


正面

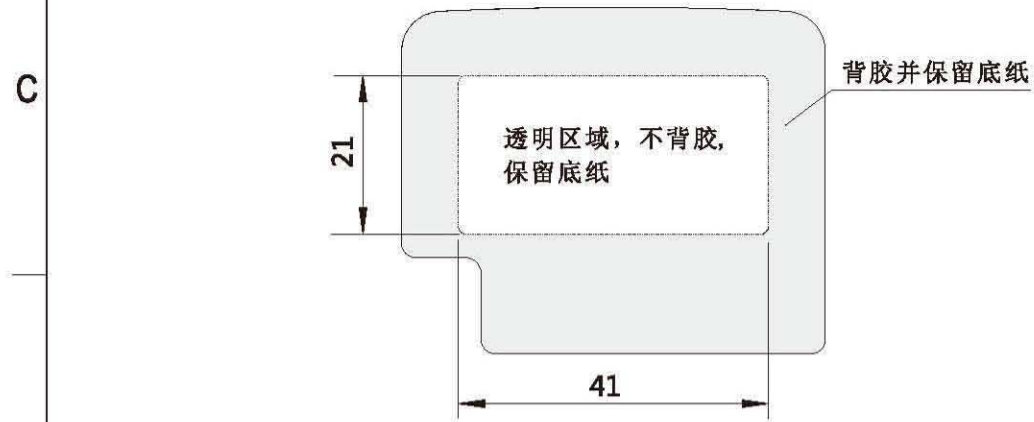

背面

REV	ECN/PCN/CR	DESCRIPTION	DESIGN
1.0	EHL014-F	新增	李琼

技术要求

- 在光滑面丝印，光滑面为反面，文字与符号的大小、位置等依1：1的电子文档；
- 颜色要求：
 底色印刷颜色色号为MR-DS193-S，要求底色色差≤1；
 文字和符号印刷 颜色色号为Pantone Cool Gray 11C；
 印刷颜色色号为Pantone Process Blue C(蓝色)；
 印刷颜色色号为Pantone 187 C(红色)；
 印刷颜色色号为Pantone 109 C(黄色)；
- 标贴外尺寸采用五金模，公差控制在±0.1mm，其它未注尺寸公差±0.1mm；
- 要求边缘光滑平整，无刀痕断口，无压痕，毛边不大于0.1mm；
- 丝印面背3M 468MP 双面胶，背胶要求粘贴力强，耐湿；
- 来料时在外包装贴上物料标贴。

APPROVALS		DATE	mindray	保密密级：秘密
DESIGN	李琼			TITLE
CHECK			DWG NO.	0155TP 主机标贴 (FDA)
CHECK			MATERIAL	8B35 磨砂面 PC t=0.125 P.CODE 0155
CHECK			SCALE	1
APPROVAL			REV.	1.0
Software & Rev: CoreIDRAW X3			PROJECTION	SIZE A4 SHEET 1 OF 1

保密：此图及其全部知识产权（含著作权）归深圳迈瑞生物医疗电子股份有限公司所有。未经深圳迈瑞生物医疗电子股份有限公司预先书面许可，严禁出于任何目的，对此图的全部或部分内容（包括但不限于图中信息、数据、运算结果等）披露、使用、拷贝或复制。
 Classified documents. This set of drawing(s) and all its intellectual property rights (including copyright) subsisting herein are property of Shenzhen Mindray Bio-medical Electronics Co., Ltd. No disclosure, use, copies or reproductions should be made of this drawing or any part(s) thereof for whatever purpose nor shall any information, data, calculations, or other contents contained in this drawing be disseminated without prior written permission of Shenzhen Mindray Bio-medical Electronics Co., Ltd.