

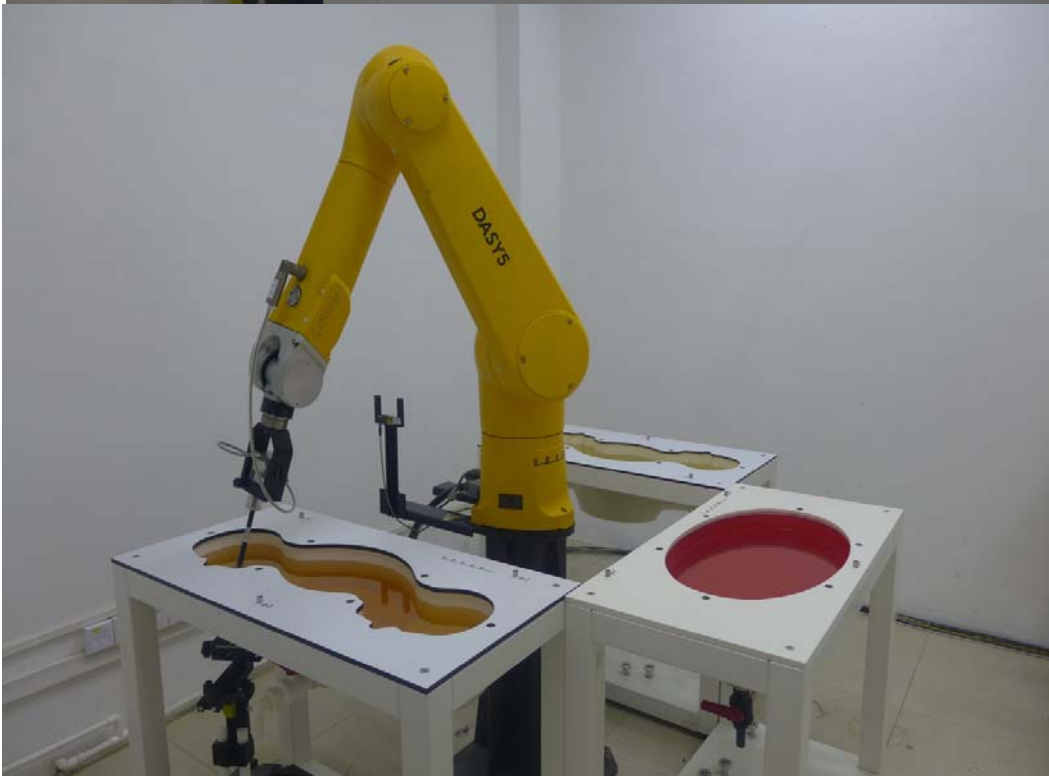
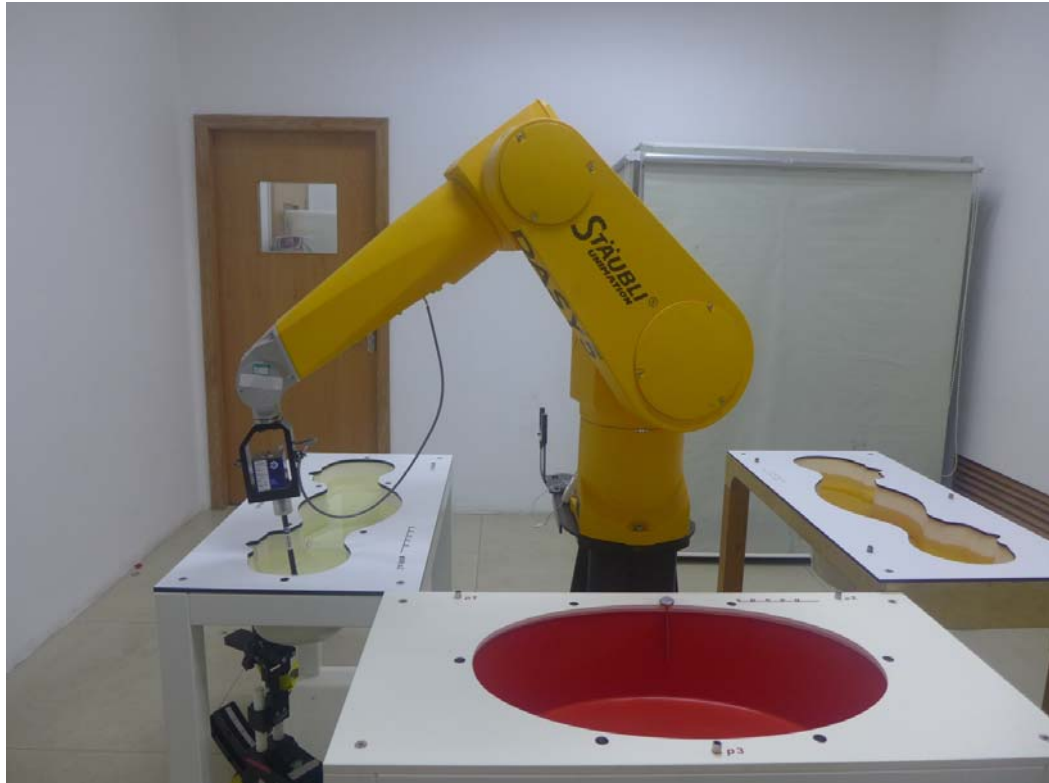


Appendix D

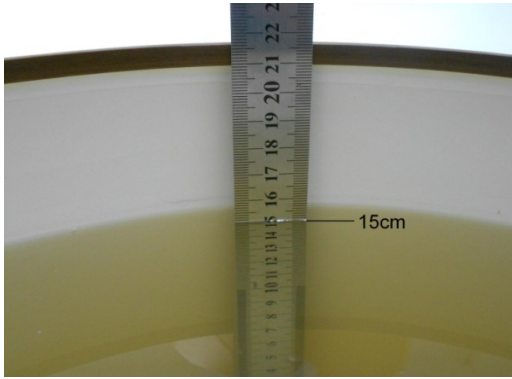



Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

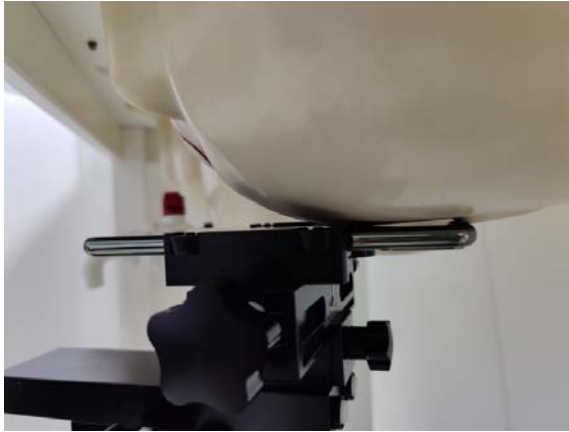

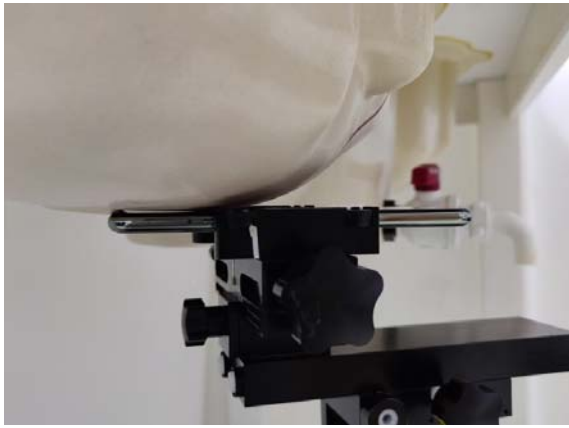



1. SAR measurement System







2. Photographs of Tissue Simulate Liquid

Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1900
 <p>15cm</p>	
Photo 3: Tissue Simulant Liquid for Head 2450	Photo 4: Tissue Simulant Liquid for Head 2600
	

3. Photographs of EUT test position

<p>Photo 5: Left touch cheek</p>	<p>Photo 6: Left tilted 15 degree</p>
	
<p>Photo 7: Right touch cheek</p>	<p>Photo 8: Right tilted 15 degree</p>
	
<p>Photo 9: Front side 10mm</p>	<p>Photo 10: Back side 10mm</p>
	

<p>Photo 11: Left side 10mm</p>	<p>Photo 12: Right side 10mm</p>
	
<p>Photo 13: Top side 10mm</p>	<p>Photo 14: Bottom side 10mm</p>
	

4. EUT Constructional Details

