

APPENDIX A: SAR TEST DATA

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, Cellular CDMA; Frequency: 820.1 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 820.1$ MHz; $\sigma = 0.936$ S/m; $\epsilon_r = 43.346$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/30/2020; Ambient Temp: 22.7°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7406; ConvF(9.61, 9.61, 9.61) @ 820.1 MHz; Calibrated: 6/23/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1583; Calibrated: 5/14/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. EVDO Rev. A, Rule Part 90S, Right Head, Cheek, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.43 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.212 W/kg

SAR(1 g) = 0.165 W/kg

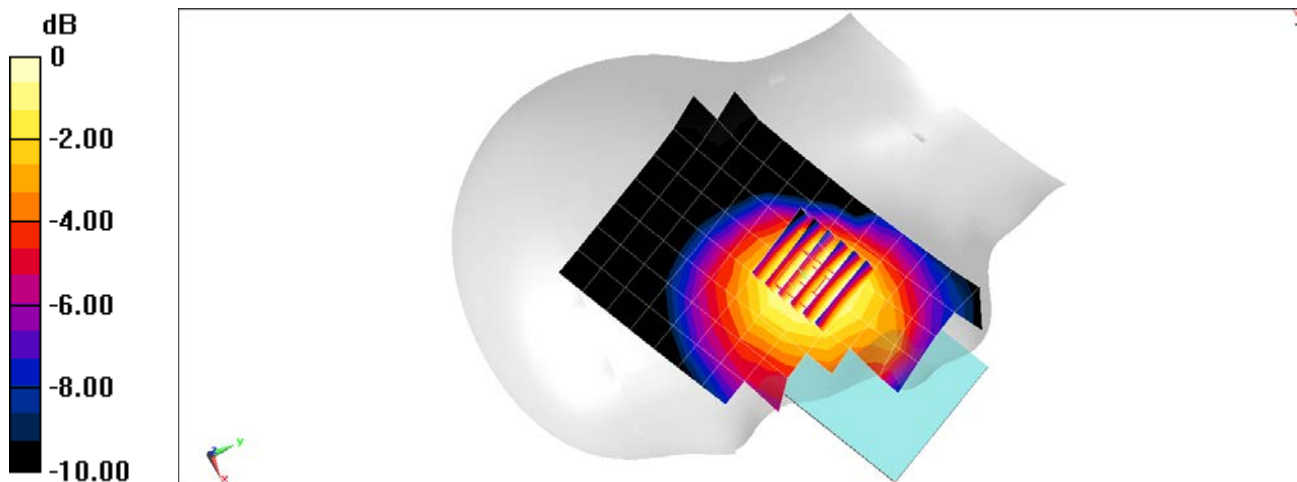

0 dB = 0.194 W/kg = -7.12 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 836.52$ MHz; $\sigma = 0.946$ S/m; $\epsilon_r = 42.969$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 10/02/2020; Ambient Temp: 22.9°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7406; ConvF(9.61, 9.61, 9.61) @ 836.52 MHz; Calibrated: 6/23/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1583; Calibrated: 5/14/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. EVDO Rev. A, Rule Part 22H, Right Head, Cheek, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 16.26 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.304 W/kg

SAR(1 g) = 0.234 W/kg

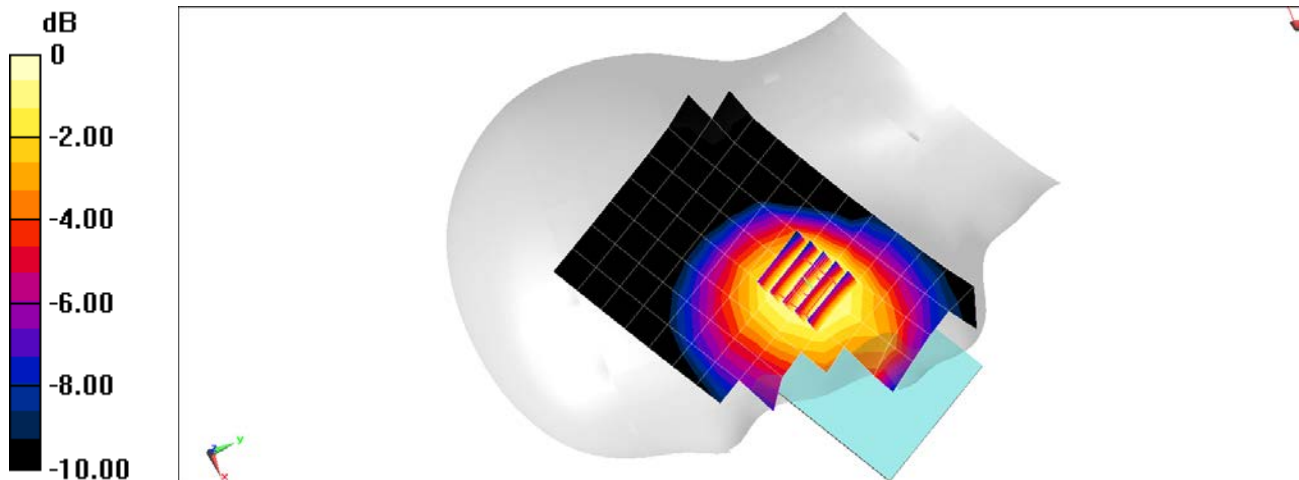

0 dB = 0.275 W/kg = -5.61 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, CDMA; Frequency: 1880 MHz; Duty Cycle: 1:1
Medium: 1900 Head Medium parameters used:
 $f = 1880 \text{ MHz}$; $\sigma = 1.443 \text{ S/m}$; $\epsilon_r = 40.771$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

Test Date: 09/28/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7406; ConvF(7.96, 7.96, 7.96) @ 1880 MHz; Calibrated: 6/23/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1583; Calibrated: 5/14/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: PCS EVDO Rev A, Right Head, Cheek, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.26 V/m; Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.244 W/kg

SAR(1 g) = 0.156 W/kg

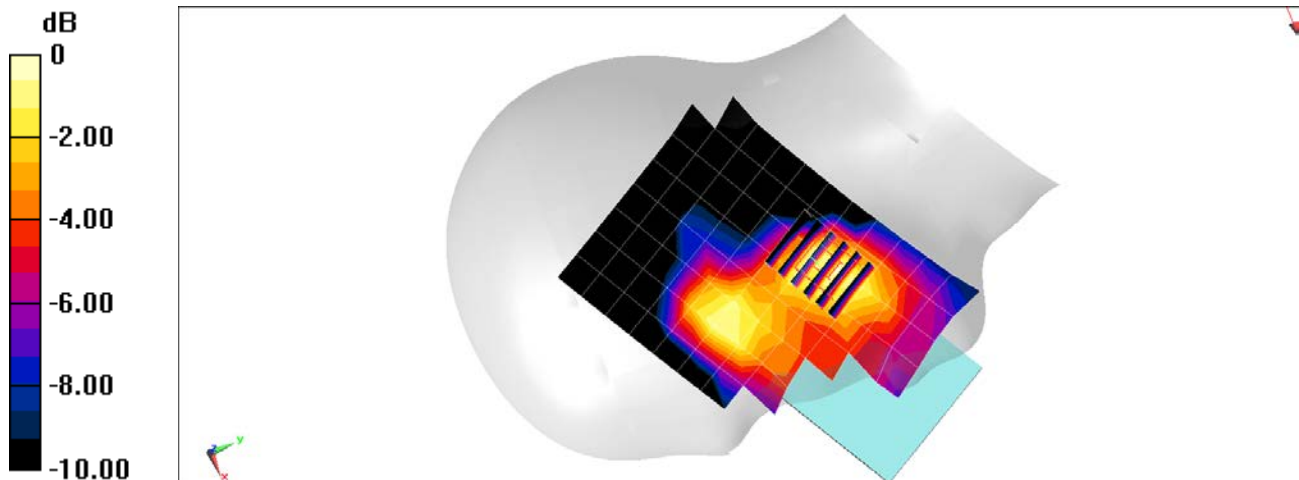

0 dB = 0.204 W/kg = -6.90 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, GSM GPRS; 3 Tx slots; Frequency: 836.6 MHz; Duty Cycle: 1:2.76
Medium: 835 Head Medium parameters used (interpolated):
 $f = 836.6$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 40.361$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/22/2020; Ambient Temp: 22.2°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7427; ConvF(9.58, 9.58, 9.58) @ 836.6 MHz; Calibrated: 2/19/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1403; Calibrated: 2/13/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: GPRS 850, Right Head, Cheek, Mid.ch, 3 Tx Slots


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 10.66 V/m; Power Drift = 0.10 dB

Peak SAR (extrapolated) = 0.120 W/kg

SAR(1 g) = 0.098 W/kg

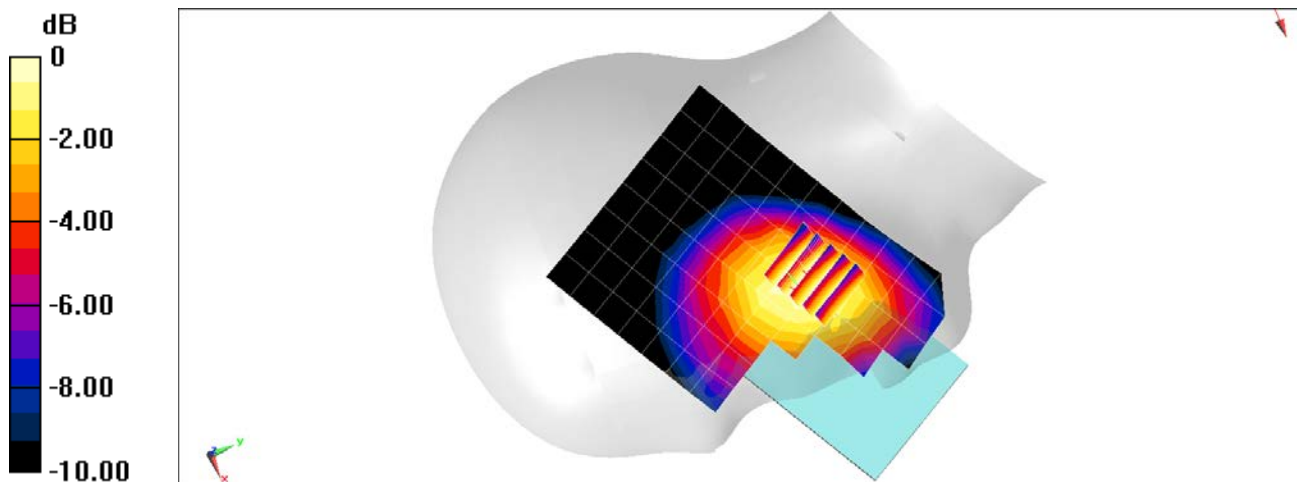

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, GSM GPRS; 3 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:2.76

Medium: 1900 Head Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.409$ S/m; $\epsilon_r = 38.908$; $\rho = 1000$ kg/m³

Phantom section: Left Section

Test Date: 09/23/2020; Ambient Temp: 23.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7532; ConvF(8.06, 8.06, 8.06) @ 1880 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: GPRS 1900, Left Head, Cheek, Mid.ch, 3 Tx Slots


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 9.139 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 0.183 W/kg

SAR(1 g) = 0.117 W/kg

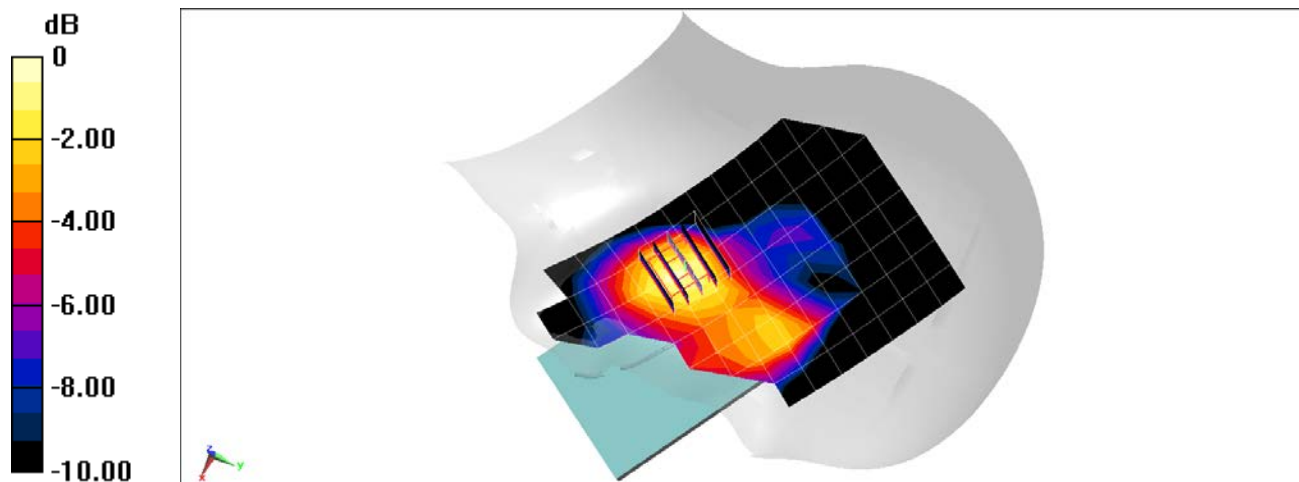

0 dB = 0.156 W/kg = -8.07 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 01579

Communication System: UID 0, UMTS; Frequency: 836.6 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 836.6$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 40.361$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/22/2020; Ambient Temp: 22.2°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7427; ConvF(9.58, 9.58, 9.58) @ 836.6 MHz; Calibrated: 2/19/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1403; Calibrated: 2/13/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 850, Right Head, Cheek, Mid.ch


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.73 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 0.197 W/kg

SAR(1 g) = 0.159 W/kg

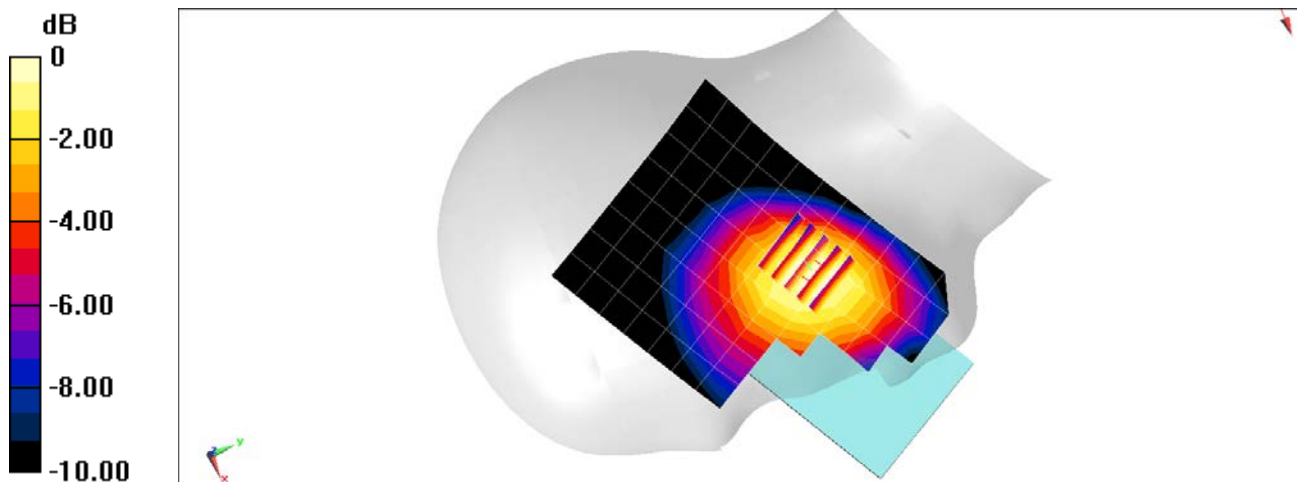

0 dB = 0.187 W/kg = -7.28 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 01581

Communication System: UID 0, UMTS; Frequency: 1732.4 MHz; Duty Cycle: 1:1
Medium: 1750 Head Medium parameters used (interpolated):
 $f = 1732.4$ MHz; $\sigma = 1.325$ S/m; $\epsilon_r = 39.269$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/18/2020; Ambient Temp: 20.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7532; ConvF(8.46, 8.46, 8.46) @ 1732.4 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1750, Left Head, Cheek, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 4.028 V/m; Power Drift = 0.11 dB

Peak SAR (extrapolated) = 0.208 W/kg

SAR(1 g) = 0.136 W/kg

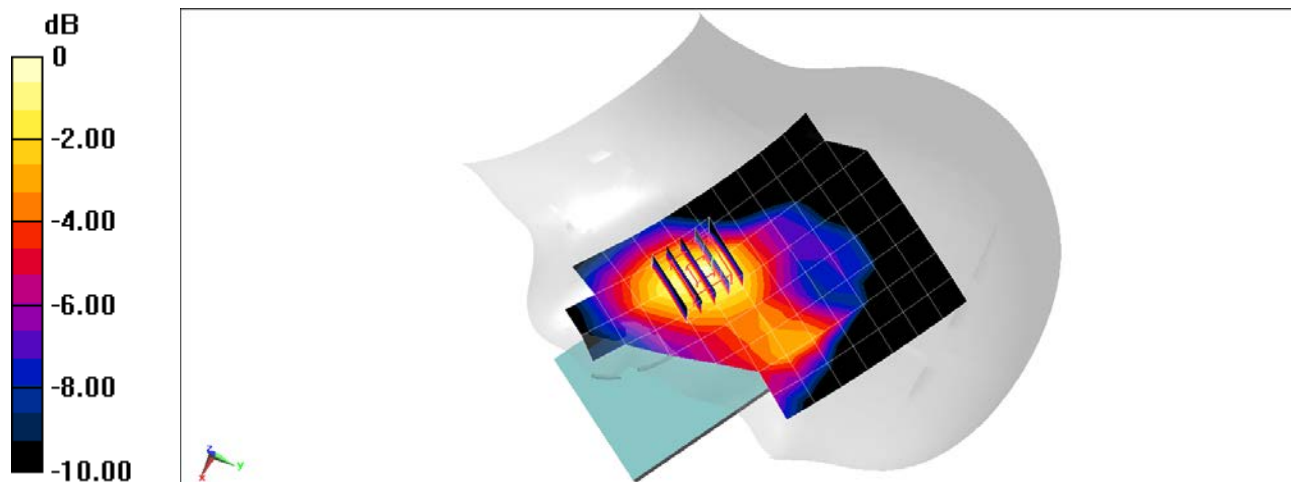

0 dB = 0.177 W/kg = -7.52 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, UMTS; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.409$ S/m; $\epsilon_r = 38.908$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Test Date: 09/23/2020; Ambient Temp: 23.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7532; ConvF(8.06, 8.06, 8.06) @ 1880 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1900, Right Head, Cheek, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.37 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.392 W/kg

SAR(1 g) = 0.234 W/kg

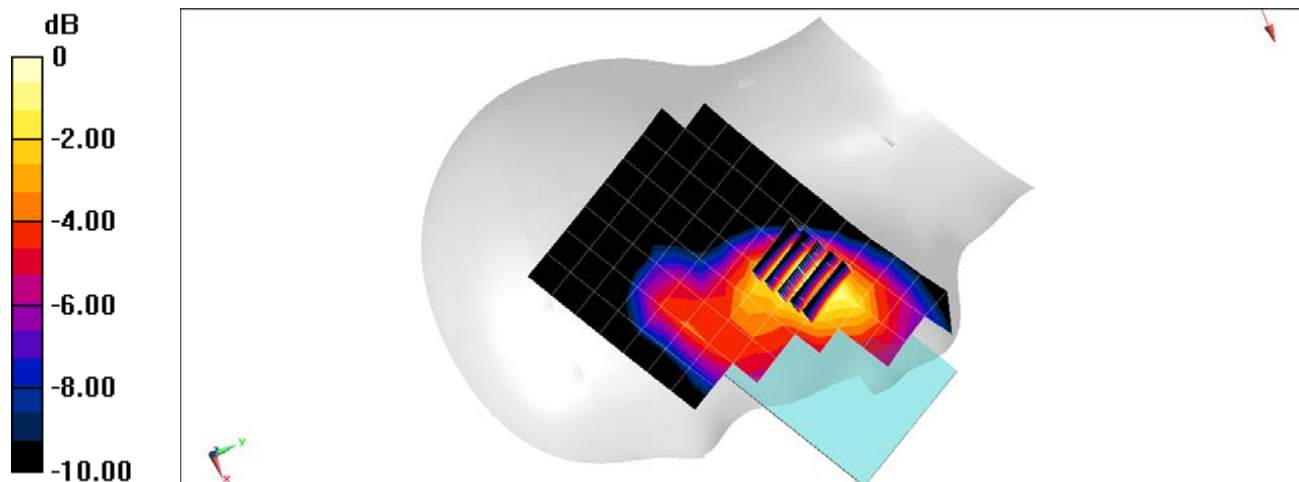

0 dB = 0.320 W/kg = -4.95 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803

Communication System: UID 0, LTE Band 71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Head Medium parameters used (interpolated):
 $f = 680.5$ MHz; $\sigma = 0.875$ S/m; $\epsilon_r = 40.656$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/22/2020; Ambient Temp: 20.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7490; ConvF(10.25, 10.25, 10.25) @ 680.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) Main use; Type: QD 000 P40 CC; Serial: 1406
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 71, Left Head, Cheek, Mid.ch,
20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.36 V/m; Power Drift = 0.18 dB

Peak SAR (extrapolated) = 0.177 W/kg

SAR(1 g) = 0.151 W/kg

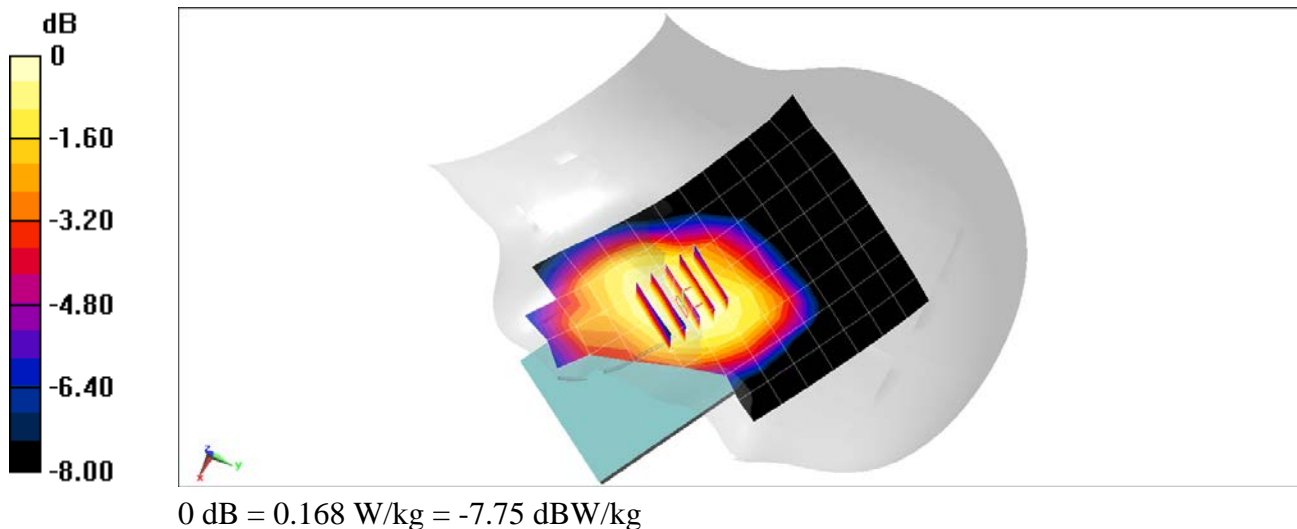

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 12; Frequency: 707.5 MHz; Duty Cycle: 1:1
Medium: 750 Head Medium parameters used (interpolated):
 $f = 707.5$ MHz; $\sigma = 0.884$ S/m; $\epsilon_r = 41.702$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/25/2020; Ambient Temp: 22.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7532; ConvF(10.72, 10.72, 10.72) @ 707.5 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 12, Right Head, Cheek, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 49 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 14.14 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 0.201 W/kg

SAR(1 g) = 0.159 W/kg

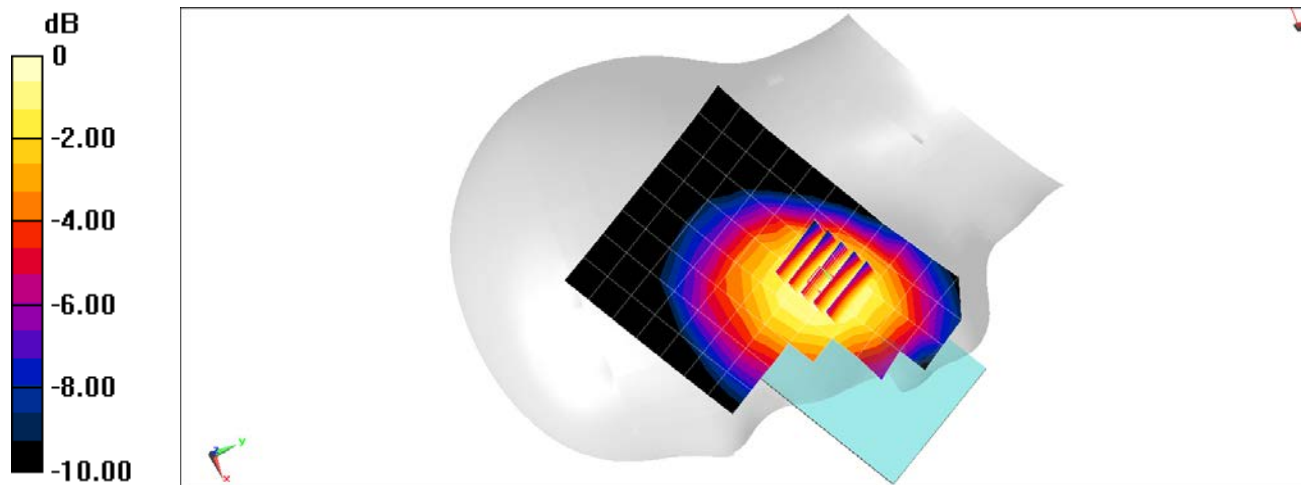

0 dB = 0.186 W/kg = -7.30 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, LTE Band 13; Frequency: 782 MHz; Duty Cycle: 1:1
Medium: 750 Head Medium parameters used (interpolated):
 $f = 782 \text{ MHz}$; $\sigma = 0.911 \text{ S/m}$; $\epsilon_r = 41.49$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

Test Date: 09/25/2020; Ambient Temp: 22.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7532; ConvF(10.72, 10.72, 10.72) @ 782 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 13, Right Head, Cheek, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.92 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.202 W/kg

SAR(1 g) = 0.160 W/kg

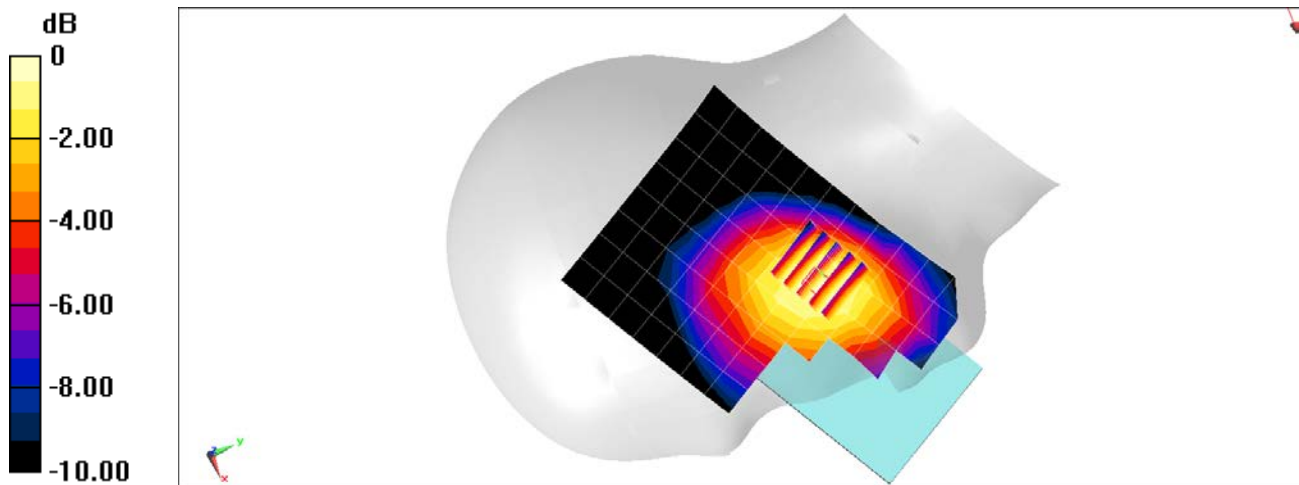

0 dB = 0.188 W/kg = -7.26 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 14; Frequency: 793 MHz; Duty Cycle: 1:1
Medium: 750 Head Medium parameters used (interpolated):
 $f = 793 \text{ MHz}$; $\sigma = 0.915 \text{ S/m}$; $\epsilon_r = 41.458$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

Test Date: 09/25/2020; Ambient Temp: 22.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7532; ConvF(10.72, 10.72, 10.72) @ 793 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 14, Right Head, Cheek, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (9x13x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 12.10 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 0.157 W/kg

SAR(1 g) = 0.124 W/kg

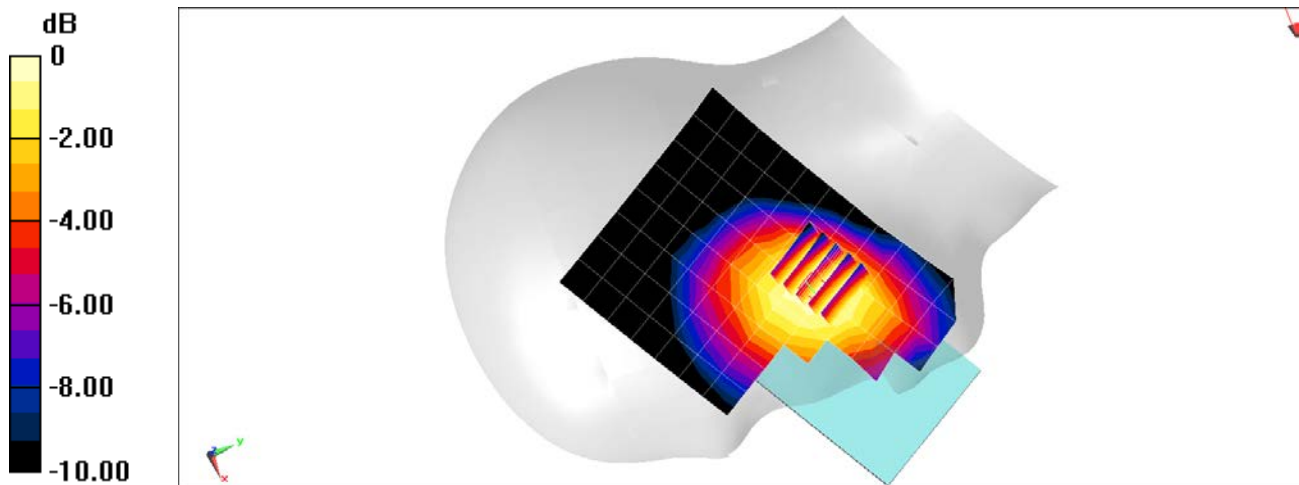

0 dB = 0.144 W/kg = -8.42 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, LTE Band 26; Frequency: 831.5 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 831.5$ MHz; $\sigma = 0.941$ S/m; $\epsilon_r = 43.306$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/29/2020; Ambient Temp: 22.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7421; ConvF(9.24, 9.24, 9.24) @ 831.5 MHz; Calibrated: 3/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn604; Calibrated: 3/19/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 26 (Cell.), Right Head, Cheek, Mid.ch,
15 MHz Bandwidth, QPSK, 1 RB, 36 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 12.06 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.149 W/kg

SAR(1 g) = 0.122 W/kg

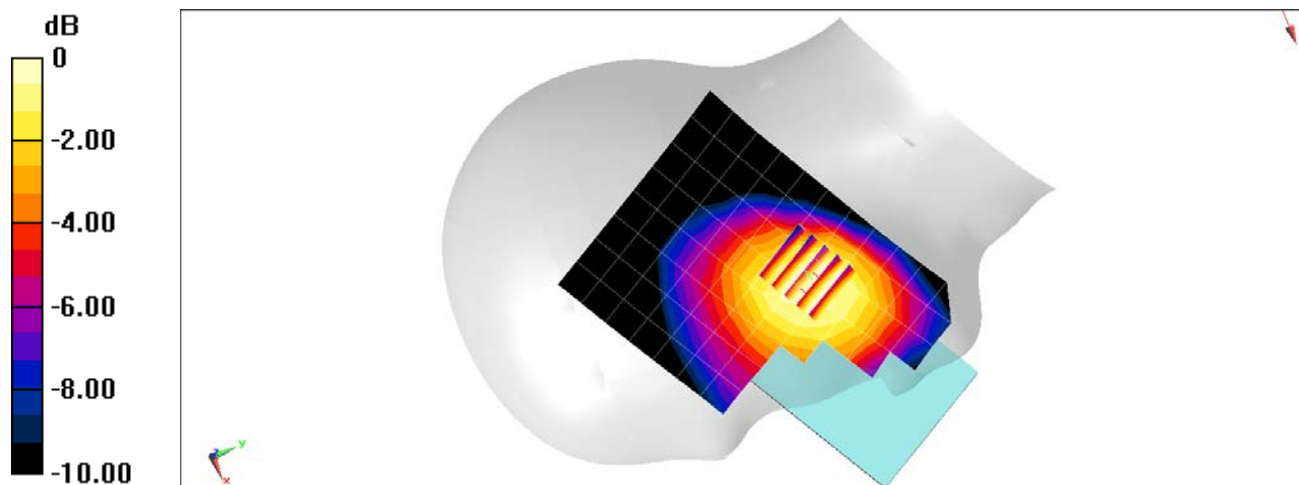

0 dB = 0.140 W/kg = -8.54 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 5 (Cell.); Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 0.891$ S/m; $\epsilon_r = 40.497$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/24/2020; Ambient Temp: 22.4°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7427; ConvF(9.58, 9.58, 9.58) @ 836.5 MHz; Calibrated: 2/19/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1403; Calibrated: 2/13/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 5 (Cell.), Right Head, Cheek, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.92 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.190 W/kg

SAR(1 g) = 0.155 W/kg

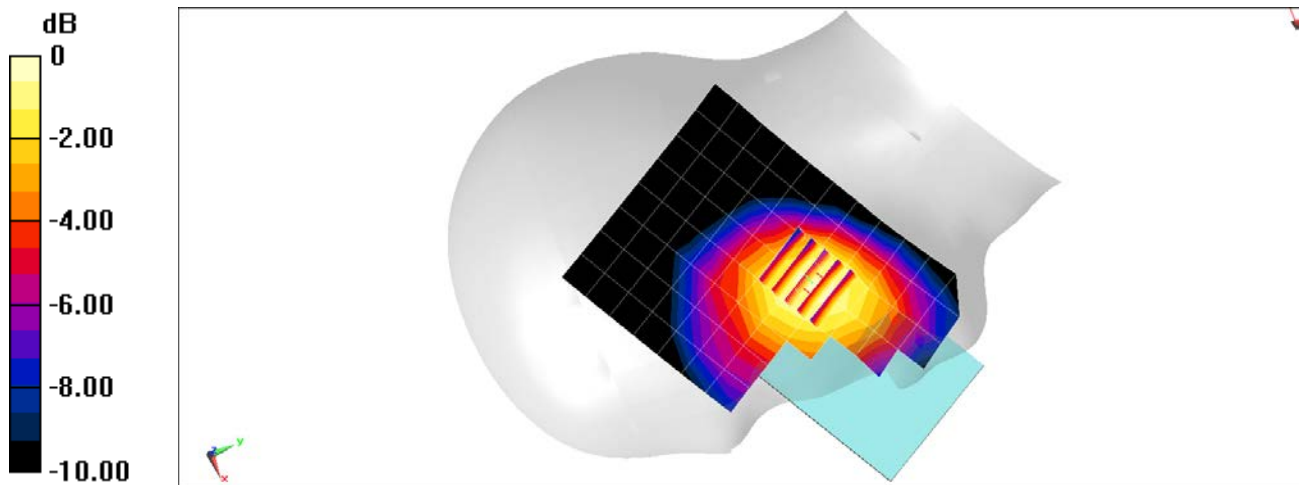

0 dB = 0.181 W/kg = -7.42 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803


Communication System: UID 0, LTE Band 66 (AWS); Frequency: 1720 MHz; Duty Cycle: 1:1
Medium: 1750 Head Medium parameters used (interpolated):
 $f = 1720$ MHz; $\sigma = 1.315$ S/m; $\epsilon_r = 38.834$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/21/2020; Ambient Temp: 20.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7532; ConvF(8.46, 8.46, 8.46) @ 1720 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 66 (AWS), Antenna 7, Left Head, Cheek, Low.ch,
20 MHz Bandwidth, QPSK, 1 RB, 99 RB Offset**

Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 19.98 V/m; Power Drift = 0.05 dB
Peak SAR (extrapolated) = 1.10 W/kg
SAR(1 g) = 0.466 W/kg

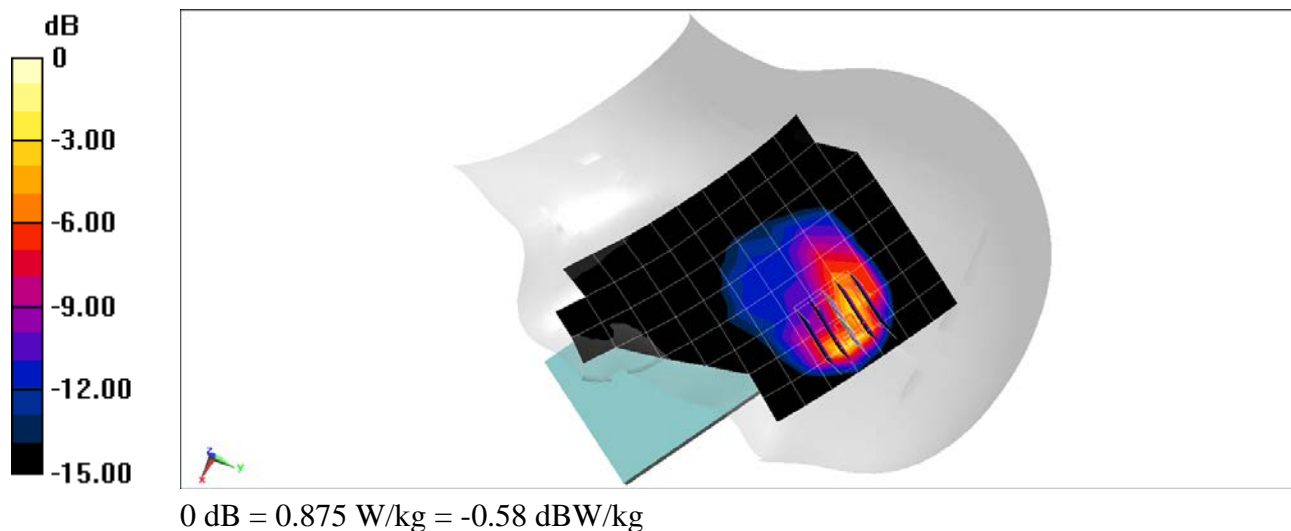

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803

Communication System: UID 0, LTE Band 25 (PCS); Frequency: 1860 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used (interpolated):

$f = 1860$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 38.979$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Test Date: 09/23/2020; Ambient Temp: 23.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7532; ConvF(8.06, 8.06, 8.06) @ 1860 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 25 (PCS), Right Head, Cheek, Low.ch,
20 MHz Bandwidth, QPSK, 1 RB, 99 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 9.933 V/m; Power Drift = 0.17 dB

Peak SAR (extrapolated) = 0.186 W/kg

SAR(1 g) = 0.115 W/kg

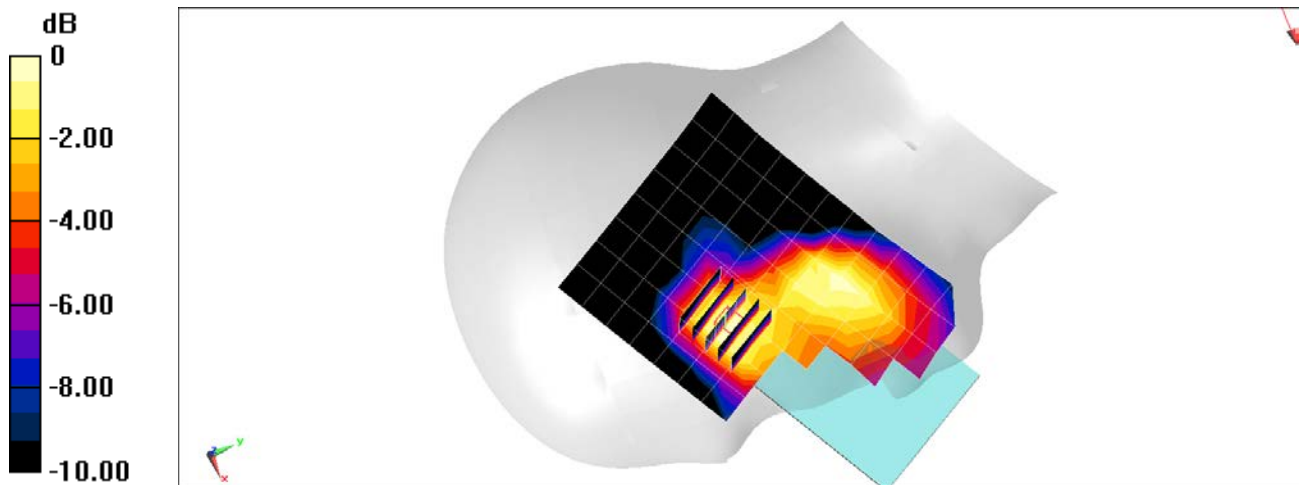

0 dB = 0.157 W/kg = -8.04 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 01581

Communication System: UID 0, LTE Band 2 (PCS); Frequency: 1860 MHz; Duty Cycle: 1:1
Medium: 1900 Head Medium parameters used (interpolated):
 $f = 1860$ MHz; $\sigma = 1.408$ S/m; $\epsilon_r = 38.763$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/28/2020; Ambient Temp: 21.9°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7427; ConvF(8.12, 8.12, 8.12) @ 1860 MHz; Calibrated: 2/19/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1403; Calibrated: 2/13/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 2 (PCS), Antenna 7, Left Head, Cheek, Low.ch,
20 MHz Bandwidth, QPSK, 1 RB, 50 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 22.86 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 1.28 W/kg

SAR(1 g) = 0.544 W/kg

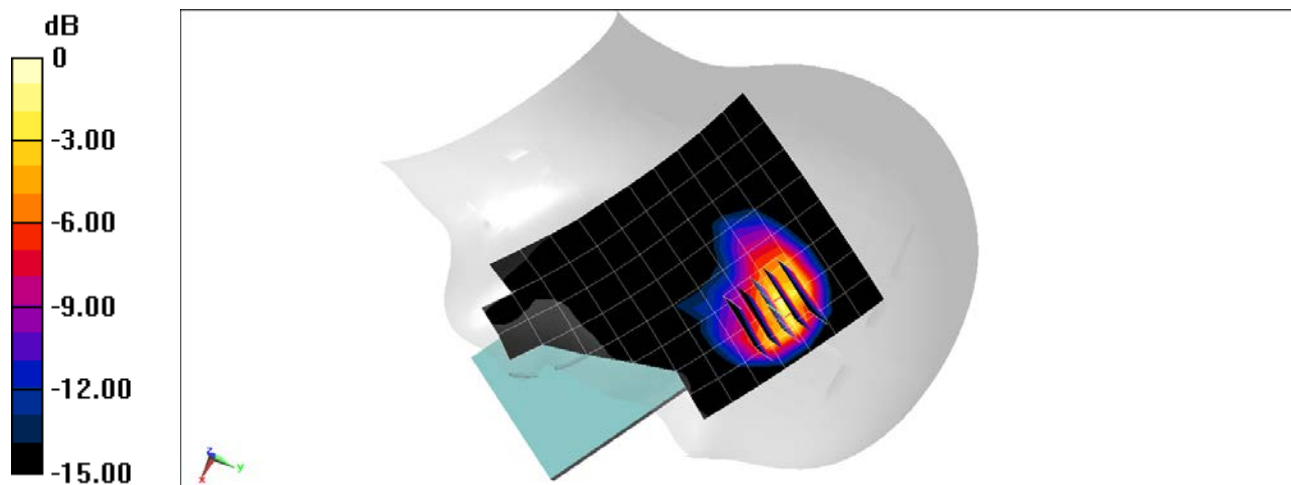

0 dB = 1.00 W/kg = 0.00 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, LTE Band 30; Frequency: 2310 MHz; Duty Cycle: 1:1
Medium: 2450 Head Medium parameters used:
 $f = 2310$ MHz; $\sigma = 1.648$ S/m; $\epsilon_r = 39.837$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/25/2020; Ambient Temp: 23.0°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 2310 MHz; Calibrated: 3/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn604; Calibrated: 3/19/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 30, Antenna 7, Left Head, Cheek, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 19.17 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 1.20 W/kg

SAR(1 g) = 0.458 W/kg

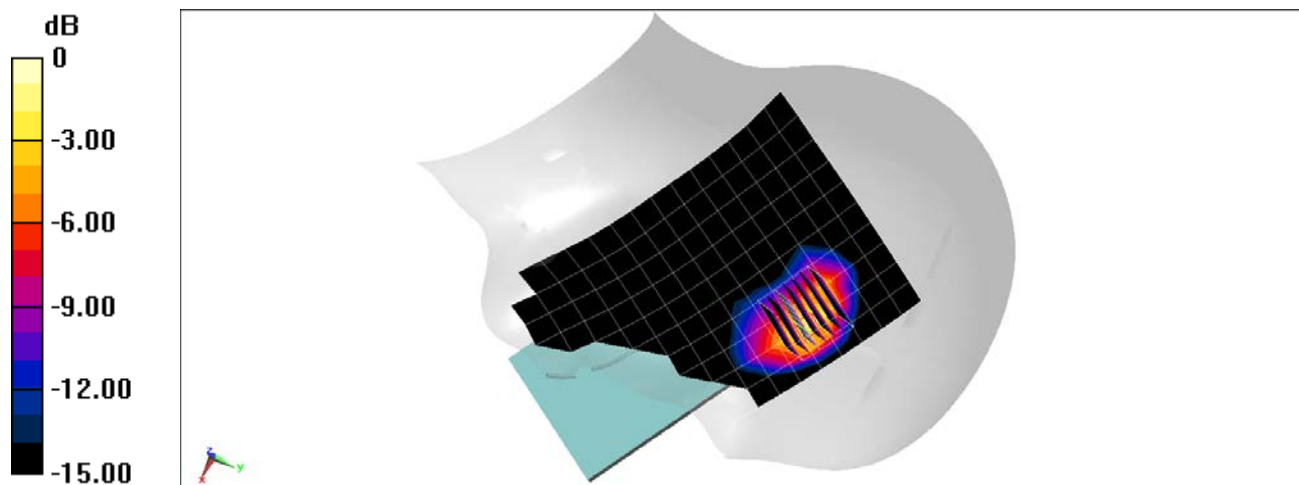

0 dB = 0.884 W/kg = -0.54 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 01581

Communication System: UID 0, LTE Band 41 (Class 3); Frequency: 2680 MHz; Duty Cycle: 1:1.58

Medium: 2450 Head Medium parameters used (interpolated):

$f = 2680$ MHz; $\sigma = 2.08$ S/m; $\epsilon_r = 38.404$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Test Date: 09/25/2020; Ambient Temp: 23.0°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7421; ConvF(7.24, 7.24, 7.24) @ 2680 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: LTE Band 41, ULCA, Right Head, Cheek,

PCC: Ch. 41490, 20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset

SCC: Ch. 41292, 20 MHz Bandwidth, QPSK, 1 RB, 99 RB Offset


Area Scan (11x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 9.930 V/m; Power Drift = 0.15 dB

Peak SAR (extrapolated) = 0.274 W/kg

SAR(1 g) = 0.137 W/kg

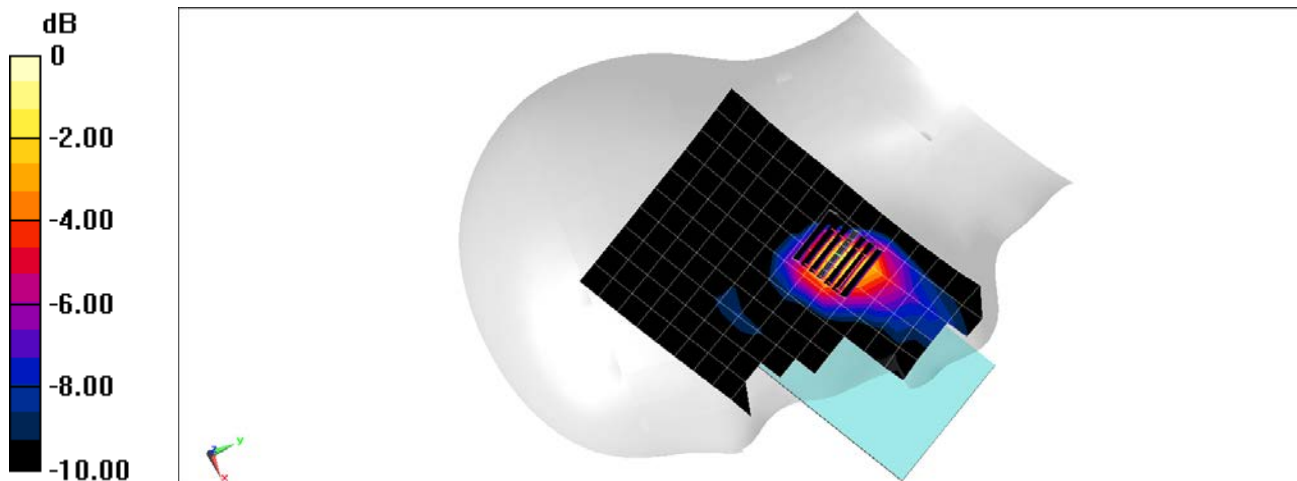

0 dB = 0.220 W/kg = -6.58 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15829

Communication System: UID 0, NR Band n71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Head Medium parameters used (interpolated):
 $f = 680.5$ MHz; $\sigma = 0.876$ S/m; $\epsilon_r = 41.774$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/25/2020; Ambient Temp: 22.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7532; ConvF(10.72, 10.72, 10.72) @ 680.5 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n71, Right Head, Cheek, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 136100, 1 RB, 1 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.73 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 0.136 W/kg

SAR(1 g) = 0.109 W/kg

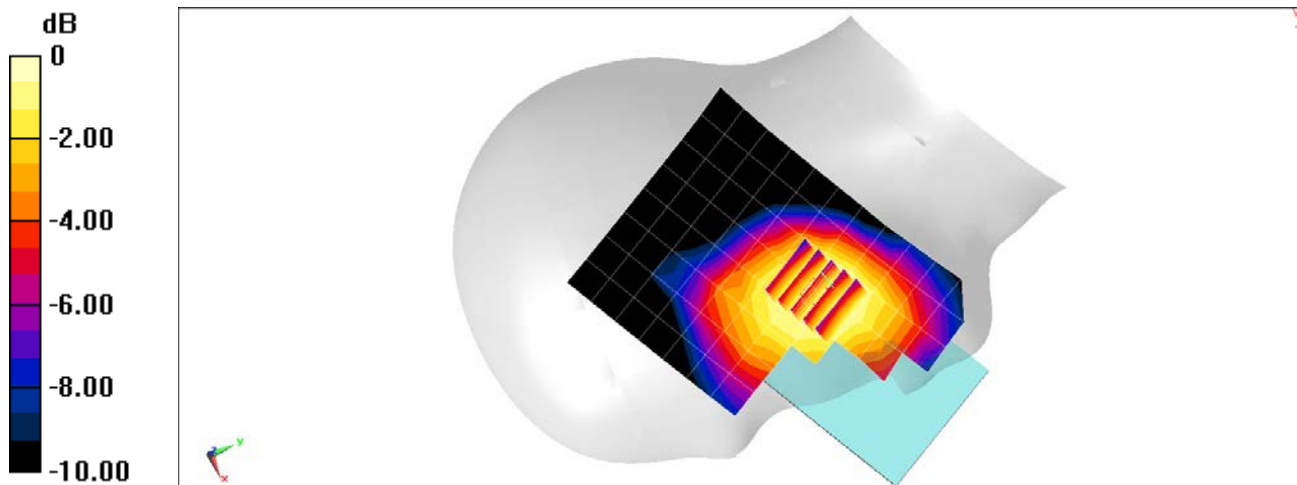

0 dB = 0.127 W/kg = -8.96 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 11257

Communication System: UID 0, NR Band n5; Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Head Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 0.943$ S/m; $\epsilon_r = 43.29$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 09/29/2020; Ambient Temp: 22.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7421; ConvF(9.24, 9.24, 9.24) @ 836.5 MHz; Calibrated: 3/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn604; Calibrated: 3/19/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n5, Right Head, Cheek, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 167300, 1 RB, 1 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 15.10 V/m; Power Drift = 0.08 dB

Peak SAR (extrapolated) = 0.240 W/kg

SAR(1 g) = 0.193 W/kg

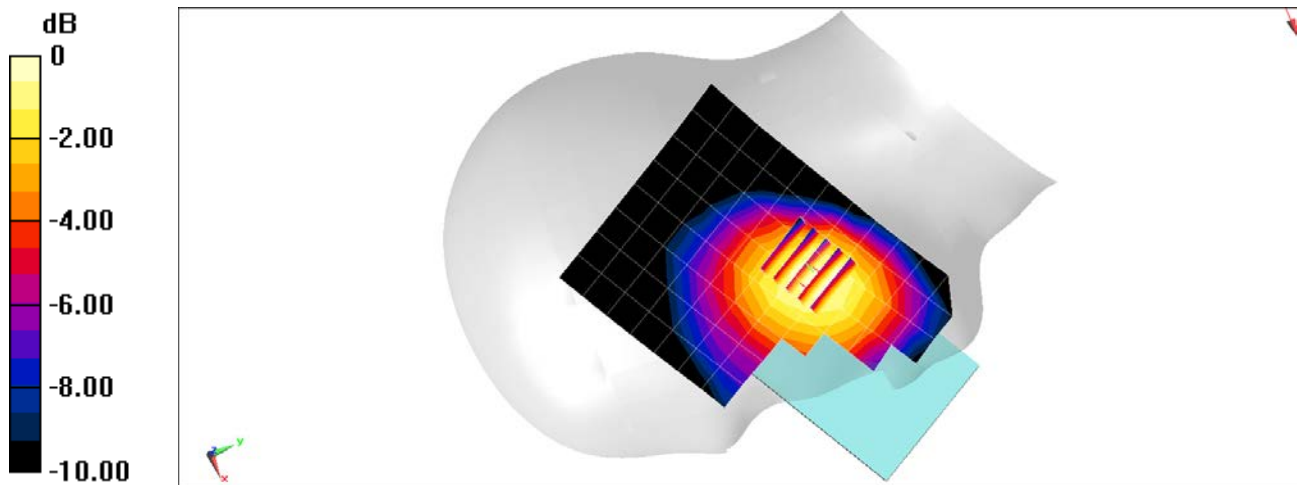

0 dB = 0.225 W/kg = -6.48 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 11257


Communication System: UID 0, NR Band n66; Frequency: 1770 MHz; Duty Cycle: 1:1
Medium: 1750 Head Medium parameters used (interpolated):
 $f = 1770$ MHz; $\sigma = 1.358$ S/m; $\epsilon_r = 38.811$; $\rho = 1000$ kg/m³
Phantom section: Left Section

Test Date: 09/29/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7427; MHz, ConvF(8.42, 8.42, 8.42) @ 1770 MHz; Calibrated: 2/19/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1403; Calibrated: 2/13/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n66, Left Head, Cheek, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 354000, 1 RB, 1 RB Offset**

Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 26.88 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 1.59 W/kg
SAR(1 g) = 0.682 W/kg;

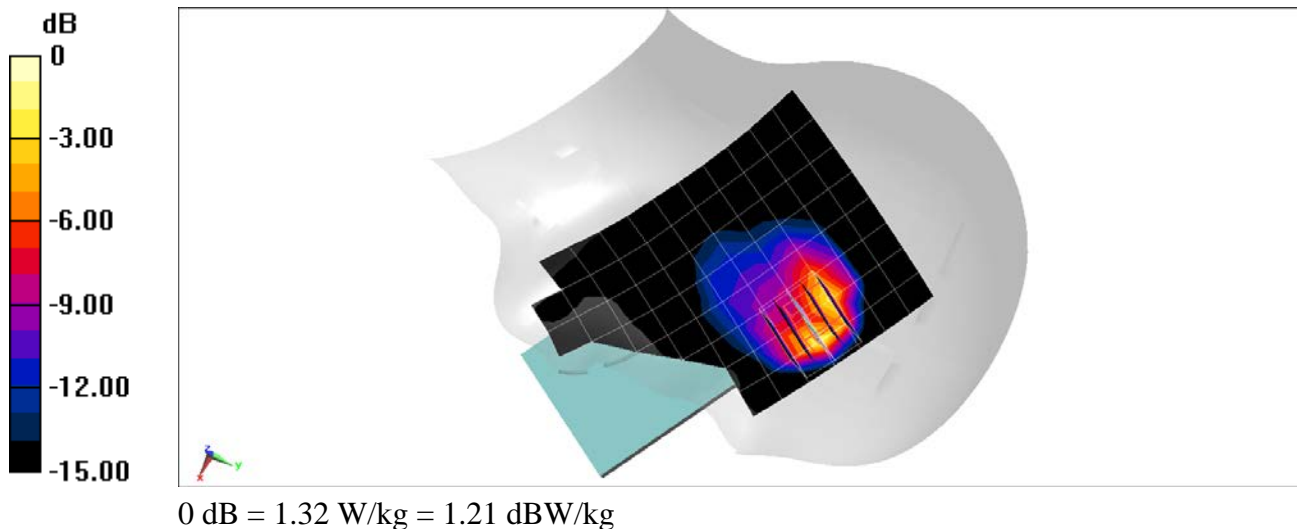

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837

Communication System: UID 0, NR Band n2; Frequency: 1900 MHz; Duty Cycle: 1:1
Medium: 1900 Head Medium parameters used (interpolated):
 $f = 1900 \text{ MHz}$; $\sigma = 1.427 \text{ S/m}$; $\epsilon_r = 38.835$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Left Section

Test Date: 09/23/2020; Ambient Temp: 23.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7532; ConvF(8.06, 8.06, 8.06) @ 1900 MHz; Calibrated: 4/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn501; Calibrated: 4/15/2020
Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n2, Left Head, Cheek, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 380000, 50 RB, 56 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 28.98 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 2.36 W/kg

SAR(1 g) = 0.976 W/kg

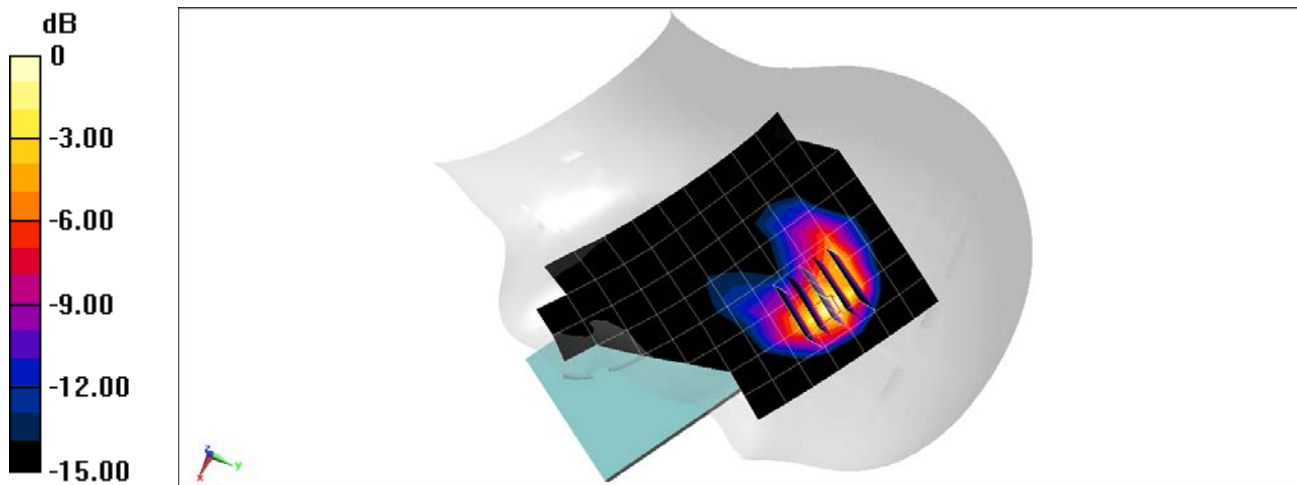

0 dB = 1.68 W/kg = 2.25 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15951

Communication System: UID 0, _IEEE 802.11b; Frequency: 2462 MHz; Duty Cycle: 1:1
Medium: 2450 Head Medium parameters used (interpolated):
 $f = 2462 \text{ MHz}$; $\sigma = 1.836 \text{ S/m}$; $\epsilon_r = 38.773$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Right Section

Test Date: 09/29/2020; Ambient Temp: 23.1°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN3589; ConvF(6.85, 6.85, 6.85) @ 2462 MHz; Calibrated: 1/21/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1558; Calibrated: 1/13/2020
Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1647
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: IEEE 802.11b, Antenna 1, 22 MHz Bandwidth, Right Head, Cheek, Ch 11, 1 Mbps


Area Scan (11x18x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (8x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 2.666 V/m; Power Drift = -0.19 dB

Peak SAR (extrapolated) = 1.56 W/kg

SAR(1 g) = 0.536 W/kg

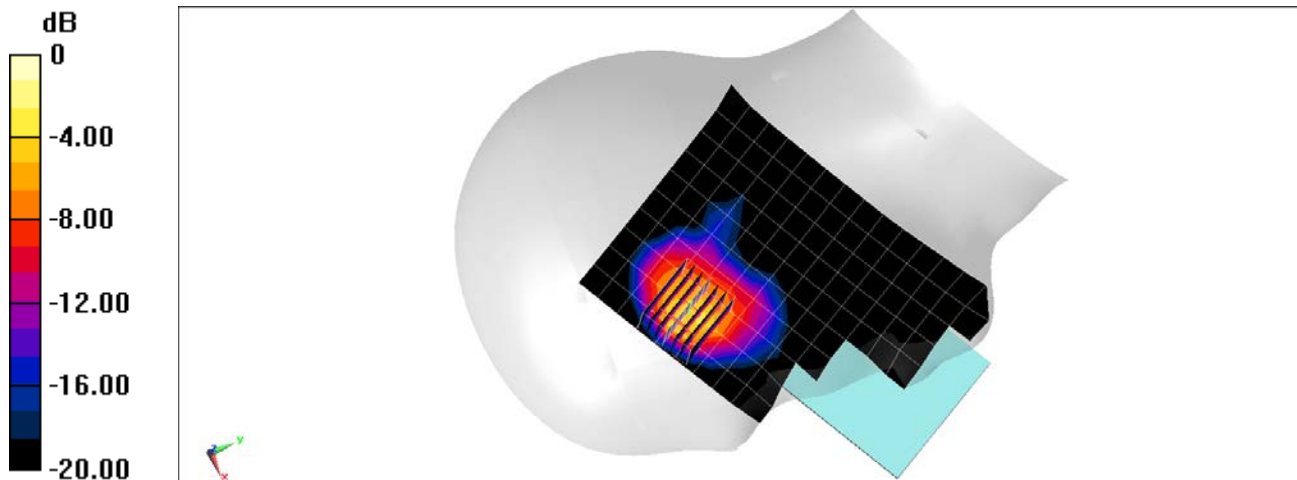

0 dB = 1.17 W/kg = 0.68 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15936

Communication System: UID 0, _IEEE 802.11n; Frequency: 5710 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Head Medium parameters used:

$f = 5710$ MHz; $\sigma = 4.947$ S/m; $\epsilon_r = 34.529$; $\rho = 1000$ kg/m³

Phantom section: Right Section

Test Date: 09/28/2020; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(4.7, 4.7, 4.7) @ 5710 MHz; Calibrated: 4/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/15/2020

Phantom: Twin-SAM V5.0(20); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: IEEE 802.11n, MIMO, U-NII-2C, 40 MHz Bandwidth,
Right Head, Cheek, Ch 142, 27 Mbps**


Area Scan (13x22x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (9x9x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Reference Value = 10.89 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 2.16 W/kg

SAR(1 g) = 0.486 W/kg

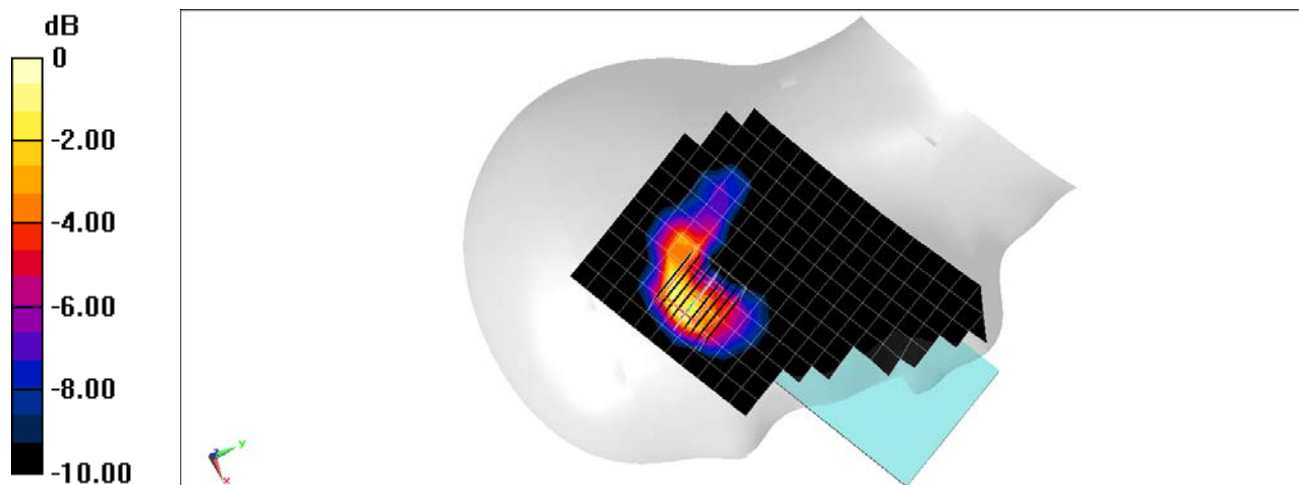

0 dB = 1.18 W/kg = 0.72 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15951

Communication System: UID 0, Bluetooth; Frequency: 2441 MHz; Duty Cycle: 1:1.300
Medium: 2450 Head Medium parameters used (interpolated):
 $f = 2441$ MHz; $\sigma = 1.823$ S/m; $\epsilon_r = 38.341$; $\rho = 1000$ kg/m³
Phantom section: Right Section

Test Date: 10/02/2020; Ambient Temp: 23.1°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN3589; ConvF(6.85, 6.85, 6.85) @ 2441 MHz; Calibrated: 1/21/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1558; Calibrated: 1/13/2020
Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1647
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Bluetooth, Right Head, Cheek, Ch 39, 1Mbps


Area Scan (11x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 11.36 V/m; Power Drift = -0.12 dB

Peak SAR (extrapolated) = 0.636 W/kg

SAR(1 g) = 0.219 W/kg

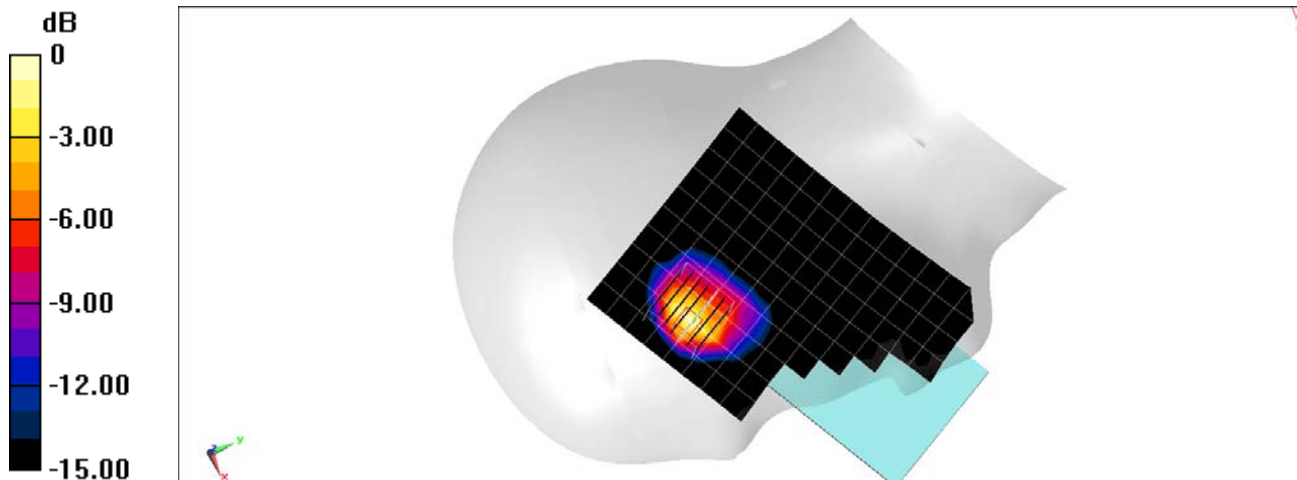

0 dB = 0.406 W/kg = -3.91 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92638

Communication System: UID 0, CDMA; Frequency: 820.1 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 820.1$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 54.755$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7308; ConvF(9.92, 9.92, 9.92) @ 820.1 MHz; Calibrated: 7/31/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1450; Calibrated: 8/11/2020
Phantom: Twin-SAM V5.0; Type: QD 000 P40 CD; Serial: 1792
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. CDMA Rule Part 90S, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 21.64 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 0.676 W/kg

SAR(1 g) = 0.419 W/kg

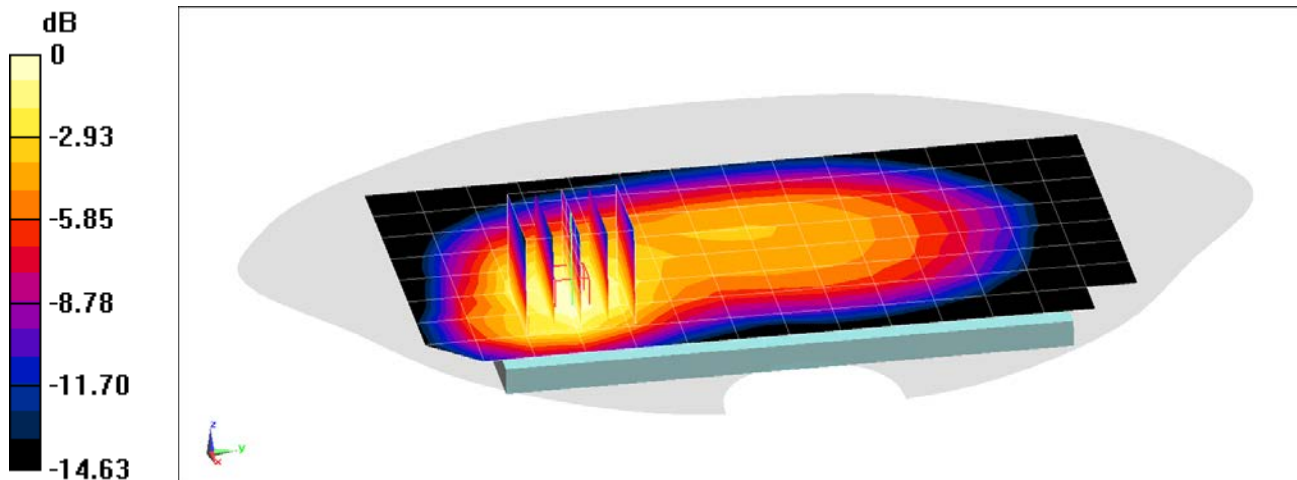

0 dB = 0.581 W/kg = -2.36 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92638

Communication System: UID 0, CDMA; Frequency: 820.1 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 820.1$ MHz; $\sigma = 0.938$ S/m; $\epsilon_r = 54.755$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7308; ConvF(9.92, 9.92, 9.92) @ 820.1 MHz; Calibrated: 7/31/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1450; Calibrated: 8/11/2020
Phantom: Twin-SAM V5.0; Type: QD 000 P40 CD; Serial: 1792
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. EVDO Rule Part 90S, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 22.16 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.720 W/kg

SAR(1 g) = 0.440 W/kg

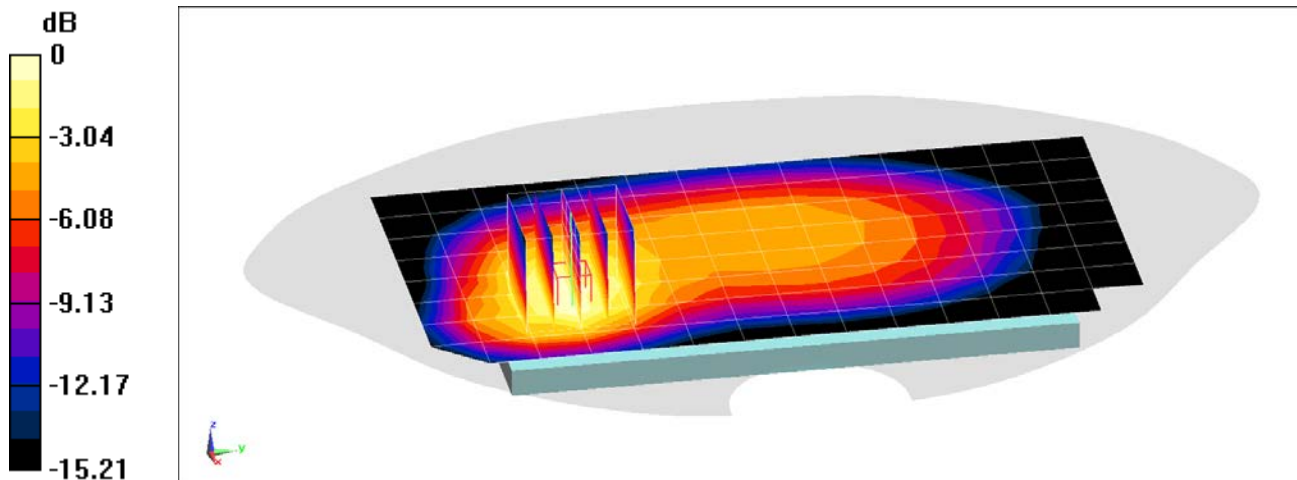

0 dB = 0.611 W/kg = -2.14 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92638

Communication System: UID 0, CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.52$ MHz; $\sigma = 0.956$ S/m; $\epsilon_r = 54.589$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7308; ConvF(9.92, 9.92, 9.92) @ 836.52 MHz; Calibrated: 7/31/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1450; Calibrated: 8/11/2020
Phantom: Twin-SAM V5.0; Type: QD 000 P40 CD; Serial: 1792
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. CDMA Rule Part 22H, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 23.63 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.818 W/kg

SAR(1 g) = 0.508 W/kg

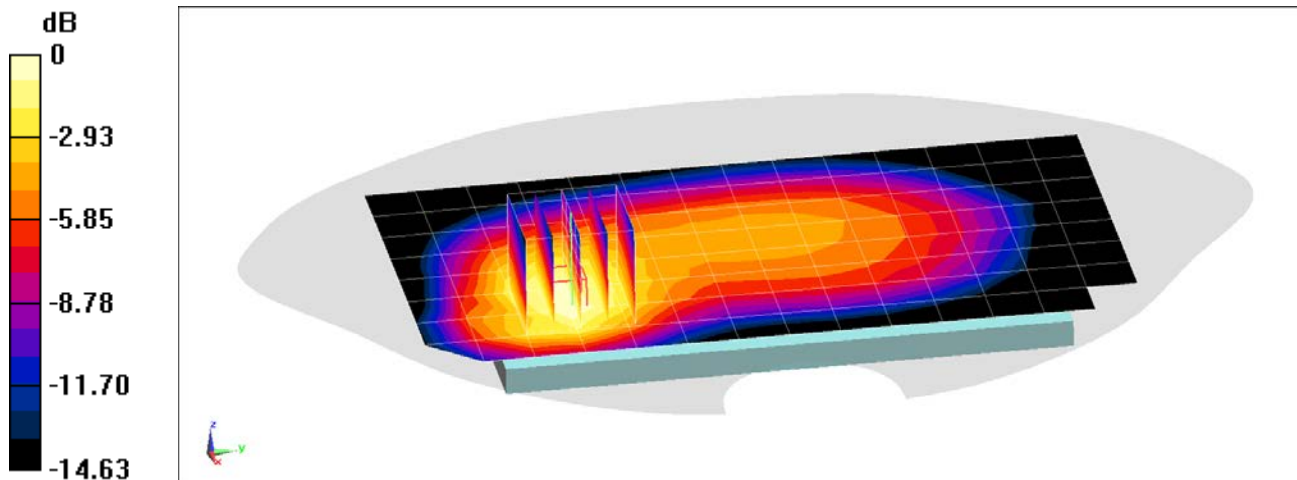

0 dB = 0.698 W/kg = -1.56 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92638

Communication System: UID 0, CDMA; Frequency: 836.52 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.52$ MHz; $\sigma = 0.956$ S/m; $\epsilon_r = 54.589$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7308; ConvF(9.92, 9.92, 9.92) @ 836.52 MHz; Calibrated: 7/31/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1450; Calibrated: 8/11/2020
Phantom: Twin-SAM V5.0; Type: QD 000 P40 CD; Serial: 1792
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Cell. EVDO Rule Part 22H, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 23.75 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.844 W/kg

SAR(1 g) = 0.516 W/kg

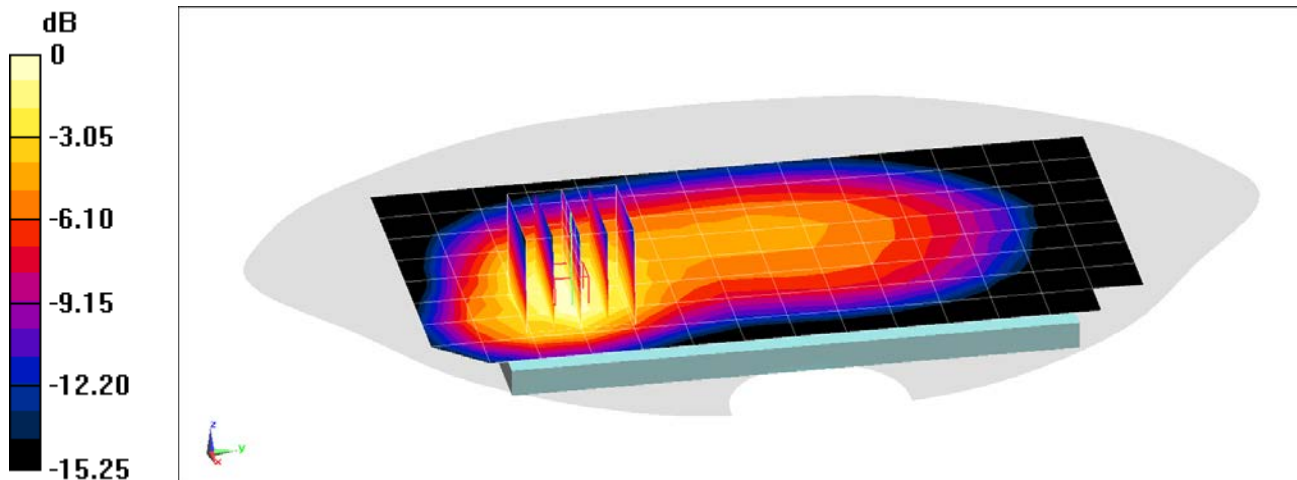

0 dB = 0.715 W/kg = -1.46 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, CDMA; Frequency: 1851.25 MHz; Duty Cycle: 1:1
Medium: 1900 Body Medium parameters used (interpolated):
 $f = 1851.25$ MHz; $\sigma = 1.488$ S/m; $\epsilon_r = 52.874$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/04/2020; Ambient Temp: 21.3°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7571; ConvF(7.56, 7.56, 7.56) @ 1851.25 MHz; Calibrated: 12/11/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1533; Calibrated: 12/5/2019
Phantom: SAM Left; Type: QD000P40CC; Serial: TP: 1375
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: PCS CDMA, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.56 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 1.11 W/kg

SAR(1 g) = 0.660 W/kg

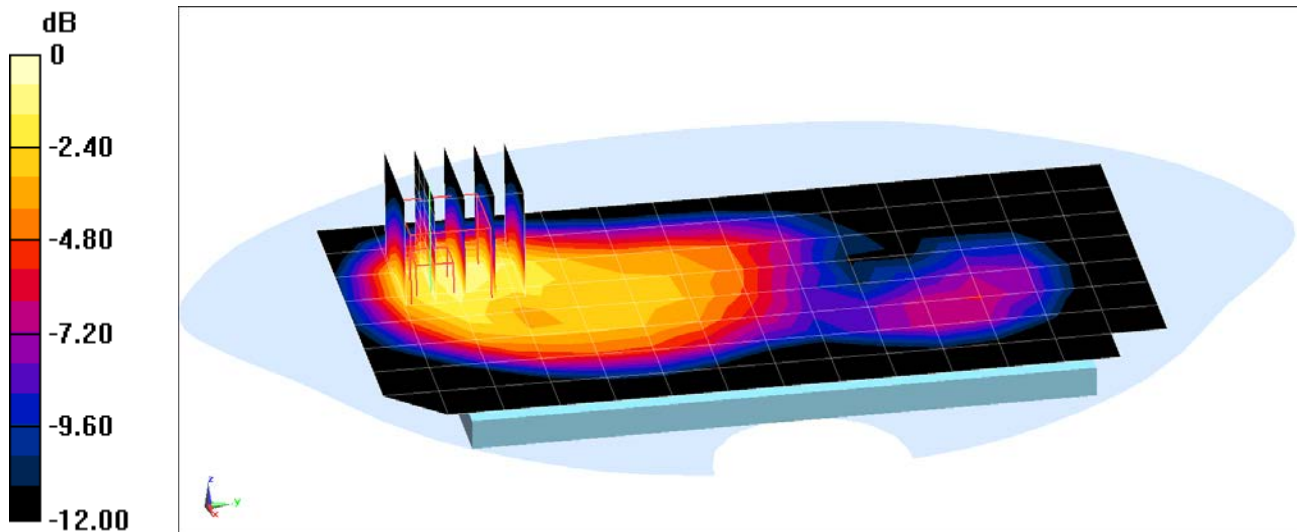

0 dB = 0.936 W/kg = -0.29 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, CDMA; Frequency: 1908.75 MHz; Duty Cycle: 1:1
Medium: 1900 Body Medium parameters used (interpolated):
 $f = 1908.75$ MHz; $\sigma = 1.551$ S/m; $\epsilon_r = 52.681$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/04/2020; Ambient Temp: 21.3°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7571; ConvF(7.56, 7.56, 7.56) @ 1908.75 MHz; Calibrated: 12/11/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1533; Calibrated: 12/5/2019
Phantom: SAM Left; Type: QD000P40CC; Serial: TP: 1375
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: PCS EVDO, Body SAR, Bottom Edge, High.ch


Area Scan (10x7x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 29.75 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 2.02 W/kg

SAR(1 g) = 1.11 W/kg

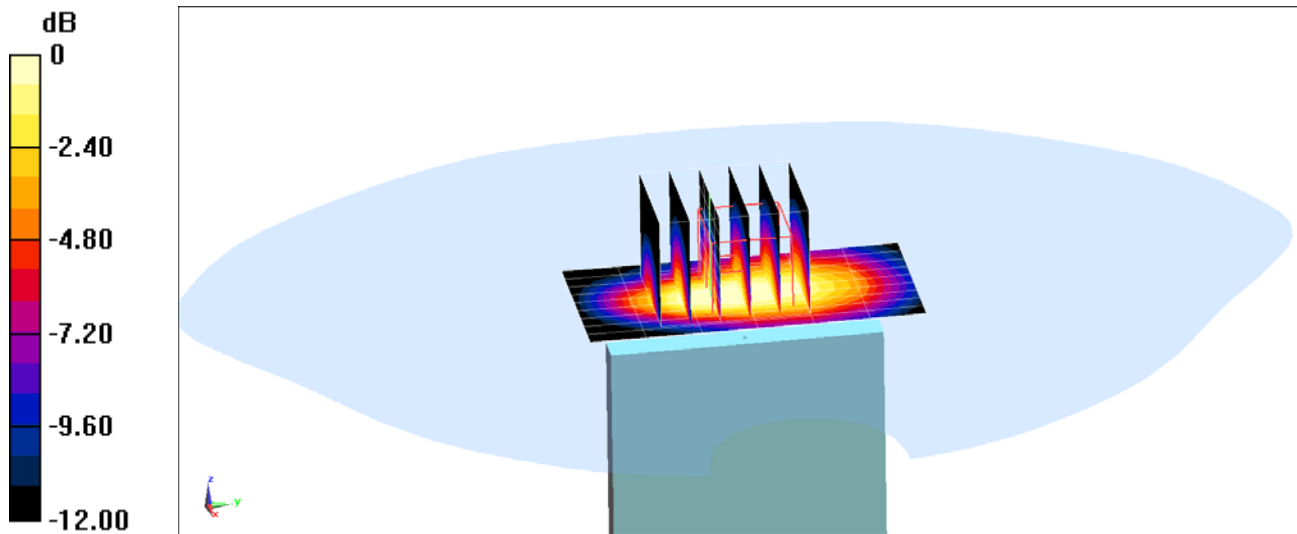

0 dB = 1.67 W/kg = 2.23 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, GSM GPRS; 3 Tx slots; Frequency: 836.6 MHz; Duty Cycle: 1:2.76
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.6$ MHz; $\sigma = 0.993$ S/m; $\epsilon_r = 54.727$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/25/2020; Ambient Temp: 25.0°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 836.6 MHz; Calibrated: 1/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn793; Calibrated: 1/14/2020
Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: GPRS 850, Body SAR, Back Side, Mid.ch, 3 Tx Slots


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 23.17 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 0.832 W/kg

SAR(1 g) = 0.504 W/kg

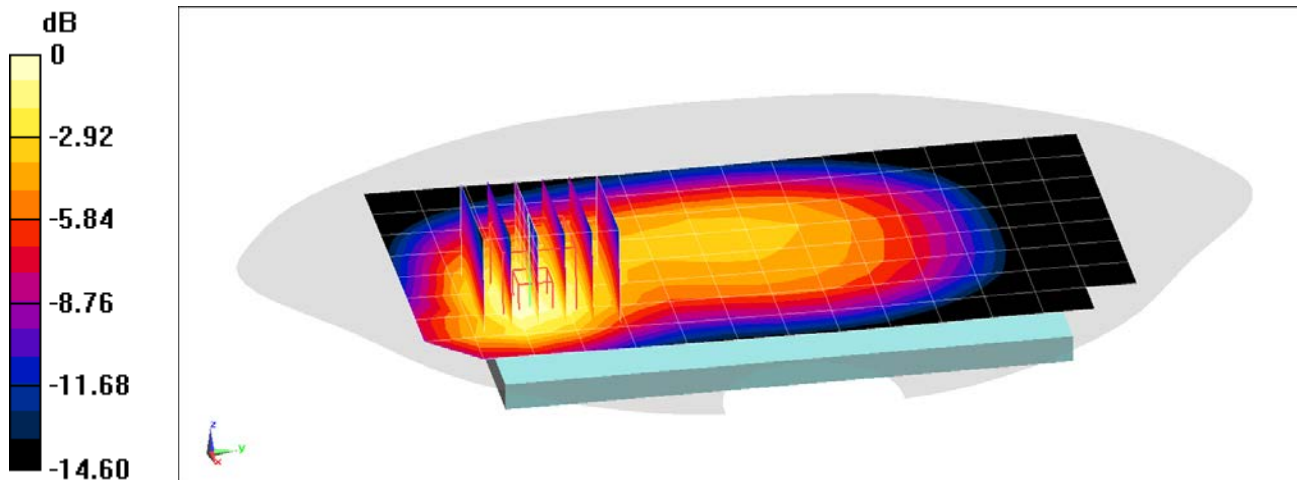

0 dB = 0.709 W/kg = -1.49 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, GSM GPRS; 3 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:2.76

Medium: 1900 Body Medium parameters used:

$f = 1880$ MHz; $\sigma = 1.565$ S/m; $\epsilon_r = 51.101$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.4°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1880 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: GPRS 1900, Body SAR, Back Side, Mid.ch, 3 Tx Slots


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.25 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 0.290 W/kg

SAR(1 g) = 0.183 W/kg

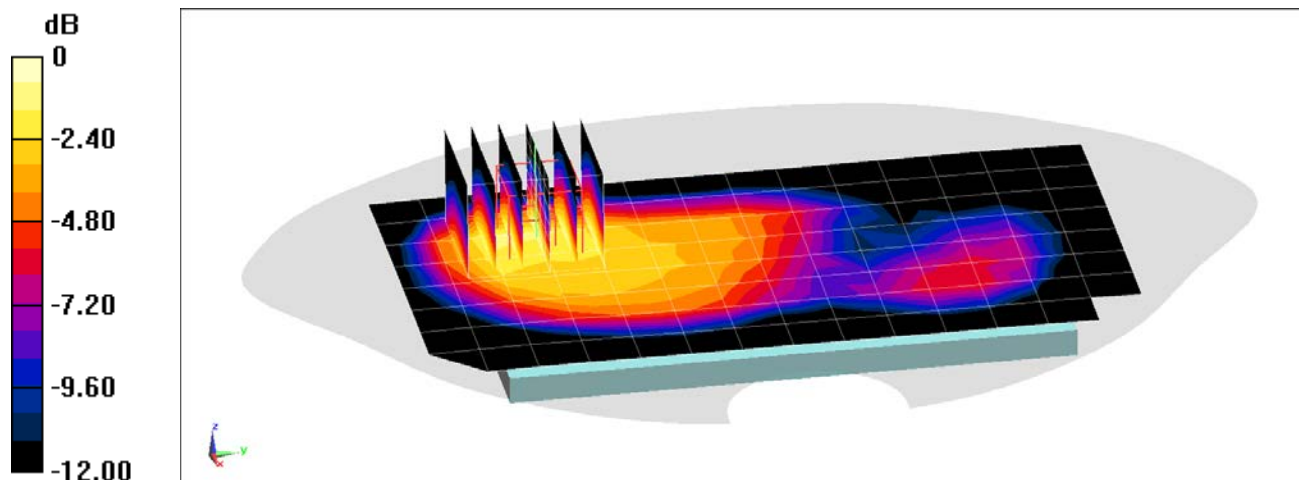

0 dB = 0.251 W/kg = -6.00 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, GSM GPRS; 3 Tx slots; Frequency: 1880 MHz; Duty Cycle: 1:2.76

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.565 \text{ S/m}$; $\epsilon_r = 51.101$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.4°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1880 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: GPRS 1900, Body SAR, Bottom Edge, Mid.ch, 3 Tx Slots


Area Scan (10x7x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 16.22 V/m; Power Drift = -0.11 dB

Peak SAR (extrapolated) = 0.627 W/kg

SAR(1 g) = 0.369 W/kg

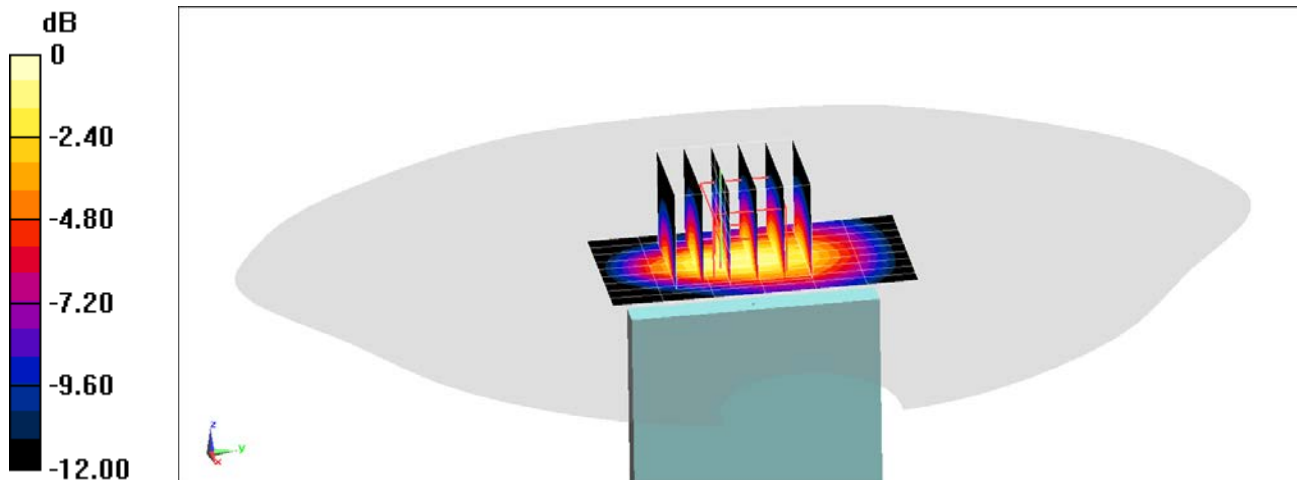

0 dB = 0.535 W/kg = -2.72 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, UMTS; Frequency: 836.6 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.6$ MHz; $\sigma = 0.994$ S/m; $\epsilon_r = 54.475$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2020; Ambient Temp: 22.3°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 836.6 MHz; Calibrated: 1/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn793; Calibrated: 1/14/2020
Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 850, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.81 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 0.582 W/kg

SAR(1 g) = 0.344 W/kg

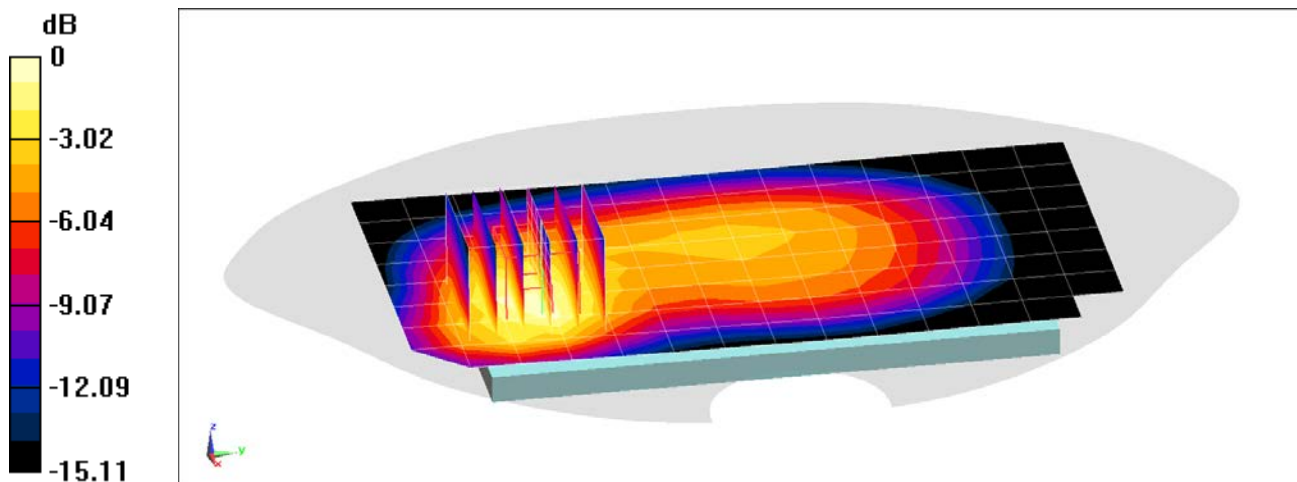

0 dB = 0.464 W/kg = -3.33 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, UMTS; Frequency: 1732.4 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1732.4$ MHz; $\sigma = 1.516$ S/m; $\epsilon_r = 52.234$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/04/2020; Ambient Temp: 20.1°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1732.4 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1750, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 18.59 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 0.837 W/kg

SAR(1 g) = 0.491 W/kg

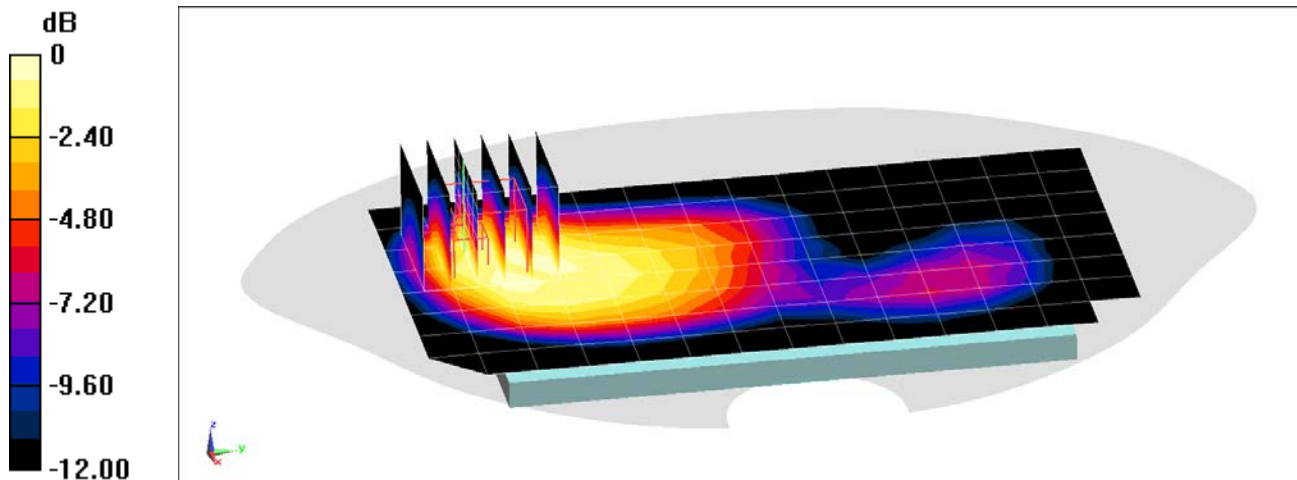

0 dB = 0.702 W/kg = -1.54 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, UMTS; Frequency: 1732.4 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1732.4$ MHz; $\sigma = 1.488$ S/m; $\epsilon_r = 52.13$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 20.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7416; ConvF(7.85, 7.85, 7.85) @ 1732.4 MHz; Calibrated: 6/22/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn701; Calibrated: 6/11/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1936
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1750, Body SAR, Bottom Edge, Mid.ch


Area Scan (10x7x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 19.84 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 0.923 W/kg

SAR(1 g) = 0.517 W/kg

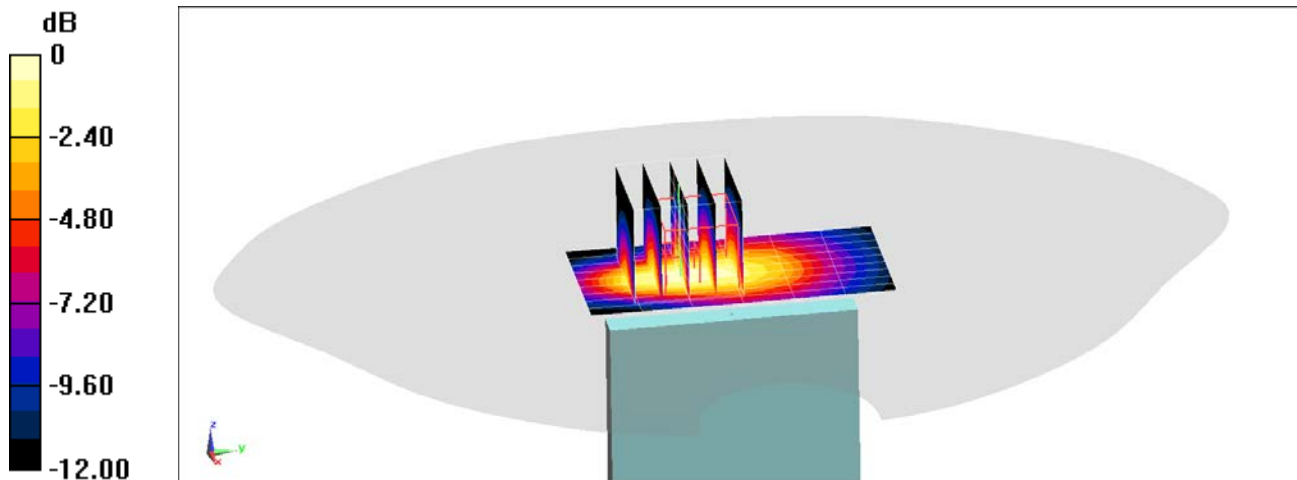

0 dB = 0.782 W/kg = -1.07 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, UMTS; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.519 \text{ S/m}$; $\epsilon_r = 51.596$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 21.5°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1880 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1900, Body SAR, Back Side, Mid.ch


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 17.48 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.690 W/kg

SAR(1 g) = 0.433 W/kg

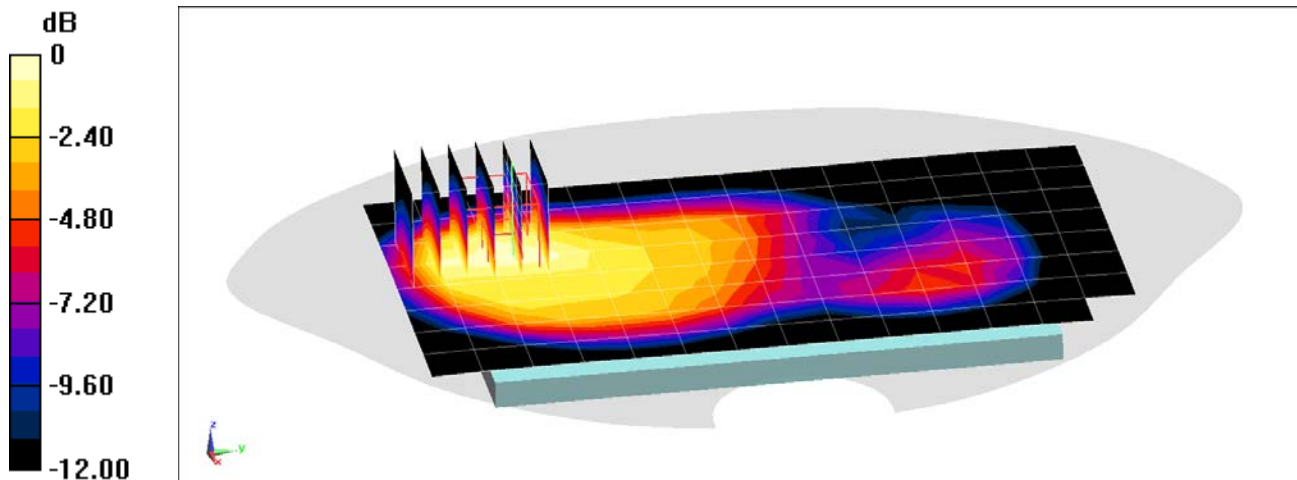

0 dB = 0.591 W/kg = -2.28 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, UMTS; Frequency: 1852.4 MHz; Duty Cycle: 1:1
Medium: 1900 Body Medium parameters used (interpolated):
 $f = 1852.4$ MHz; $\sigma = 1.548$ S/m; $\epsilon_r = 53.362$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/01/2020; Ambient Temp: 21.1°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN3837; ConvF(7.68, 7.68, 7.68) @ 1852.4 MHz; Calibrated: 1/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn793; Calibrated: 1/14/2020
Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: UMTS 1900, Body SAR, Bottom Edge, Low.ch


Area Scan (10x9x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 22.68 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 1.34 W/kg

SAR(1 g) = 0.728 W/kg

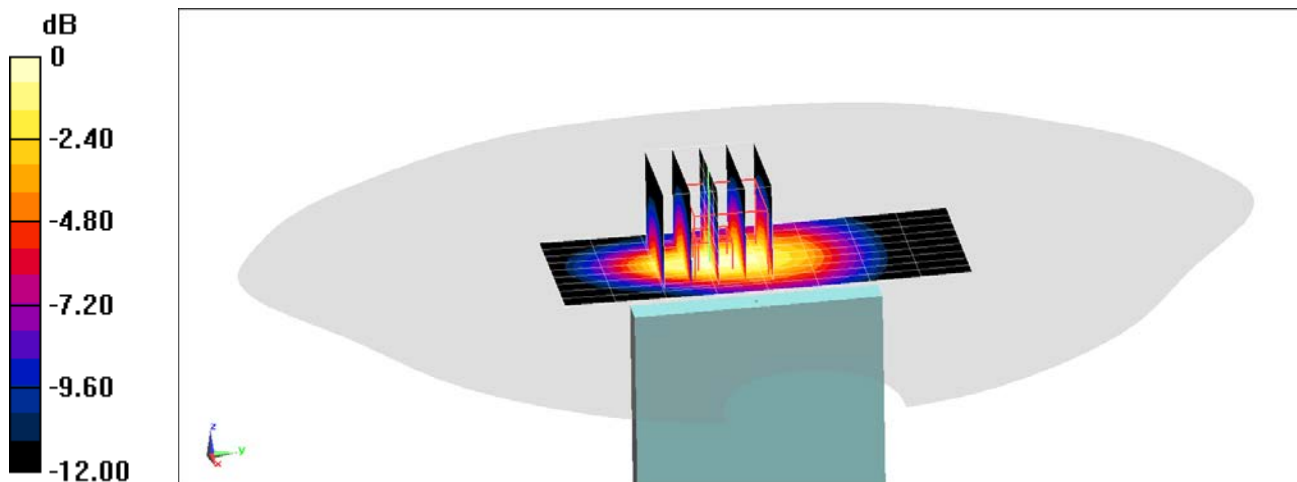

0 dB = 1.12 W/kg = 0.49 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated):
 $f = 680.5 \text{ MHz}$; $\sigma = 0.969 \text{ S/m}$; $\epsilon_r = 54.128$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7490; ConvF(10.37, 10.37, 10.37) @ 680.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 71, Body SAR, Back Side, Mid.ch,
20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 16.67 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.388 W/kg

SAR(1 g) = 0.255 W/kg

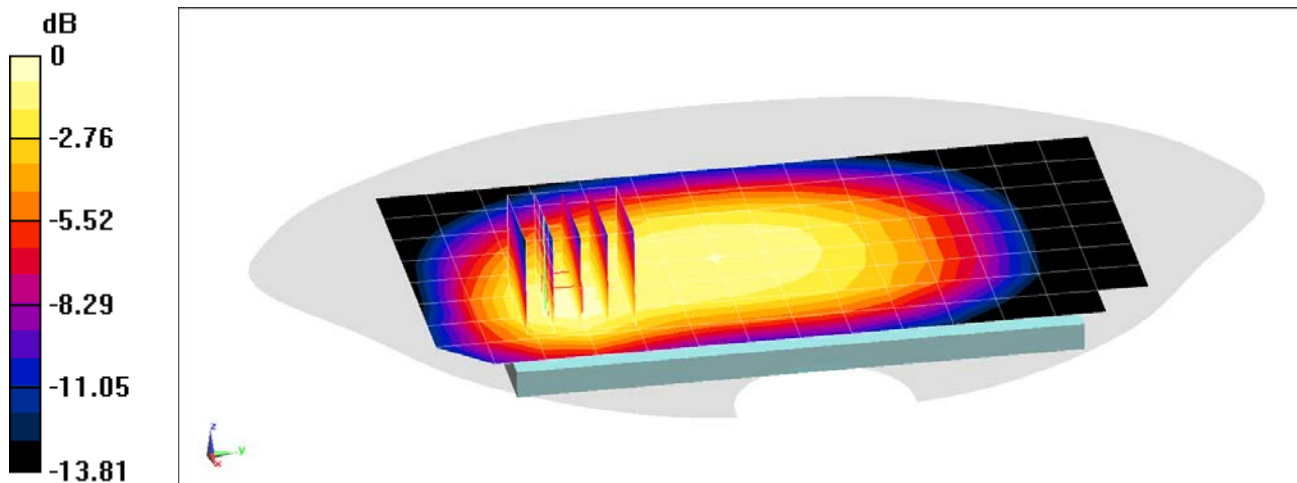

0 dB = 0.332 W/kg = -4.79 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated):
 $f = 680.5 \text{ MHz}$; $\sigma = 0.969 \text{ S/m}$; $\epsilon_r = 54.128$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7490; ConvF(10.37, 10.37, 10.37) @ 680.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 71, Body SAR, Left Edge, Mid.ch,
20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (10x13x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.56 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 0.569 W/kg

SAR(1 g) = 0.389 W/kg

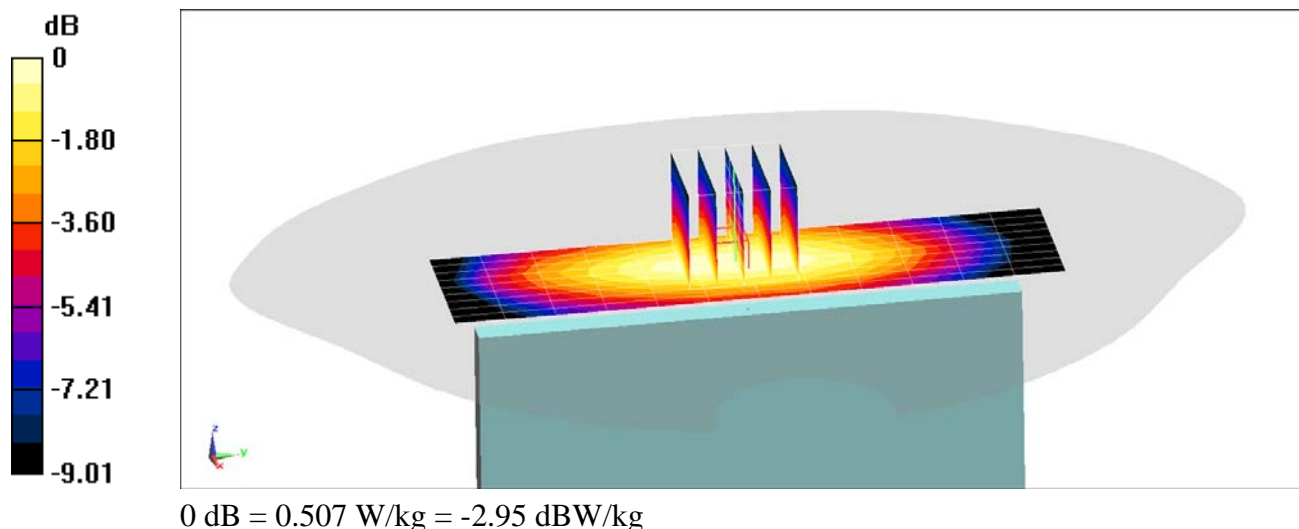

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 12; Frequency: 707.5 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated):
 $f = 707.5$ MHz; $\sigma = 0.962$ S/m; $\epsilon_r = 54.201$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 20.0°C; Tissue Temp: 19.9°C

Probe: EX3DV4 - SN3837; ConvF(9.55, 9.55, 9.55) @ 707.5 MHz; Calibrated: 1/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn793; Calibrated: 1/14/2020
Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 12, Body SAR, Back Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 49 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 16.56 V/m; Power Drift = 0.11 dB

Peak SAR (extrapolated) = 0.542 W/kg

SAR(1 g) = 0.328 W/kg

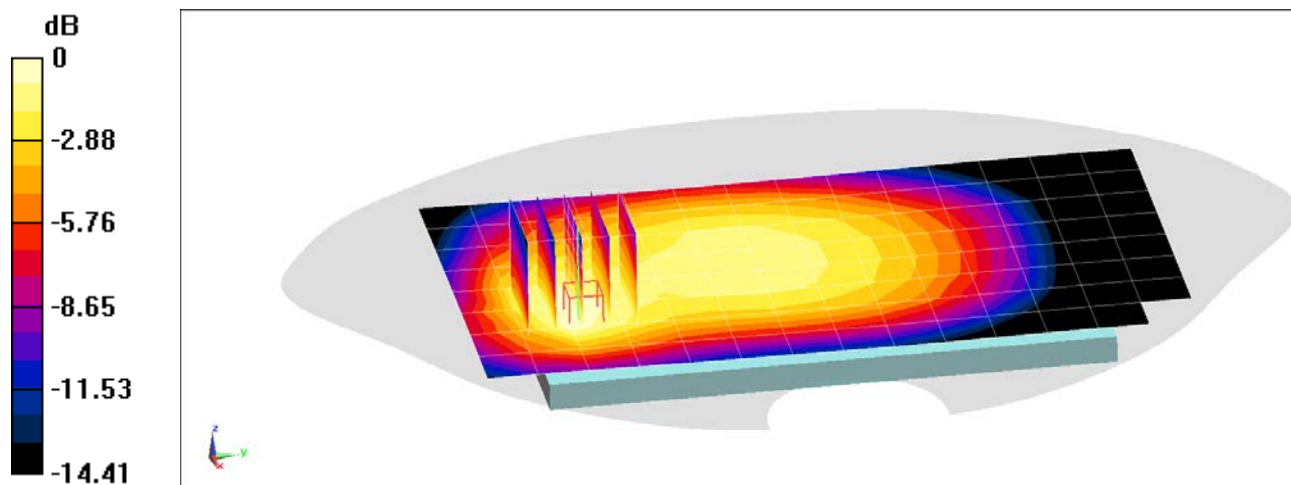

0 dB = 0.462 W/kg = -3.35 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 13; Frequency: 782 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated)
 $f = 782 \text{ MHz}$; $\sigma = 0.979 \text{ S/m}$; $\epsilon_r = 54.856$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 782 MHz; Calibrated: 7/16/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1402; Calibrated: 7/9/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 13, Body SAR, Back Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 15.06 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.325 W/kg

SAR(1 g) = 0.206 W/kg

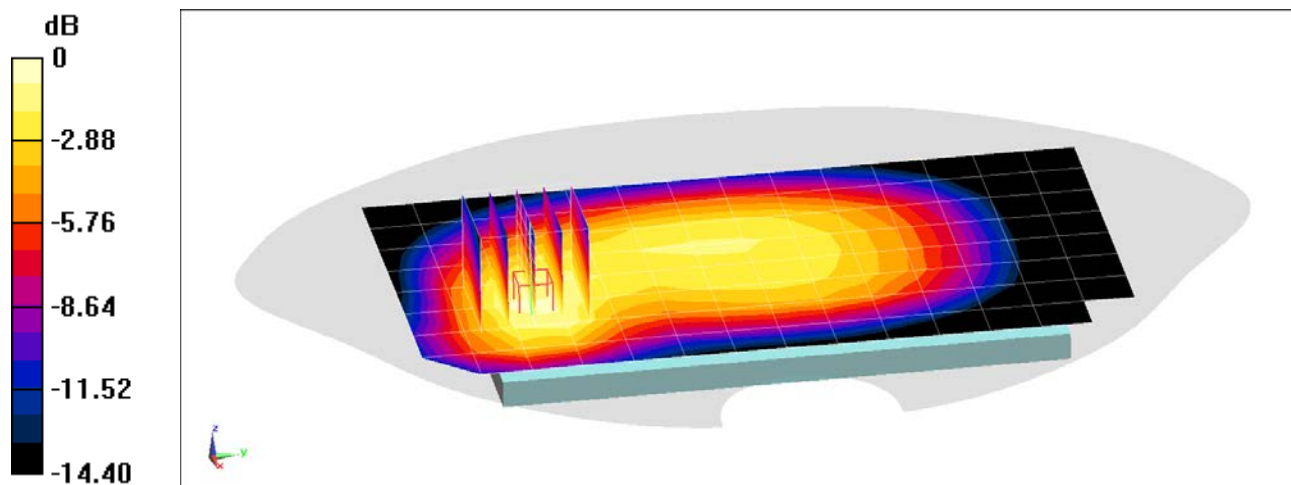

0 dB = 0.281 W/kg = -5.51 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 14; Frequency: 793 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 793 \text{ MHz}$; $\sigma = 0.983 \text{ S/m}$; $\epsilon_r = 54.837$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 793 MHz; Calibrated: 7/16/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1402; Calibrated: 7/9/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 14, Body SAR, Back Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 14.57 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.314 W/kg

SAR(1 g) = 0.198 W/kg

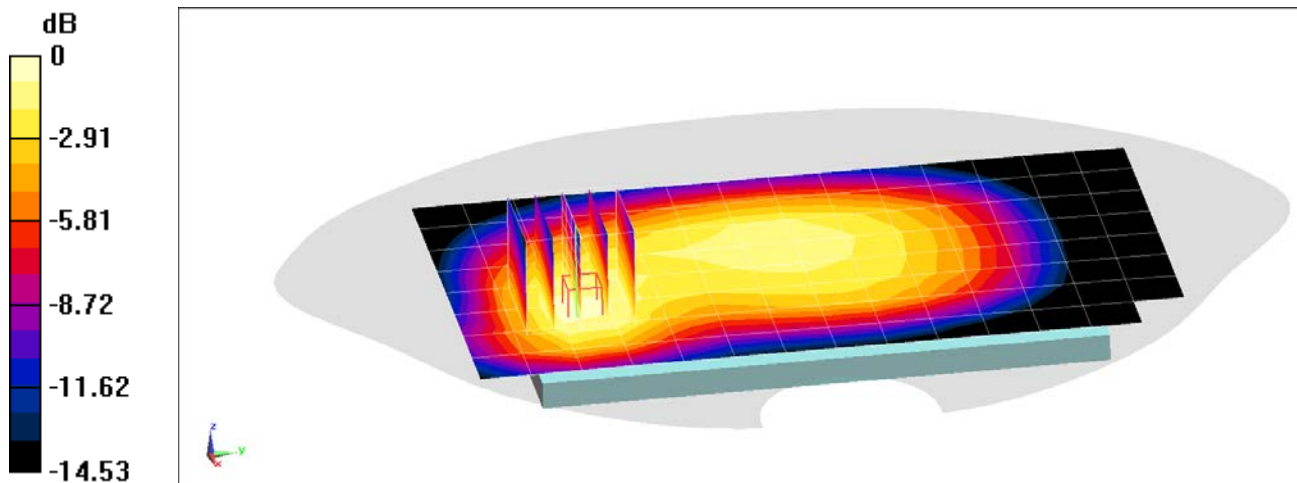

0 dB = 0.267 W/kg = -5.73 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 14; Frequency: 793 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 793 \text{ MHz}$; $\sigma = 0.983 \text{ S/m}$; $\epsilon_r = 54.837$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 793 MHz; Calibrated: 7/16/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1402; Calibrated: 7/9/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 14, Body SAR, Front Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 14.47 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 0.313 W/kg

SAR(1 g) = 0.202 W/kg

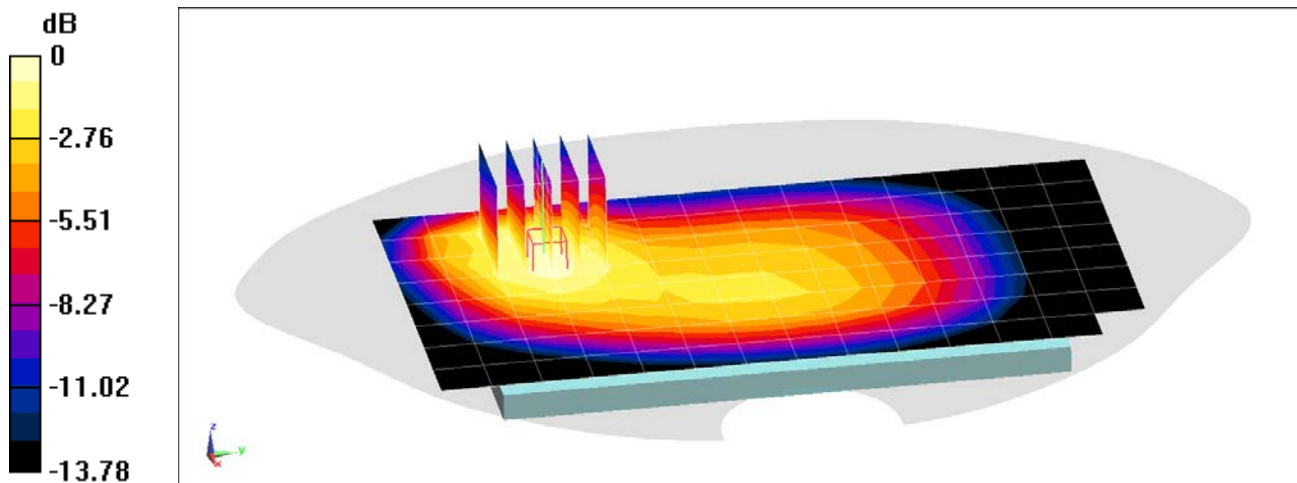

0 dB = 0.269 W/kg = -5.70 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803

Communication System: UID 0, LTE Band 26; Frequency: 831.5 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 831.5$ MHz; $\sigma = 1.013$ S/m; $\epsilon_r = 53.367$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(10.18, 10.18, 10.18) @ 831.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 26 (Cell.), Body SAR, Back Side, Mid.ch,
15 MHz Bandwidth, QPSK, 1 RB, 36 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 17.35 V/m; Power Drift = 0.16 dB

Peak SAR (extrapolated) = 0.478 W/kg

SAR(1 g) = 0.298 W/kg

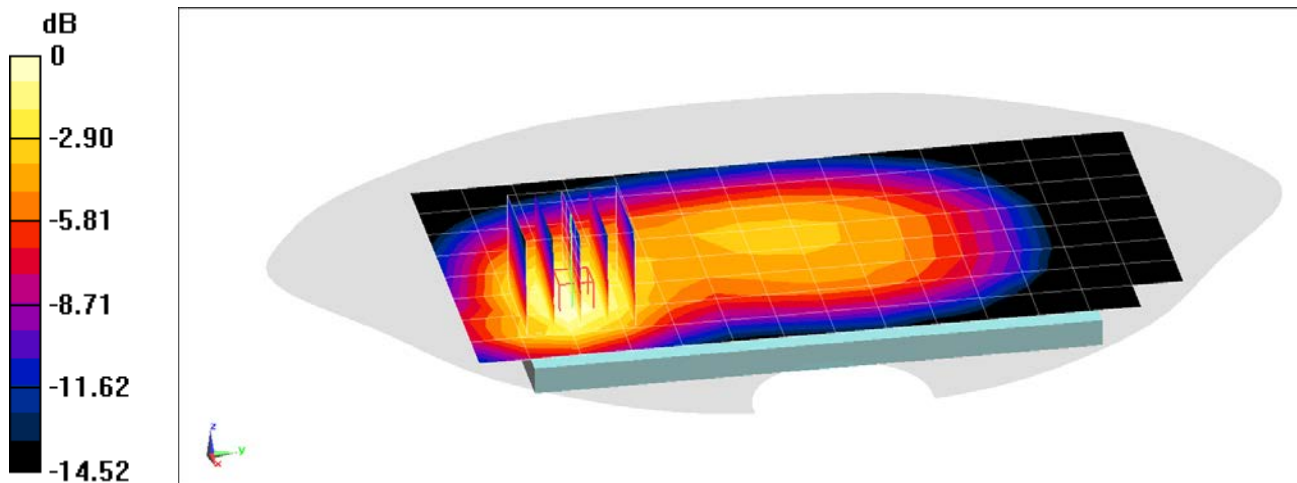

0 dB = 0.414 W/kg = -3.83 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803


Communication System: UID 0, LTE Band 5; Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 1.015$ S/m; $\epsilon_r = 53.352$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(10.18, 10.18, 10.18) @ 836.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 5 (Cell.), Body SAR, Back Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**

Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 19.50 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 0.571 W/kg
SAR(1 g) = 0.361 W/kg

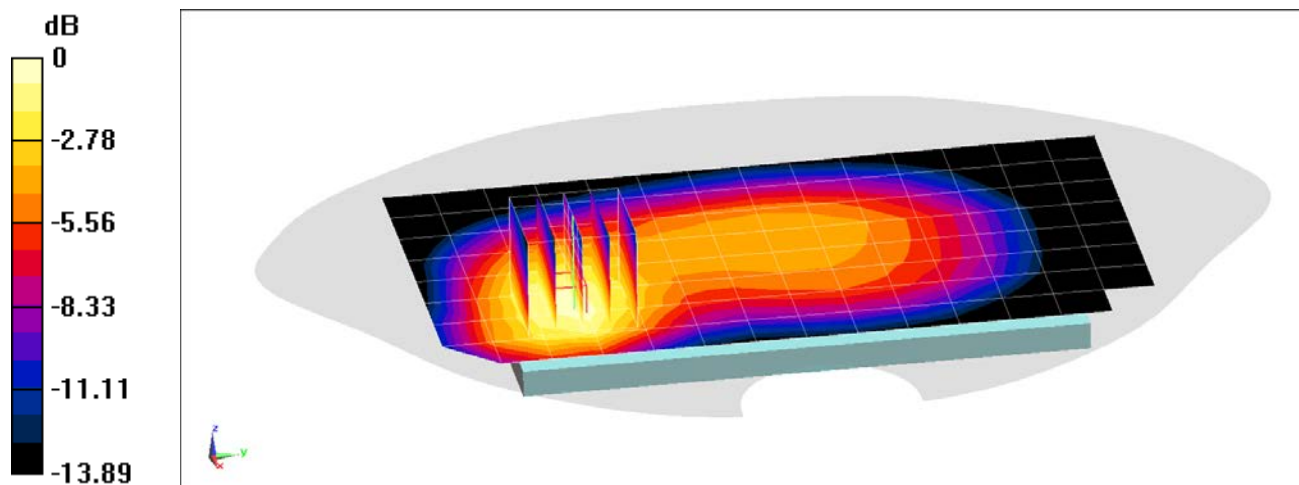

0 dB = 0.483 W/kg = -3.16 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803

Communication System: UID 0, LTE Band 5 (Cell.); Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 1.011$ S/m; $\epsilon_r = 53.732$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 24.5°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 836.5 MHz; Calibrated: 1/20/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn793; Calibrated: 1/14/2020
Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 5 (Cell.), Body SAR, Front Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.06 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 0.639 W/kg

SAR(1 g) = 0.387 W/kg

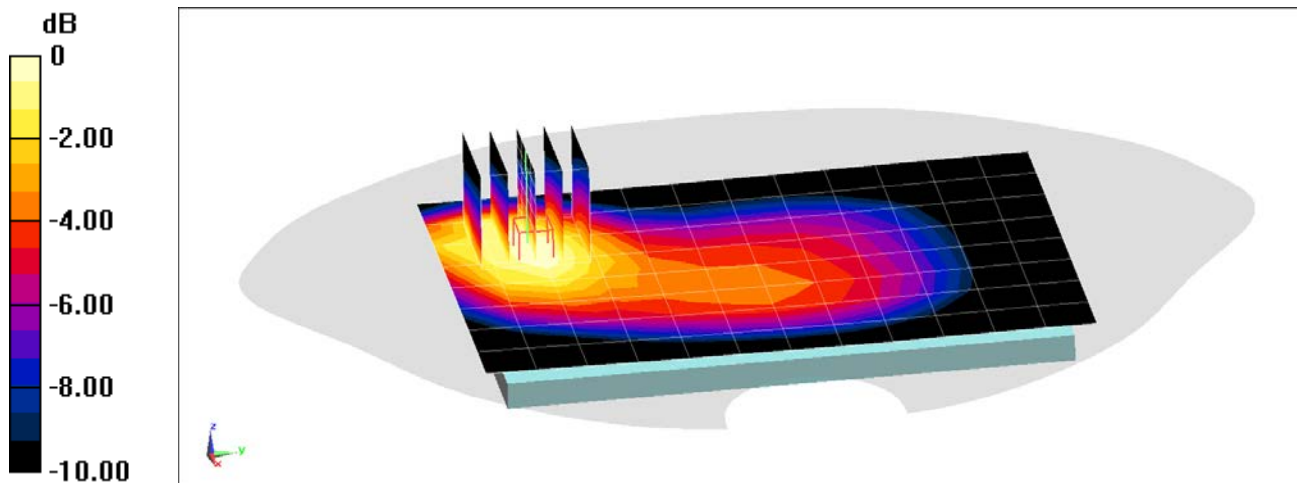

0 dB = 0.539 W/kg = -2.68 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837

Communication System: UID 0, _LTE Band 66 (AWS); Frequency: 1770 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1770 \text{ MHz}$; $\sigma = 1.525 \text{ S/m}$; $\epsilon_r = 51.999$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 20.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7416; ConvF(7.85, 7.85, 7.85) @ 1770 MHz; Calibrated: 6/22/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn701; Calibrated: 6/11/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1936
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 66 (AWS), Antenna 2, Body SAR, Back Side, High.ch,
20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 15.41 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 0.572 W/kg

SAR(1 g) = 0.346 W/kg

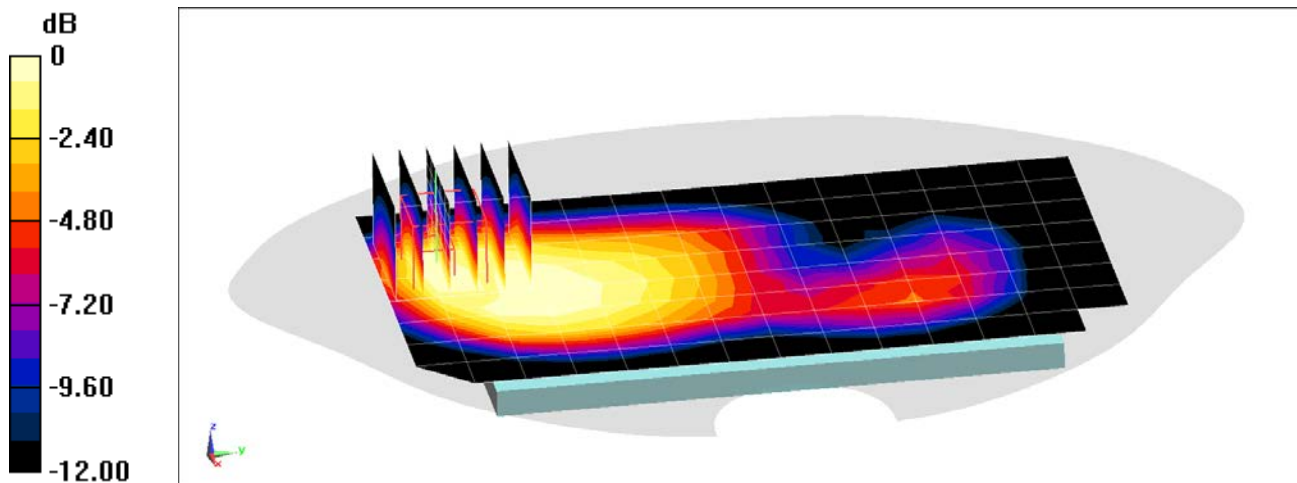

0 dB = 0.481 W/kg = -3.18 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837

Communication System: UID 0, _LTE Band 66 (AWS); Frequency: 1770 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1770$ MHz; $\sigma = 1.525$ S/m; $\epsilon_r = 51.999$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 20.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7416; ConvF(7.85, 7.85, 7.85) @ 1770 MHz; Calibrated: 6/22/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn701; Calibrated: 6/11/2020
Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1936
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 66 (AWS), Antenna 2, Body SAR, Bottom Edge, High.ch,
20 MHz Bandwidth, QPSK, 50 RB, 50 RB Offset**


Area Scan (11x9x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 20.69 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 1.06 W/kg

SAR(1 g) = 0.590 W/kg

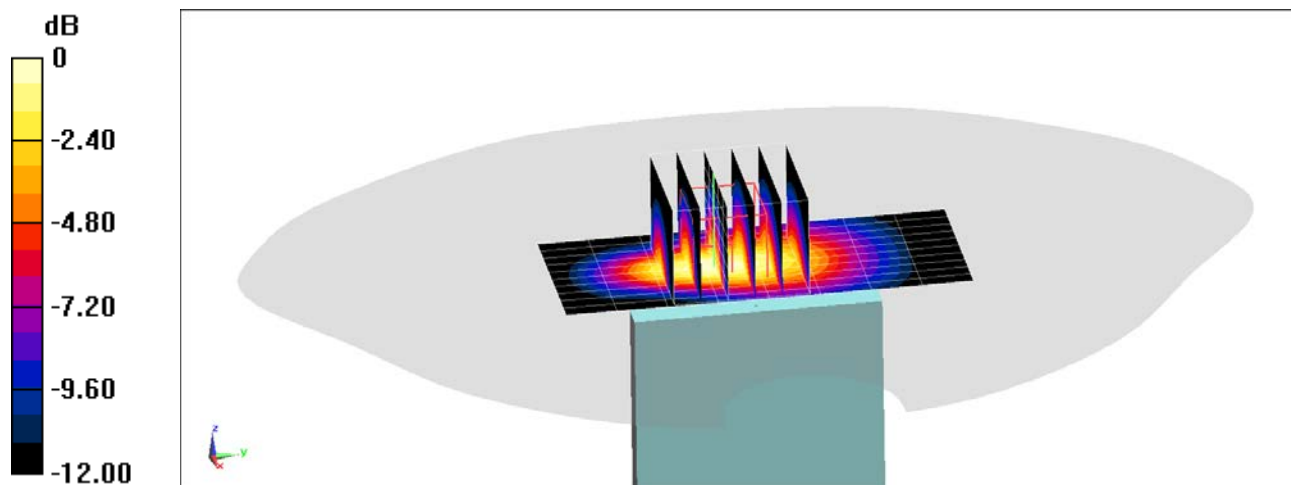

0 dB = 0.889 W/kg = -0.51 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 25 (PCS); Frequency: 1860 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1860 \text{ MHz}$; $\sigma = 1.55 \text{ S/m}$; $\epsilon_r = 51.119$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.4°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1860 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 25 (PCS), Body SAR, Back Side, Low.ch,
20 MHz Bandwidth, QPSK, 1 RB, 99 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 15.68 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 0.570 W/kg

SAR(1 g) = 0.356 W/kg

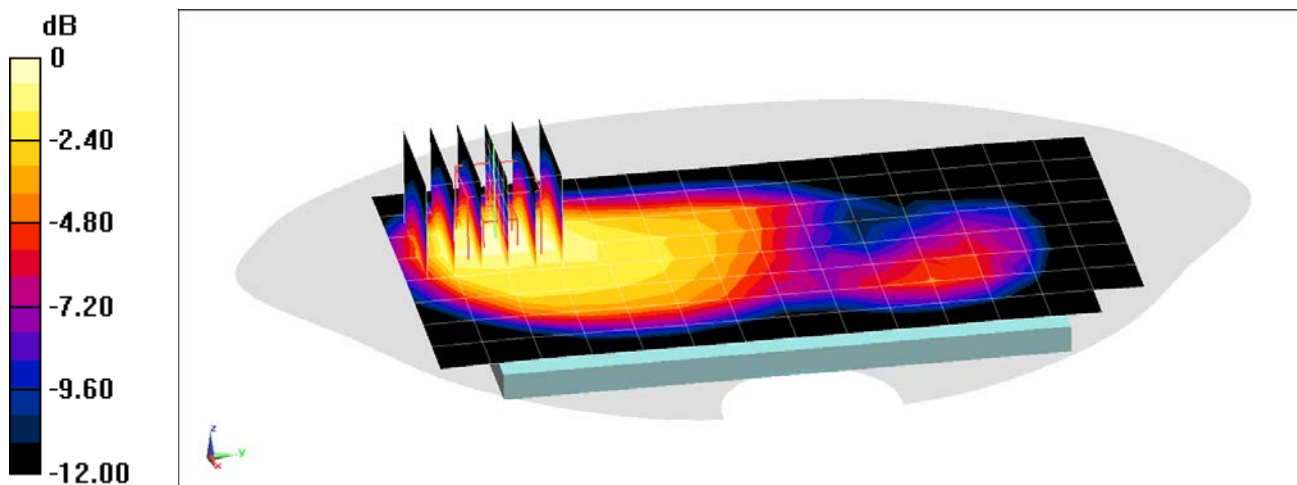

0 dB = 0.488 W/kg = -3.12 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 25 (PCS); Frequency: 1905 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1905$ MHz; $\sigma = 1.58$ S/m; $\epsilon_r = 51.08$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.4°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1905 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 25 (PCS), Body SAR, Bottom Edge, High.ch,
20 MHz Bandwidth, QPSK, 50 RB, 0 RB Offset**


Area Scan (11x9x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 19.70 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 0.931 W/kg

SAR(1 g) = 0.546 W/kg

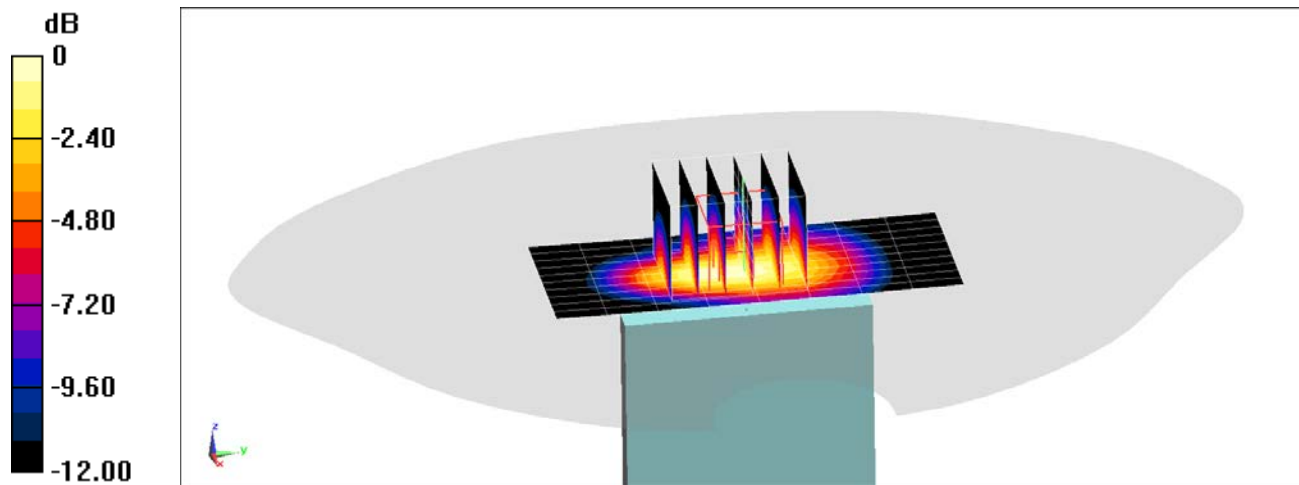

0 dB = 0.803 W/kg = -0.95 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15787

Communication System: UID 0, LTE Band 2 (PCS); Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.589$ S/m; $\epsilon_r = 51.095$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 23.1°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7490; ConvF(8.22, 8.22, 8.22) @ 1900 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 2 (PCS), Antenna 7, Body SAR, Back Side, High.ch,
20 MHz Bandwidth, QPSK, 1 RB, 50 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (6x6x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 12.74 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.423 W/kg

SAR(1 g) = 0.231 W/kg

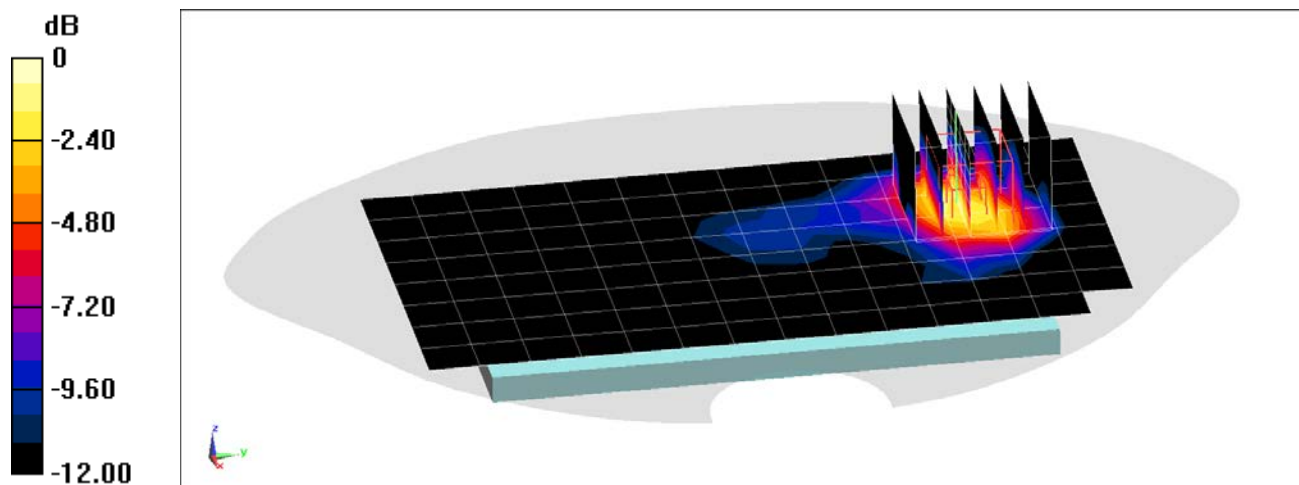

0 dB = 0.351 W/kg = -4.55 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15803

Communication System: UID 0, LTE Band 30; Frequency: 2310 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2310 \text{ MHz}$; $\sigma = 1.896 \text{ S/m}$; $\epsilon_r = 51.325$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/19/2020; Ambient Temp: 22.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7421; ConvF(7.63, 7.63, 7.63) @ 2310 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: LTE Band 30, Antenna 1, Body SAR, Back Side, Mid.ch,
10 MHz Bandwidth, QPSK, 1 RB, 25 RB Offset**


Area Scan (10x18x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (10x8x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 17.26 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 0.945 W/kg

SAR(1 g) = 0.462 W/kg

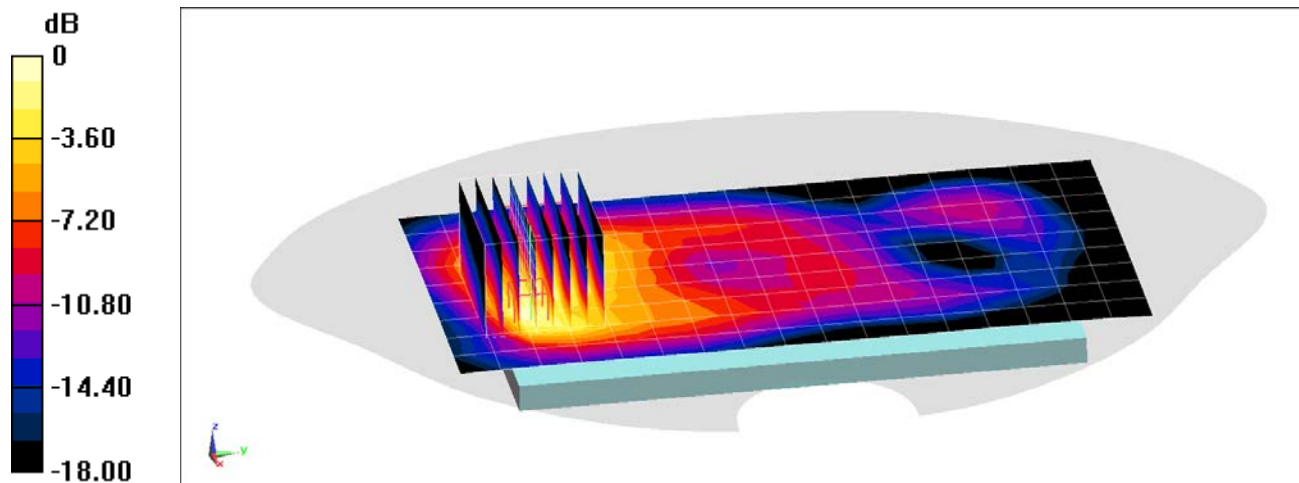

0 dB = 0.775 W/kg = -1.11 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 41 (Class 3); Frequency: 2680 MHz; Duty Cycle: 1:1.58

Medium: 2450 Body Medium parameters used (interpolated):

$f = 2680$ MHz; $\sigma = 2.304$ S/m; $\epsilon_r = 50.263$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/20/2020; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7427; ConvF(7.08, 7.08, 7.08) @ 2680 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: LTE Band 41, ULCA, Body SAR, Back Side

PCC: Ch. 41490, 20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset

SCC: Ch. 41292, 20 MHz Bandwidth, QPSK, 1 RB 99 RB Offset


Area Scan (11x16x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 12.14 V/m; Power Drift = -0.19 dB

Peak SAR (extrapolated) = 0.624 W/kg

SAR(1 g) = 0.299 W/kg

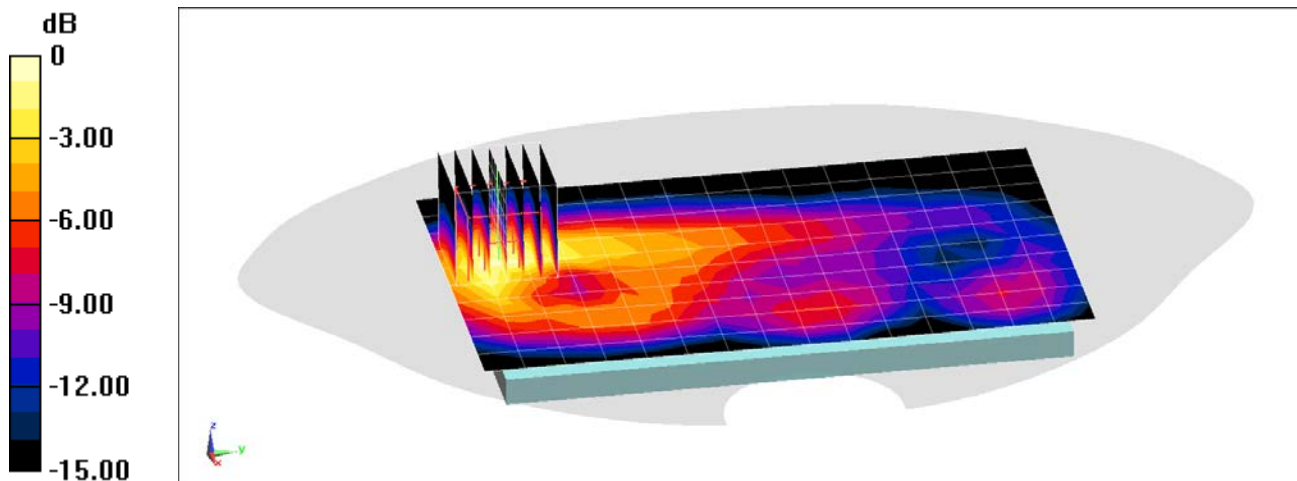

0 dB = 0.495 W/kg = -3.05 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15811

Communication System: UID 0, LTE Band 41 (Class 3); Frequency: 2680 MHz; Duty Cycle: 1:1.58

Medium: 2450 Body Medium parameters used (interpolated):

$f = 2680$ MHz; $\sigma = 2.304$ S/m; $\epsilon_r = 50.263$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/20/2020; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7427; ConvF(7.08, 7.08, 7.08) @ 2680 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: LTE Band 41, ULCA, Body SAR, Bottom Edge

PCC: Ch. 41490, 20 MHz Bandwidth, QPSK, 1 RB, 0 RB Offset

SCC: Ch. 41292, 20 MHz Bandwidth, QPSK, 1 RB 99 RB Offset


Area Scan (11x10x1): Measurement grid: dx=5mm, dy=12mm

Zoom Scan (7x8x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 15.98 V/m; Power Drift = 0.07 dB

Peak SAR (extrapolated) = 1.13 W/kg

SAR(1 g) = 0.501 W/kg

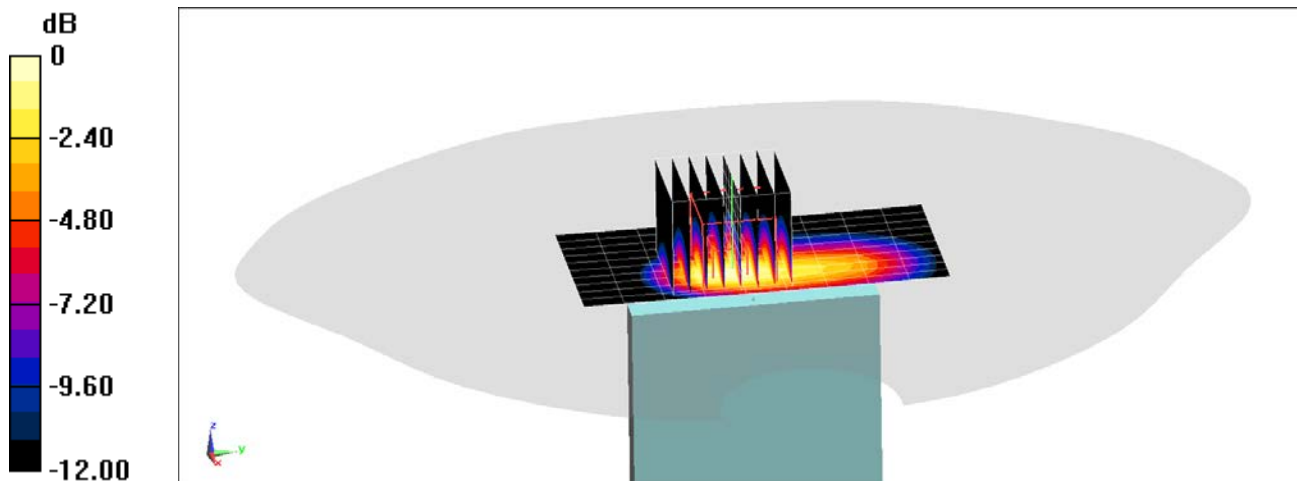

0 dB = 0.868 W/kg = -0.61 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15829

Communication System: UID 0, NR Band n71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated):
 $f = 680.5 \text{ MHz}$; $\sigma = 0.94 \text{ S/m}$; $\epsilon_r = 53.955$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/25/2020; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 680.5 MHz; Calibrated: 7/16/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1402; Calibrated: 7/9/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n71, Body SAR, Back Side, 20 MHz Bandwidth,
CP-OFDM QPSK, Ch. 136100, 1 RB, 1 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 15.08 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 0.316 W/kg

SAR(1 g) = 0.204 W/kg

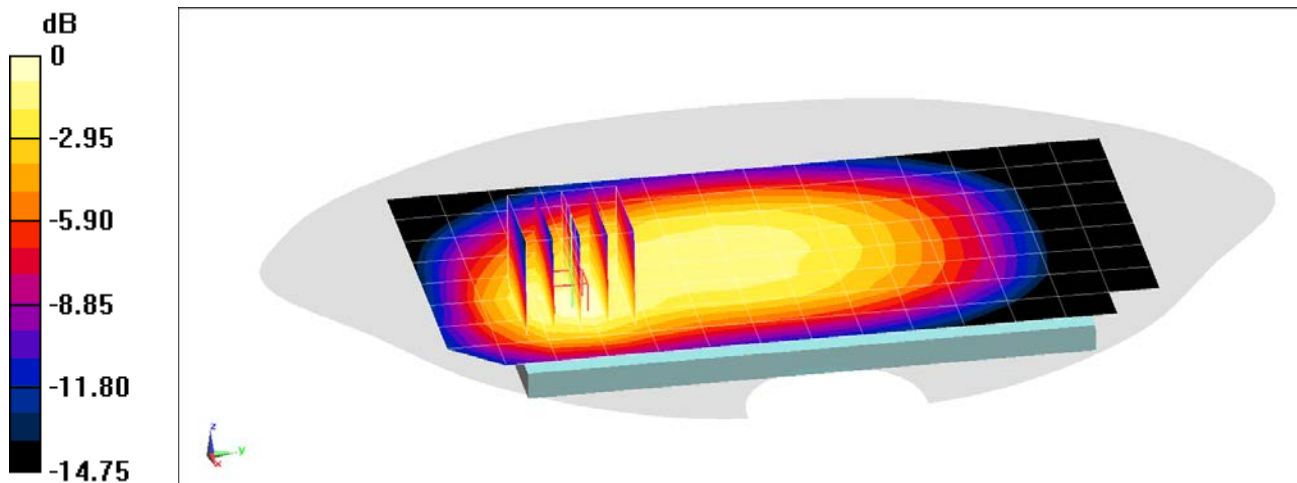

0 dB = 0.275 W/kg = -5.61 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15829

Communication System: UID 0, NR Band n71; Frequency: 680.5 MHz; Duty Cycle: 1:1
Medium: 750 Body Medium parameters used (interpolated):
 $f = 680.5 \text{ MHz}$; $\sigma = 0.94 \text{ S/m}$; $\epsilon_r = 53.955$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/25/2020; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 680.5 MHz; Calibrated: 7/16/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1402; Calibrated: 7/9/2020
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n71, Body SAR, Left Edge, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 136100, 1 RB, 1 RB Offset**


Area Scan (11x15x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 16.67 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 0.387 W/kg

SAR(1 g) = 0.253 W/kg

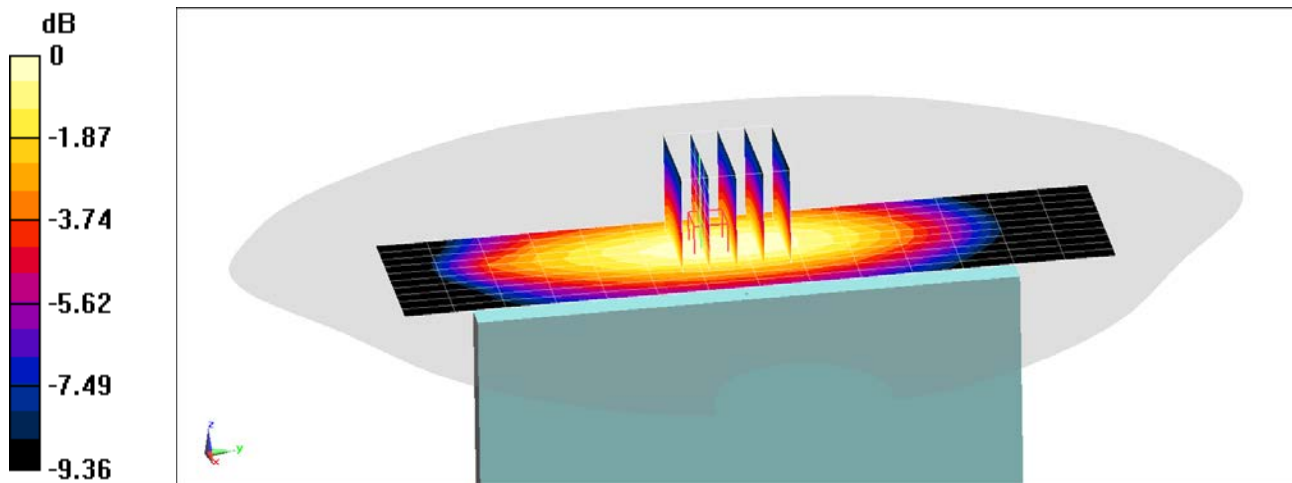

0 dB = 0.338 W/kg = -4.71 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837


Communication System: UID 0, NR Band n5; Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 1.015$ S/m; $\epsilon_r = 53.352$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(10.18, 10.18, 10.18) @ 836.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n5, Body SAR, Back Side, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 167300, 50 RB, 28 RB Offset**

Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 18.97 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 0.556 W/kg
SAR(1 g) = 0.346 W/kg

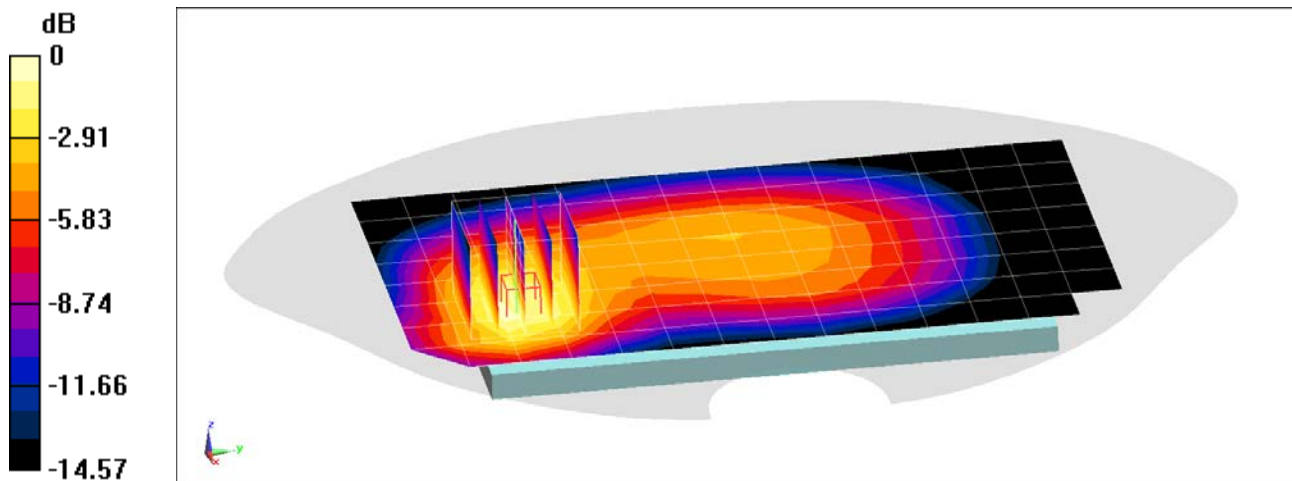

0 dB = 0.480 W/kg = -3.19 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837


Communication System: UID 0, NR Band n5; Frequency: 836.5 MHz; Duty Cycle: 1:1
Medium: 835 Body Medium parameters used (interpolated):
 $f = 836.5$ MHz; $\sigma = 1.015$ S/m; $\epsilon_r = 53.352$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(10.18, 10.18, 10.18) @ 836.5 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n5, Body SAR, Front Side, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 167300, 50 RB, 28 RB Offset**

Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm
Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm
Reference Value = 19.90 V/m; Power Drift = -0.02 dB
Peak SAR (extrapolated) = 0.621 W/kg
SAR(1 g) = 0.385 W/kg

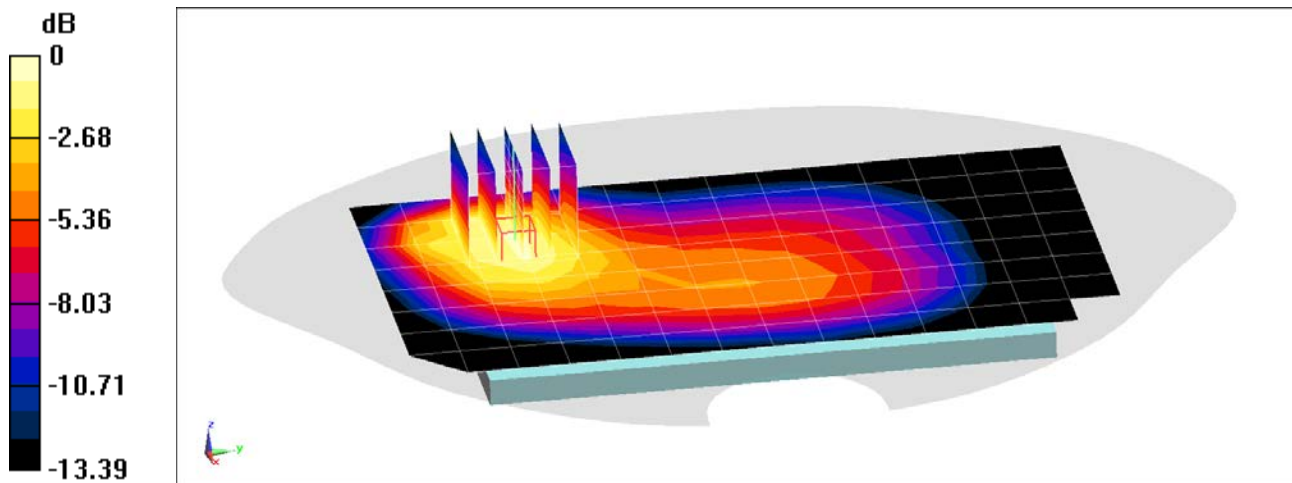

0 dB = 0.527 W/kg = -2.78 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837

Communication System: UID 0, NR Band n66; Frequency: 1745 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1745 \text{ MHz}$; $\sigma = 1.507 \text{ S/m}$; $\epsilon_r = 51.902$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1745 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n66, Body SAR, Back Side, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 349000, 1 RB, 1 RB Offset**


Area Scan (9x15x1): Measurement grid: $dx=15\text{mm}$, $dy=15\text{mm}$

Zoom Scan (5x5x7)/Cube 0: Measurement grid: $dx=8\text{mm}$, $dy=8\text{mm}$, $dz=5\text{mm}$

Reference Value = 13.87 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.511 W/kg

SAR(1 g) = 0.269 W/kg

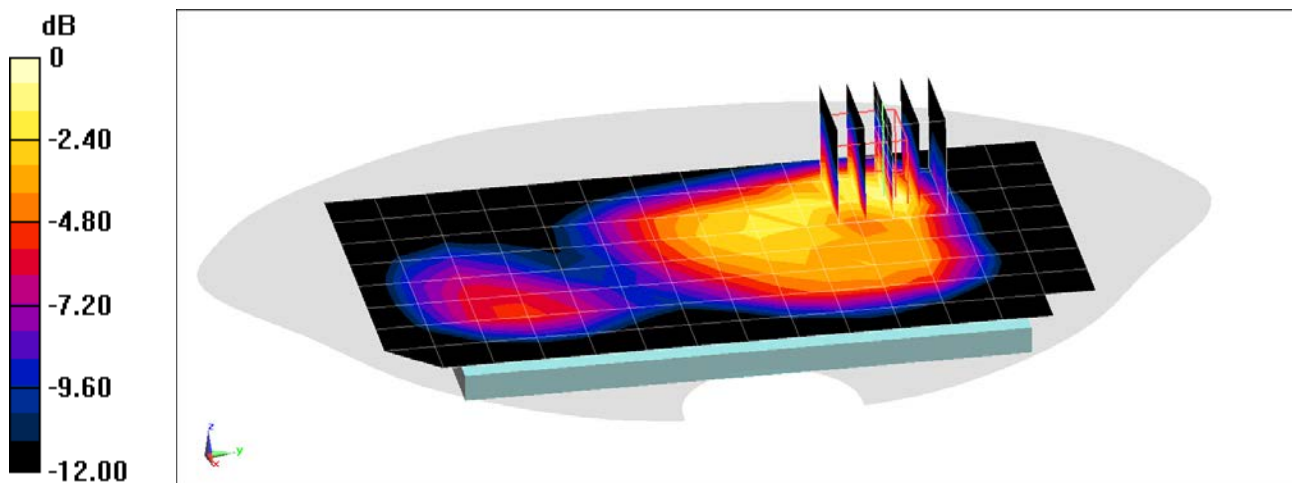

0 dB = 0.408 W/kg = -3.89 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15829

Communication System: UID 0, NR Band n66; Frequency: 1720 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1720 \text{ MHz}$; $\sigma = 1.466 \text{ S/m}$; $\epsilon_r = 52.191$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 18.9°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF(8.01, 8.01, 8.01) @ 1720 MHz; Calibrated: 11/21/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1213; Calibrated: 11/13/2019
Phantom: Twin-SAM V4.0; Type: QD 000 P40 CA; Serial: 1275
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n66, Body SAR, Right Edge, 20 MHz Bandwidth,
CP-OFDM QPSK, Ch. 344000, 1 RB, 1 RB Offset**


Area Scan (10x13x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 13.33 V/m; Power Drift = 0.00 dB

Peak SAR (extrapolated) = 0.449 W/kg

SAR(1 g) = 0.231 W/kg

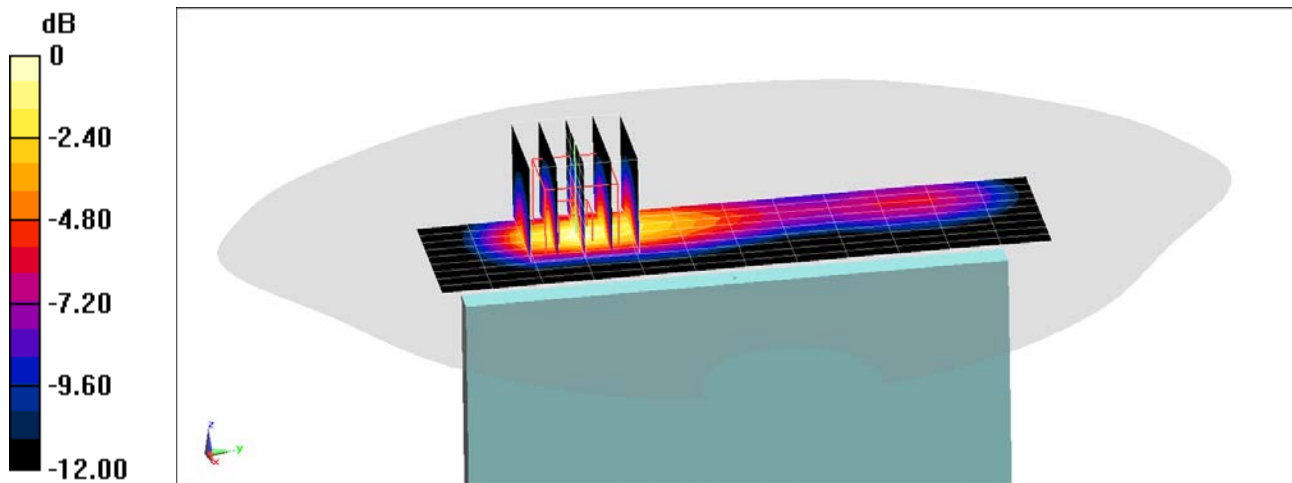

0 dB = 0.376 W/kg = -4.25 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15795

Communication System: UID 0, NR Band n2; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.567 \text{ S/m}$; $\epsilon_r = 53.325$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/01/2020; Ambient Temp: 21.1°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN3837; ConvF(7.68, 7.68, 7.68) @ 1880 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n2, Body SAR, Back Side, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 376000 50 RB, 28 RB Offset**


Area Scan (9x13x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 21.80 V/m; Power Drift = -0.05 dB

Peak SAR (extrapolated) = 1.20 W/kg

SAR(1 g) = 0.655 W/kg

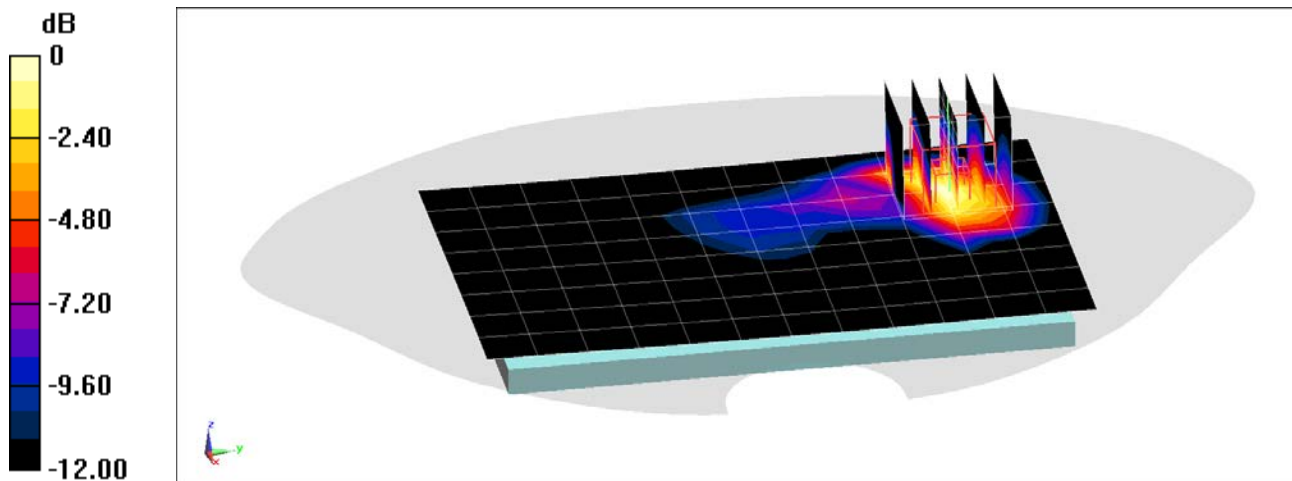

0 dB = 0.997 W/kg = -0.01 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 11257

Communication System: UID 0, NR Band n2; Frequency: 1860 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1860$ MHz; $\sigma = 1.564$ S/m; $\epsilon_r = 51.145$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 23.1°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7490; ConvF(8.22, 8.22, 8.22) @ 1860 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n2, Body SAR, Back Side, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 372000, 50 RB, 56 RB Offset**


Area Scan (9x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 11.42 V/m; Power Drift = 0.04

Peak SAR (extrapolated) = 0.450 W/kg

SAR(1 g) = 0.242 W/kg

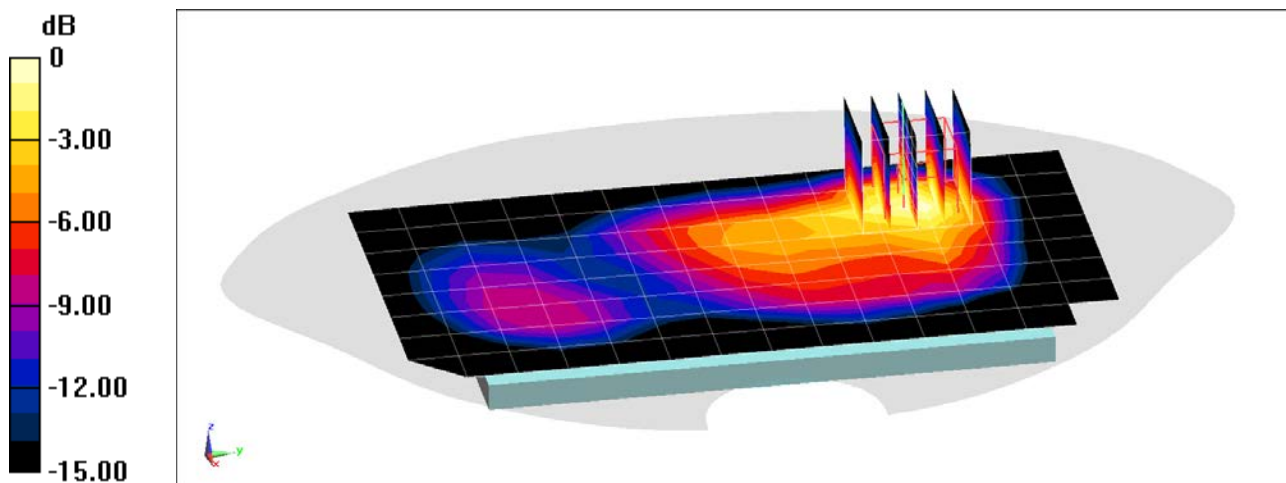

0 dB = 0.351 W/kg = -4.55 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15936

Communication System: UID 0, _IEEE 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1
Medium: 2450 Body Medium parameters used (interpolated):
f = 2412 MHz; $\sigma = 1.946$ S/m; $\epsilon_r = 50.666$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/15/2020; Ambient Temp: 22.0°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(7.73, 7.73, 7.73) @ 2412 MHz; Calibrated: 4/21/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1502; Calibrated: 4/15/2020
Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: IEEE 802.11b, Antenna 1, 22 MHz Bandwidth, Body SAR, Ch 1, 1 Mbps, Back Side


Area Scan (11x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 11.16 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 0.443 W/kg

SAR(1 g) = 0.219 W/kg

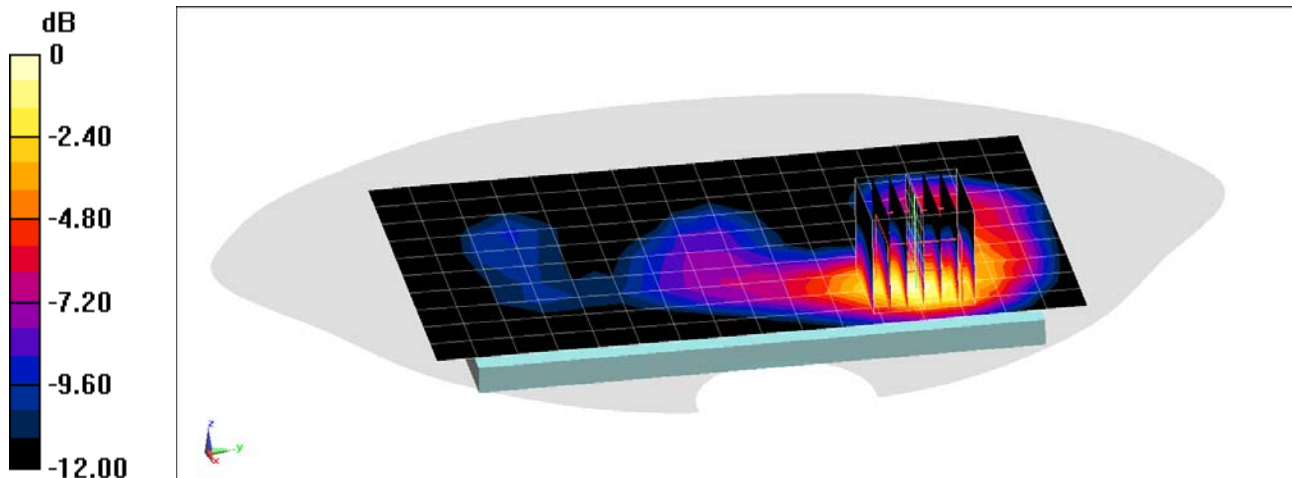

0 dB = 0.353 W/kg = -4.52 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15936


Communication System: UID 0, _IEEE 802.11b; Frequency: 2412 MHz; Duty Cycle: 1:1
Medium: 2450 Body Medium parameters used (interpolated):
 $f = 2412 \text{ MHz}$; $\sigma = 1.946 \text{ S/m}$; $\epsilon_r = 50.666$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/15/2020; Ambient Temp: 22.0°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(7.73, 7.73, 7.73) @ 2412 MHz; Calibrated: 4/21/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1502; Calibrated: 4/15/2020
Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: IEEE 802.11b, Antenna 1, 22 MHz Bandwidth, Body SAR, Ch 1, 1 Mbps, Left Edge

Area Scan (10x17x1): Measurement grid: dx=5mm, dy=12mm
Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
Reference Value = 13.22 V/m; Power Drift = 0.02 dB
Peak SAR (extrapolated) = 0.610 W/kg
SAR(1 g) = 0.297 W/kg

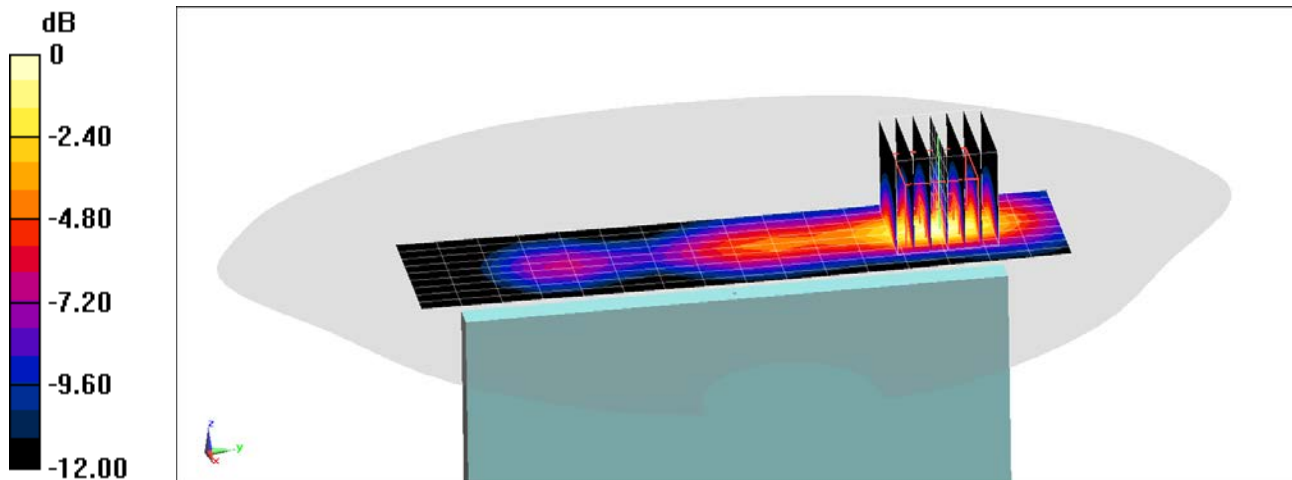

0 dB = 0.497 W/kg = -3.04 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15928

Communication System: UID 0, 802.11a 5.2-5.8 GHz Band; Frequency: 5785 MHz; Duty Cycle: 1:1
Medium: 5200-5800 Body Medium parameters used:
 $f = 5785$ MHz; $\sigma = 6.17$ S/m; $\epsilon_r = 47.758$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.4°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7538; ConvF(4.17, 4.17, 4.17) @ 5785 MHz; Calibrated: 5/18/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn728; Calibrated: 5/20/2020
Phantom: Front; Type: QD 000 P40 CD; Serial: 1686
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: IEEE 802.11a, Antenna 2, U-NII-3, 20 MHz Bandwidth,
Body SAR, Ch 157, 6 Mbps, Back Side**


Area Scan (9x9x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (7x7x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Reference Value = 1.446 V/m; Power Drift = -0.19 dB

Peak SAR (extrapolated) = 0.747 W/kg

SAR(1 g) = 0.163 W/kg

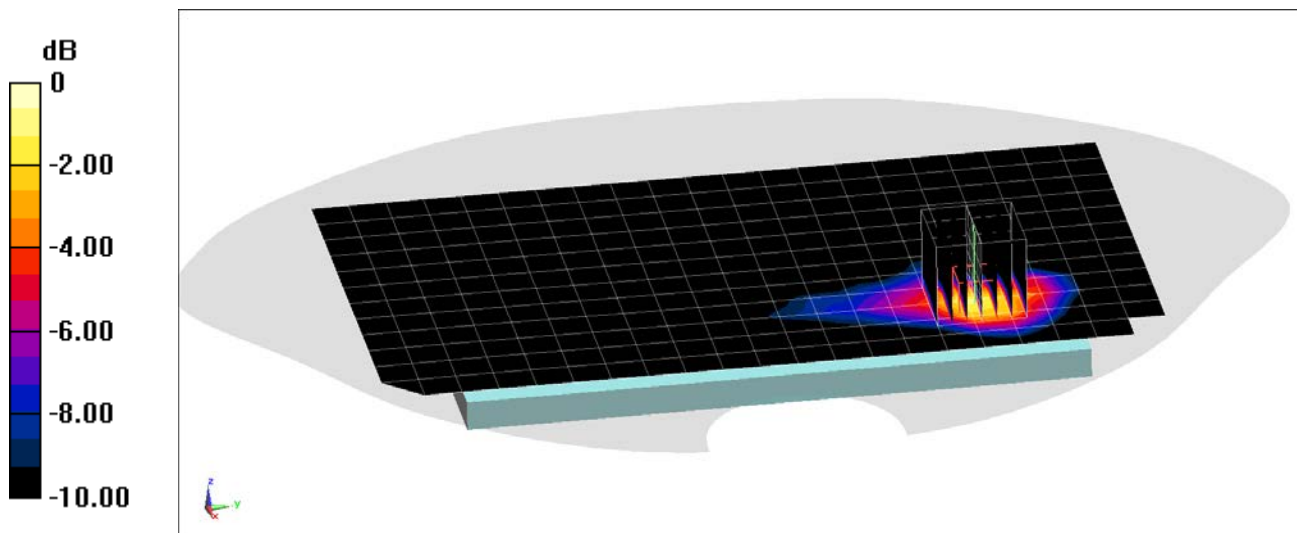

0 dB = 0.417 W/kg = -3.80 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15928

Communication System: UID 0, Bluetooth; Frequency: 2441 MHz; Duty Cycle: 1:1.300
Medium: 2450 Body Medium parameters used (interpolated):
 $f = 2441$ MHz; $\sigma = 2.004$ S/m; $\epsilon_r = 51.888$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/21/2020; Ambient Temp: 23.2°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7409; ConvF(7.24, 7.24, 7.24) @ 2441 MHz; Calibrated: 6/23/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1334; Calibrated: 6/18/2020
Phantom: LeftTwin-SAM V5.0; Type: QD 000 P40 CD; Serial: TP1375
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Bluetooth, Body SAR, Ch 39, 1 Mbps, Back Side


Area Scan (11x17x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 3.194 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 0.0450 W/kg

SAR(1 g) = 0.021 W/kg

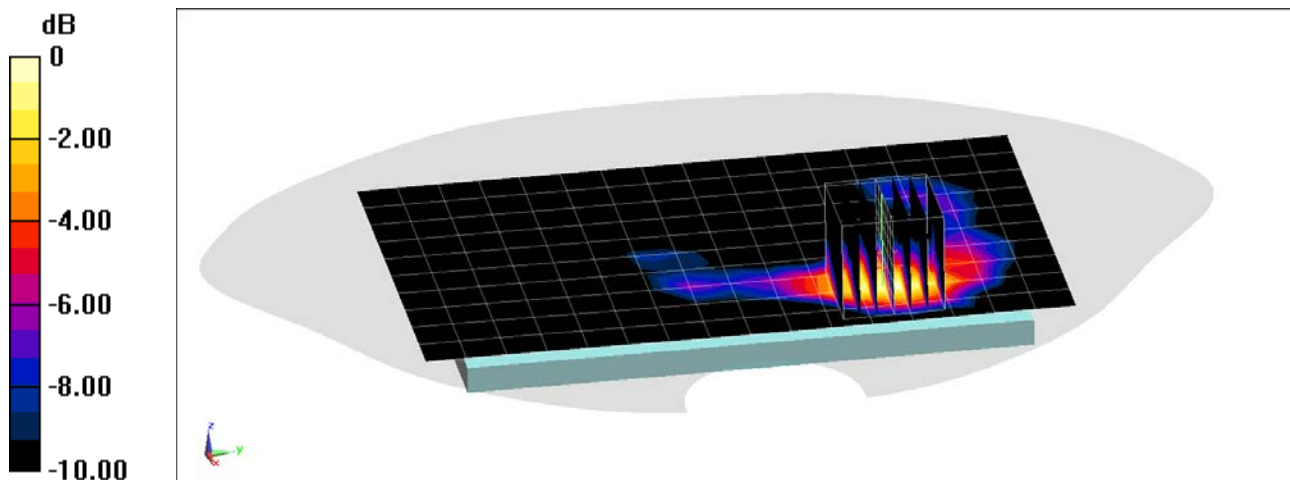

0 dB = 0.0352 W/kg = -14.53 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15928

Communication System: UID 0, Bluetooth; Frequency: 2441 MHz; Duty Cycle: 1:1.300

Medium: 2450 Body Medium parameters used (interpolated):

$f = 2441$ MHz; $\sigma = 2.004$ S/m; $\epsilon_r = 51.888$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/21/2020; Ambient Temp: 23.2°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7409; ConvF(7.24, 7.24, 7.24) @ 2441 MHz; Calibrated: 6/23/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/18/2020

Phantom: LeftTwin-SAM V5.0; Type: QD 000 P40 CD; Serial: TP1375

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: Bluetooth, Body SAR, Ch 39, 1 Mbps, Left Edge


Area Scan (10x16x1): Measurement grid: dx=5mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 4.935 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 0.0960 W/kg

SAR(1 g) = 0.042 W/kg

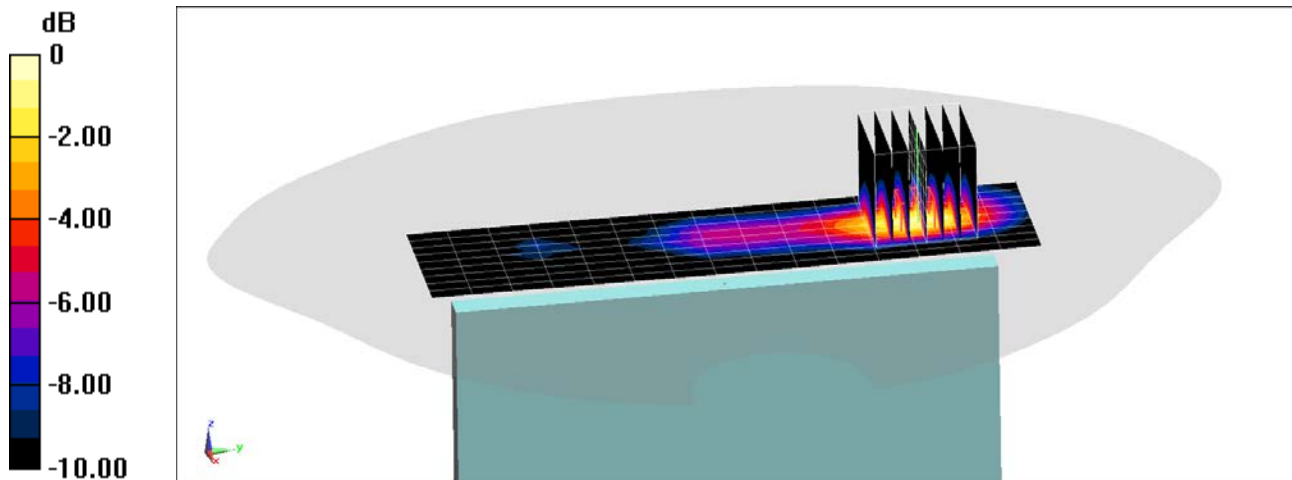

0 dB = 0.0753 W/kg = -11.23 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 92679

Communication System: UID 0, CDMA; Frequency: 1880 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1880 \text{ MHz}$; $\sigma = 1.518 \text{ S/m}$; $\epsilon_r = 52.781$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 0.0 cm

Test Date: 10/04/2020; Ambient Temp: 21.3°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7571; ConvF(7.56, 7.56, 7.56) @ 1880 MHz; Calibrated: 12/11/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1533; Calibrated: 12/5/2019

Phantom: SAM Left; Type: QD000P40CC; Serial: TP: 1375

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

Mode: PCS EVDO, Phablet SAR, Bottom Edge, Mid.ch


Area Scan (10x9x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (10x10x8)/Cube 0: Measurement grid: dx=3.8mm, dy=3.8mm, dz=1.4mm; Graded Ratio: 1.4

Reference Value = 72.47 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 26.2 W/kg

SAR(10 g) = 2.58 W/kg

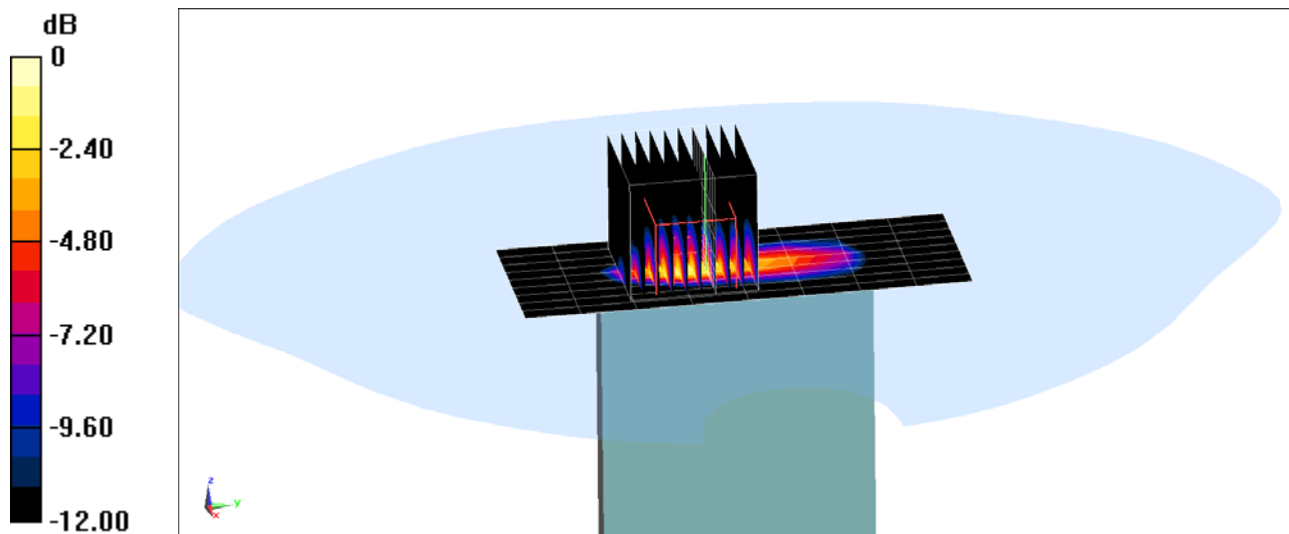

0 dB = 14.3 W/kg = 11.55 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15083

Communication System: UID 0, NR Band n66; Frequency: 1745 MHz; Duty Cycle: 1:1
Medium: 1750 Body Medium parameters used (interpolated):
 $f = 1745 \text{ MHz}$; $\sigma = 1.495 \text{ S/m}$; $\epsilon_r = 52.334$; $\rho = 1000 \text{ kg/m}^3$
Phantom section: Flat Section; Space: 0.2 cm

Test Date: 09/30/2020; Ambient Temp: 20.3°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1745 MHz; Calibrated: 12/13/2019
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn1532; Calibrated: 12/5/2019
Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n66, Phablet SAR, Right Edge, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 349000, 50 RB, 28 RB Offset**


Area Scan (10x15x1): Measurement grid: $dx=5\text{mm}$, $dy=15\text{mm}$

Zoom Scan (13x13x8)/Cube 0: Measurement grid: $dx=2.7\text{mm}$, $dy=2.7\text{mm}$, $dz=1.4\text{mm}$; Graded Ratio: 1.4

Reference Value = 56.52 V/m; Power Drift = -0.07 dB

Peak SAR (extrapolated) = 14.2 W/kg

SAR(10 g) = 1.51 W/kg

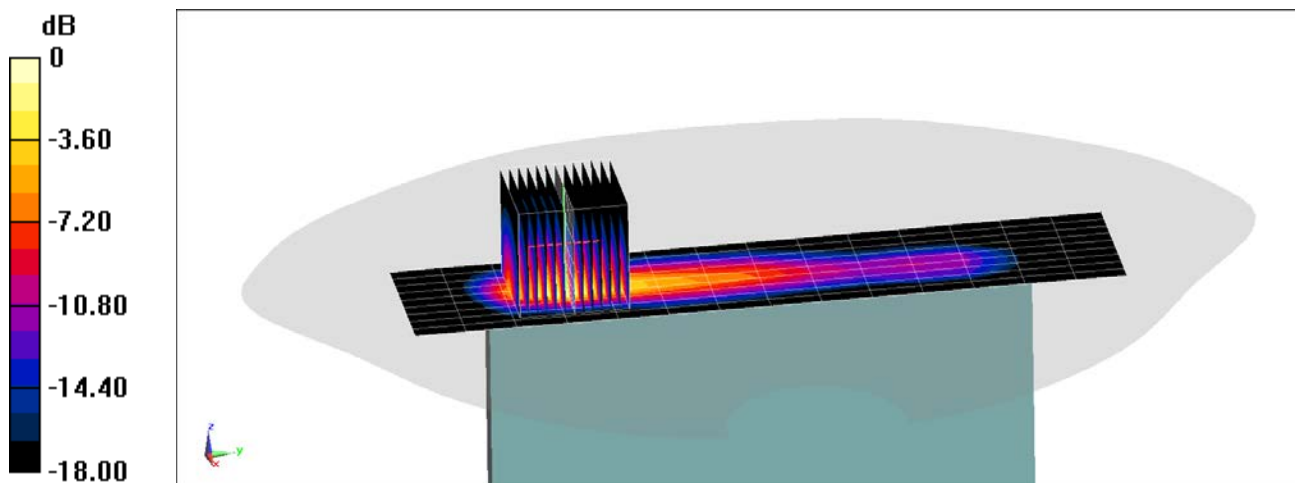

0 dB = 8.48 W/kg = 9.28 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15837

Communication System: UID 0, NR Band n2; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.589$ S/m; $\epsilon_r = 51.095$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 0.2 cm

Test Date: 09/28/2020; Ambient Temp: 23.1°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7490; ConvF(8.22, 8.22, 8.22) @ 1900 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: NR Band n2, Phablet SAR, Right Edge, 20 MHz Bandwidth,
DFT-s-OFDM QPSK, Ch. 380000, 1 RB, 104 RB Offset**


Area Scan (11x15x1): Measurement grid: dx=5mm, dy=15mm

Zoom Scan (12x12x8)/Cube 0: Measurement grid: dx=2.8mm, dy=2.8mm, dz=1.4mm; Graded Ratio: 1.4

Reference Value = 56.11 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 13.2 W/kg

SAR(10 g) = 1.59 W/kg

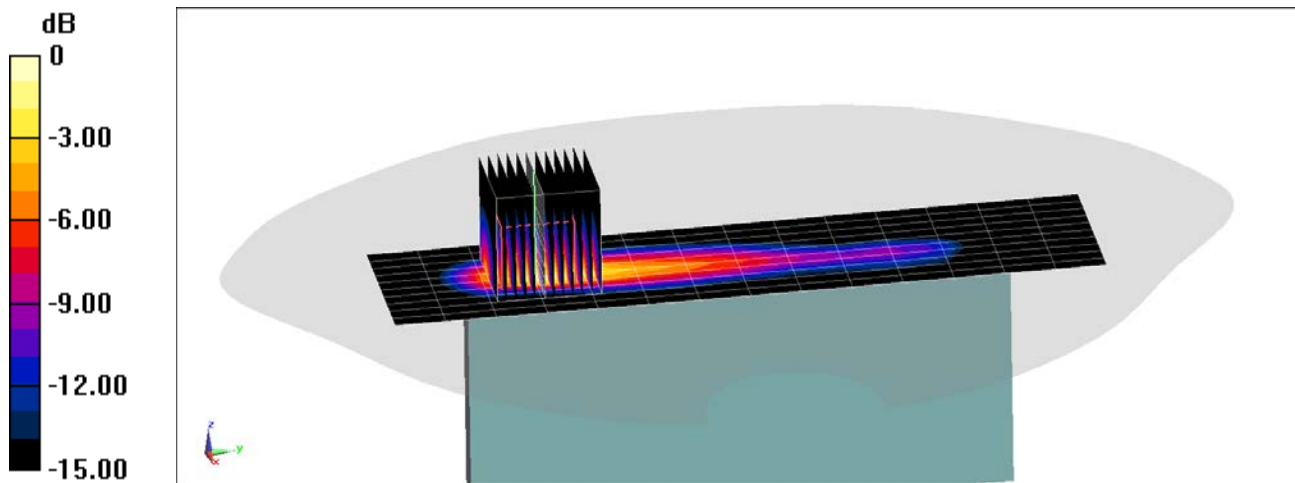

0 dB = 8.20 W/kg = 9.14 dBW/kg

PCTEST

DUT: ZNFK920AM; Type: Portable Handset; Serial: 15928

Communication System: UID 0, 802.11a 5.2-5.8 GHz Band; Frequency: 5280 MHz; Duty Cycle: 1:1
Medium: 5200-5800 Body Medium parameters used:
 $f = 5280$ MHz; $\sigma = 5.453$ S/m; $\epsilon_r = 48.541$; $\rho = 1000$ kg/m³
Phantom section: Flat Section; Space: 0.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.5°C; Tissue Temp: 24.1°C

Probe: EX3DV4 - SN7538; ConvF(4.6, 4.6, 4.6) @ 5280 MHz; Calibrated: 5/18/2020
Sensor-Surface: 1.4mm (Mechanical Surface Detection)
Electronics: DAE4 Sn728; Calibrated: 5/20/2020
Phantom: Front; Type: QD 000 P40 CD; Serial: 1686
Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

**Mode: IEEE 802.11a, Antenna 2, U-NII-2A, 20 MHz Bandwidth,
Phablet SAR, Ch 56, 6 Mbps, Left Edge**


Area Scan (10x22x1): Measurement grid: dx=5mm, dy=10mm

Zoom Scan (9x9x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Reference Value = 2.480 V/m; Power Drift = 0.20 dB

Peak SAR (extrapolated) = 8.47 W/kg

SAR(10 g) = 0.449 W/kg

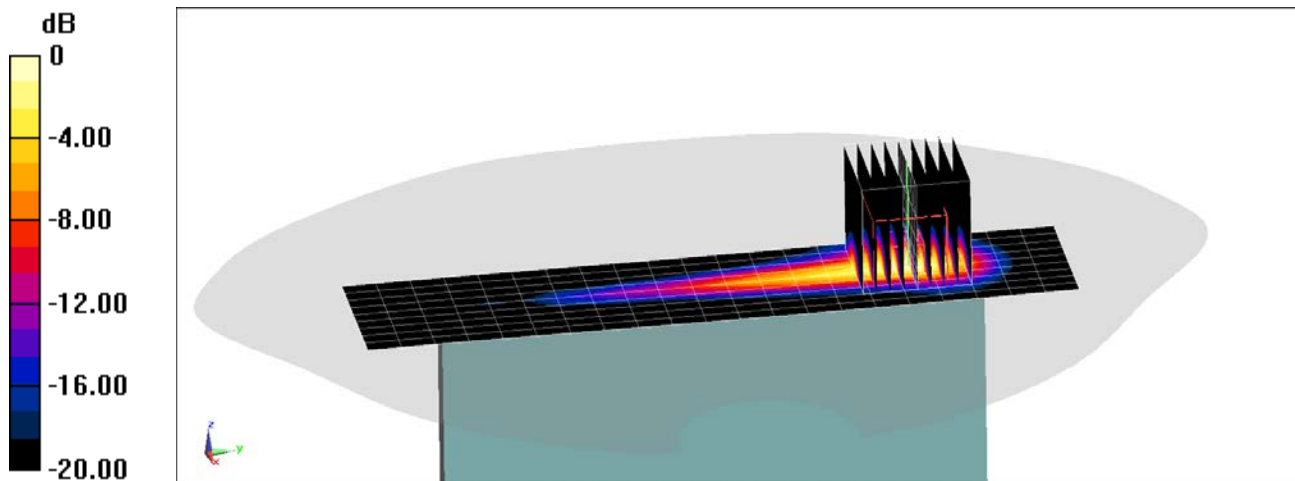

0 dB = 4.50 W/kg = 6.53 dBW/kg

APPENDIX B: SYSTEM VERIFICATION

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Head Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.894 \text{ S/m}$; $\epsilon_r = 40.461$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/22/2020; Ambient Temp: 20.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7490; ConvF(10.25, 10.25, 10.25) @ 750 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) Main use; Type: QD 000 P40 CC; Serial: 1406

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.55 W/kg

SAR(1 g) = 1.69 W/kg

Deviation(1 g) = 1.56%

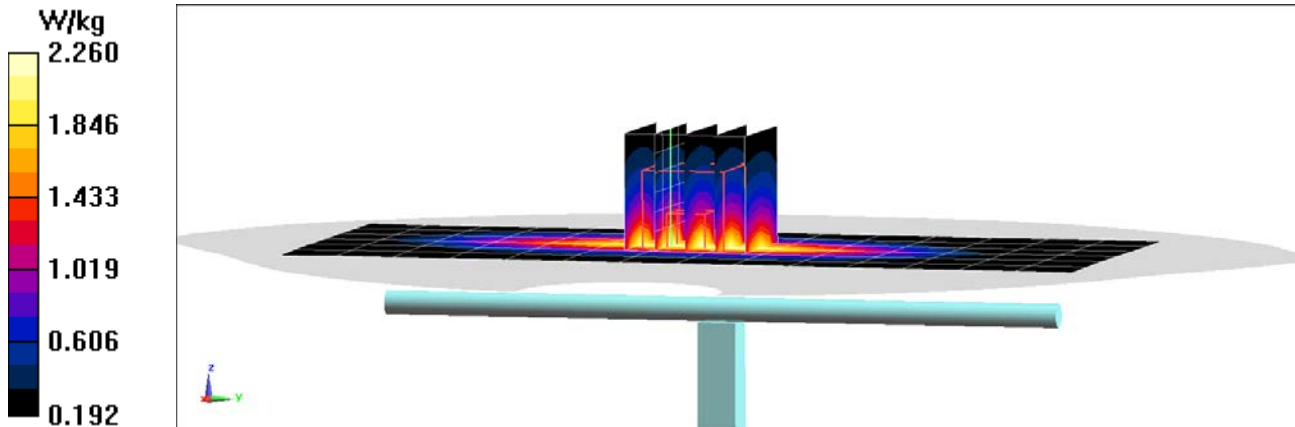

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Head Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.9 \text{ S/m}$; $\epsilon_r = 41.583$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/25/2020; Ambient Temp: 22.1°C; Tissue Temp: 21.3°C

Probe: EX3DV4 - SN7532; ConvF(10.72, 10.72, 10.72) @ 750 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.50 W/kg

SAR(1 g) = 1.66 W/kg

Deviation(1 g) = -0.24%

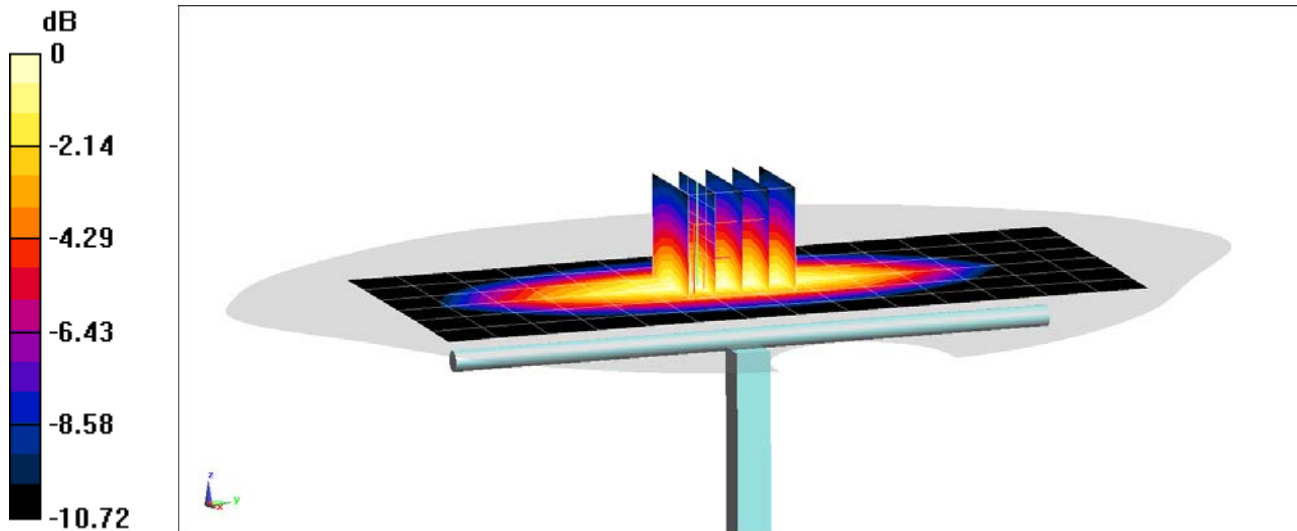

0 dB = 2.26 W/kg = 3.54 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d040

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.89 \text{ S/m}$; $\epsilon_r = 40.38$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/22/2020; Ambient Temp: 22.2°C; Tissue Temp: 20.6°C

Probe: EX3DV4 - SN7427; ConvF(9.58, 9.58, 9.58) @ 835 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.72 W/kg

SAR(1 g) = 1.84 W/kg

Deviation(1 g) = -3.16%

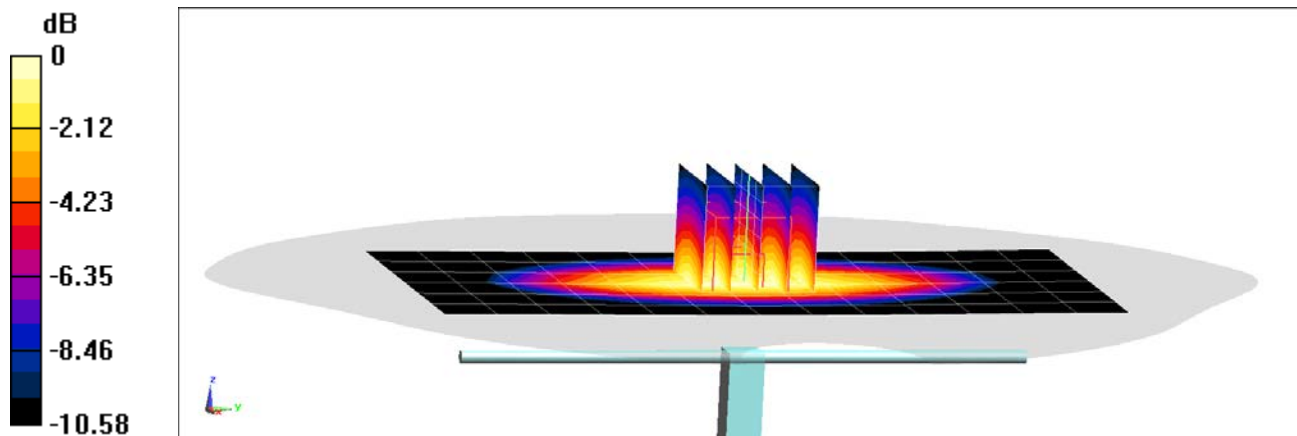

0 dB = 2.44 W/kg = 3.87 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d040

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.89 \text{ S/m}$; $\epsilon_r = 40.516$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/24/2020; Ambient Temp: 22.4°C; Tissue Temp: 21.2°C

Probe: EX3DV4 - SN7427; ConvF(9.58, 9.58, 9.58) @ 835 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.87 W/kg

SAR(1 g) = 1.98 W/kg

Deviation(1 g) = 4.21%

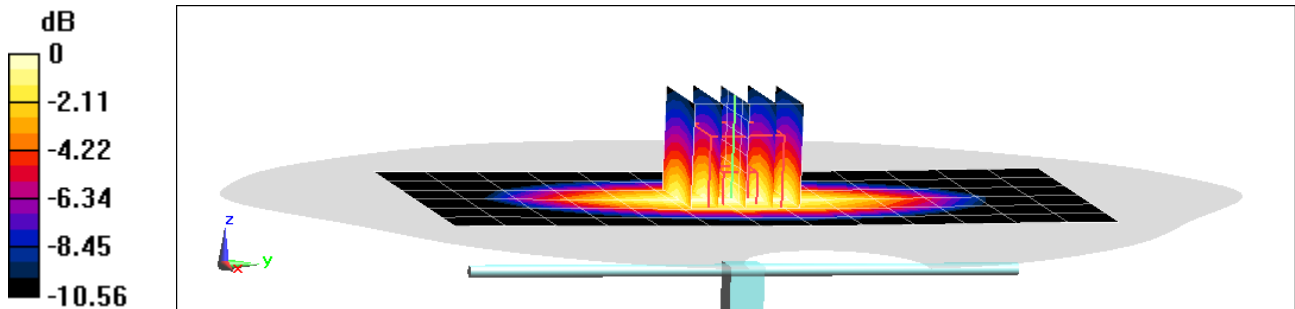

0 dB = 2.60 W/kg = 4.15 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d132

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.941 \text{ S/m}$; $\epsilon_r = 43.307$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/30/2020; Ambient Temp: 22.7°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7406; ConvF(9.61, 9.61, 9.61) @ 835 MHz; Calibrated: 6/23/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 5/14/2020

Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.90 W/kg

SAR(1 g) = 1.92 W/kg

Deviation(1 g) = -0.52%

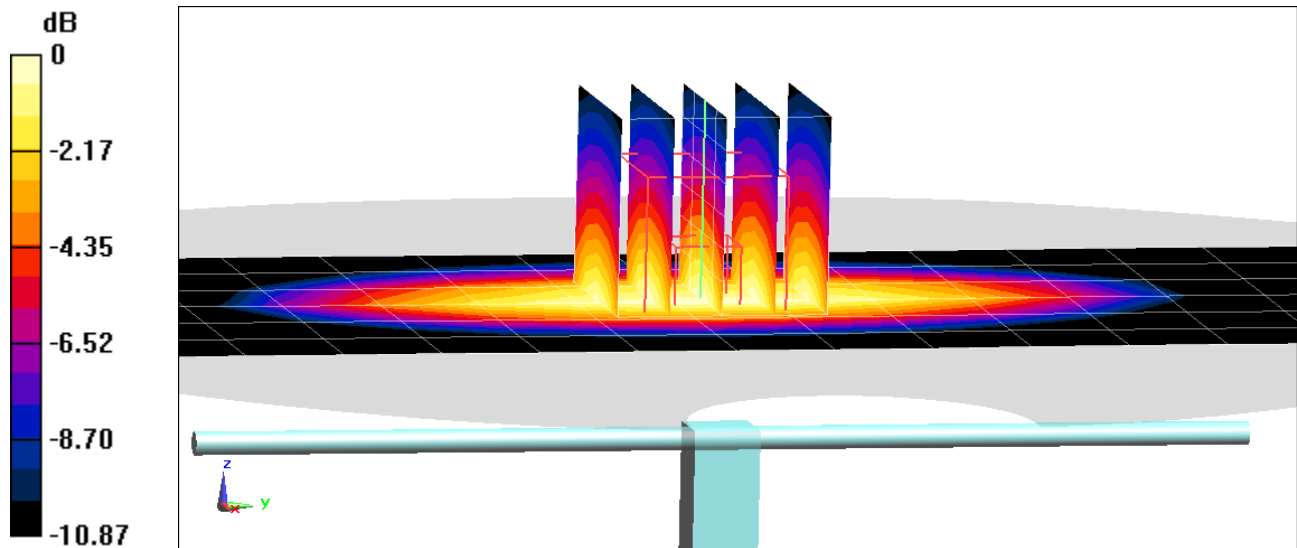

0 dB = 2.58 W/kg = 4.12 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d132

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.945 \text{ S/m}$; $\epsilon_r = 42.974$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 10/02/2020; Ambient Temp: 22.9°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN7406; ConvF(9.61, 9.61, 9.61) @ 835 MHz; Calibrated: 6/23/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 5/14/2020

Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.05 W/kg

SAR(1 g) = 1.96 W/kg

Deviation(1 g) = 1.55%

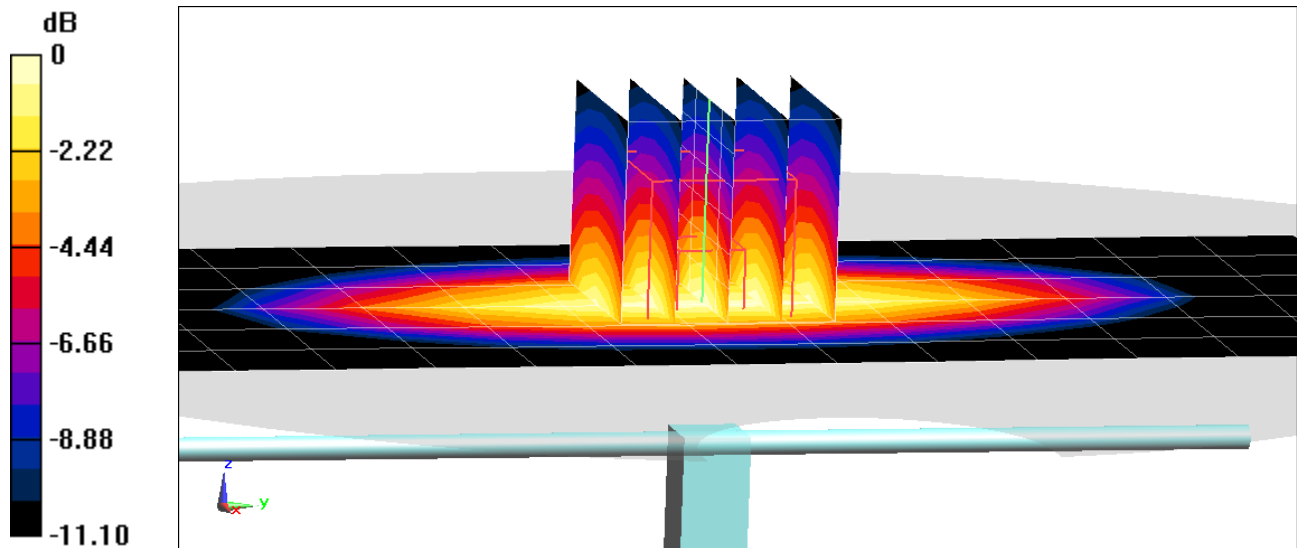

0 dB = 2.67 W/kg = 4.27 dBW/kg

PCTEST

DUT: Dipole 850 MHz; Type: D850V2; Serial: 1009

Communication System: UID 0, CW; Frequency: 850 MHz; Duty Cycle: 1:1

Medium: 835 Head Medium parameters used:

$f = 850 \text{ MHz}$; $\sigma = 0.948 \text{ S/m}$; $\epsilon_r = 43.257$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/29/2020; Ambient Temp: 22.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7421; ConvF(9.24, 9.24, 9.24) @ 850 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

850 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.19 W/kg

SAR(1 g) = 2.14 W/kg

Deviation(1 g) = 5.94%

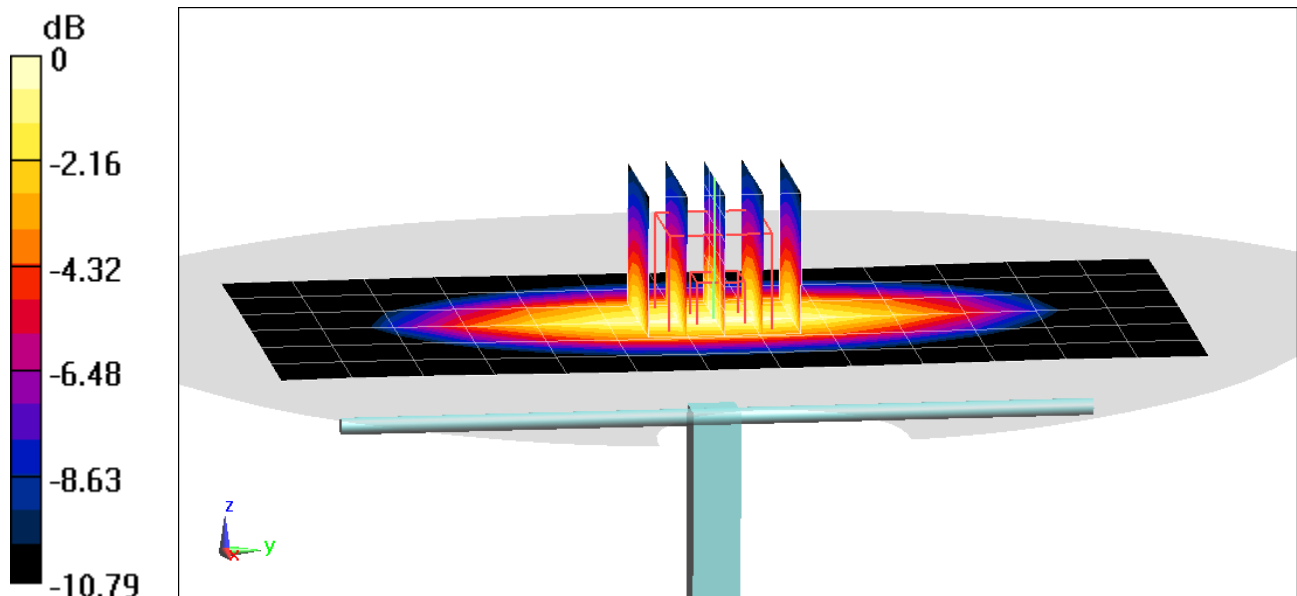

0 dB = 2.87 W/kg = 4.58 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1083

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Head Medium parameters used:

$f = 1750$ MHz; $\sigma = 1.339$ S/m; $\epsilon_r = 39.194$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/18/2020; Ambient Temp: 20.5°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7532; ConvF(8.46, 8.46, 8.46) @ 1750 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.90 W/kg

SAR(1 g) = 3.71 W/kg

Deviation(1 g) = 2.77%

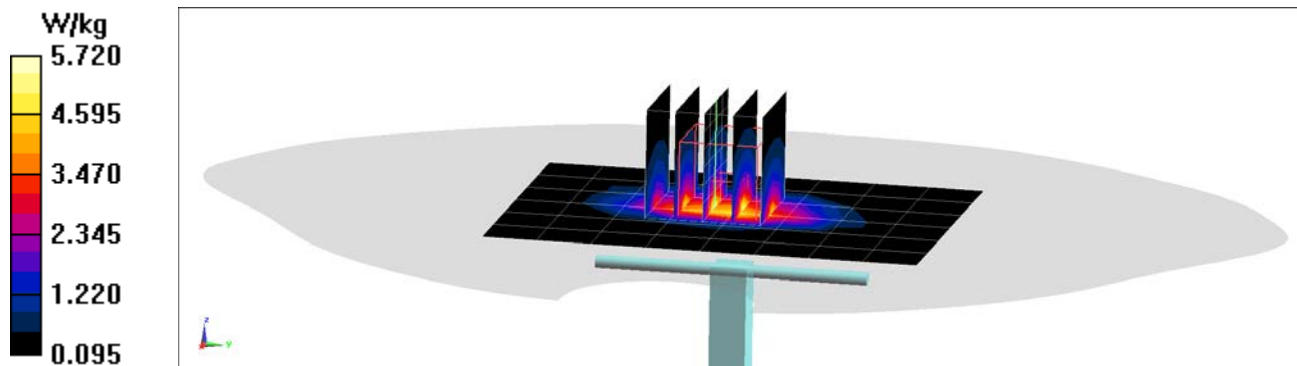

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1092

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Head Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.342 \text{ S/m}$; $\epsilon_r = 38.703$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/21/2020; Ambient Temp: 20.7°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7532; ConvF(8.46, 8.46, 8.46) @ 1750 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.71 W/kg

SAR(1 g) = 3.6 W/kg

Deviation(1 g) = -0.28%

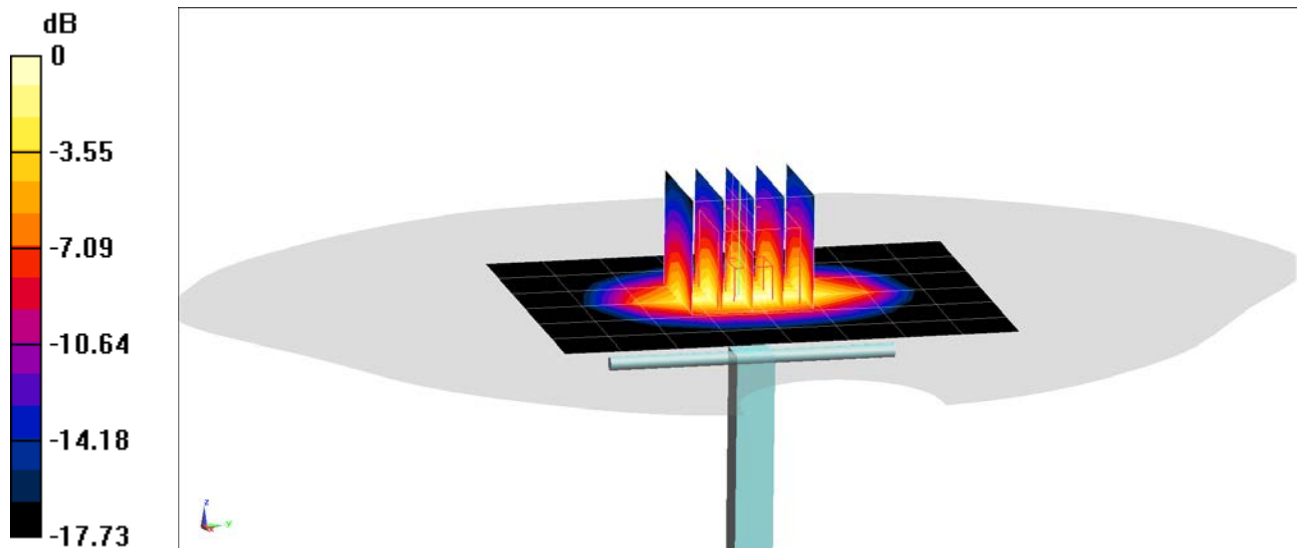

0 dB = 5.56 W/kg = 7.45 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1092

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Head Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.339 \text{ S/m}$; $\epsilon_r = 38.888$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/29/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7427; ConvF(8.42, 8.42, 8.42) @ 1750 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.86 W/kg

SAR(1 g) = 3.66 W/kg

Deviation(1 g) = 1.39%

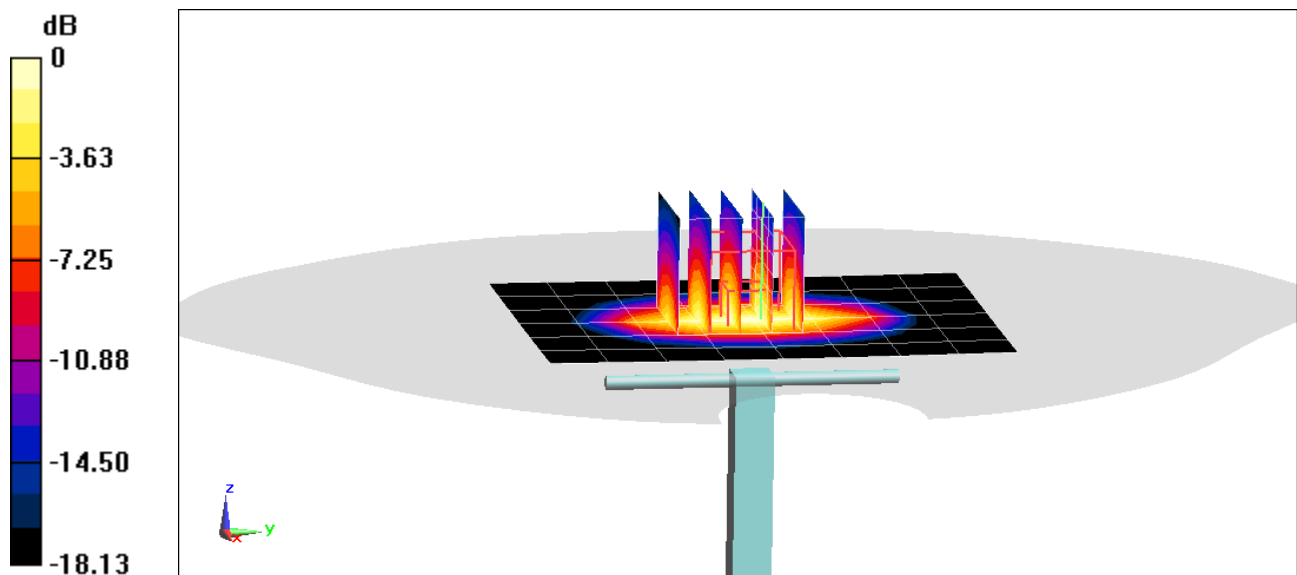

0 dB = 5.60 W/kg = 7.48 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d026

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.427$ S/m; $\epsilon_r = 38.835$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/23/2020; Ambient Temp: 23.5°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7532; ConvF(8.06, 8.06, 8.06) @ 1900 MHz; Calibrated: 4/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn501; Calibrated: 4/15/2020

Phantom: Twin-SAM V8.0_Left; Type: QD 000 P41 AA; Serial: 1935

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.43 W/kg

SAR(1 g) = 3.85 W/kg

Deviation(1 g) = -4.23%

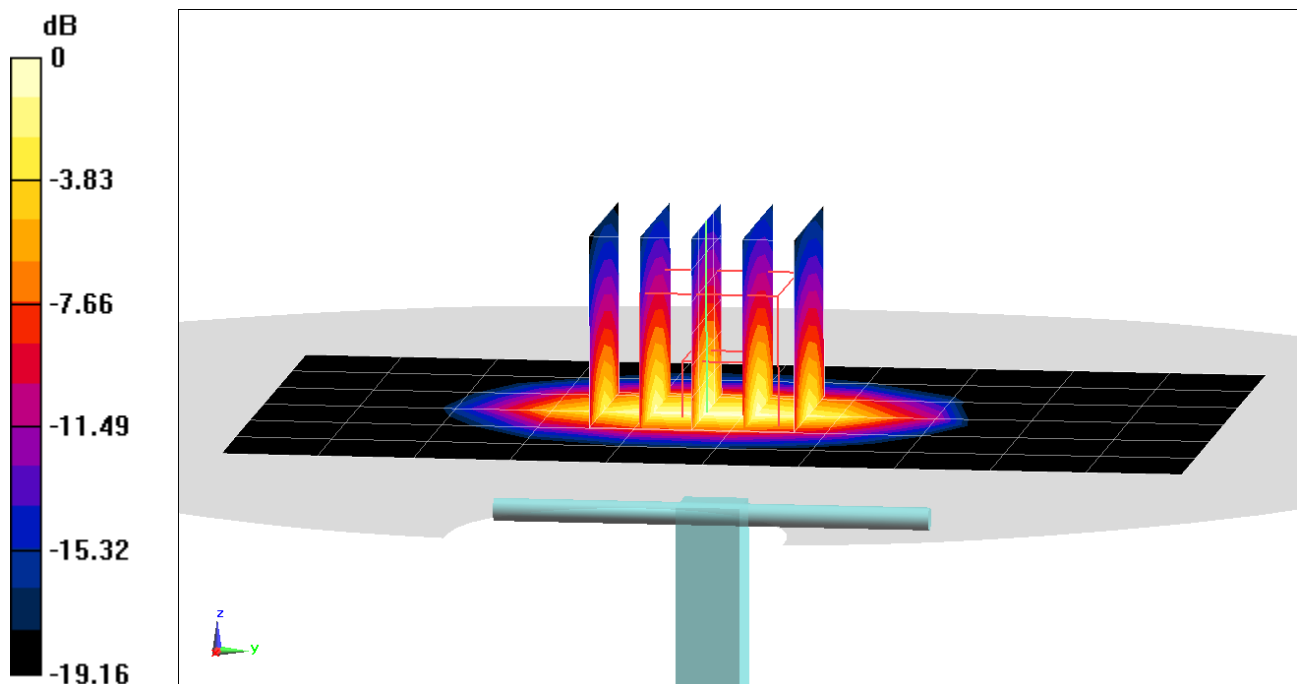

0 dB = 6.13 W/kg = 7.87 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d030

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used (interpolated):

$f = 1900 \text{ MHz}$; $\sigma = 1.444 \text{ S/m}$; $\epsilon_r = 38.617$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 21.9°C; Tissue Temp: 22.0°C

Probe: EX3DV4 - SN7427; ConvF(8.12, 8.12, 8.12) @ 1900 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.77 W/kg

SAR(1 g) = 3.99 W/kg

Deviation(1 g) = 0.00%

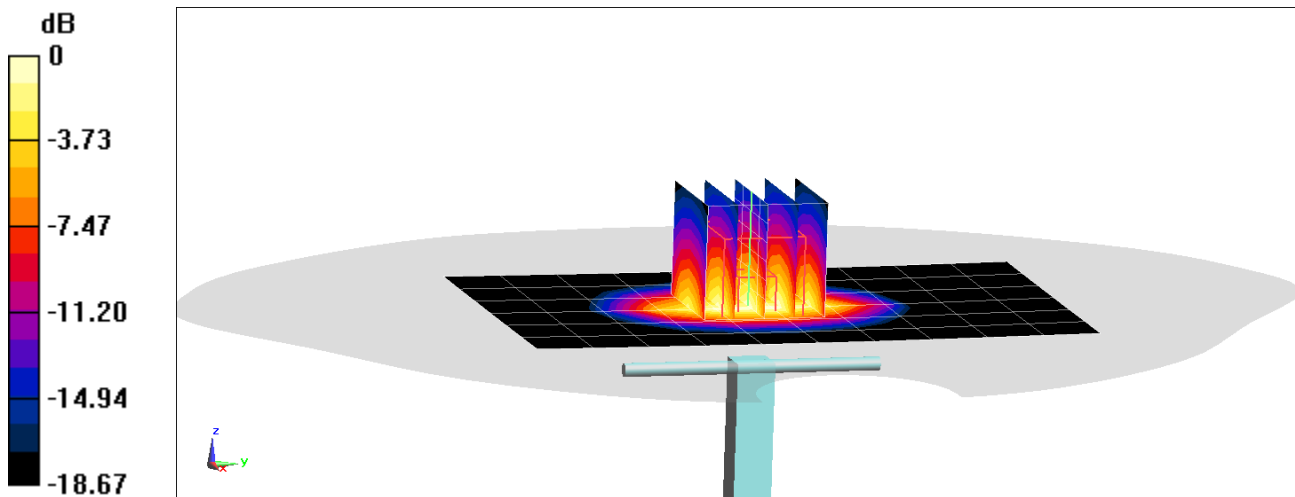

0 dB = 6.38 W/kg = 8.05 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d148

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Head Medium parameters used:

$f = 1900$ MHz; $\sigma = 1.456$ S/m; $\epsilon_r = 40.754$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7406; ConvF(7.96, 7.96, 7.96) @ 1900 MHz; Calibrated: 6/23/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1583; Calibrated: 5/14/2020

Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1966

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.63 W/kg

SAR(1 g) = 4.06 W/kg

Deviation(1 g) = 3.84%

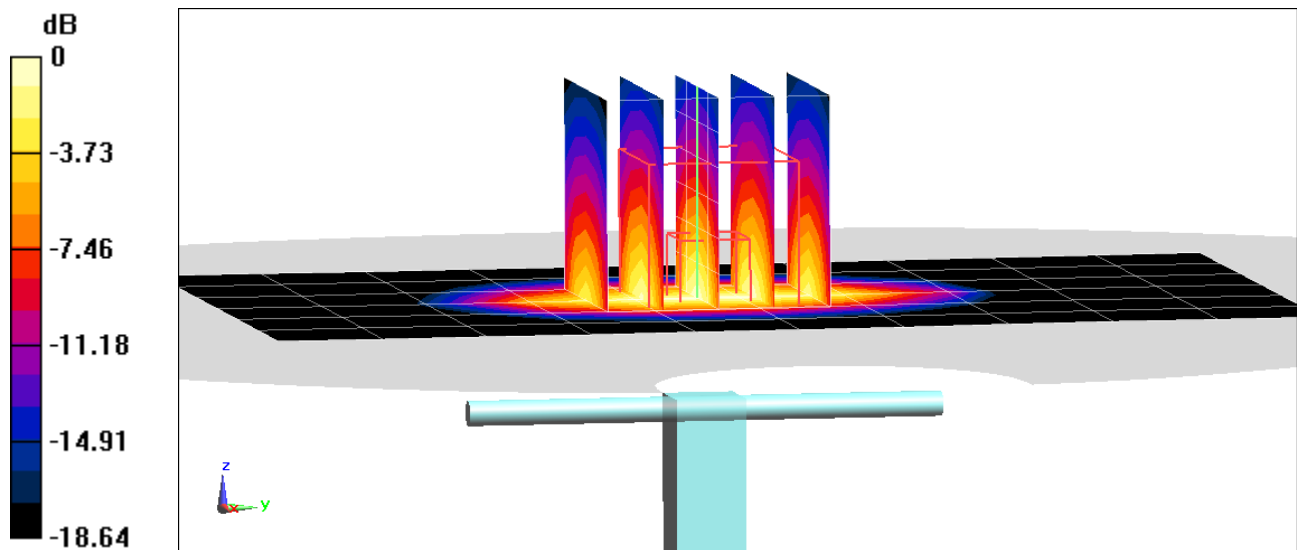

PCTEST

DUT: Dipole 2300 MHz; Type: D2300V2; Serial: 1038

Communication System: UID 0, CW; Frequency: 2300 MHz; Duty Cycle: 1:1

Medium: 2450 Head Medium parameters used:

$f = 2300$ MHz; $\sigma = 1.637$ S/m; $\epsilon_r = 39.875$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/25/2020; Ambient Temp: 23.0°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 2300 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2300 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 10.3 W/kg

SAR(1 g) = 5.07 W/kg

Deviation(1 g) = 2.84%

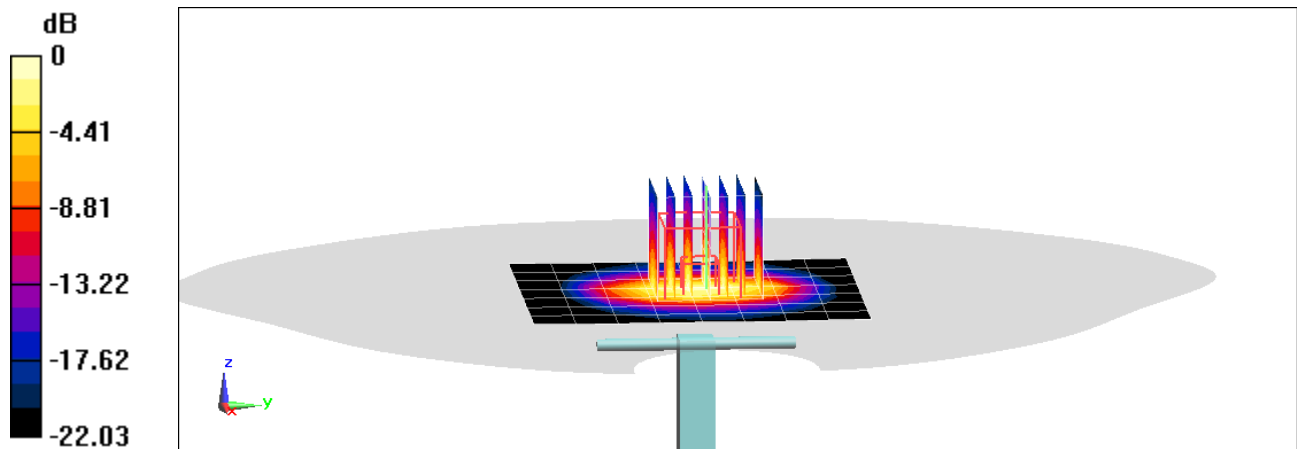

0 dB = 8.34 W/kg = 9.21 dBW/kg

PCTEST

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 981

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Head Medium parameters used:

$f = 2450$ MHz; $\sigma = 1.827$ S/m; $\epsilon_r = 38.791$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0cm

Test Date: 09/29/2020; Ambient Temp: 23.1°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN3589; ConvF(6.85, 6.85, 6.85) @ 2450 MHz; Calibrated: 1/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1558; Calibrated: 1/13/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1647

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2450 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 11.0 W/kg

SAR(1 g) = 5.19 W/kg

Deviation(1 g) = -0.76%

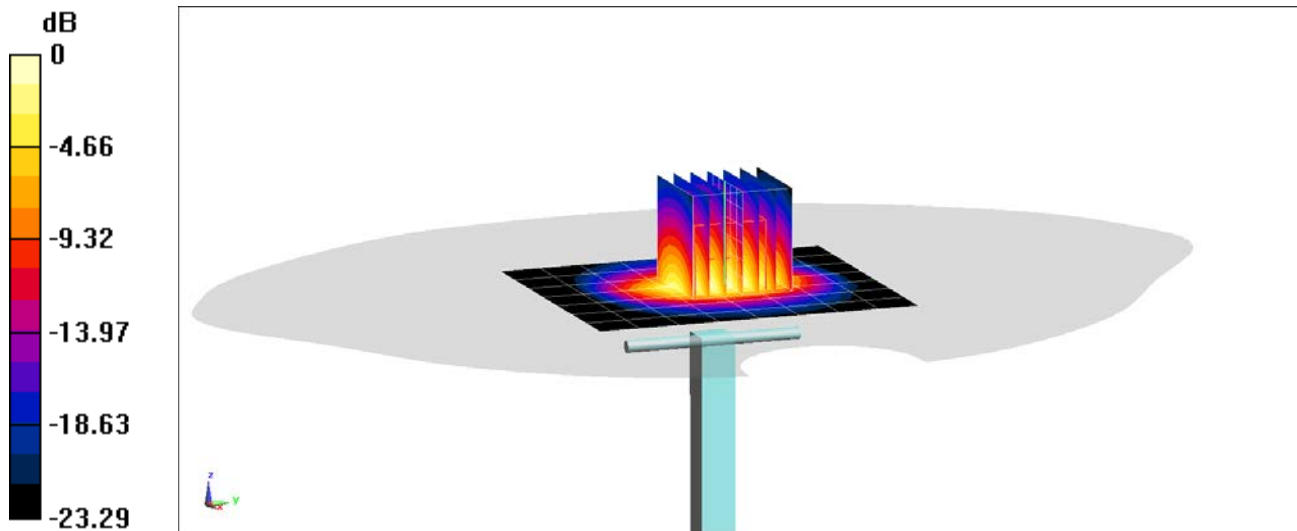

0 dB = 8.75 W/kg = 9.42 dBW/kg

PCTEST

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 981

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Head Medium parameters used:

$f = 2450 \text{ MHz}$; $\sigma = 1.83 \text{ S/m}$; $\epsilon_r = 38.329$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/02/2020; Ambient Temp: 23.1°C; Tissue Temp: 22.9°C

Probe: EX3DV4 - SN3589; ConvF(6.85, 6.85, 6.85) @ 2450 MHz; Calibrated: 1/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1558; Calibrated: 1/13/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1647

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2450 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 11.3 W/kg

SAR(1 g) = 5.35 W/kg

Deviation(1 g) = 2.29%

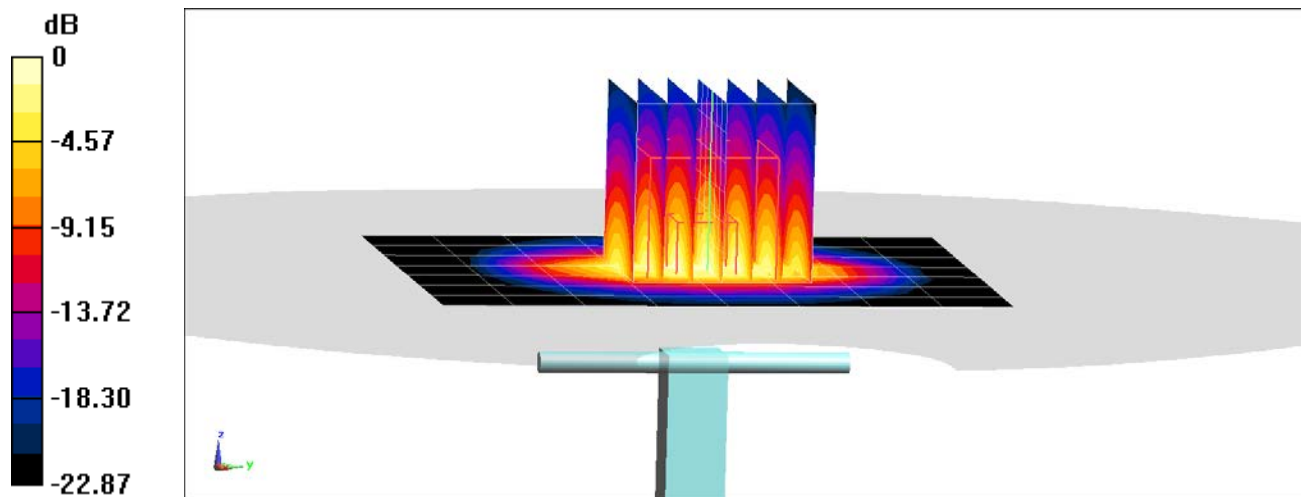

0 dB = 9.08 W/kg = 9.58 dBW/kg

PCTEST

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: 1042

Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: 2450 Head Medium parameters used:

$f = 2600$ MHz; $\sigma = 1.986$ S/m; $\epsilon_r = 38.727$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/25/2020; Ambient Temp: 23.0°C; Tissue Temp: 23.7°C

Probe: EX3DV4 - SN7421; ConvF(7.24, 7.24, 7.24) @ 2600 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2600 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 13.6 W/kg

SAR(1 g) = 6.03 W/kg

Deviation(1 g) = 4.51%

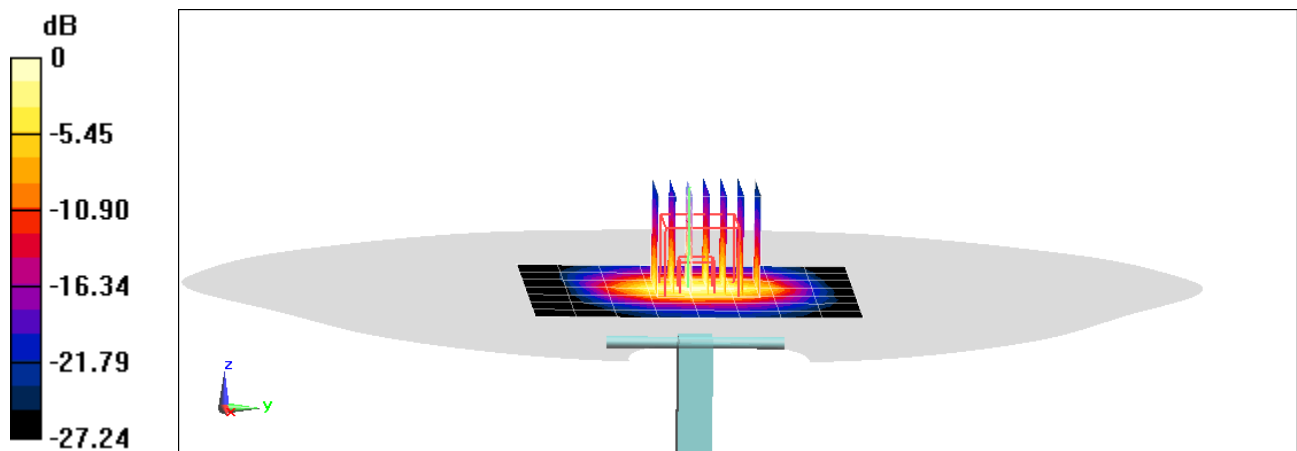

0 dB = 10.5 W/kg = 10.21 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1120

Communication System: UID 0, CW; Frequency: 5250 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Head Medium parameters used:

$f = 5250$ MHz; $\sigma = 4.494$ S/m; $\epsilon_r = 35.188$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(5.14, 5.14, 5.14) @ 5250 MHz; Calibrated: 4/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/15/2020

Phantom: Twin-SAM V5.0(20); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5250 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.2 W/kg

SAR(1 g) = 3.9 W/kg

Deviation(1 g) = -2.86%

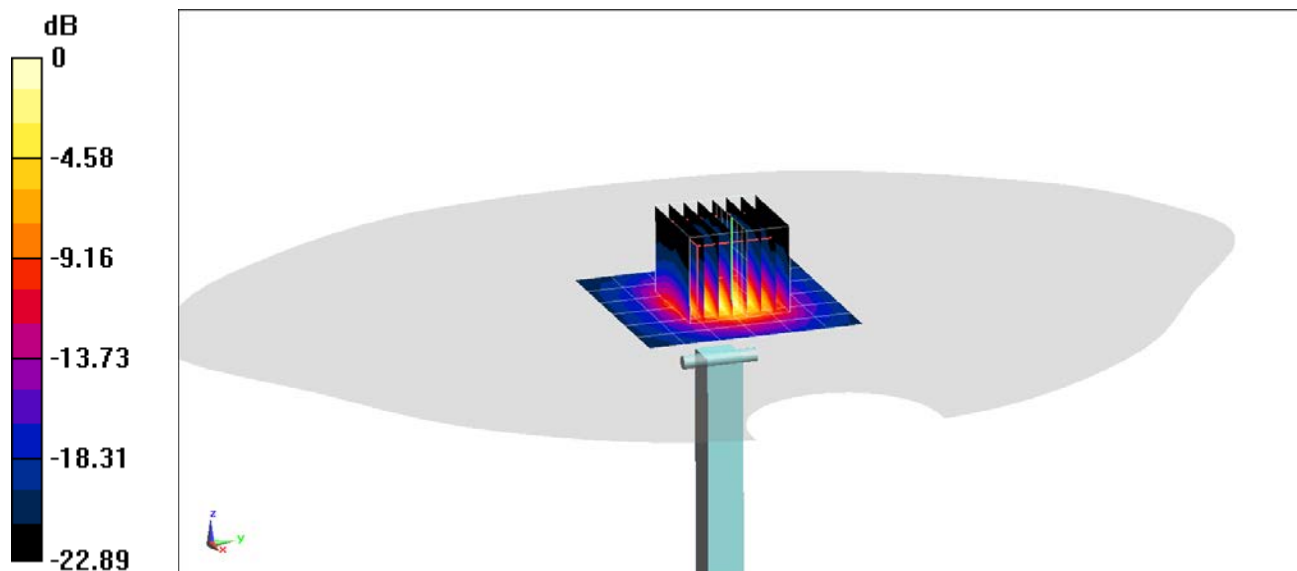

0 dB = 8.93 W/kg = 9.51 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1120

Communication System: UID 0, CW; Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Head Medium parameters used:

$f = 5600$ MHz; $\sigma = 4.839$ S/m; $\epsilon_r = 34.706$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(4.75, 4.75, 4.75) @ 5600 MHz; Calibrated: 4/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/15/2020

Phantom: Twin-SAM V5.0(20); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5600 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.3 W/kg

SAR(1 g) = 4.09 W/kg

Deviation(1 g) = -2.15%

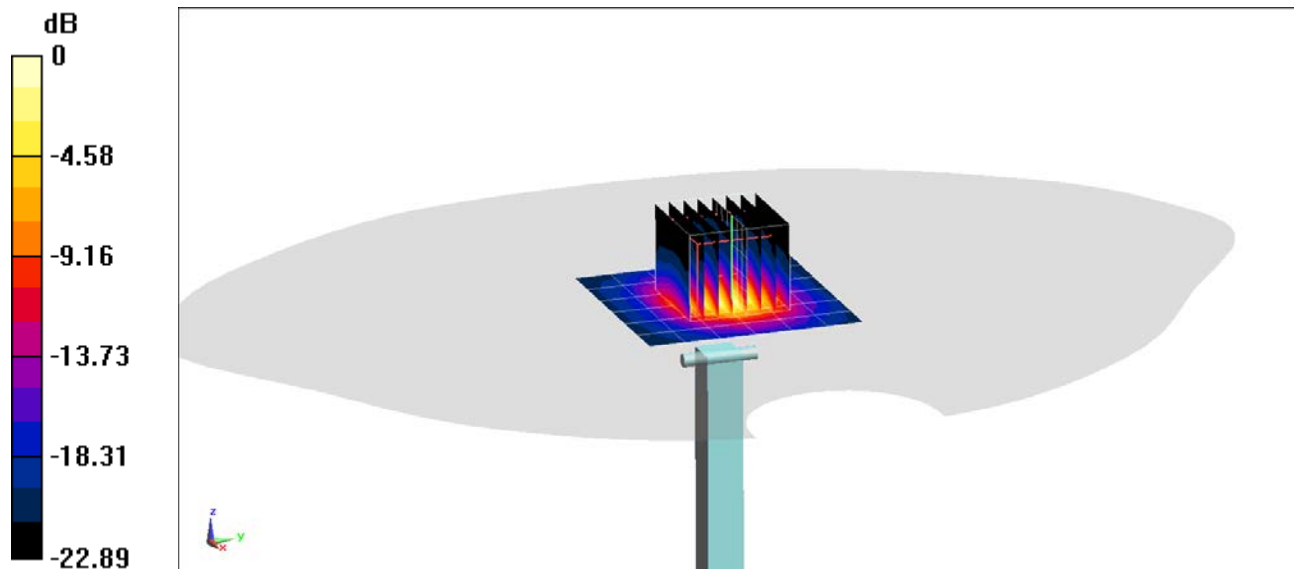

0 dB = 9.86 W/kg = 9.94 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1120

Communication System: UID 0, CW; Frequency: 5750 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Head Medium parameters used:

$f = 5750$ MHz; $\sigma = 5.001$ S/m; $\epsilon_r = 34.562$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 22.5°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(4.7, 4.7, 4.7) @ 5750 MHz; Calibrated: 4/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/15/2020

Phantom: Twin-SAM V5.0(20); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5750 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x7)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.0 W/kg

SAR(1 g) = 3.94 W/kg

Deviation(1 g) = -1.99%

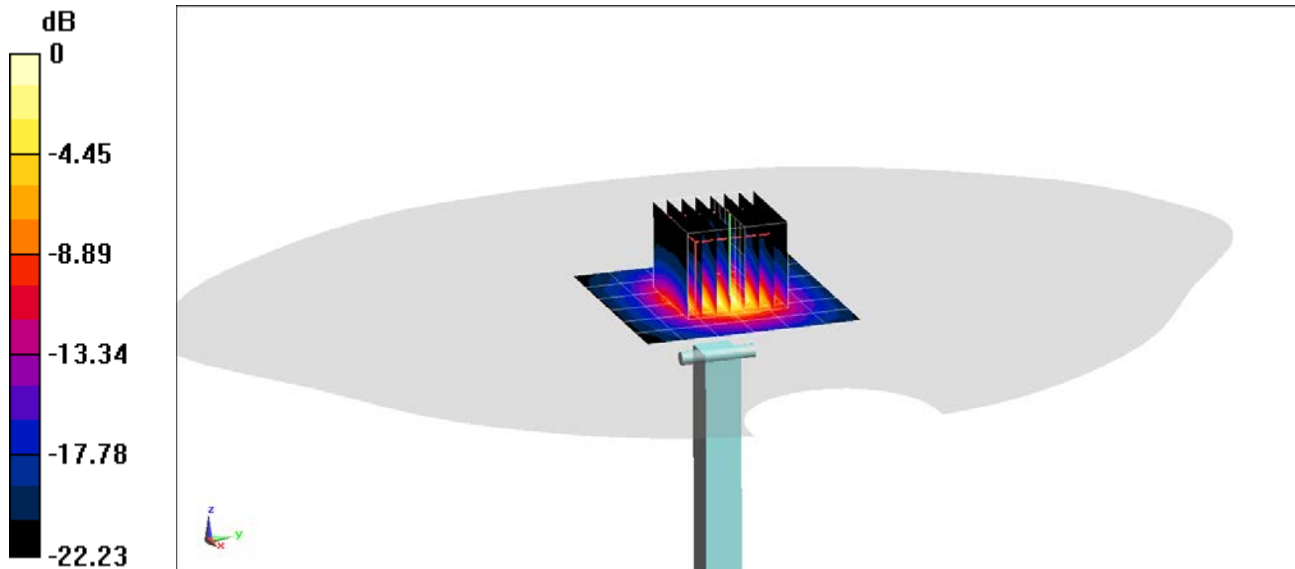

0 dB = 9.42 W/kg = 9.74 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.967 \text{ S/m}$; $\epsilon_r = 54.919$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/23/2020; Ambient Temp: 21.9°C; Tissue Temp: 21.6°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 750 MHz; Calibrated: 7/16/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1402; Calibrated: 7/9/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.80 W/kg

SAR(1 g) = 1.73 W/kg

Deviation(1 g) = 0.93%

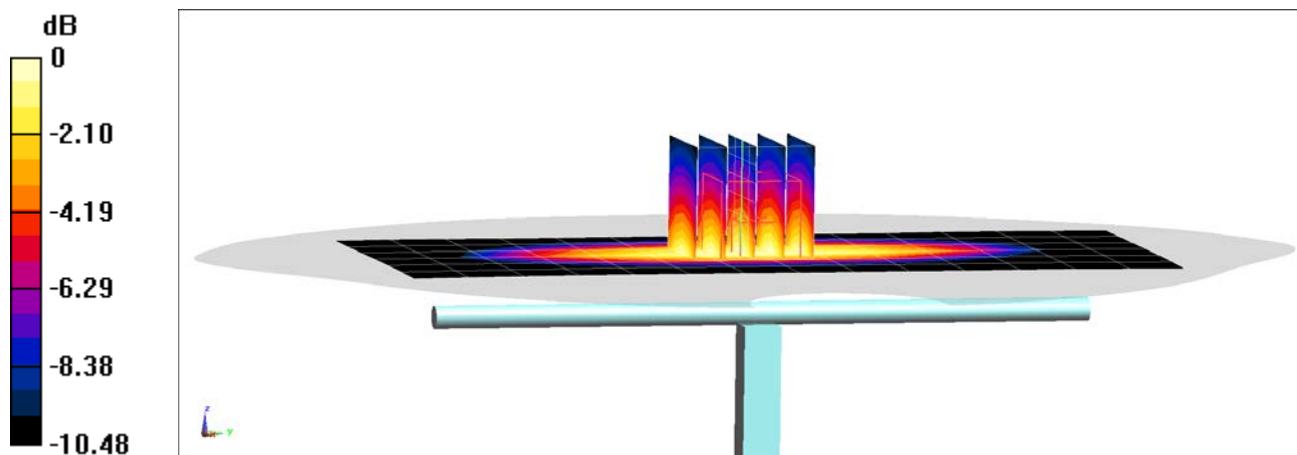

0 dB = 2.65 W/kg = 4.23 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.965 \text{ S/m}$; $\epsilon_r = 53.809$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/25/2020; Ambient Temp: 22.3°C; Tissue Temp: 21.9°C

Probe: EX3DV4 - SN7491; ConvF(10.44, 10.44, 10.44) @ 750 MHz; Calibrated: 7/16/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1402; Calibrated: 7/9/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1596

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.71 W/kg

SAR(1 g) = 1.74 W/kg

Deviation(1 g) = 1.52%

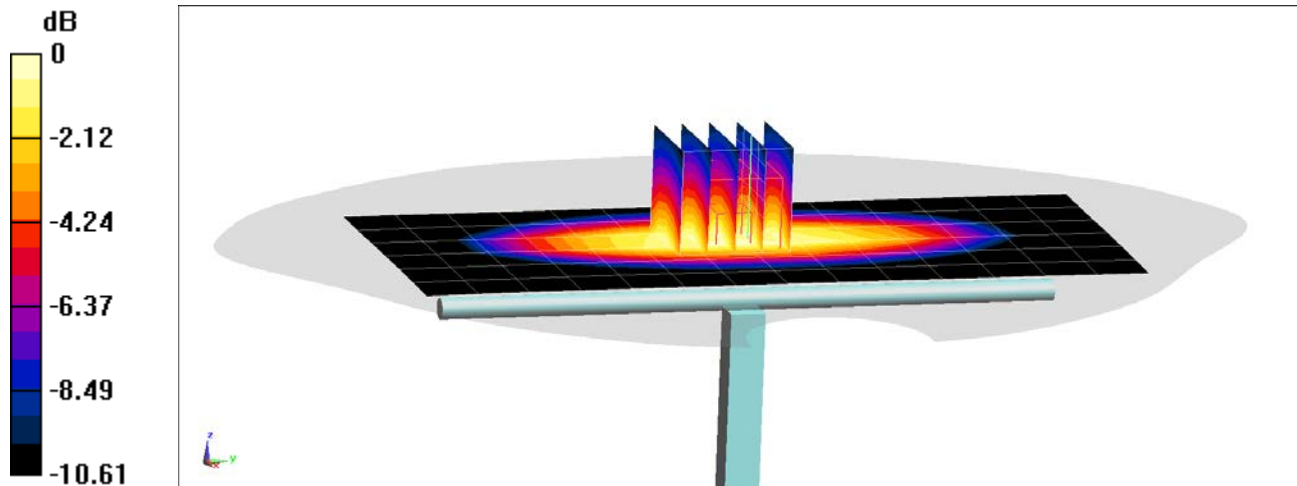

0 dB = 2.35 W/kg = 3.71 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.978 \text{ S/m}$; $\epsilon_r = 54.116$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/30/2020; Ambient Temp: 20.0°C; Tissue Temp: 19.9°C

Probe: EX3DV4 - SN3837; ConvF(9.55, 9.55, 9.55) @ 750 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.77 W/kg

SAR(1 g) = 1.8 W/kg

Deviation(1 g) = 5.02%

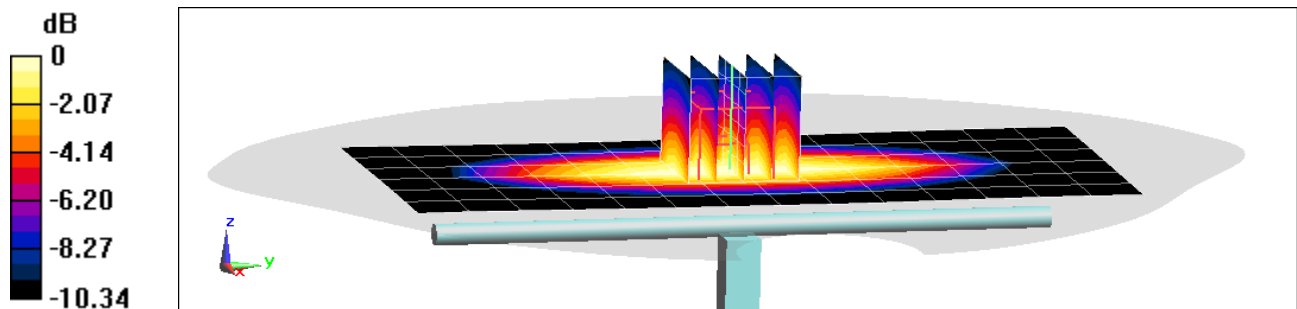

0 dB = 2.43 W/kg = 3.86 dBW/kg

PCTEST

DUT: Dipole 750 MHz; Type: D750V3; Serial: 1034

Communication System: UID 0, CW; Frequency: 750 MHz; Duty Cycle: 1:1

Medium: 750 Body Medium parameters used (interpolated):

$f = 750 \text{ MHz}$; $\sigma = 0.993 \text{ S/m}$; $\epsilon_r = 53.971$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/30/2020; Ambient Temp: 22.7°C; Tissue Temp: 21.4°C

Probe: EX3DV4 - SN7490; ConvF(10.37, 10.37, 10.37) @ 750 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

750 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x15x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.65 W/kg

SAR(1 g) = 1.7 W/kg

Deviation(1 g) = -0.82%

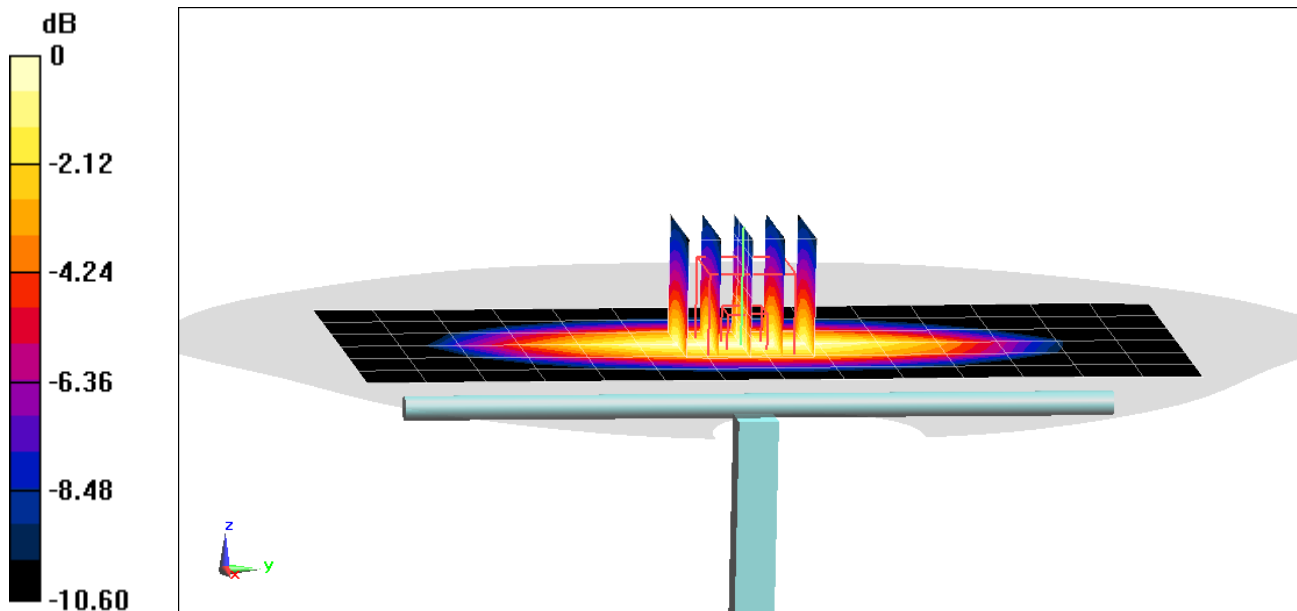

0 dB = 2.32 W/kg = 3.65 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d040

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 1.014 \text{ S/m}$; $\epsilon_r = 53.355$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(10.18, 10.18, 10.18) @ 835 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.12 W/kg

SAR(1 g) = 1.99 W/kg

Deviation(1 g) = 4.41%

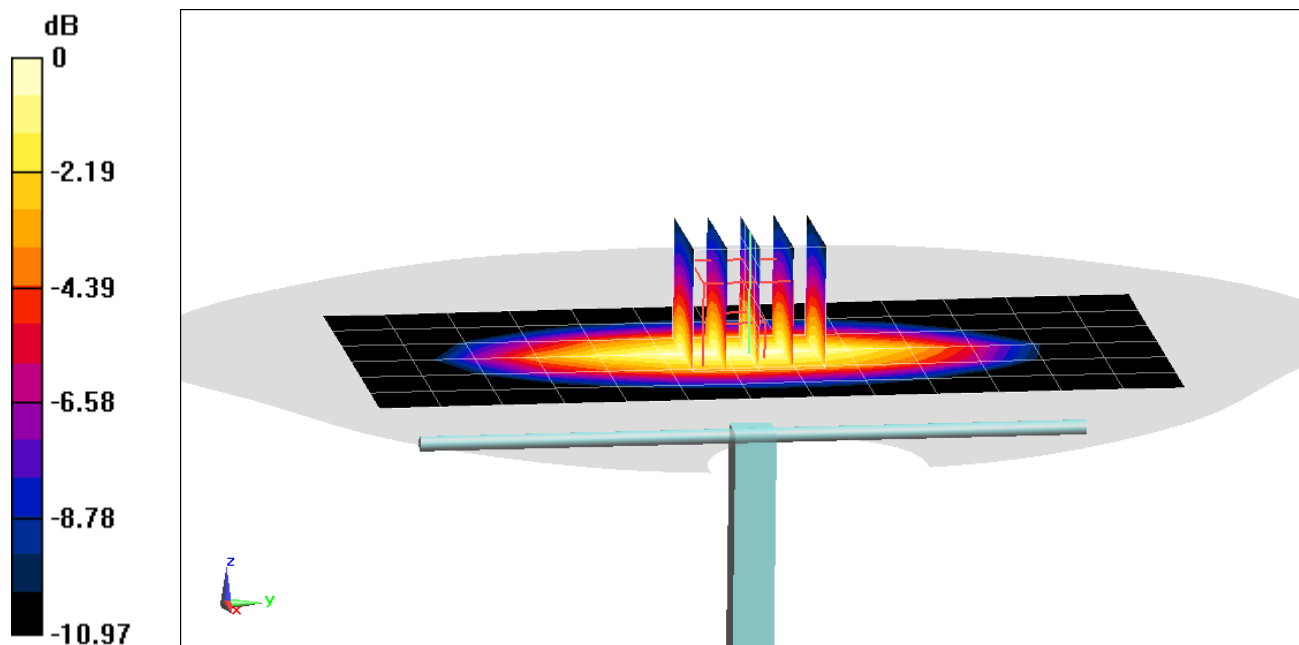

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d132

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body; Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 0.954 \text{ S/m}$; $\epsilon_r = 54.606$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/28/2020; Ambient Temp: 22.0°C; Tissue Temp: 21.5°C

Probe: EX3DV4 - SN7308; ConvF(9.92, 9.92, 9.92) @ 835 MHz; Calibrated: 7/31/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1450; Calibrated: 8/11/2020

Phantom: Twin-SAM V5.0; Type: QD 000 P40 CD; Serial: 1792

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 2.92 W/kg

SAR(1 g) = 1.88 W/kg

Deviation(1 g) = -5.62%

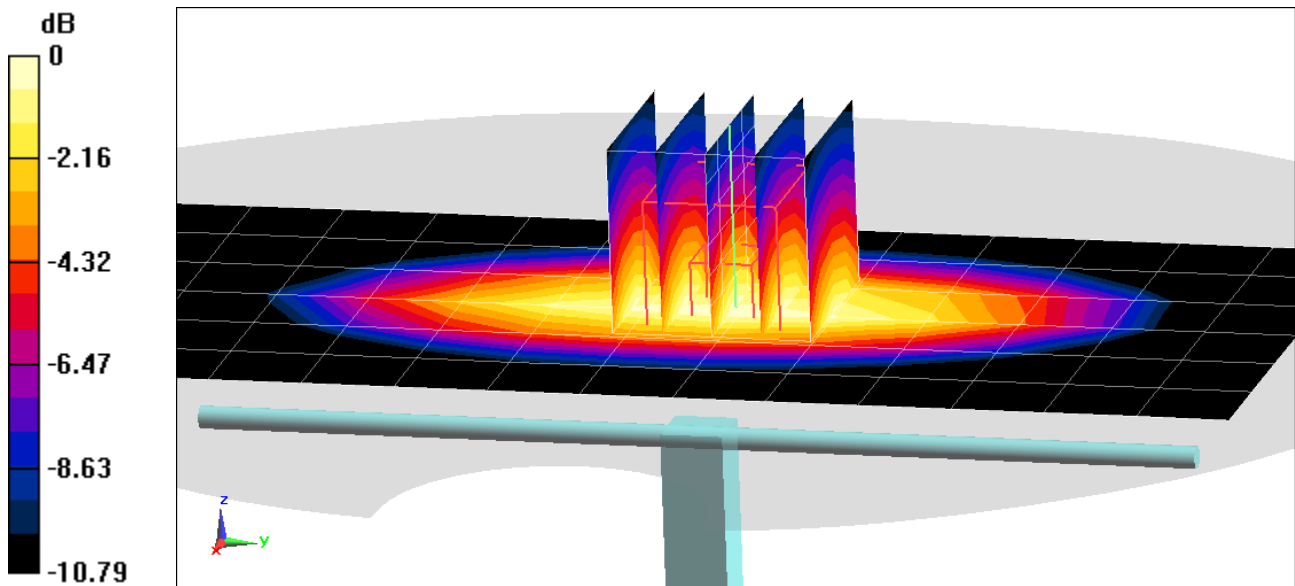

0 dB = 2.55 W/kg = 4.07 dBW/kg

PCTEST

DUT: Dipole 835 MHz; Type: D835V2; Serial: 4d040

Communication System: UID 0, CW; Frequency: 835 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 835 \text{ MHz}$; $\sigma = 1.01 \text{ S/m}$; $\epsilon_r = 53.737$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/28/2020; Ambient Temp: 24.5°C; Tissue Temp: 22.1°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 835 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

835 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.18 W/kg

SAR(1 g) = 2.07 W/kg

Deviation(1 g) = 8.60%

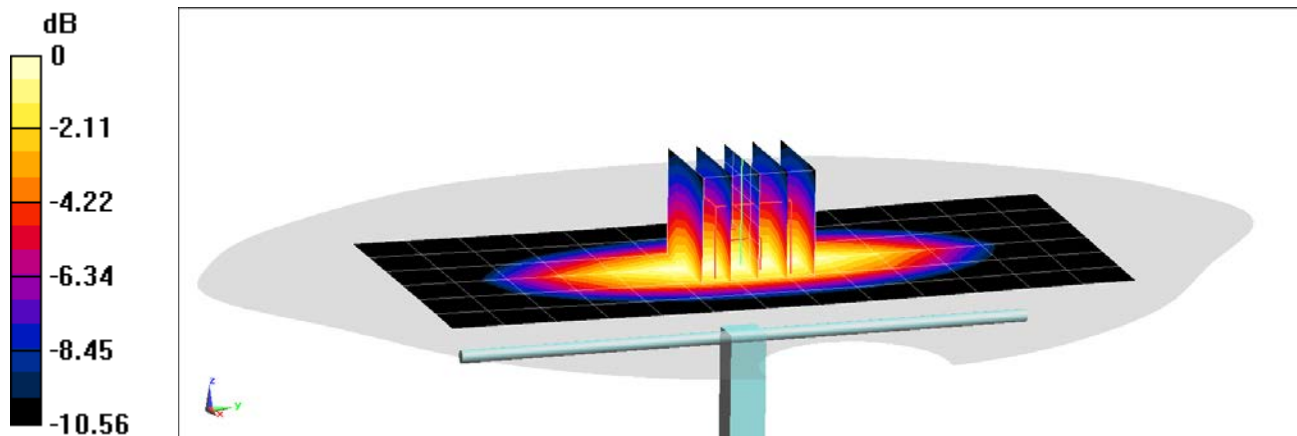

0 dB = 2.79 W/kg = 4.46 dBW/kg

PCTEST

DUT: Dipole 850 MHz; Type: D850V2; Serial: 1009

Communication System: UID 0, CW; Frequency: 850 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 850 \text{ MHz}$; $\sigma = 1 \text{ S/m}$; $\epsilon_r = 54.436$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/23/2020; Ambient Temp: 22.3°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 850 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

850 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.28 W/kg

SAR(1 g) = 2.05 W/kg

Deviation(1 g) = 2.50%

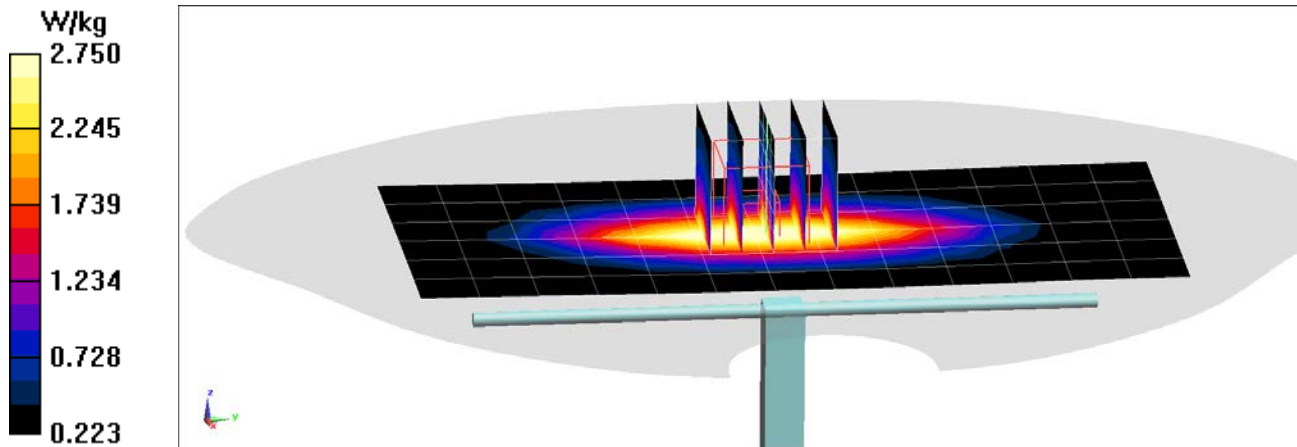

PCTEST

DUT: Dipole 850 MHz; Type: D850V2; Serial: 1009

Communication System: UID 0, CW; Frequency: 850 MHz; Duty Cycle: 1:1

Medium: 835 Body Medium parameters used:

$f = 850 \text{ MHz}$; $\sigma = 0.998 \text{ S/m}$; $\epsilon_r = 54.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.5 cm

Test Date: 09/25/2020; Ambient Temp: 25.0°C; Tissue Temp: 21.8°C

Probe: EX3DV4 - SN3837; ConvF(9.37, 9.37, 9.37) @ 850 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

850 MHz System Verification at 23.0 dBm (200 mW)


Area Scan (7x14x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 3.45 W/kg

SAR(1 g) = 2.17 W/kg

Deviation(1 g) = 8.50%

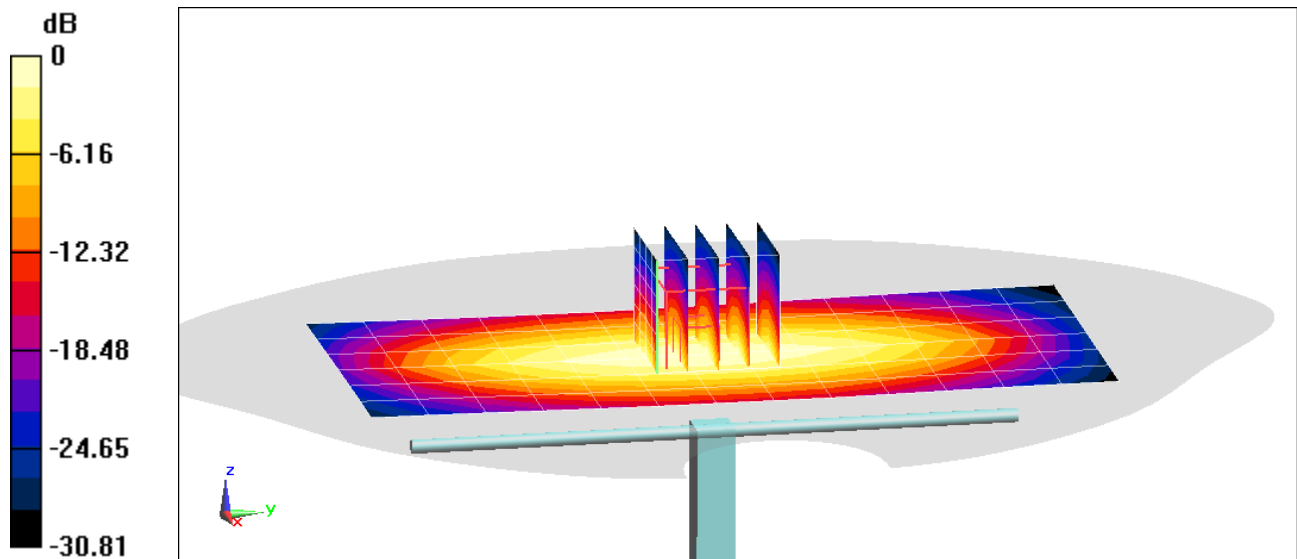

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1083

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750$ MHz; $\sigma = 1.505$ S/m; $\epsilon_r = 52.063$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 20.1°C; Tissue Temp: 19.4°C

Probe: EX3DV4 - SN7416; ConvF(7.85, 7.85, 7.85) @ 1750 MHz; Calibrated: 6/22/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn701; Calibrated: 6/11/2020

Phantom: Twin-SAM V8.0; Type: QD 000 P41 Ax; Serial: 1936

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.89 W/kg

SAR(1 g) = 3.78 W/kg

Deviation(1 g) = 1.89%

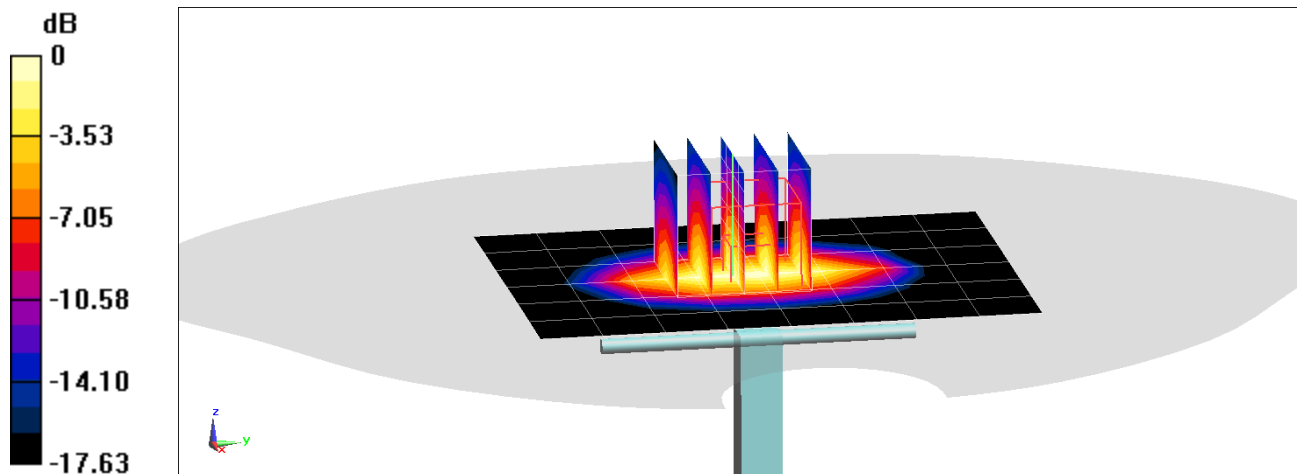

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1083

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.51 \text{ S/m}$; $\epsilon_r = 51.895$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 23.3°C; Tissue Temp: 21.1°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1750 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.45 W/kg

SAR(1 g) = 3.59 W/kg

Deviation(1 g) = -3.23%

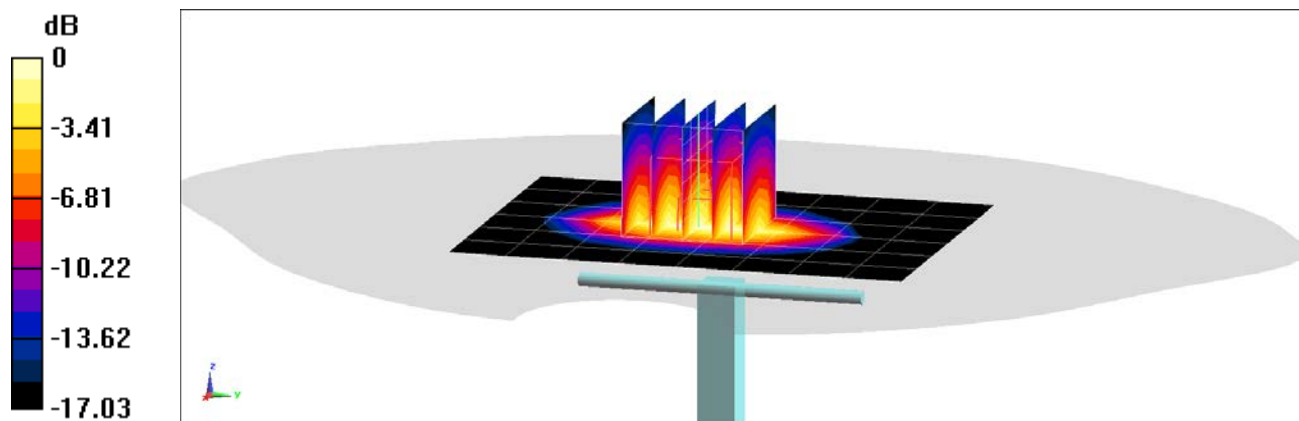

0 dB = 5.52 W/kg = 7.42 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1083

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750 \text{ MHz}$; $\sigma = 1.494 \text{ S/m}$; $\epsilon_r = 52.105$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 18.9°C; Tissue Temp: 20.5°C

Probe: EX3DV4 - SN7420; ConvF(8.01, 8.01, 8.01) @ 1750 MHz; Calibrated: 11/21/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1213; Calibrated: 11/13/2019

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CA; Serial: 1275

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.22 W/kg

SAR(1 g) = 3.94 W/kg

Deviation(1 g) = 6.20%

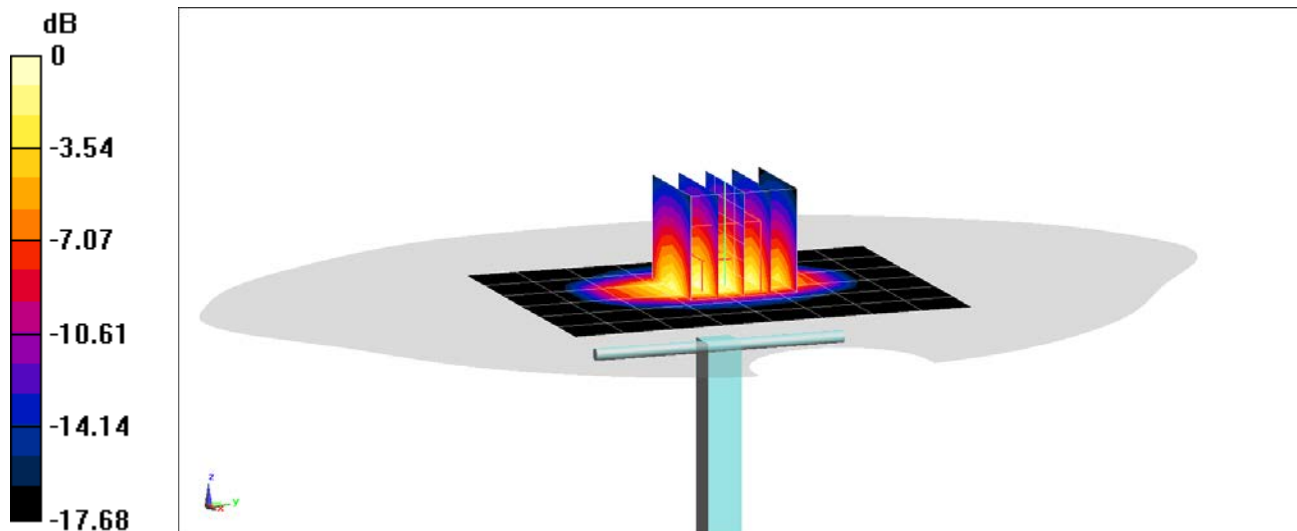

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1092

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750$ MHz; $\sigma = 1.498$ S/m; $\epsilon_r = 52.327$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 20.3°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1750 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.48 W/kg

SAR(10 g) = 1.9 W/kg

Deviation(10 g) = -2.06%

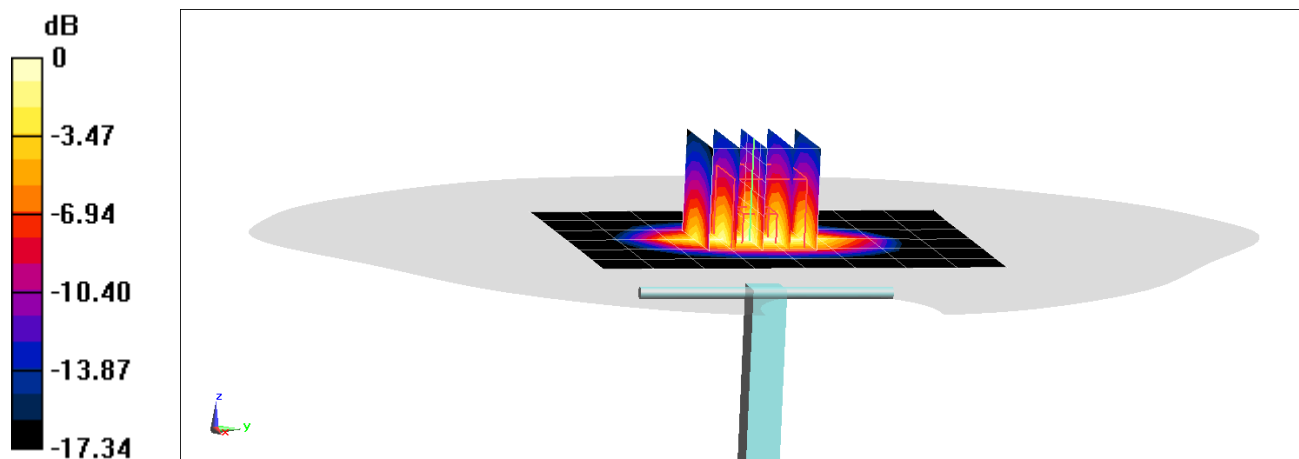

0 dB = 5.51 W/kg = 7.41 dBW/kg

PCTEST

DUT: Dipole 1750 MHz; Type: D1750V2; Serial: 1083

Communication System: UID 0, CW; Frequency: 1750 MHz; Duty Cycle: 1:1

Medium: 1750 Body Medium parameters used:

$f = 1750$ MHz; $\sigma = 1.528$ S/m; $\epsilon_r = 52.206$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/04/2020; Ambient Temp: 20.1°C; Tissue Temp: 20.7°C

Probe: EX3DV4 - SN7490; ConvF(8.54, 8.54, 8.54) @ 1750 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1750 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x9x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 6.73 W/kg

SAR(1 g) = 3.81 W/kgg

Deviation(1 g) = 2.70%

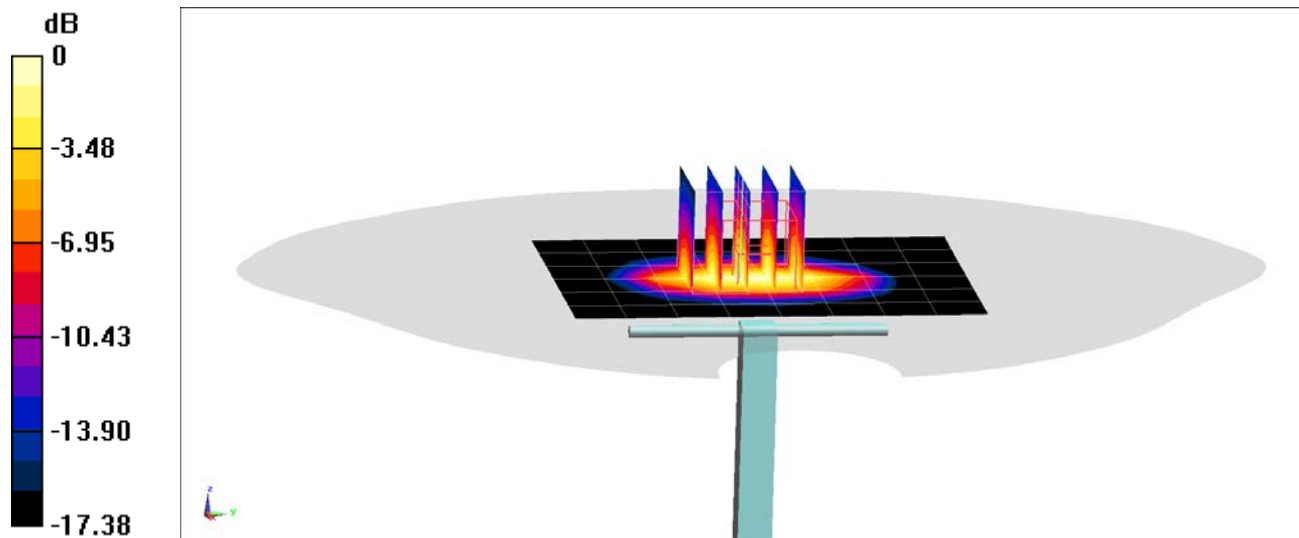

0 dB = 5.67 W/kg = 7.54 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d180

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.577$ S/m; $\epsilon_r = 51.084$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.4°C; Tissue Temp: 23.8°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1900 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.53 W/kg

SAR(1 g) = 4.21 W/kg

Deviation(1 g) = 7.95%

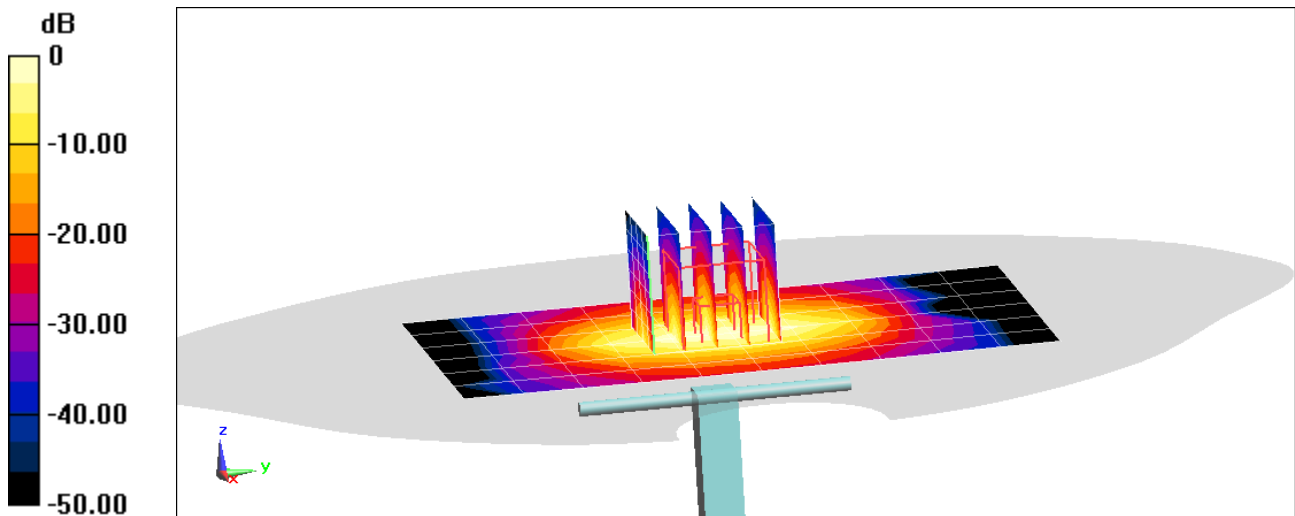

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d030

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.541$ S/m; $\epsilon_r = 51.517$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/24/2020; Ambient Temp: 21.5°C; Tissue Temp: 23.0°C

Probe: EX3DV4 - SN7421; ConvF(7.68, 7.68, 7.68) @ 1900 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.60 W/kg

SAR(1 g) = 4.25 W/kg

Deviation(1 g) = 6.52%

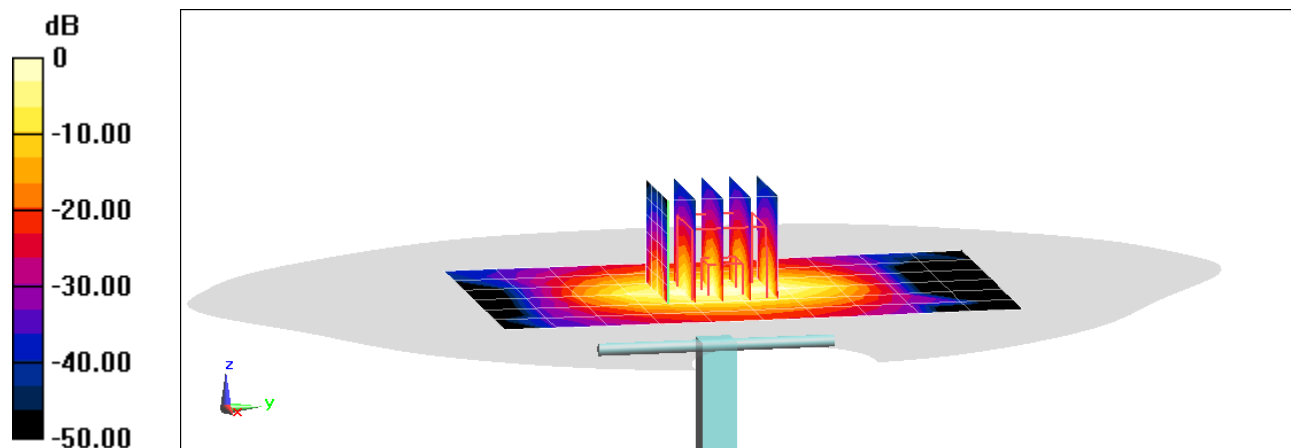

0 dB = 6.59 W/kg = 8.19 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d030

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900$ MHz; $\sigma = 1.589$ S/m; $\epsilon_r = 51.095$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/28/2020; Ambient Temp: 23.1°C; Tissue Temp: 21.7°C

Probe: EX3DV4 - SN7490; ConvF(8.22, 8.22, 8.22) @ 1900 MHz; Calibrated: 12/13/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1532; Calibrated: 12/5/2019

Phantom: Twin-SAM V4.0 (20) SUB use; Type: QD 000 P40 CC; Serial: 1403

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.22 W/kg

SAR(1 g) = 4.04 W/kg; SAR(10 g) = 2.1 W/kg

Deviation(1 g) = 1.25%; Deviation(10 g) = -0.47%

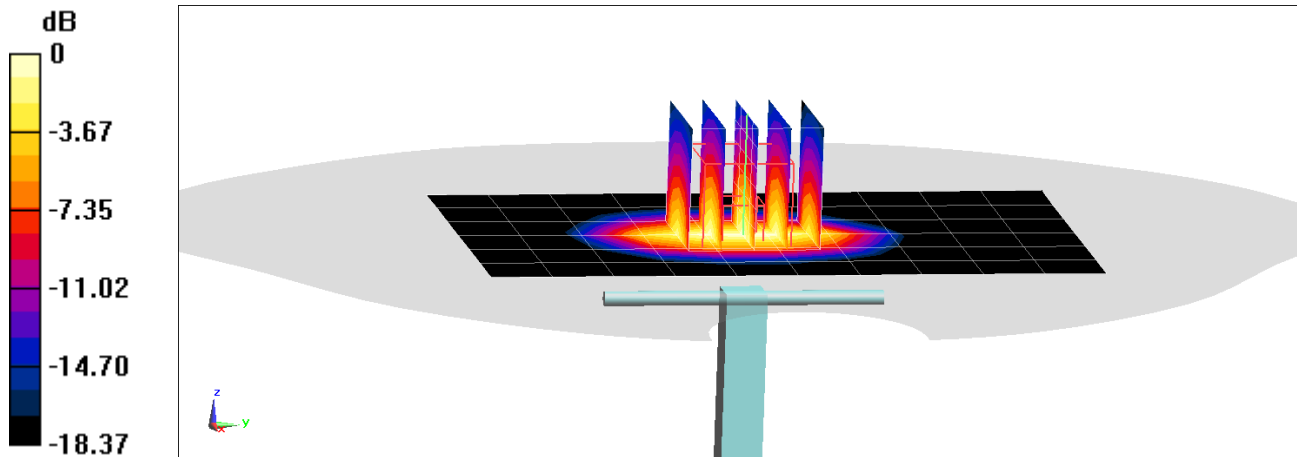

0 dB = 6.16 W/kg = 7.90 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d030

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used (interpolated):

$f = 1900 \text{ MHz}$; $\sigma = 1.58 \text{ S/m}$; $\epsilon_r = 53.304$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/01/2020; Ambient Temp: 21.1°C; Tissue Temp: 20.4°C

Probe: EX3DV4 - SN3837; ConvF(7.68, 7.68, 7.68) @ 1900 MHz; Calibrated: 1/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn793; Calibrated: 1/14/2020

Phantom: Twin-SAM V4.0 Main; Type: QD 000 P40 CC; Serial: 1114

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.72 W/kg

SAR(1 g) = 4.22 W/kg

Deviation(1 g) = 5.76%

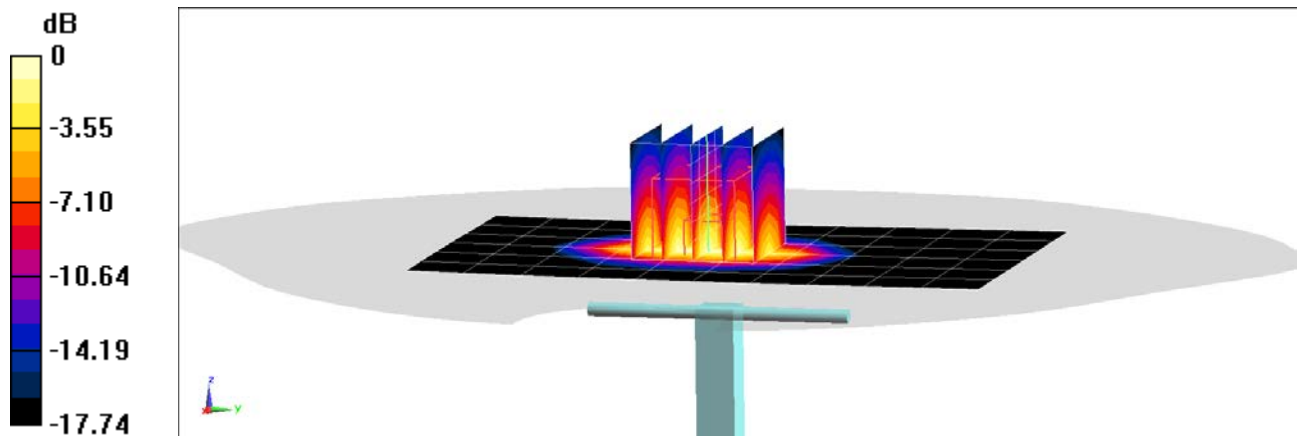

0 dB = 6.56 W/kg = 8.17 dBW/kg

PCTEST

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: 5d080

Communication System: UID 0, CW; Frequency: 1900 MHz; Duty Cycle: 1:1

Medium: 1900 Body Medium parameters used:

$f = 1900 \text{ MHz}$; $\sigma = 1.54 \text{ S/m}$; $\epsilon_r = 52.713$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 10/04/2020; Ambient Temp: 21.3°C; Tissue Temp: 22.6°C

Probe: EX3DV4 - SN7571; ConvF(7.56, 7.56, 7.56) @ 1900 MHz; Calibrated: 12/11/2019

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1533; Calibrated: 12/5/2019

Phantom: SAM Left; Type: QD000P40CC; Serial: TP: 1375

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

1900 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (7x11x1): Measurement grid: dx=15mm, dy=15mm

Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Peak SAR (extrapolated) = 7.69 W/kg

SAR(1 g) = 4.1 W/kg; SAR(10 g) = 2.11 W/kg

Deviation(1 g) = 4.59%; Deviation(10 g) = 2.43%

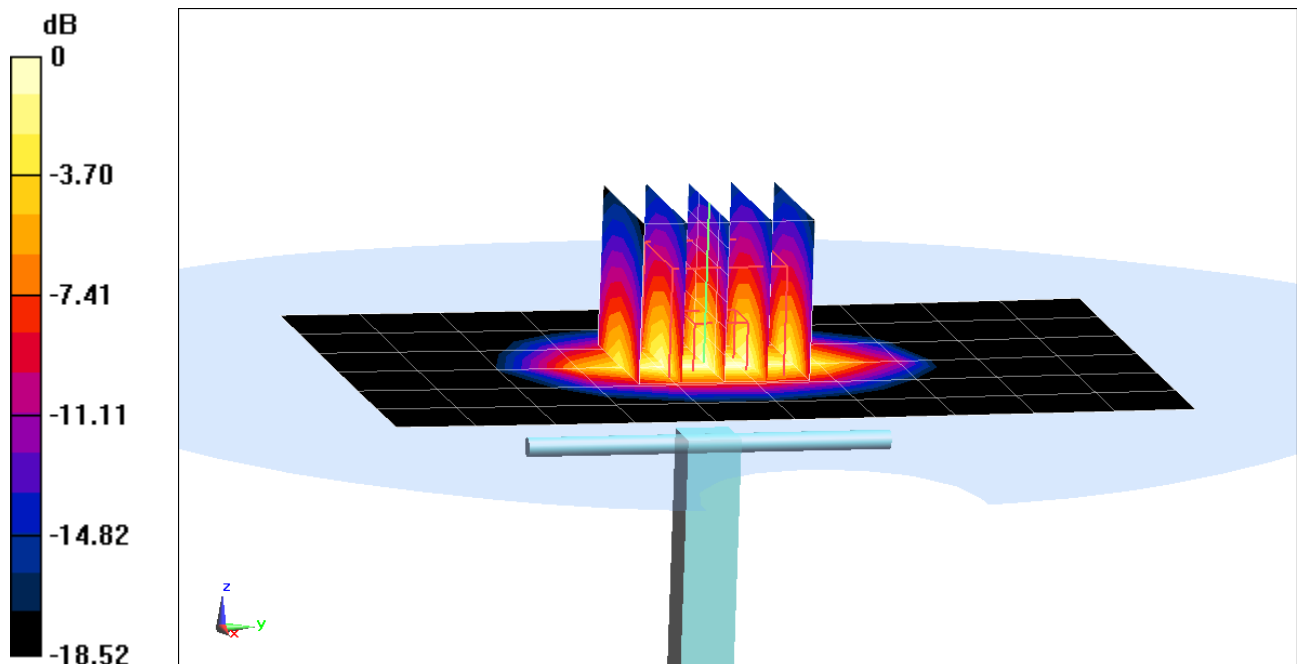

0 dB = 6.37 W/kg = 8.04 dBW/kg

PCTEST

DUT: Dipole 2300 MHz; Type: D2300V3; Serial: 1038

Communication System: UID 0, CW; Frequency: 2300 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2300$ MHz; $\sigma = 1.887$ S/m; $\epsilon_r = 51.335$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/19/2020; Ambient Temp: 22.5°C; Tissue Temp: 23.5°C

Probe: EX3DV4 - SN7421; ConvF(7.63, 7.63, 7.63) @ 2300 MHz; Calibrated: 3/20/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn604; Calibrated: 3/19/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CC; Serial: 1179

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2300 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 9.48 W/kg

SAR(1 g) = 4.88 W/kg

Deviation(1 g) = 4.50%

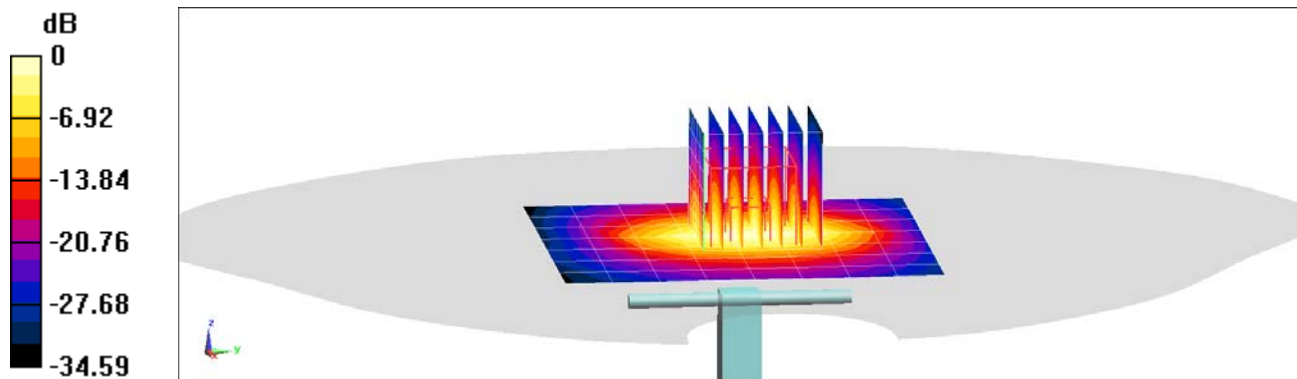

0 dB = 7.74 W/kg = 8.89 dBW/kg

PCTEST

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 882

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2450$ MHz; $\sigma = 1.989$ S/m; $\epsilon_r = 50.544$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/15/2020; Ambient Temp: 22.0°C; Tissue Temp: 22.8°C

Probe: EX3DV4 - SN7402; ConvF(7.73, 7.73, 7.73) @ 2450 MHz; Calibrated: 4/21/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1502; Calibrated: 4/15/2020

Phantom: Twin-SAM V5.0 (30); Type: QD 000 P40 CD; Serial: 1868

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2450 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 11.2 W/kg

SAR(1 g) = 5.33 W/kg

Deviation(1 g) = 3.50%

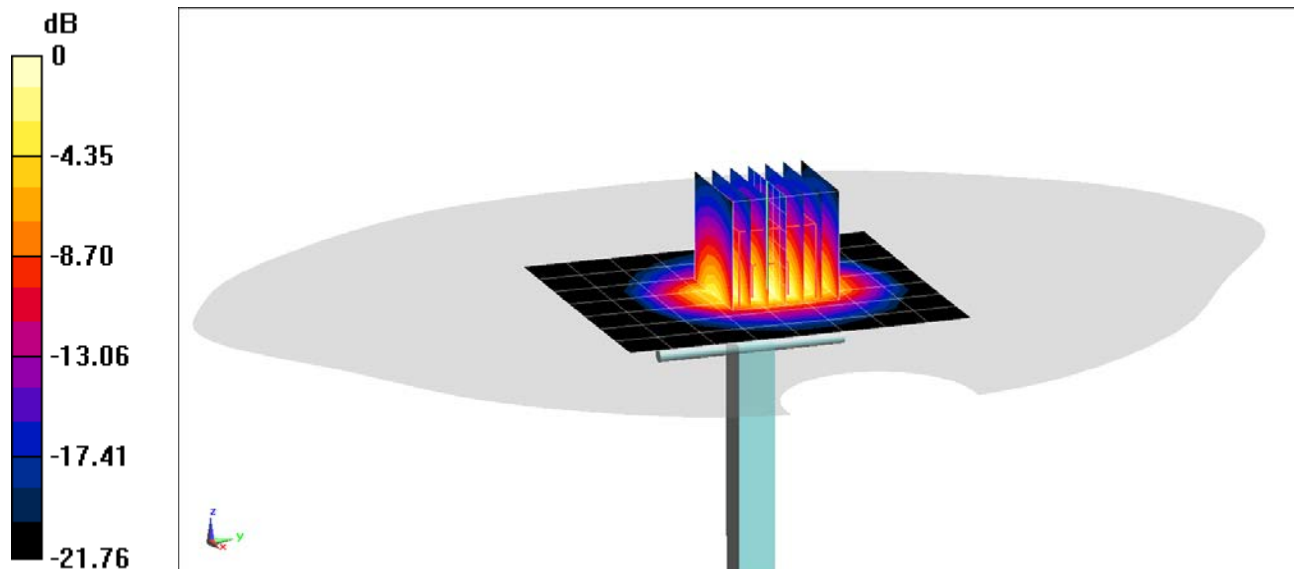

0 dB = 8.96 W/kg = 9.52 dBW/kg

PCTEST

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: 981

Communication System: UID 0, CW; Frequency: 2450 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2450$ MHz; $\sigma = 2.014$ S/m; $\epsilon_r = 51.864$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/21/2020; Ambient Temp: 23.2°C; Tissue Temp: 23.1°C

Probe: EX3DV4 - SN7409; ConvF(7.24, 7.24, 7.24) @ 2450 MHz; Calibrated: 6/23/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1334; Calibrated: 6/18/2020

Phantom: LeftTwin-SAM V5.0; Type: QD 000 P40 CD; Serial: TP1375

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2450 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 11.1 W/kg

SAR(1 g) = 5.24 W/kg

Deviation(1 g) = 2.95%

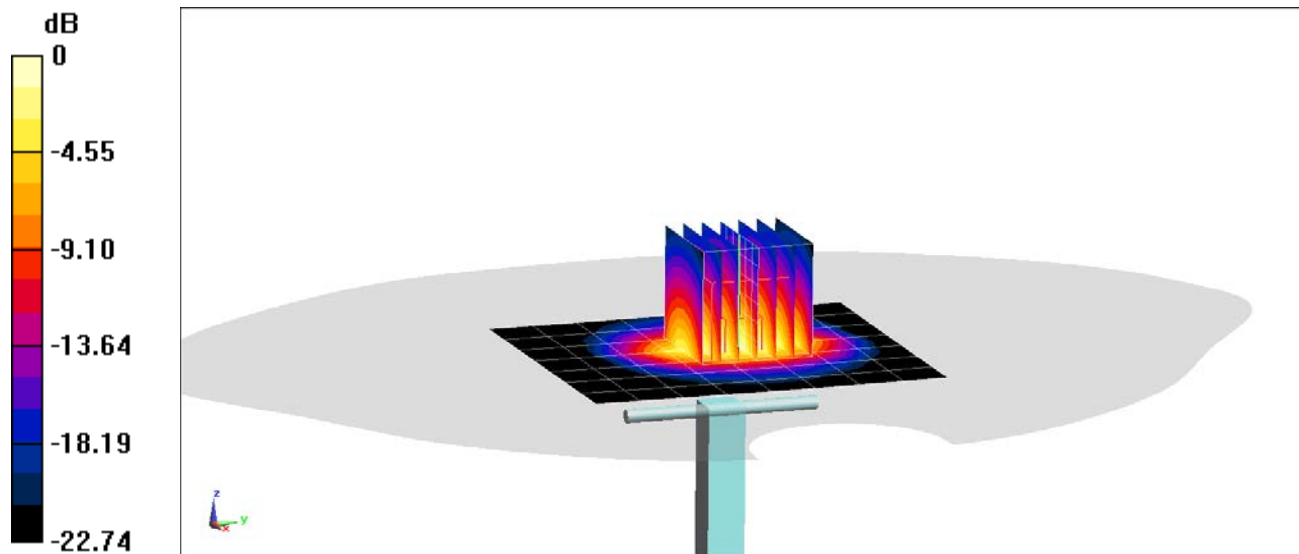

PCTEST

DUT: Dipole 2600 MHz; Type: D2600V2; Serial: 1009

Communication System: UID 0, CW; Frequency: 2600 MHz; Duty Cycle: 1:1

Medium: 2450 Body Medium parameters used:

$f = 2600$ MHz; $\sigma = 2.207$ S/m; $\epsilon_r = 50.517$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/20/2020; Ambient Temp: 21.1°C; Tissue Temp: 21.0°C

Probe: EX3DV4 - SN7427; ConvF(7.08, 7.08, 7.08) @ 2600 MHz; Calibrated: 2/19/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn1403; Calibrated: 2/13/2020

Phantom: Twin-SAM V4.0; Type: QD 000 P40 CD; Serial: 1736

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

2600 MHz System Verification at 20.0 dBm (100 mW)


Area Scan (8x9x1): Measurement grid: dx=12mm, dy=12mm

Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Peak SAR (extrapolated) = 12.9 W/kg

SAR(1 g) = 5.78 W/kg

Deviation(1 g) = 4.14%

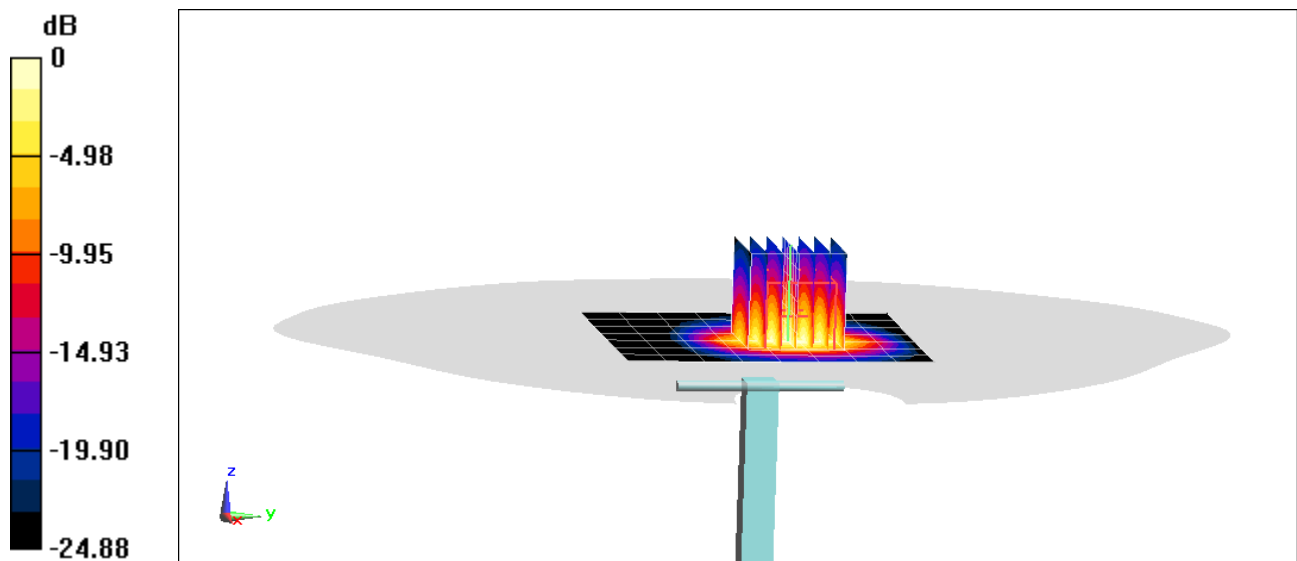

0 dB = 10.1 W/kg = 10.04 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1237

Communication System: UID 0, CW; Frequency: 5250 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Body Medium parameters used:

$f = 5250$ MHz; $\sigma = 5.418$ S/m; $\epsilon_r = 48.595$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.5°C; Tissue Temp: 24.1°C

Probe: EX3DV4 - SN7538; ConvF(4.6, 4.6, 4.6) @ 5250 MHz; Calibrated: 5/18/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn728; Calibrated: 5/20/2020

Phantom: Front; Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5250 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 14.6 W/kg

SAR(10 g) = 1.01 W/kg

Deviation(10 g) = -4.72%

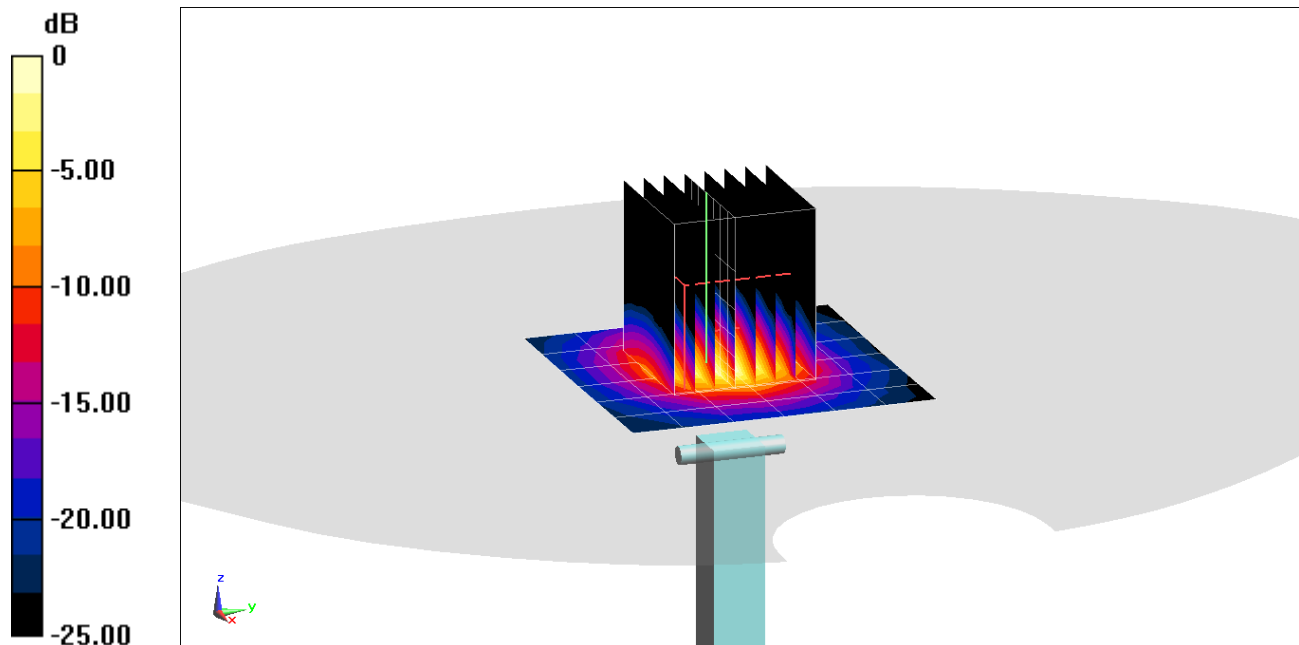

0 dB = 8.22 W/kg = 9.15 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1237

Communication System: UID 0, CW; Frequency: 5250 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Body Medium parameters used:

$f = 5250$ MHz; $\sigma = 5.462$ S/m; $\epsilon_r = 48.612$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.4°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7538; ConvF(4.6, 4.6, 4.6) @ 5250 MHz; Calibrated: 5/18/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn728; Calibrated: 5/20/2020

Phantom: Front; Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5250 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 15.2 W/kg

SAR(1 g) = 3.67 W/kg

Deviation(1 g) = -2.91%

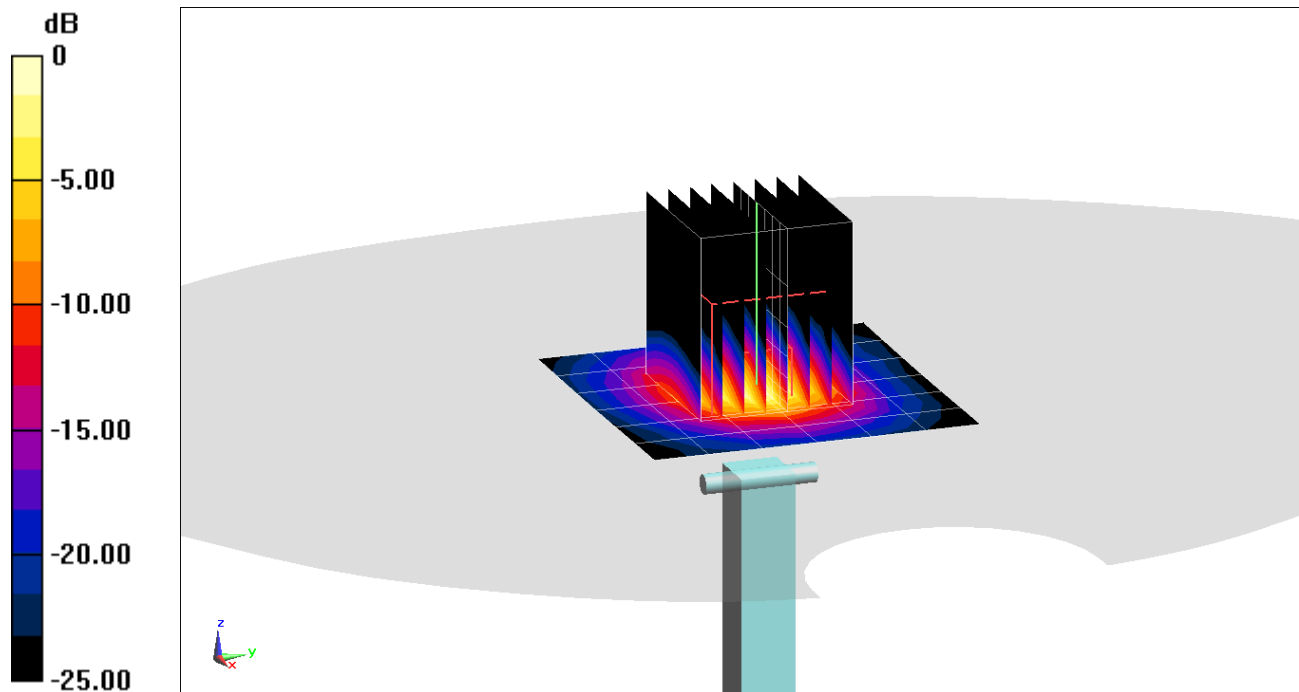

0 dB = 8.84 W/kg = 9.46 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1237

Communication System: UID 0, CW; Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Body Medium parameters used:

$f = 5600$ MHz; $\sigma = 5.889$ S/m; $\epsilon_r = 48.045$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/22/2020; Ambient Temp: 23.5°C; Tissue Temp: 24.1°C

Probe: EX3DV4 - SN7538; ConvF(4.09, 4.09, 4.09) @ 5600 MHz; Calibrated: 5/18/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn728; Calibrated: 5/20/2020

Phantom: Front; Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5600 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.2 W/kg

SAR(10 g) = 1.09 W/kg

Deviation(10 g) = -0.91%

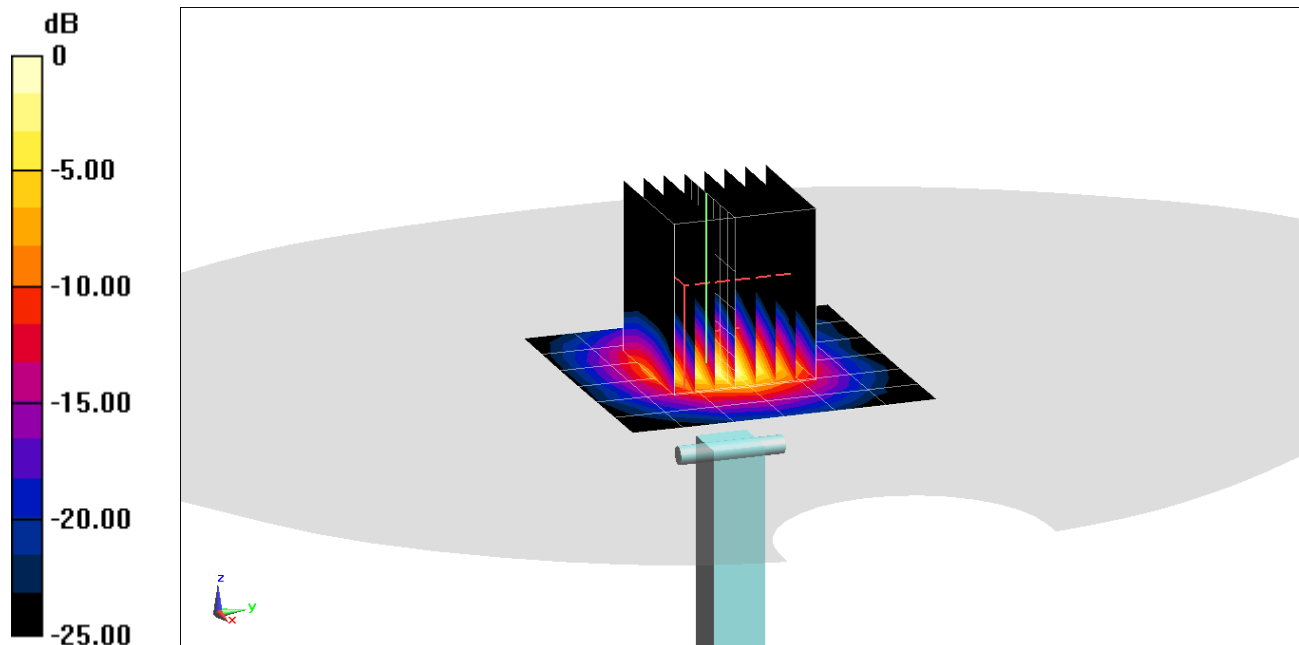

0 dB = 9.27 W/kg = 9.67 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1237

Communication System: UID 0, CW; Frequency: 5600 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Body Medium parameters used:

$f = 5600$ MHz; $\sigma = 5.92$ S/m; $\epsilon_r = 48.039$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.4°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7538; ConvF(4.09, 4.09, 4.09) @ 5600 MHz; Calibrated: 5/18/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn728; Calibrated: 5/20/2020

Phantom: Front; Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5600 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 4 W/kg

Deviation(1 g) = 1.91%

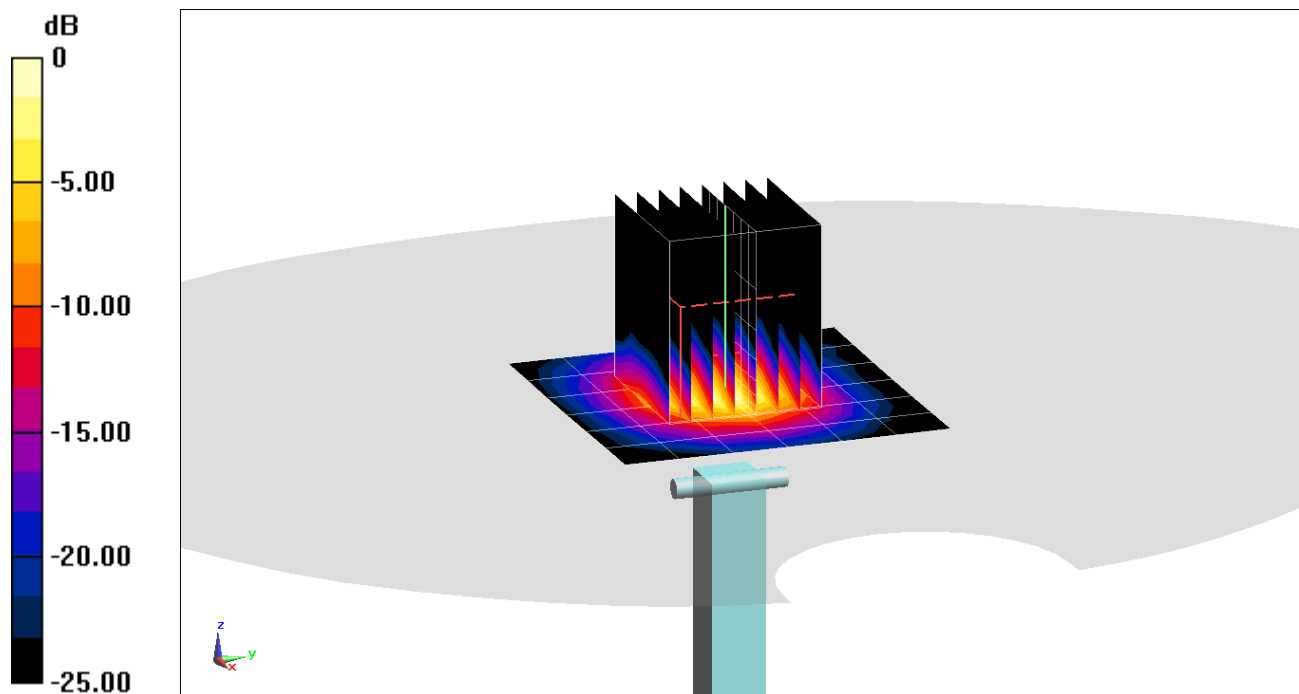

0 dB = 9.62 W/kg = 9.83 dBW/kg

PCTEST

DUT: Dipole 5 GHz; Type: D5GHzV2; Serial: 1237

Communication System: UID 0, CW; Frequency: 5750 MHz; Duty Cycle: 1:1

Medium: 5200-5800 Body Medium parameters used:

$f = 5750$ MHz; $\sigma = 6.125$ S/m; $\epsilon_r = 47.813$; $\rho = 1000$ kg/m³

Phantom section: Flat Section; Space: 1.0 cm

Test Date: 09/30/2020; Ambient Temp: 22.4°C; Tissue Temp: 22.5°C

Probe: EX3DV4 - SN7538; ConvF(4.17, 4.17, 4.17) @ 5750 MHz; Calibrated: 5/18/2020

Sensor-Surface: 1.4mm (Mechanical Surface Detection)

Electronics: DAE4 Sn728; Calibrated: 5/20/2020

Phantom: Front; Type: QD 000 P40 CD; Serial: 1686

Measurement SW: DASY52, Version 52.10 (4);SEMCAD X Version 14.6.14 (7483)

5750 MHz System Verification at 17.0 dBm (50 mW)


Area Scan (7x7x1): Measurement grid: dx=10mm, dy=10mm

Zoom Scan (8x8x8)/Cube 0: Measurement grid: dx=4mm, dy=4mm, dz=1.4mm; Graded Ratio: 1.4

Peak SAR (extrapolated) = 17.8 W/kg

SAR(1 g) = 3.71 W/kg

Deviation(1 g) = -2.24%

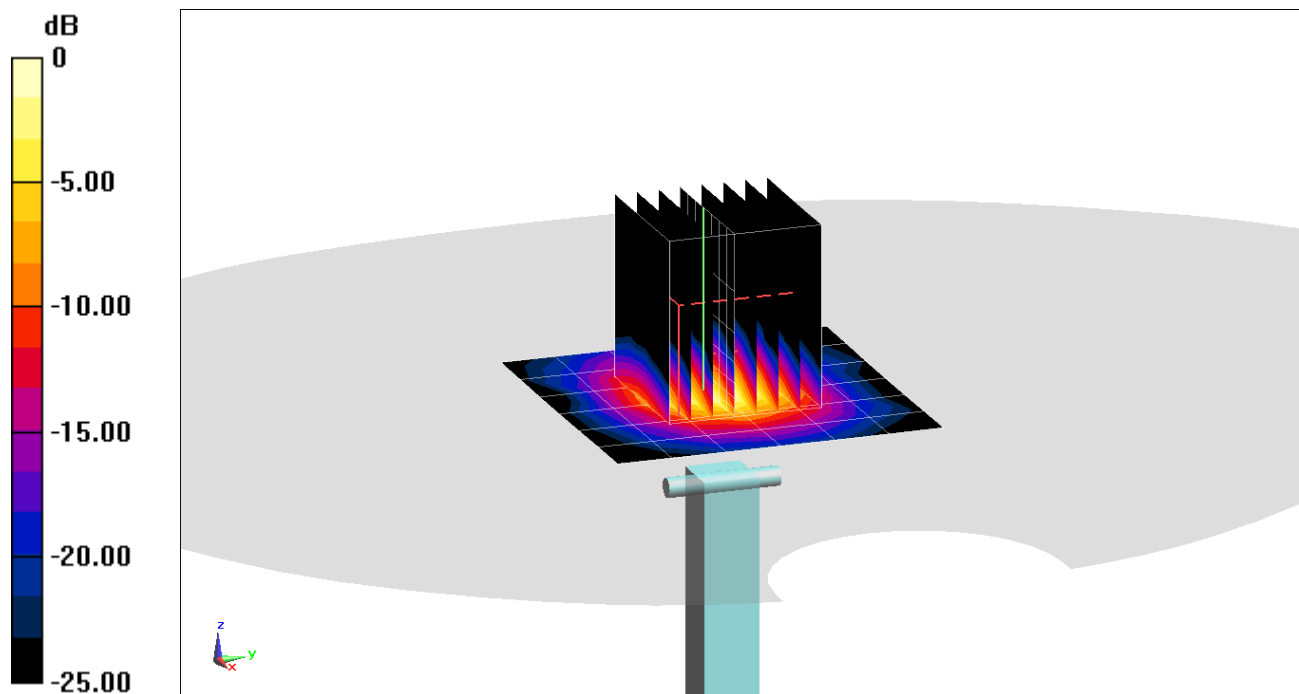

0 dB = 9.30 W/kg = 9.68 dBW/kg

APPENDIX C: SAR TISSUE SPECIFICATIONS

Measurement Procedure for Tissue verification:

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity ϵ' can be calculated from the below equation (Pournaropoulos and Misra):



$$Y = \frac{j2\omega\epsilon_r\epsilon_0}{[\ln(b/a)]^2} \int_a^b \int_a^b \int_0^\pi \cos\phi' \frac{\exp[-j\omega r(\mu_0\epsilon_r'\epsilon_0)^{1/2}]}{r} d\phi' d\rho' d\rho$$

where Y is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho' \cos\phi'$, ω is the angular frequency, and $j = \sqrt{-1}$.

3 Composition / Information on ingredients		
3.2 Mixtures		
Description: Aqueous solution with surfactants and inhibitors		
Declarable, or hazardous components:		
CAS: 107-21-1 EINECS: 203-473-3 Reg.nr.: 01-2119456816-28-0000	Ethenediol STOT RE 2, H373; Acute Tox. 4, H302	>1.0-4.9%
CAS: 68608-26-4 EINECS: 271-781-5 Reg.nr.: 01-2119527859-22-0000	Sodium petroleum sulfonate Eye Irrit. 2, H319	< 2.9%
CAS: 107-41-5 EINECS: 203-489-0 Reg.nr.: 01-2119539582-35-0000	Hexylene Glycol / 2-Methyl-pentane-2,4-diol Skin Irrit. 2, H315; Eye Irrit. 2, H319	< 2.9%
CAS: 68920-66-1 NLP: 500-236-9 Reg.nr.: 01-2119489407-26-0000	Alkoxylated alcohol, > C₁₆ Aquatic Chronic 2, H411; Skin Irrit. 2, H315; Eye Irrit. 2, H319	< 2.0%
Additional information:		
For the wording of the listed risk phrases refer to section 16. Not mentioned CAS-, EINECS- or registration numbers are to be regarded as Proprietary/Confidential. The specific chemical identity and/or exact percentage concentration of proprietary components is withheld as a trade secret.		

Figure C-1

Note: Liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

FCC ID: ZNFK920AM		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 09/15/20 - 10/04/20	DUT Type: Portable Handset			APPENDIX C: Page 1 of 3

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MBBL600-6000V6)
Product No.	SL AAM U16 BC (Batch: 181029-1)
Manufacturer	SPEAG



Measurement Method
TSL dielectric parameters measured using calibrated DAK probe.

Target Parameters
Target parameters as defined in the KDB 865864 compliance standard.

Test Condition
Ambient Condition 22°C ; 30% humidity
TSL Temperature 22°C
Test Date 30-Oct-18
Operator CL

Additional Information
TSL Density
TSL Heat-capacity

f [MHz]	Measured			Target		Diff.to Target [%]	
	e'	e''	sigma	eps	sigma	Δ-eps	Δ-sigma
800	55.1	21.3	0.95	55.3	0.97	-0.4	-2.1
825	55.1	20.8	0.98	55.2	0.98	-0.3	-2.0
835	55.1	20.6	0.96	55.1	0.99	0.0	-2.5
850	55.1	20.4	0.96	55.2	0.99	-0.1	-3.0
900	55.0	19.7	0.98	55.0	1.05	0.0	-6.7
1400	54.2	15.6	1.22	54.1	1.28	0.2	-4.7
1450	54.1	15.4	1.24	54.0	1.30	0.2	-4.6
1500	54.1	15.3	1.27	53.9	1.33	0.3	-4.5
1550	54.0	15.1	1.30	53.9	1.36	0.2	-4.4
1600	53.9	15.0	1.33	53.8	1.39	0.2	-4.3
1625	53.9	14.9	1.35	53.8	1.41	0.3	-4.3
1640	53.9	14.9	1.36	53.7	1.42	0.3	-4.2
1650	53.8	14.9	1.36	53.7	1.43	0.2	-4.9
1700	53.8	14.8	1.40	53.6	1.46	0.4	-4.1
1750	53.7	14.7	1.43	53.4	1.49	0.5	-4.0
1800	53.7	14.6	1.46	53.3	1.52	0.8	-3.9
1810	53.7	14.6	1.47	53.3	1.52	0.8	-3.3
1825	53.7	14.6	1.48	53.3	1.52	0.8	-2.6
1850	53.6	14.5	1.50	53.3	1.52	0.6	-1.3
1900	53.5	14.5	1.53	53.3	1.52	0.4	0.7
1950	53.5	14.5	1.67	53.3	1.52	0.4	3.3
2000	53.4	14.4	1.60	53.3	1.52	0.2	5.3
2050	53.4	14.4	1.64	53.2	1.57	0.3	4.5
2100	53.3	14.4	1.68	53.2	1.62	0.2	3.7
2150	53.3	14.4	1.72	53.1	1.68	0.4	3.6
2200	53.2	14.4	1.76	53.0	1.71	0.3	2.9
2250	53.1	14.4	1.81	53.0	1.76	0.2	2.8
2300	53.1	14.4	1.85	52.9	1.81	0.4	2.2
2350	53.0	14.5	1.89	52.8	1.85	0.3	2.2
2400	52.9	14.5	1.94	52.8	1.90	0.2	2.1
2450	52.9	14.5	1.98	52.7	1.95	0.4	1.5
2500	52.8	14.6	2.03	52.6	2.02	0.3	0.5
2550	52.7	14.6	2.07	52.6	2.09	0.2	-1.0
2600	52.6	14.7	2.12	52.5	2.16	0.2	-1.9

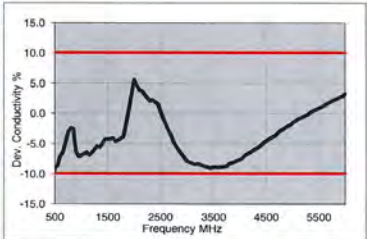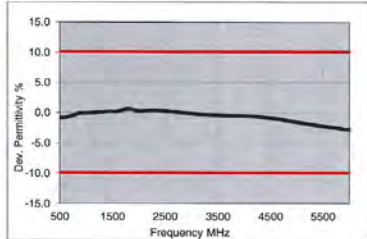

3500	51.1	15.5	3.02	51.3	3.31	-0.4	-8.8
3700	50.8	15.7	3.24	51.1	3.55	-0.5	-8.8
5200	48.1	18.2	5.27	49.0	5.30	-1.8	-0.6
5250	48.0	18.3	5.34	49.0	5.36	-1.9	-0.4
5300	47.9	18.4	5.41	48.9	5.42	-2.0	-0.2
5500	47.5	16.6	5.70	48.6	5.65	-2.2	0.8
5600	47.3	18.8	5.84	48.5	5.77	-2.3	1.3
5700	47.1	18.9	5.99	48.3	5.88	-2.5	1.8
5800	47.0	19.0	6.14	48.2	6.00	-2.6	2.3

TSL Dielectric Parameters

1

Figure C-2
600 – 5800 MHz Body Tissue Equivalent Matter

FCC ID: ZNFK920AM		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 09/15/20 - 10/04/20	DUT Type: Portable Handset			APPENDIX C: Page 2 of 3

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HBBL600-10000V6)
Product No.	SL AAH U16 BC (Batch: 181031-2)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated DAK probe.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition



Ambient Condition 22°C ; 30% humidity
 TSL Temperature 22°C
 Test Date 31-Oct-18
 Operator CL

Additional Information

TSL Density
 TSL Heat-capacity

Results

f [MHz]	Measured			Target		Diff.to Target [%]	
	e'	e''	sigma	eps	sigma	Δ-eps	Δ-sigma
800	43.8	20.5	0.91	41.7	0.90	5.1	1.4
825	43.8	20.1	0.92	41.6	0.91	5.3	1.5
850	43.8	19.9	0.93	41.5	0.91	5.4	2.0
880	43.7	19.7	0.93	41.5	0.92	5.3	1.5
900	43.5	16.9	0.95	41.5	0.97	4.8	-2.1
1400	42.5	15.0	1.17	40.6	1.18	4.7	-0.8
1450	42.5	14.8	1.19	40.5	1.20	4.9	-0.8
1600	42.2	14.3	1.27	40.3	1.28	4.7	-1.1
1625	42.2	14.2	1.29	40.3	1.30	4.8	-0.7
1640	42.2	14.2	1.30	40.3	1.31	4.8	-0.5
1650	42.1	14.2	1.30	40.2	1.31	4.6	-1.0
1700	42.1	14.0	1.33	40.2	1.34	4.8	-0.9
1750	42.0	13.9	1.36	40.1	1.37	4.8	-0.8
1800	41.9	13.9	1.39	40.0	1.40	4.7	-0.7
1810	41.9	13.8	1.40	40.0	1.40	4.7	0.0
1825	41.9	13.8	1.41	40.0	1.40	4.7	0.7
1850	41.8	13.8	1.42	40.0	1.40	4.5	1.4
1900	41.8	13.7	1.45	40.0	1.40	4.5	3.6
1950	41.7	13.7	1.48	40.0	1.40	4.3	5.7
2000	41.6	13.6	1.51	40.0	1.40	4.0	7.9
2050	41.6	13.6	1.55	39.9	1.44	4.2	7.3
2100	41.5	13.5	1.58	39.8	1.49	4.2	6.1
2150	41.4	13.5	1.62	39.7	1.53	4.2	5.7
2200	41.4	13.5	1.65	39.6	1.58	4.4	4.6
2250	41.3	13.5	1.69	39.6	1.62	4.4	4.2
2300	41.2	13.5	1.72	39.5	1.67	4.4	3.2
2350	41.1	13.5	1.76	39.4	1.71	4.4	2.9
2400	41.1	13.5	1.80	39.3	1.76	4.6	2.5
2450	41.0	13.5	1.84	39.2	1.80	4.6	2.2
2500	40.9	13.5	1.88	39.1	1.85	4.5	1.4
2550	40.8	13.5	1.92	39.1	1.91	4.4	0.6
2600	40.8	13.6	1.96	39.0	1.96	4.0	-0.2
3500	39.2	14.1	2.74	37.9	2.91	3.3	-5.8
3700	38.9	14.2	2.93	37.7	3.12	3.1	-6.1

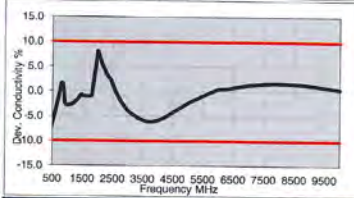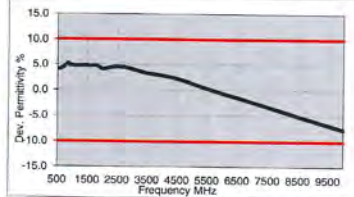

5200	36.3	15.8	4.57	38.0	4.66	0.9	-1.7
5250	36.2	15.9	4.63	35.9	4.71	0.8	-1.6
5300	36.1	15.9	4.69	35.9	4.76	0.7	-1.4
5500	35.8	16.1	4.92	35.6	4.96	0.3	-0.9
5600	35.6	16.2	5.04	35.5	5.07	0.1	-0.6
5700	35.4	16.2	5.15	35.4	5.17	0.0	-0.3
5800	35.2	16.3	5.27	35.3	5.27	-0.2	0.0
6000	34.9	16.5	5.50	35.1	5.48	-0.6	0.5
6500	34.0	16.9	6.12	34.5	6.07	-1.4	0.9
7000	33.1	17.3	6.74	33.9	6.65	-2.3	1.3
7500	32.2	17.6	7.36	33.3	7.24	-3.2	1.6
8000	31.4	17.9	7.97	32.7	7.84	-4.1	1.7
8500	30.5	18.2	8.59	32.1	8.45	-5.0	1.6
9000	29.7	18.4	9.20	31.5	9.08	-5.9	1.3
9500	28.9	18.5	9.80	31.0	9.71	-6.8	0.9
10000	28.1	18.7	10.40	30.4	10.36	-7.6	0.4

TSL Dielectric Parameters

Figure C-3
600 – 5800 MHz Head Tissue Equivalent Matter

FCC ID: ZNFK920AM		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 09/15/20 - 10/04/20	DUT Type: Portable Handset			APPENDIX C: Page 3 of 3



APPENDIX D: SAR SYSTEM VALIDATION

Per FCC KDB Publication 865664 D02v01r02, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in FCC KDB Publication 865664 D01v01r04 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

Table D-1
SAR System Validation Summary – 1g



SAR System	Freq. (MHz)	Date	Probe SN	Probe Cal Point		Cond. (σ)	Perm. (εr)	CW VALIDATION			MOD. VALIDATION		
								SENSITIVITY	PROBE LINEARITY	PROBE ISOTROPY	MOD. TYPE	DUTY FACTOR	PAR
AM7	750	5/20/2020	7490	750	Head	0.881	41.800	PASS	PASS	PASS	N/A	N/A	N/A
AM8	750	6/25/2020	7532	750	Head	0.901	42.435	PASS	PASS	PASS	N/A	N/A	N/A
AM1	835	3/12/2020	7427	835	Head	0.887	41.650	PASS	PASS	PASS	GMSK	PASS	N/A
L	835	7/6/2020	7406	835	Head	0.903	42.760	PASS	PASS	PASS	GMSK	PASS	N/A
AM4	835	5/12/2020	7421	835	Head	0.866	39.960	PASS	PASS	PASS	GMSK	PASS	N/A
AM8	1750	6/25/2020	7532	1750	Head	1.324	40.239	PASS	PASS	PASS	N/A	N/A	N/A
AM1	1750	3/12/2020	7427	1750	Head	1.324	39.689	PASS	PASS	PASS	N/A	N/A	N/A
AM8	1900	9/23/2020	7532	1900	Head	1.427	38.835	PASS	PASS	PASS	GMSK	PASS	N/A
AM1	1900	3/12/2020	7427	1900	Head	1.424	39.945	PASS	PASS	PASS	GMSK	PASS	N/A
L	1900	7/7/2020	7406	1900	Head	1.403	40.885	PASS	PASS	PASS	GMSK	PASS	N/A
AM4	2300	5/14/2020	7421	2300	Head	1.683	39.500	PASS	PASS	PASS	N/A	N/A	N/A
E	2450	2/5/2020	3589	2450	Head	1.823	38.835	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
AM4	2600	5/13/2020	7421	2600	Head	1.887	37.346	PASS	PASS	PASS	TDD	PASS	N/A
K2	5250	6/11/2020	7402	5250	Head	4.534	35.720	PASS	PASS	PASS	OFDM	N/A	PASS
K2	5600	6/11/2020	7402	5600	Head	4.872	35.230	PASS	PASS	PASS	OFDM	N/A	PASS
K2	5750	6/11/2020	7402	5750	Head	5.030	35.060	PASS	PASS	PASS	OFDM	N/A	PASS
AM3	750	9/16/2020	7491	750	Body	0.948	54.825	PASS	PASS	PASS	N/A	N/A	N/A
AM6	750	3/10/2020	3837	750	Body	0.955	53.889	PASS	PASS	PASS	N/A	N/A	N/A
AM7	750	5/18/2020	7490	750	Body	0.965	53.605	PASS	PASS	PASS	N/A	N/A	N/A
AM7	835	5/18/2020	7490	835	Body	0.998	53.350	PASS	PASS	PASS	GMSK	PASS	N/A
P	835	9/8/2020	7308	835	Body	0.977	54.530	PASS	PASS	PASS	GMSK	PASS	N/A
AM6	835	3/10/2020	3837	835	Body	0.992	54.144	PASS	PASS	PASS	GMSK	PASS	N/A
AM5	1750	7/6/2020	7416	1750	Body	1.437	51.230	PASS	PASS	PASS	N/A	N/A	N/A
AM7	1750	5/13/2020	7490	1750	Body	1.449	51.065	PASS	PASS	PASS	N/A	N/A	N/A
AM2	1750	12/5/2019	7420	1750	Body	1.526	51.265	PASS	PASS	PASS	N/A	N/A	N/A
AM4	1900	4/22/2020	7421	1900	Body	1.577	52.969	PASS	PASS	PASS	GMSK	PASS	N/A
AM7	1900	5/13/2020	7490	1900	Body	1.582	50.652	PASS	PASS	PASS	GMSK	PASS	N/A
AM6	1900	3/4/2020	3837	1900	Body	1.583	51.670	PASS	PASS	PASS	GMSK	PASS	N/A
J	1900	1/1/2020	7571	1900	Body	1.579	51.919	PASS	PASS	PASS	GMSK	PASS	N/A
AM4	2300	5/27/2020	7421	2300	Body	1.892	52.110	PASS	PASS	PASS	N/A	N/A	N/A
K	2450	7/7/2020	7409	2450	Body	2.018	51.180	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
K2	2450	7/21/2020	7402	2450	Body	1.996	51.910	PASS	PASS	PASS	OFDM/TDD	PASS	PASS
AM1	2600	4/13/2020	7427	2600	Body	2.156	51.414	PASS	PASS	PASS	TDD	PASS	N/A
G	5250	8/16/2020	7538	5250	Body	5.476	47.185	PASS	PASS	PASS	OFDM	N/A	PASS
G	5600	8/16/2020	7538	5600	Body	5.937	46.607	PASS	PASS	PASS	OFDM	N/A	PASS
G	5750	8/16/2020	7538	5750	Body	6.140	46.354	PASS	PASS	PASS	OFDM	N/A	PASS

FCC ID ZNFK920AM	 <small>Proud to be part of</small>	SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 09/15/20 - 10/04/20	DUT Type: Portable Handset			APPENDIX D: Page 1 of 2

**Table D-2
SAR System Validation Summary – 10g**

SAR System	Freq. (MHz)	Date	Probe SN	Probe Cal Point		Cond. (σ)	Perm. (ϵ_r)	CW VALIDATION			MOD. VALIDATION		
								SENSITIVITY	PROBE LINEARITY	PROBE ISOTROPY	MOD. TYPE	DUTY FACTOR	PAR
AM7	1750	5/13/2020	7490	1750	Body	1.449	51.065	PASS	PASS	PASS	N/A	N/A	N/A
AM7	1900	5/13/2020	7490	1900	Body	1.582	50.652	PASS	PASS	PASS	GMSK	PASS	N/A
J	1900	1/1/2020	7571	1900	Body	1.579	51.919	PASS	PASS	PASS	GMSK	PASS	N/A
G	5250	8/16/2020	7538	5250	Body	5.476	47.185	PASS	PASS	PASS	OFDM	N/A	PASS
G	5600	8/16/2020	7538	5600	Body	5.937	46.607	PASS	PASS	PASS	OFDM	N/A	PASS

NOTE: While the probes have been calibrated for both CW and modulated signals, all measurements were performed using communication systems calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r04 for scenarios when CW probe calibrations are used with other signal types. SAR systems were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to FCC KDB Publication 865664 D01v01r04.

FCC ID ZNFK920AM		SAR EVALUATION REPORT		Approved by: Quality Manager
Test Dates: 09/15/20 - 10/04/20	DUT Type: Portable Handset			APPENDIX D: Page 2 of 2

APPENDIX F: PROBE AND DIPOLE CALIBRATION CERTIFICATES



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No. **D750V3-1034 May18**

CALIBRATION CERTIFICATE

Object **D750V3 - SN:1034**

Calibration procedure(s) **QA/CAL-05.v10
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 18, 2018**

*SC ✓
5/31/2018
BN ✓
05/01/2019
ATM ✓
6/11/2020*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	04-Apr-18 (No. 217-02672/02673)	Apr-19
Power sensor NRP-Z91	SN: 103244	04-Apr-18 (No. 217-02672)	Apr-19
Power sensor NRP-Z91	SN: 103245	04-Apr-18 (No. 217-02673)	Apr-19
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-18 (No. 217-02682)	Apr-19
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-18 (No. 217-02683)	Apr-19
Reference Probe EX3DV4	SN: 7349	30-Dec-17 (No. EX3-7349_Dec17)	Dec-18
DAE4	SN: 601	26-Oct-17 (No. DAE4-601_Oct17)	Oct-18
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter EPM-442A	SN: GB37480704	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: US37292783	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
Power sensor HP 8481A	SN: MY41092317	07-Oct-16 (in house check Oct-16)	In house check: Oct-18
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-16)	In house check: Oct-18
Network Analyzer HP 8753E	SN: US37390585	18-Oct-01 (in house check Oct-17)	In house check: Oct-18

Calibrated by: **Manu Seitz** (Name), **Laboratory Technician** (Function), *[Signature]* (Signature)

Approved by: **Kajla Pokovic** (Name), **Technical Manager** (Function), *[Signature]* (Signature)

Issued: May 22, 2018

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 0108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.1
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	750 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.9	0.89 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.0 ± 6 %	0.89 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.09 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	8.32 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.36 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.42 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.5	0.96 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	54.7 ± 6 %	0.96 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.15 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	8.57 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.42 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	5.67 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	55.3 Ω + 0.0 j Ω
Return Loss	- 26.0 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	50.0 Ω - 3.2 j Ω
Return Loss	- 29.8 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.034 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	July 06, 2011

DASY5 Validation Report for Head TSL

Date: 17.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1034

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750$ MHz; $\sigma = 0.89$ S/m; $\epsilon_r = 41$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.22, 10.22, 10.22) @ 750 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 59.66 V/m; Power Drift = -0.03 dB

Peak SAR (extrapolated) = 3.18 W/kg

SAR(1 g) = 2.09 W/kg; SAR(10 g) = 1.36 W/kg

Maximum value of SAR (measured) = 2.82 W/kg

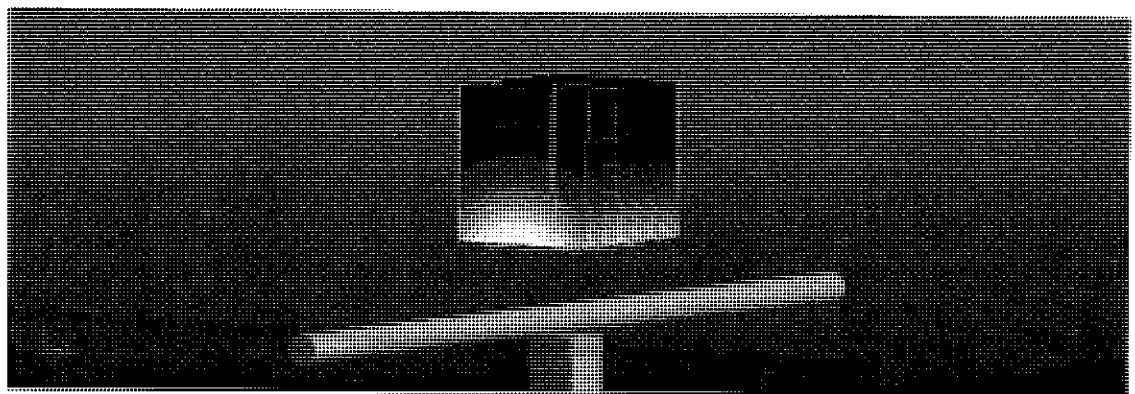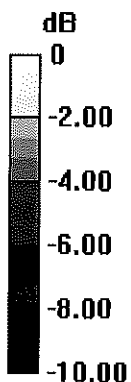

0 dB = 2.82 W/kg = 4.50 dBW/kg


Impedance Measurement Plot for Head TSL

17 May 2018 09:39:14

CH1 S11 1 U FS


1: 55.279 Ω 0.0430 Ω 9.1180 pF 750.000 000 MHz

*
De1
CA
Avg
16
H1d

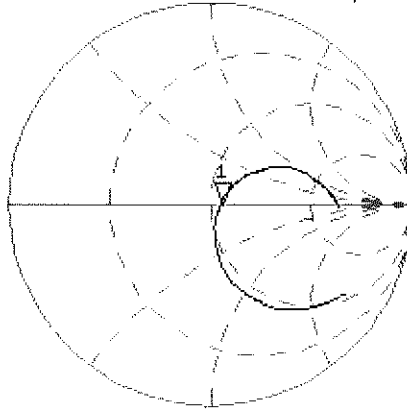

CH2 S11 LOG 5 dB/REF -20 dB 1:-25.993 dB 750.000 000 MHz

CA
Avg
16
H1d

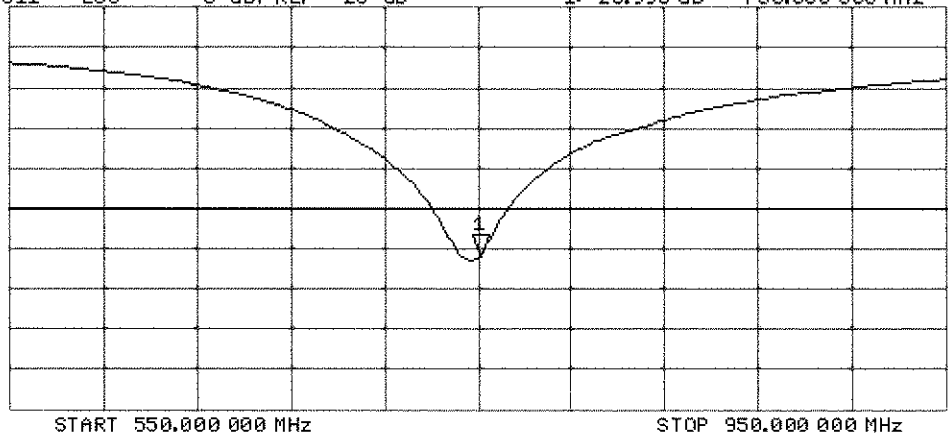

DASY5 Validation Report for Body TSL

Date: 18.05.2018

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 750 MHz; Type: D750V3; Serial: D750V3 - SN:1034

Communication System: UID 0 - CW; Frequency: 750 MHz

Medium parameters used: $f = 750$ MHz; $\sigma = 0.96$ S/m; $\epsilon_r = 54.7$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.19, 10.19, 10.19) @ 750 MHz; Calibrated: 30.12.2017
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 26.10.2017
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.1(1476); SEMCAD X 14.6.11(7439)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.60 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 3.16 W/kg

SAR(1 g) = 2.15 W/kg; SAR(10 g) = 1.42 W/kg

Maximum value of SAR (measured) = 2.83 W/kg

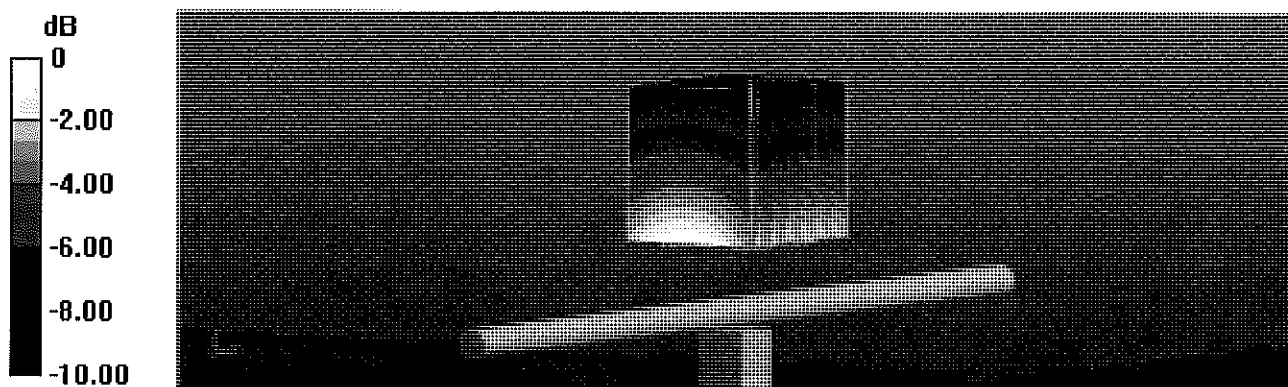


0 dB = 2.83 W/kg = 4.52 dBW/kg

Impedance Measurement Plot for Body TSL


18 May 2018 09:54:01
 CH1 S11 1 U FS 1: 49.951 $\hat{\omega}$ -3.2324 $\hat{\omega}$ 65.649 pF 750.000 000 MHz

*
 De1
 Cor
 Avg
 16
 H1d

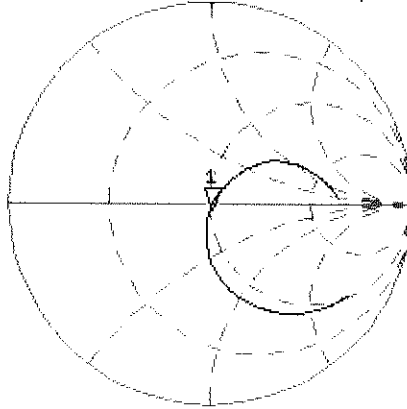

CH2 S11 LOG 5 dB/REF -20 dB 1: -29.809 dB 750.000 000 MHz

Cor
 Avg
 16
 H1d

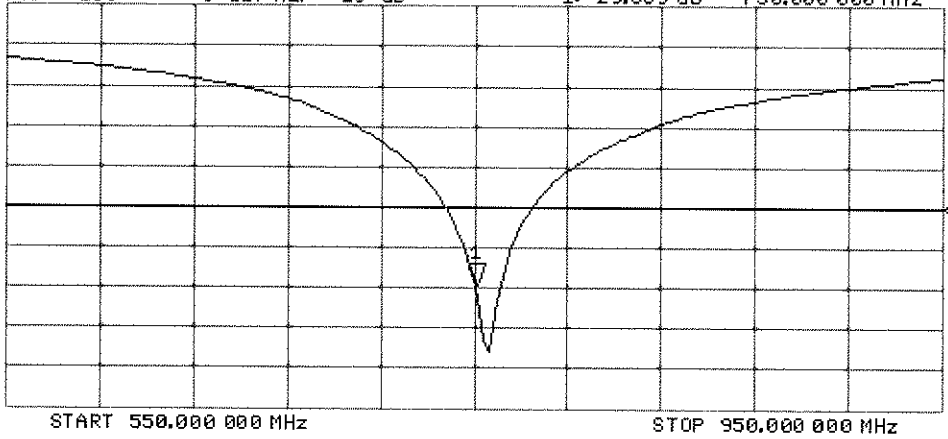

Certification of Calibration

Object D750V3 – SN: 1034

Calibration procedure(s) Procedure for Calibration Extension for SAR Dipoles.

Extended Calibration date: May 16, 2019

Description: SAR Validation Dipole at 750 MHz.

Calibration Equipment used:

Manufacturer	Model	Description	Cal Date	Cal Interval	Cal Due	Serial Number
Agilent	8753ES	S-Parameter Network Analyzer	10/2/2018	Annual	10/2/2019	US39170118
Agilent	N5182A	MXG Vector Signal Generator	6/15/2018	Annual	6/15/2019	MY47420837
Amplifier Research	15S1G6	Amplifier	CBT	N/A	CBT	343972
Anritsu	ML2495A	Power Meter	10/21/2018	Annual	10/21/2019	941001
Anritsu	MA2411B	Pulse Power Sensor	10/30/2018	Annual	10/30/2019	1207470
Anritsu	MA2411B	Pulse Power Sensor	11/20/2018	Annual	11/20/2019	1339007
Control Company	4040	Temperature / Humidity Monitor	2/28/2018	Biennial	2/28/2020	150761911
Control Company	4352	Ultra Long Stem Thermometer	2/28/2018	Biennial	2/28/2020	170330160
Keysight	772D	Dual Directional Coupler	CBT	N/A	CBT	MY52180215
Keysight Technologies	85033E	Standard Mechanical Calibration Kit (DC to 9GHz, 3.5mm)	6/4/2018	Annual	6/4/2019	MY53401181
Mini-Circuits	BW-N20W5+	DC to 18 GHz Precision Fixed 20 dB Attenuator	CBT	N/A	CBT	N/A
Mini-Circuits	NLP-2950+	Low Pass Filter DC to 2700 MHz	CBT	N/A	CBT	N/A
Narda	4772-3	Attenuator (3dB)	CBT	N/A	CBT	9406
Pasternack	PE2208-6	Bidirectional Coupler	CBT	N/A	CBT	N/A
Pasternack	PE5011-1	Torque Wrench	7/19/2017	Biennial	7/19/2019	N/A
SPEAG	DAKS-3.5	Portable DAK	9/11/2018	Annual	9/11/2019	1045
SPEAG	EX3DV4	SAR Probe	7/20/2018	Annual	7/20/2019	7416
SPEAG	DAE4	Dasy Data Acquisition Electronics	7/10/2018	Annual	7/10/2019	1402

Measurement Uncertainty = $\pm 23\%$ (k=2)

	Name	Function	Signature
Calibrated By:	Parker Jones	Team Lead Engineer	<i>Parker Jones</i>
Approved By:	Kaitlin O'Keefe	Senior Technical Manager	<i>KOK</i>

DIPOLE CALIBRATION EXTENSION



Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:

1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.



The following dipole was checked to pass the above 3 requirements to have 2-year calibration period from the calibration date:

Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Head (1g) W/kg @ 23.0 dBm	Measured Head SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Head (10g) W/kg @ 23.0 dBm	Measured Head SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Head (Ohm) Real	Measured Impedance Head (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Head (Ohm) Imaginary	Measured Impedance Head (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Head (dB)	Measured Return Loss Head (dB)	Deviation (%)	PASS/FAIL
5/18/2018	5/16/2019	1.034	1.664	1.65	-0.84%	1.064	1.08	-0.37%	55.3	54.4	0.9	0	-2.2	2.2	-26	-26.5	-1.90%	PASS
Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Body (1g) W/kg @ 23.0 dBm	Measured Body SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Body (10g) W/kg @ 23.0 dBm	Measured Body SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Body (Ohm) Real	Measured Impedance Body (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Body (Ohm) Imaginary	Measured Impedance Body (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Body (dB)	Measured Return Loss Body (dB)	Deviation (%)	PASS/FAIL
5/18/2018	5/16/2019	1.034	1.714	1.81	5.60%	1.134	1.19	4.94%	50	51.7	1.7	-3.2	-1	2.2	-29.8	-31	-3.90%	PASS

Impedance & Return-Loss Measurement Plot for Head TSL

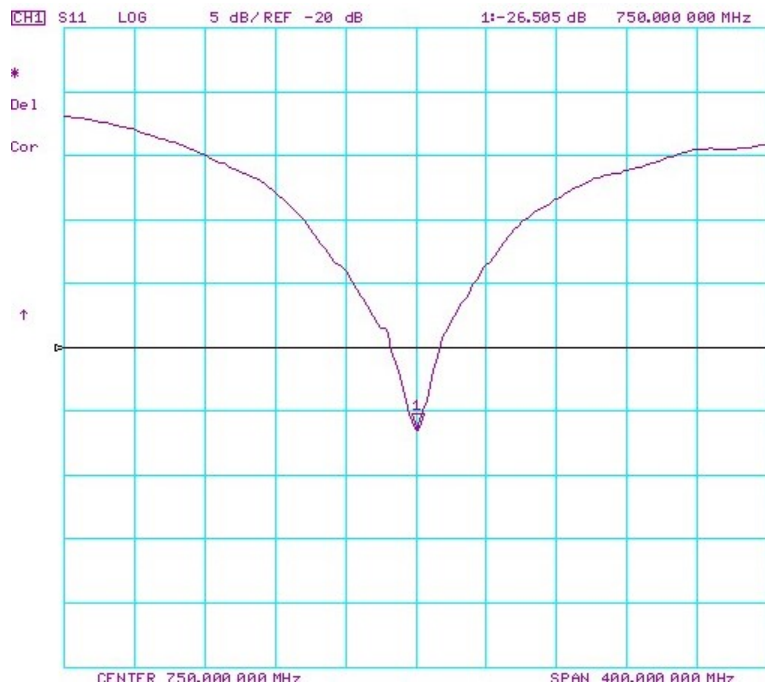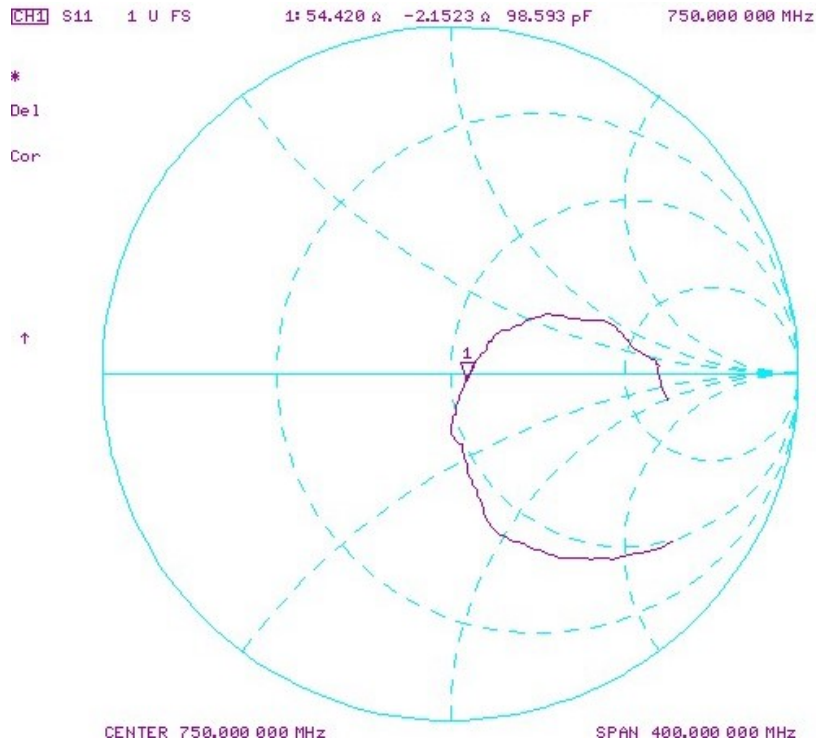

Impedance & Return-Loss Measurement Plot for Body TSL

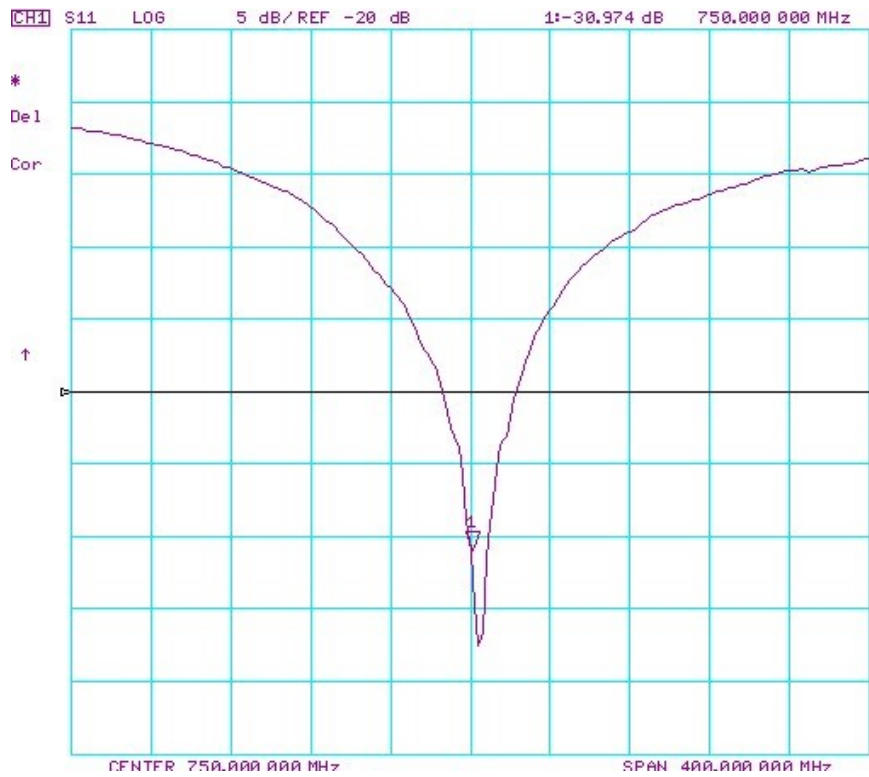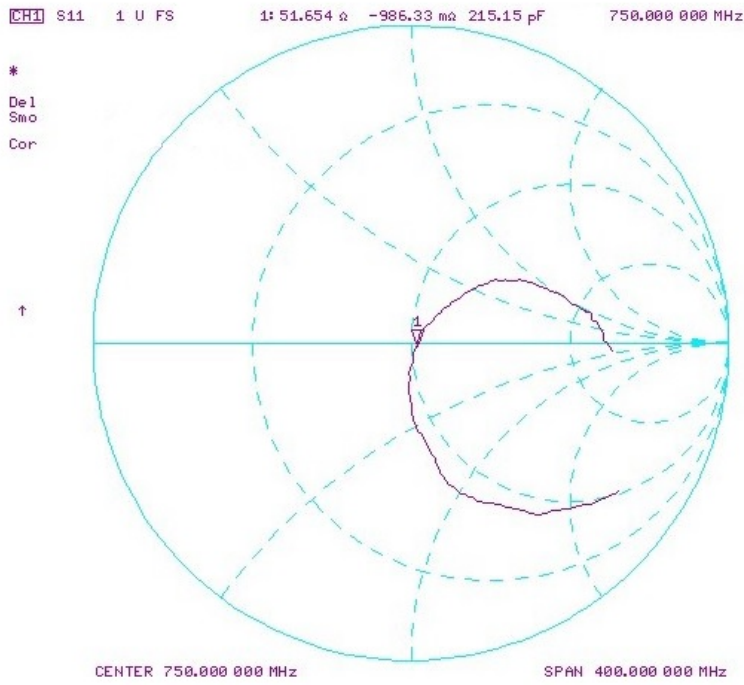

Certification of Calibration

Object: D750V3 – SN: 1034

Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.

Extended Calibration date: May 18, 2020

Description: SAR Validation Dipole at 750 MHz.

Calibration Equipment used:

Manufacturer	Model	Description	Cal Date	Cal Interval	Cal Due	Serial Number
Agilent	8753ES	S-Parameter Network Analyzer	1/16/2020	Annual	1/16/2021	US39170118
Agilent	N5182A	MXG Vector Signal Generator	8/19/2019	Annual	8/19/2020	MY47420837
Amplifier Research	15S1G6	Amplifier	CBT	N/A	CBT	343972
Anritsu	MA2411B	Pulse Power Sensor	1/21/2020	Annual	1/21/2021	1207470
Anritsu	MA2411B	Pulse Power Sensor	1/21/2020	Annual	1/21/2021	1339007
Anritsu	ML2495A	Power Meter	1/15/2020	Annual	1/15/2021	1328004
Control Company	62344-734	Therm./ Clock/ Humidity Monitor	3/18/2019	Biennial	3/18/2021	192038436
Control Company	4352	Ultra Long Stem Thermometer	8/2/2018	Biennial	8/2/2020	181292000
Keysight Technologies	85033E	Standard Mechanical Calibration Kit (DC to 9GHz, 3.5mm)	7/2/2019	Annual	7/2/2020	MY53401181
MiniCircuits	VLF-6000+	Low Pass Filter	CBT	N/A	CBT	N/A
Mini-Circuits	BW-N20W5+	DC to 18 GHz Precision Fixed 20 dB Attenuator	CBT	N/A	CBT	N/A
Narda	4772-3	Attenuator (3dB)	CBT	N/A	CBT	9406
Pasternack	PE2208-6	Bidirectional Coupler	CBT	N/A	CBT	N/A
Pasternack	NC-100	Torque Wrench	5/23/2018	Biennial	5/23/2020	N/A
SPEAG	DAE4	Dasy Data Acquisition Electronics	2/13/2020	Annual	2/13/2021	1403
SPEAG	DAE4	Dasy Data Acquisition Electronics	3/19/2020	Annual	3/19/2021	604
SPEAG	DAK-3.5	Dielectric Assessment Kit	5/12/2020	Annual	5/12/2021	1070
SPEAG	EX3DV4	SAR Probe	2/19/2020	Annual	2/19/2021	7427
SPEAG	EX3DV4	SAR Probe	3/20/2020	Annual	3/20/2021	7421

Measurement Uncertainty = $\pm 23\%$ (k=2)

	Name	Function	Signature
Calibrated By:	Parker Jones	Team Lead Engineer	<i>Parker Jones</i>
Approved By:	Kaitlin O'Keefe	Managing Director	<i>KOK</i>

DIPOLE CALIBRATION EXTENSION

Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:



1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 3-year calibration period from the calibration date:



Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Head (1g) W/kg @ 23.0 dBm	Measured Head SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Head (10g) W/kg @ 23.0 dBm	Measured Head SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Head (Ohm) Real	Measured Impedance Head (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Head (Ohm) Imaginary	Measured Impedance Head (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Head (dB)	Measured Return Loss Head (dB)	Deviation (%)	PASS/FAIL
5/18/2018	5/18/2020	1.034	1.664	1.63	-2.04%	1.064	1.08	-0.37%	55.3	52.2	-3.1	0	-2.4	2.4	-26	-30.3	-16.50%	PASS

Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Body (1g) W/kg @ 23.0 dBm	Measured Body SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Body (10g) W/kg @ 23.0 dBm	Measured Body SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Body (Ohm) Real	Measured Impedance Body (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Body (Ohm) Imaginary	Measured Impedance Body (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Body (dB)	Measured Return Loss Body (dB)	Deviation (%)	PASS/FAIL
5/18/2018	5/18/2020	1.034	1.714	1.73	0.93%	1.134	1.15	1.41%	50	48.9	-1.1	-3.2	-3	0.2	-29.8	-29.6	0.70%	PASS

Impedance & Return-Loss Measurement Plot for Head TSL

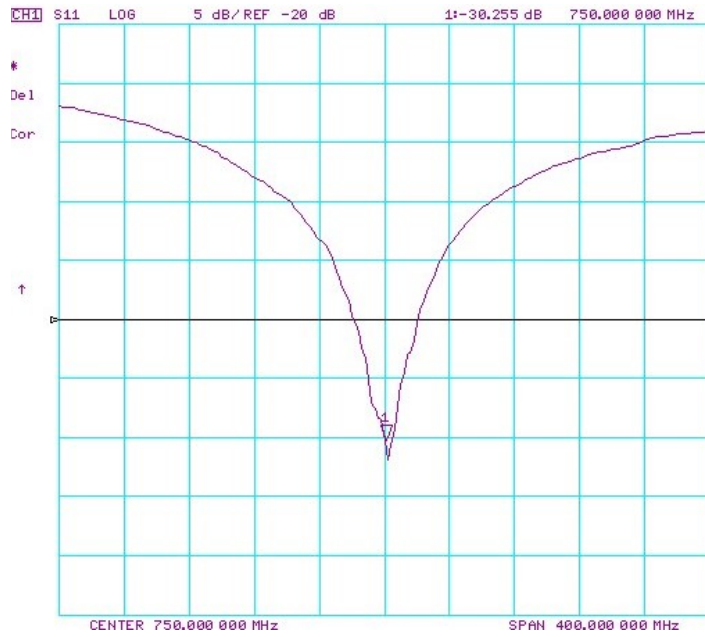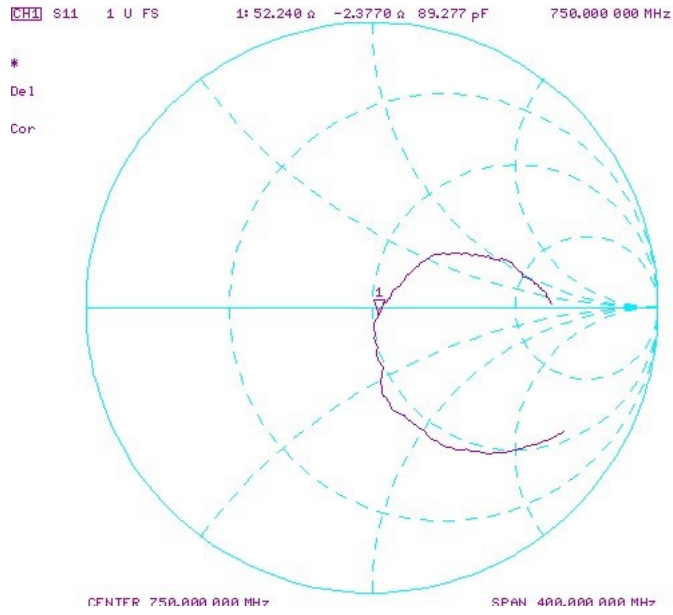

Impedance & Return-Loss Measurement Plot for Body TSL

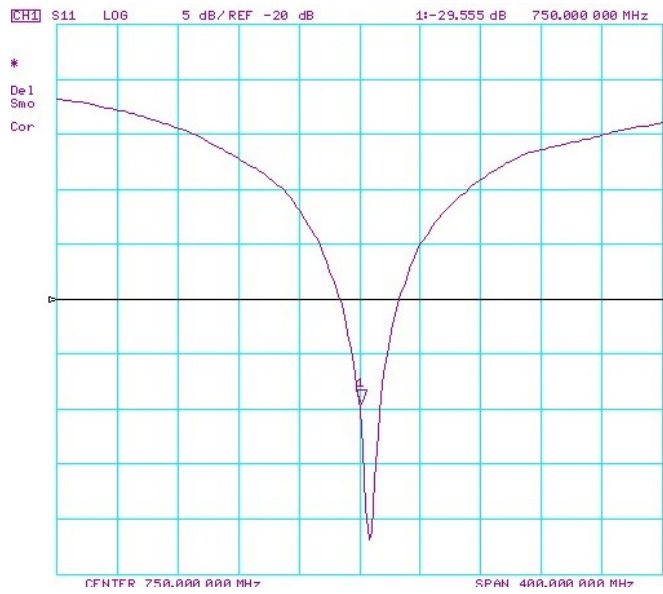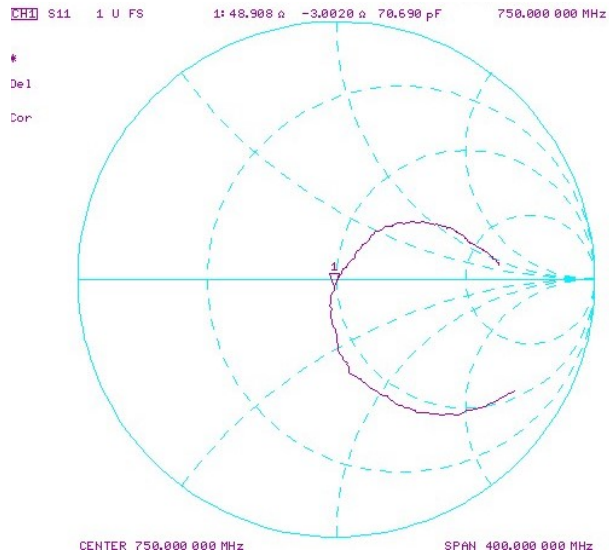



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client: **PC Test**

Certificate No.: **D835V2-4d040_Jun19**

CALIBRATION CERTIFICATE

Object: **D835V2 - SN:4d040**

Calibration procedure(s): **QA CAL-05.v11
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **June 20, 2019**

✓
ATM
6/28/19
✓
ATM
7/2/20

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-19 (No. 217-02894)	Apr-20
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-19 (No. 217-02895)	Apr-20
Reference Probe EX3DV4	SN: 7349	29-May-19 (No. EX3-7349_May19)	May-20
DAE4	SN: 601	30-Mar-19 (No. DAE4-601_Apr19)	Apr-20

Secondary Standards	ID #	Check Date (In house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Feb-19)	In house check: Oct-20
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-18)	In house check: Oct-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-18)	In house check: Oct-19

Calibrated by: **Manu Sellz** (Name), **Laboratory Technician** (Function), [Signature]

Approved by: **Katja Pokovic** (Name), **Technical Manager** (Function), [Signature]

Issued: June 21, 2019

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.2
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	41.8 ± 6 %	0.91 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.39 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.50 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.54 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.13 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	0.98 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.40 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.53 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.57 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.24 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	49.6 Ω - 4.1 j Ω
Return Loss	- 27.7 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	46.6 Ω - 6.5 j Ω
Return Loss	- 22.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.393 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------

DASY5 Validation Report for Head TSL

Date: 20.06.2019

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d040

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.91$ S/m; $\epsilon_r = 41.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(9.89, 9.89, 9.89) @ 835 MHz; Calibrated: 29.05.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2019
- Phantom: Flat Phantom 4.9 (front); Type: QD 00L P49 AA; Serial: 1001
- DASY52 52.10.2(1504); SEMCAD X 14.6.12(7470)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 63.05 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 3.60 W/kg


SAR(1 g) = 2.39 W/kg; SAR(10 g) = 1.54 W/kg

Maximum value of SAR (measured) = 3.19 W/kg

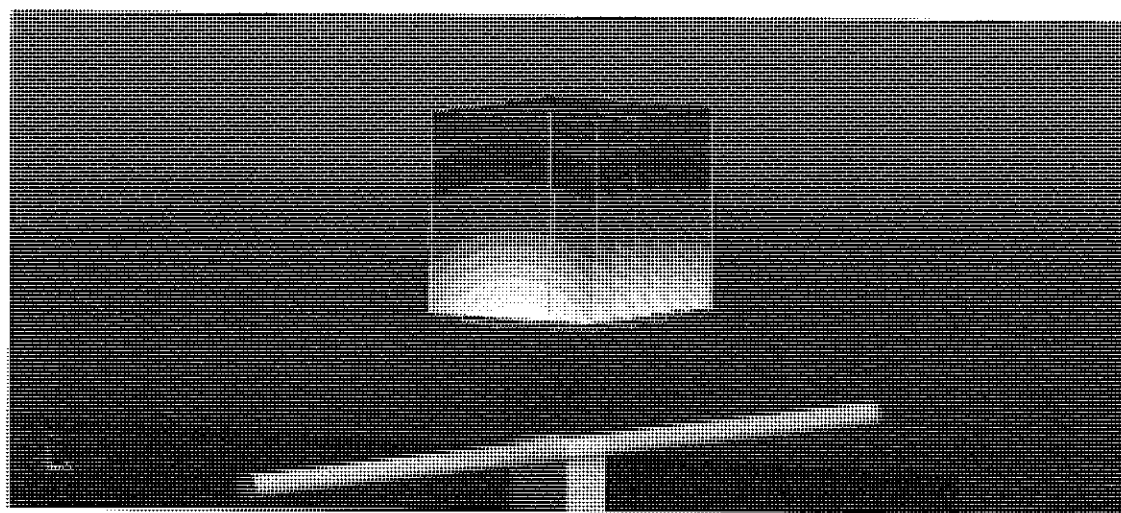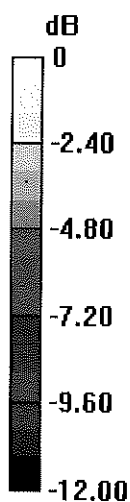

0 dB = 3.19 W/kg = 5.04 dBW/kg

Impedance Measurement Plot for Head TSL

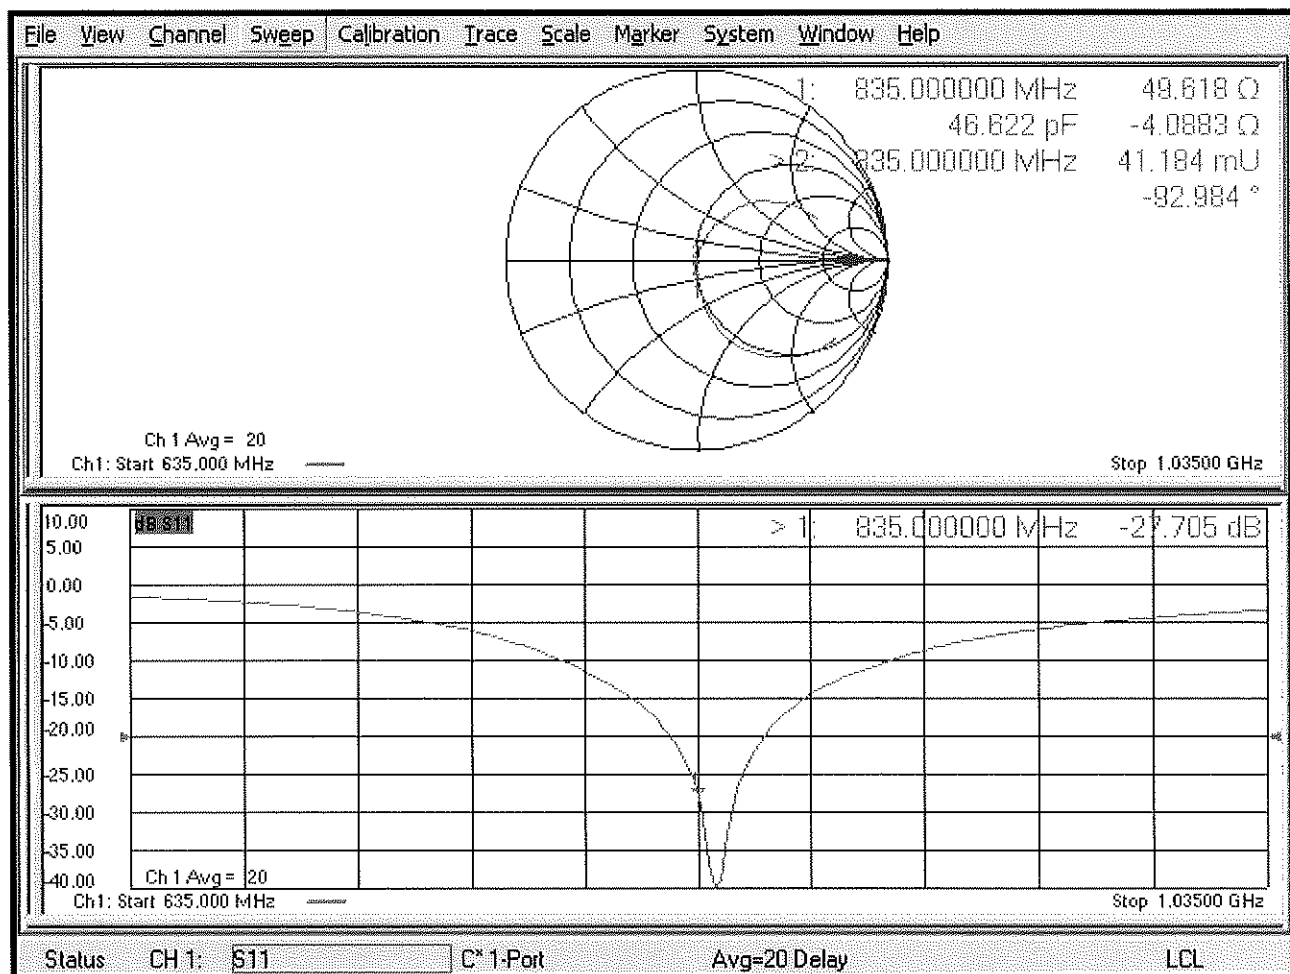

DASY5 Validation Report for Body TSL

Date: 13.06.2019

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d040

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835$ MHz; $\sigma = 0.98$ S/m; $\epsilon_r = 55.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: EX3DV4 - SN7349; ConvF(10.16, 10.16, 10.16) @ 835 MHz; Calibrated: 29.05.2019
- Sensor-Surface: 1.4mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2019
- Phantom: Flat Phantom 4.9 (Back); Type: QD 00R P49 AA; Serial: 1005
- DASY52 52.10.2(1504); SEMCAD X 14.6.12(7470)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 57.73 V/m; Power Drift = -0.08 dB

Peak SAR (extrapolated) = 3.59 W/kg


SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 3.21 W/kg

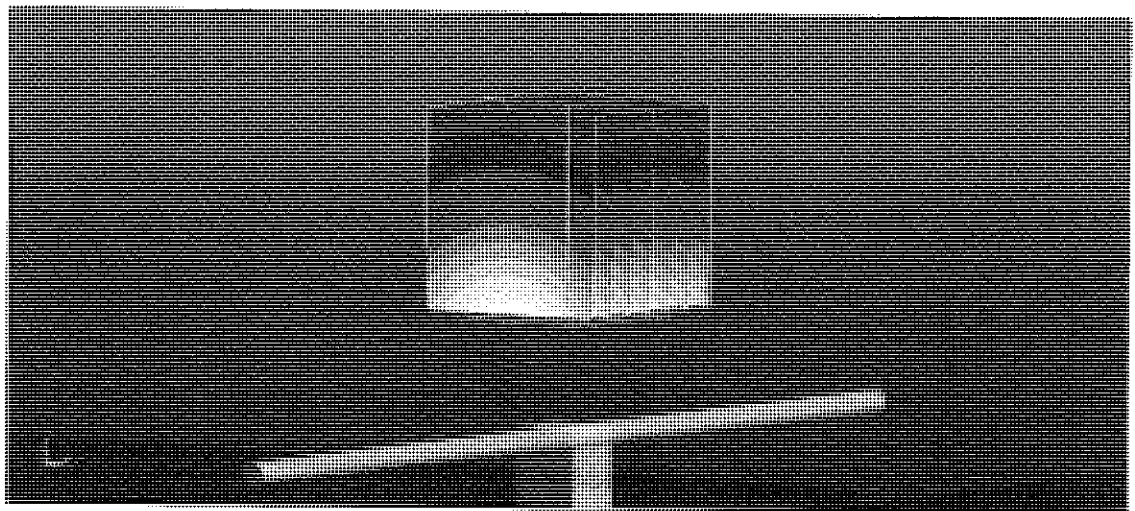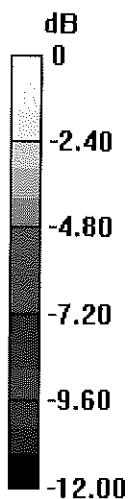

0 dB = 3.21 W/kg = 5.07 dBW/kg

Impedance Measurement Plot for Body TSL

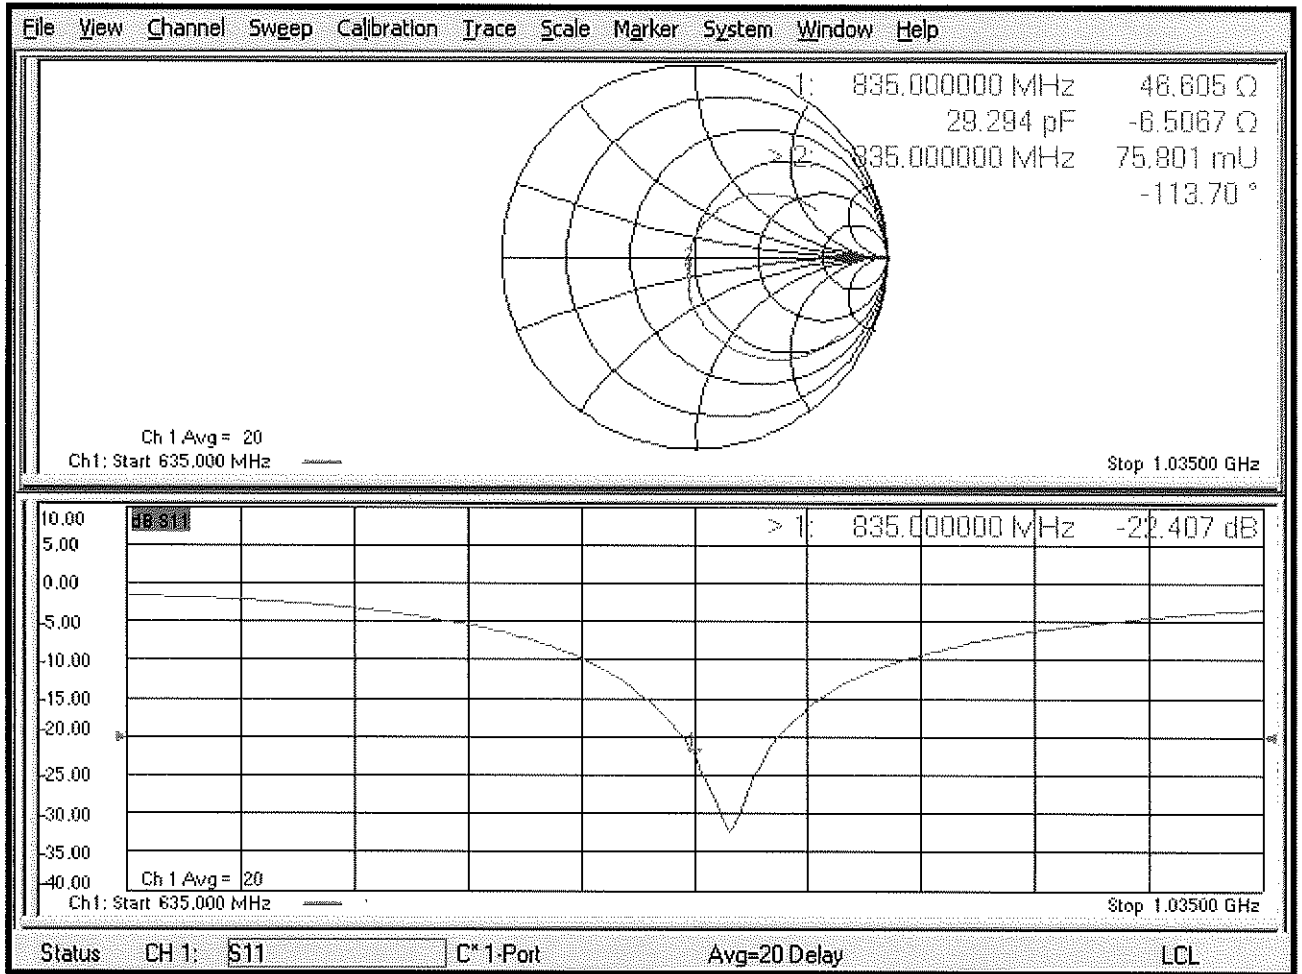

Certification of Calibration

Object: D835V2 – SN: 4d040
 Calibration procedure(s): Procedure for Calibration Extension for SAR Dipoles.
 Extended Calibration date: June 20, 2020
 Description: SAR Validation Dipole at 835 MHz.

Calibration Equipment used:

Manufacturer	Model	Description	Cal Date	Cal Interval	Cal Due	Serial Number
Agilent	8753ES	S-Parameter Network Analyzer	1/16/2020	Annual	1/16/2021	US39170118
Agilent	N5182A	MXG Vector Signal Generator	8/19/2019	Annual	8/19/2020	MY47420837
Amplifier Research	15S1G6	Amplifier	CBT	N/A	CBT	343972
Anritsu	MA2411B	Pulse Power Sensor	1/21/2020	Annual	1/21/2021	1207470
Anritsu	MA2411B	Pulse Power Sensor	1/21/2020	Annual	1/21/2021	1339007
Anritsu	ML2495A	Power Meter	1/15/2020	Annual	1/15/2021	1328004
Control Company	62344-734	Therm./ Clock/ Humidity Monitor	3/18/2019	Biennial	3/18/2021	192038436
Control Company	4352	Ultra Long Stem Thermometer	8/2/2018	Biennial	8/2/2020	181292000
Keysight Technologies	85033E	Standard Mechanical Calibration Kit (DC to 9GHz, 3.5mm)	7/2/2019	Annual	7/2/2020	MY53401181
MiniCircuits	VLF-6000+	Low Pass Filter	CBT	N/A	CBT	N/A
Mini-Circuits	BW-N20W5+	DC to 18 GHz Precision Fixed 20 dB Attenuator	CBT	N/A	CBT	N/A
Narda	4772-3	Attenuator (3dB)	CBT	N/A	CBT	9406
Pasternack	PE2208-6	Bidirectional Coupler	CBT	N/A	CBT	N/A
Seekonk	NC-100	Torque Wrench	7/18/2019	Annual	7/18/2020	N/A
SPEAG	DAE4	Dasy Data Acquisition Electronics	1/14/2020	Annual	1/14/2021	793
SPEAG	DAE4	Dasy Data Acquisition Electronics	3/19/2020	Annual	3/19/2021	604
SPEAG	DAK-3.5	Dielectric Assessment Kit	5/12/2020	Annual	5/12/2021	1070
SPEAG	EX3DV4	SAR Probe	1/20/2020	Annual	1/20/2021	3837
SPEAG	EX3DV4	SAR Probe	3/20/2020	Annual	3/20/2021	7421

Measurement Uncertainty = $\pm 23\%$ (k=2)

	Name	Function	Signature
Calibrated By:	Parker Jones	Team Lead Engineer	<i>Parker Jones</i>
Approved By:	Kaitlin O'Keefe	Managing Director	<i>KOK</i>

DIPOLE CALIBRATION EXTENSION

Per KDB 865664 D01, calibration intervals of up to three years may be considered for reference dipoles when it is demonstrated that the SAR target, impedance and return loss of a dipole have remained stable according to the following requirements:



1. The measured SAR does not deviate more than 10% from the target on the calibration certificate.
2. The return-loss does not deviate more than 20% from the previous measurement and meets the required 20dB minimum return-loss requirement.
3. The measurement of real or imaginary parts of impedance does not deviate more than 5Ω from the previous measurement.

The following dipole was checked to pass the above 3 requirements to have 2-year calibration period from the calibration date:



Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Head (1g) W/kg @ 23.0 dBm	Measured Head SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Head (10g) W/kg @ 23.0 dBm	Measured Head SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Head (Ohm) Real	Measured Impedance Head (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Head (Ohm) Imaginary	Measured Impedance Head (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Head (dB)	Measured Return Loss Head (dB)	Deviation (%)	PASS/FAIL
6/20/2019	6/20/2020	1.383	1.900	2	5.26%	1.226	1.31	6.85%	49.6	49	0.6	-4.1	-2.8	1.3	-27.7	-30.6	-10.50%	PASS

Calibration Date	Extension Date	Certificate Electrical Delay (ns)	Certificate SAR Target Body (1g) W/kg @ 23.0 dBm	Measured Body SAR (1g) W/kg @ 23.0 dBm	Deviation 1g (%)	Certificate SAR Target Body (10g) W/kg @ 23.0 dBm	Measured Body SAR (10g) W/kg @ 23.0 dBm	Deviation 10g (%)	Certificate Impedance Body (Ohm) Real	Measured Impedance Body (Ohm) Real	Difference (Ohm) Real	Certificate Impedance Body (Ohm) Imaginary	Measured Impedance Body (Ohm) Imaginary	Difference (Ohm) Imaginary	Certificate Return Loss Body (dB)	Measured Return Loss Body (dB)	Deviation (%)	PASS/FAIL
6/20/2019	6/20/2020	1.393	1.906	2.04	7.03%	1.248	1.34	7.37%	46.6	45.6	1	-6.5	-5.2	1.3	-22.4	-23.1	-3.10%	PASS

Impedance & Return-Loss Measurement Plot for Head TSL

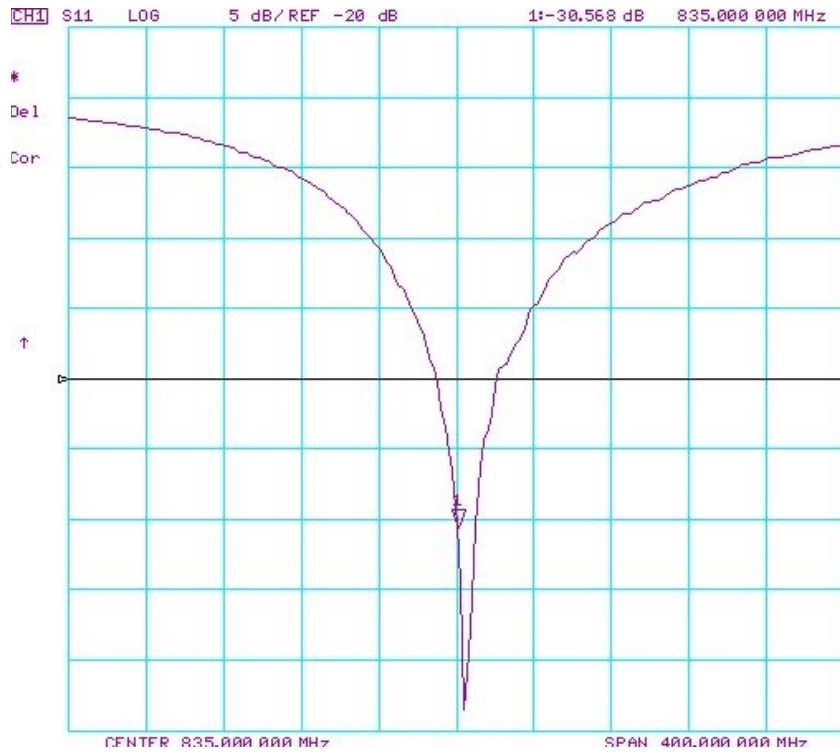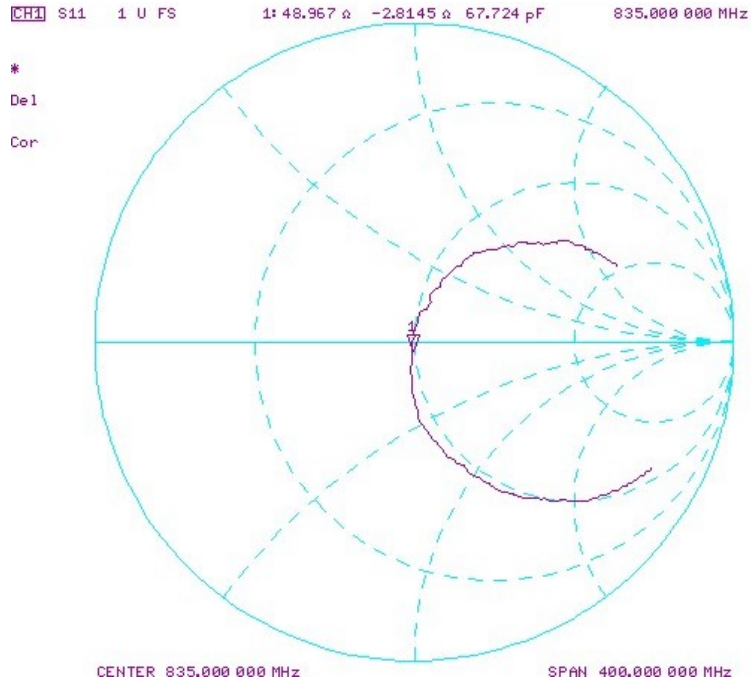

Impedance & Return-Loss Measurement Plot for Body TSL

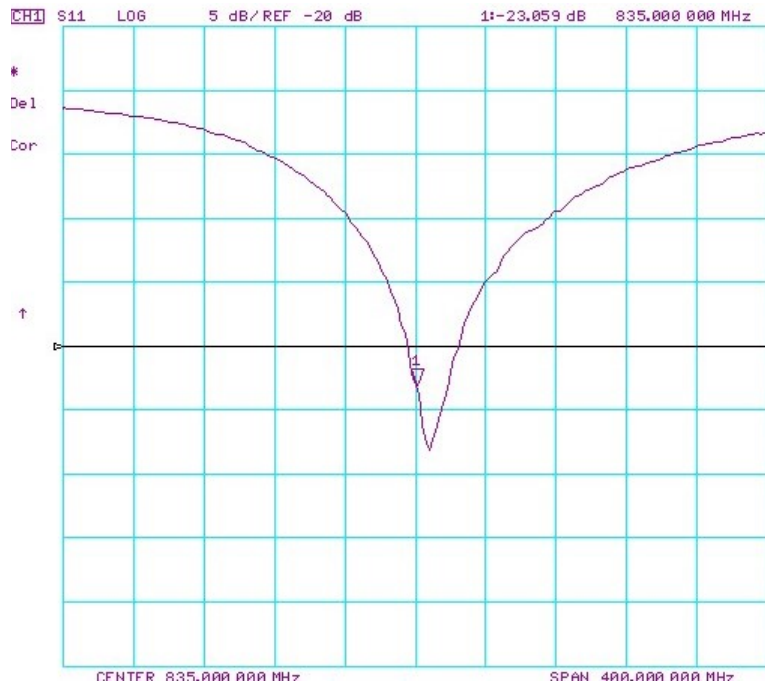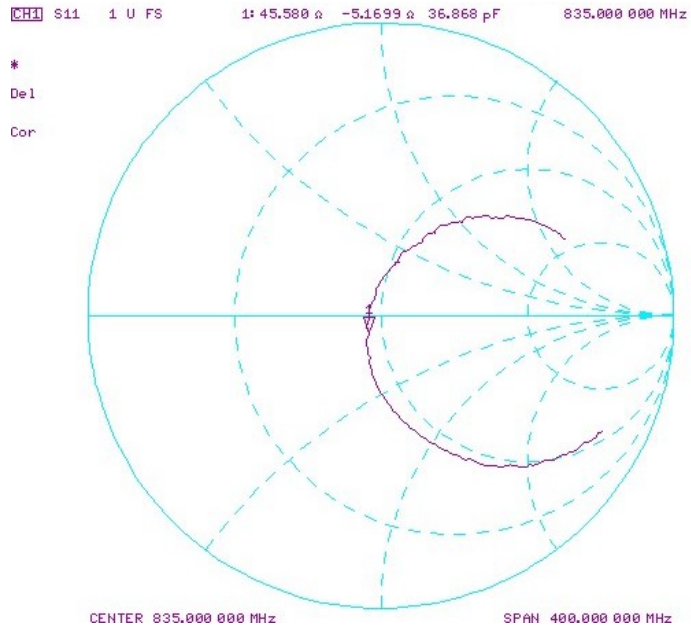



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Client **PC Test**

Certificate No: **D835V2-4d132_Jan20**

CALIBRATION CERTIFICATE

Object **D835V2 - SN:4d132**

Calibration procedure(s) **QA CAL-05.v11
Calibration Procedure for SAR Validation Sources between 0.7-3 GHz**

Calibration date: **January 13, 2020**

*BN ✓
02-05-2020*

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter NRP	SN: 104778	03-Apr-19 (No. 217-02892/02893)	Apr-20
Power sensor NRP-Z91	SN: 103244	03-Apr-19 (No. 217-02892)	Apr-20
Power sensor NRP-Z91	SN: 103245	03-Apr-19 (No. 217-02893)	Apr-20
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-19 (No. 217-02894)	Apr-20
Type-N mismatch combination	SN: 5047.2 / 06327	04-Apr-19 (No. 217-02895)	Apr-20
Reference Probe EX3DV4	SN: 7349	31-Dec-19 (No. EX3-7349_Dec19)	Dec-20
DAE4	SN: 601	27-Dec-19 (No. DAE4-601_Dec19)	Dec-20

Secondary Standards	ID #	Check Date (in house)	Scheduled Check
Power meter E4419B	SN: GB39512475	30-Oct-14 (in house check Feb-19)	In house check: Oct-20
Power sensor HP 8481A	SN: US37292783	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
Power sensor HP 8481A	SN: MY41092317	07-Oct-15 (in house check Oct-18)	In house check: Oct-20
RF generator R&S SMT-06	SN: 100972	15-Jun-15 (in house check Oct-18)	In house check: Oct-20
Network Analyzer Agilent E8358A	SN: US41080477	31-Mar-14 (in house check Oct-19)	In house check: Oct-20

Calibrated by:	Name Leif Klysner	Function Laboratory Technician	Signature
----------------	-----------------------------	--	---------------

Approved by:	Name Katja Pokovic	Technical Manager Technical Manager	
--------------	------------------------------	---	--

Issued: January 21, 2020

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 0108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Measurement procedure for the assessment of Specific Absorption Rate (SAR) from hand-held and body-mounted devices used next to the ear (frequency range of 300 MHz to 6 GHz)", July 2016
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.10.3
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz \pm 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 \pm 0.2) °C	42.6 \pm 6 %	0.91 mho/m \pm 6 %
Head TSL temperature change during test	< 0.5 °C	---	---

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.42 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.65 W/kg \pm 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.58 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.30 W/kg \pm 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 \pm 0.2) °C	55.1 \pm 6 %	0.99 mho/m \pm 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.53 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.96 W/kg \pm 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.68 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.64 W/kg \pm 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.4 Ω - 3.1 j Ω
Return Loss	- 30.0 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.7 Ω - 5.5 j Ω
Return Loss	- 24.8 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.385 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
-----------------	-------