Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
S wiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

CALIBRATION CERTIFICATE

Accreditation No.: SCS 0108

Client

PC Test

Certificate No: D835V2-4d119_Apr15

Object	D835V2 - SN:4d	119 military among the continue of the	·
Calibration procedure(s)	QA CAL-05.v9 Calibration procedure for dipole validation kits above 700 MHz 4/29		
Calibration date:	April 13, 2015		e sa seria artik artik Kikasio (se
The measurements and the tince	rtainties with confidence p	ional standards, which realize the physical unprobability are given on the following pages are facility: environment temperature $(22 \pm 3)^{\circ}$ 0	nd are part of the certificate.
Primary Standards	ID #	Cal Data (0, 115	
Power meter EPM-442A	GB37480704	Cal Date (Certificate No.)	Scheduled Calibration
Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02020)	Oct-15
Reference 20 dB Attenuator	SN: 5058 (20k)	07-Oct-14 (No. 217-02021)	Oct-15
Type-N mismatch combination	SN: 5047.2 / 06327	01-Apr-15 (No. 217-02131)	Mar-16
Reference Probe ES3DV3	SN: 3205	01-Apr-15 (No. 217-02134)	Mar-16
DAE4	SN: 601	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15
, ·	514. 001	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15
	Name	Function	Signature
Calibrated by:	Israe Elnaouq	Laboratory Technician	Moreon Charge
Approved by:	Katja Pokovic	Technical Manager	Ally-
This calibration certificate shall no	ot be reproduced except in	full without written approval of the laboratory.	Issued: April 13, 2015

Certificate No: D835V2-4d119_Apr15

Page 1 of 8

Calibration Laboratory of

Schmid & Partner **Engineering AG** Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst S Service suisse d'étalonnage

Servizio svizzero di taratura S

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF

sensitivity in TSL / NORM x,y,z

N/A

not applicable or not measured

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D835V2-4d119_Apr15

Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	V OZ0.0
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	with opacer
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.9 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.43 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.38 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.57 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	6.11 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	55.4 ± 6 %	1.01 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.37 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.20 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.55 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.06 W/kg ± 16.5 % (k=2)

Certificate No: D835V2-4d119_Apr15

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	50.2 Ω - 2.2 jΩ
Return Loss	- 33.3 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω - 4.9 ϳΩ
Return Loss	- 25.1 dB

General Antenna Parameters and Design

Flectrical Doloy (one dispetion)	
Electrical Delay (one direction)	1 000
	1.386 ns

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 29, 2010

Certificate No: D835V2-4d119_Apr15

DASY5 Validation Report for Head TSL

Date: 13.04.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d119

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz; $\sigma = 0.94$ S/m; $\varepsilon_r = 40.9$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.2, 6.2, 6.2); Calibrated: 30.12.2014;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

• DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 56.77 V/m P

Reference Value = 56.77 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.64 W/kg


SAR(1 g) = 2.43 W/kg; SAR(10 g) = 1.57 W/kg

Maximum value of SAR (measured) = 2.85 W/kg

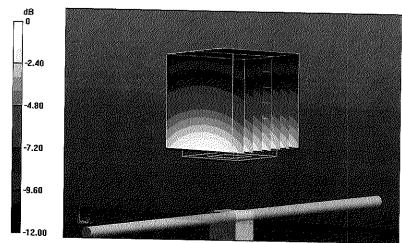

0 dB = 2.85 W/kg = 4.55 dBW/kg

Impedance Measurement Plot for Head TSL

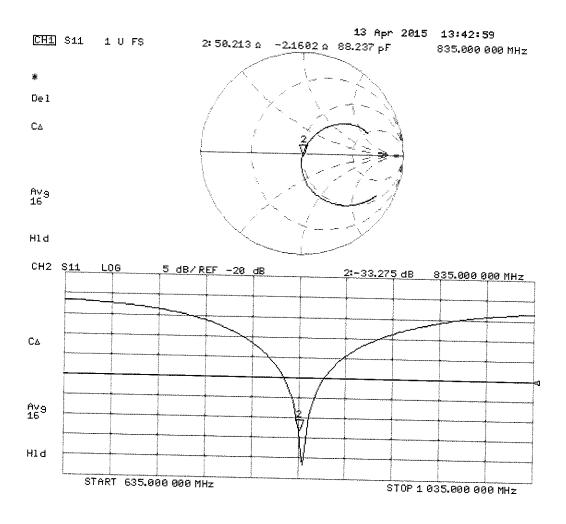

DASY5 Validation Report for Body TSL

Date: 13.04.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN:4d119

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: f = 835 MHz; $\sigma = 1.01$ S/m; $\epsilon_r = 55.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(6.17, 6.17, 6.17); Calibrated: 30.12.2014;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001

DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 54.44 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 3.52 W/kg


SAR(1 g) = 2.37 W/kg; SAR(10 g) = 1.55 W/kg

Maximum value of SAR (measured) = 2.77 W/kg

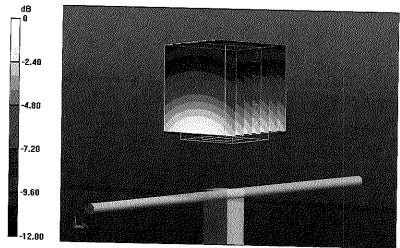

0 dB = 2.77 W/kg = 4.42 dBW/kg

Impedance Measurement Plot for Body TSL

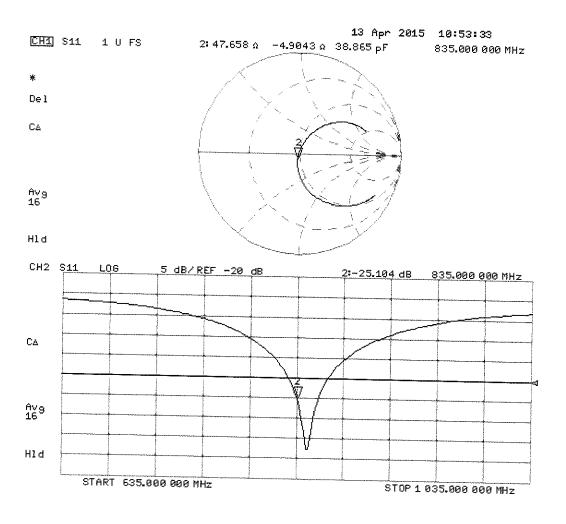

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: D1900V2-5d149 Jul15

1	CALIBRATION CERTIFICATE

Object

D1900V2 - SN:5d149

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

UU√ 8/4/1°

Calibration date:

July 14, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 \pm 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02021)	Oct-15
Reference 20 dB Attenuator	SN: 5058 (20k)	01-Apr-15 (No. 217-02131)	Mar-16
Type-N mismatch combination	SN: 5047.2 / 06327	01-Apr-15 (No. 217-02134)	Mar-16
Reference Probe ES3DV3	SN: 3205	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15
DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15
	Name	Function	Signature

Calibrated by:

Leif Klysner

Function

Laboratory Technician

Signature

Approved by:

Katja Pokovic

Technical Manager

Issued: July 14, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: D1900V2-5d149_Jul15

Page 1 of 8

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL

tissue simulating liquid

ConvF N/A

sensitivity in TSL / NORM x,y,z not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

e) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point.
 No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d149_Jul15

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	39.7 ± 6 %	1.38 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.1 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.7 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.34 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.5 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.7 ± 6 %	1.54 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C		

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	10.2 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	40.4 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.49 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.8 W/kg ± 16.5 % (k=2)

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.4 Ω + 5.6 jΩ
Return Loss	- 24.9 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω + 6.1 jΩ
Return Loss	- 23.5 dB

General Antenna Parameters and Design

Florida de Dalace / como Pro (U. A.)	
Electrical Delay (one direction)	1.197 ns
(1111)	11107 110

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 11, 2011

DASY5 Validation Report for Head TSL

Date: 14.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d149

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.38 \text{ S/m}$; $\varepsilon_r = 39.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5, 5, 5); Calibrated: 30.12.2014;

Sensor-Surface: 3mm (Mechanical Surface Detection)

Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

• DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 99.22 V/m; Power Drift = 0.02 dB

Peak SAR (extrapolated) = 18.3 W/kg


SAR(1 g) = 10.1 W/kg; SAR(10 g) = 5.34 W/kg

Maximum value of SAR (measured) = 12.9 W/kg

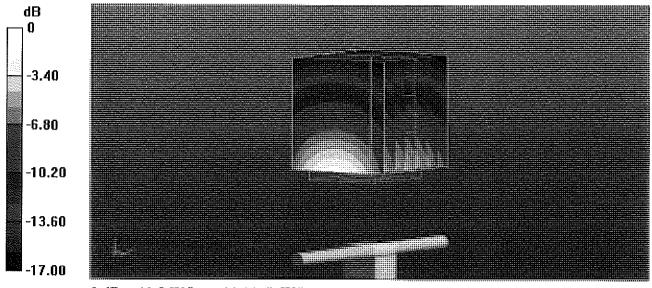

0 dB = 12.9 W/kg = 11.11 dBW/kg

Impedance Measurement Plot for Head TSL

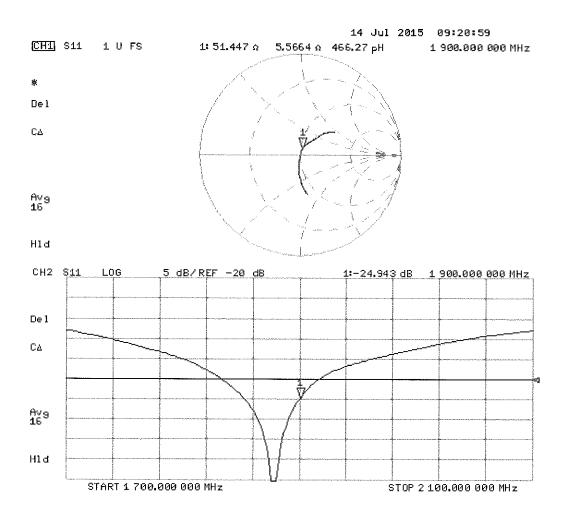

DASY5 Validation Report for Body TSL

Date: 14.07.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d149

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.54 \text{ S/m}$; $\varepsilon_r = 52.7$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

• Probe: ES3DV3 - SN3205; ConvF(4.65, 4.65, 4.65); Calibrated: 30.12.2014;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 18.08.2014

• Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.96 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 17.2 W/kg


SAR(1 g) = 10.2 W/kg; SAR(10 g) = 5.49 W/kg

Maximum value of SAR (measured) = 12.9 W/kg

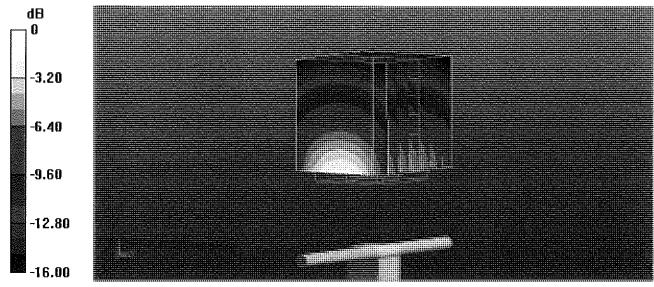

0 dB = 12.9 W/kg = 11.11 dBW/kg

Impedance Measurement Plot for Body TSL

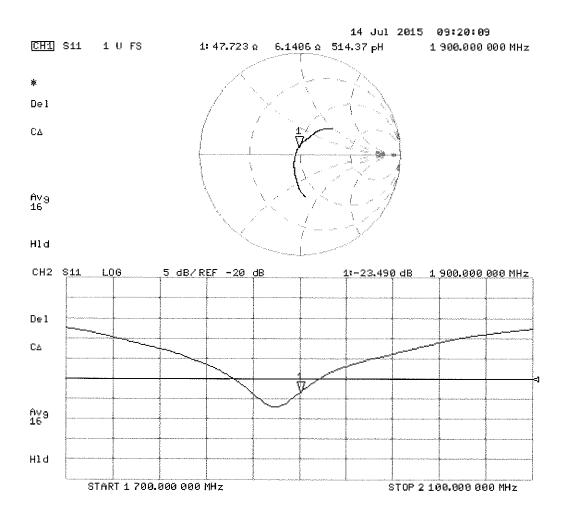

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étatonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

PC Test

Certificate No: ES3-3288 Sep15

CALIBRATION CERTIFICATE

Object

ES3DV3 - SN:32B8

Calibration procedure(\$)

QA CAL-01.v9; QA CAL-23.v5; QA CAL-25.v6 Calibration procedure for obsimetric E-field probes

Calibration date:

September 18, 2015

This delibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature $(22 \pm 3)^{\circ}$ C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ΙD	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: \$5054 (3c)	01-Apr-15 (Na. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	\$N; \$5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 560	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	i ID	Check Date (in house)	Scheduled Check
RF generator HP 66490	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	U\$37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Name Function Signature

Calibrated by: Michael Weber Eathoratory Technician

Approved by: Katja Pokovic Technical Manager

issued: September 19, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3288_Sep15 Page 1 of 13

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage

Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization φ φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center).

i.e., $\vartheta = 0$ is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y.z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z; A, B, C, D are numerical linearization parameters assessed based on
 the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor
 media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip
 (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: E\$3-3288_Sep15 Page 2 of 13

Probe ES3DV3

SN:3288

Manufactured: July 6, 2010

Calibrated:

September 18, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m)²) ^A	1.05	1.16	0.92	± 10.1 %
DCP (mV) ^B	106.9	106.9	107.4	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc [®]
0	CW	†x	0.0	0.0		0.00	190.7	(k=2)
	7	* ΄ Υ	0.0		1.0	~~		±3.0 %
•••		····		0.0	1.0		181.4	
10010-	SAR Validation (Square, 100ms, 10ms)	<u></u>	0.0	0.0	1.0	45.05	179.1	<u> </u>
CAA	The state of the s	X i	2.55	61.8	10.9	10.00	38.D	±1.2 %
		<u> </u>	99.34	97.0	21.5		36.6	
10011-	UMTS-FDD (WCDMA)	Ž	6.26	70.5	13.9		35.2	<u> </u>
CAB	i	X	3.28	67.4 ;—	18.7	2.91	129.4	±0.5 %
		Y	3,60	69.3	19.8		143.8	
40010		Z	3.38	67.9	18.8	-11.	143,0	```
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	Х	3.07	70.1	19.4	1.87	131.0	±0.7 %
		. γ	3.79	74.2	21.4		145.4	
4 AB 4 B	1000	Z	3.15	70.5	19.4	[144.5	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM. 6 Mbps)	X	10.64	69.8	22.8	9.46	122.7	±2.7 %
	<u> </u>	Y	10.89	70.2	22.9		140.0	
		Z	10,70	70.2	23.0		136.7	· · · · · · · · · · · · · · · · · · ·
10021- DAB	GSM-FDD (TDMA, GMSK)	Х	10.49	86.3	22.8	9.39	138.5	±2.2 %
		Υ	13.76	90.7	24.6		145.7	
		Z	7.99	82.4	21.3		141.8	
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	×	9.73	85.3	22.7	9.57	149,4	±2.7 %
		Υ	9.12	84.3	22.7		131.8	
		Z	8.21	83.4	22.1	•	134.8	
1002 4 - DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	34.75	99.7	24.5	6.56	135.8	±2.5 %
		Υ	22.21	94.5	23.5		148.5	
	****	Z	8.93	81,8	18.8		148.3	
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	×	51,22	100.0 .	22.6	4.80	132.9	±1.9 %
		Υ	45.95	99.6	23.0		139.7	
		Z	14.90	87.0	19.2		138.0	
10028- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	х	56.25	99.8	21.6	3.55	141.8	±1.9 %
		ΙΥ	61.05	99.6	21.6		149.8	
		z z	70.48	99.7	20.8		126.6	
10032- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	х	98.24	98.4	18.0	1.16	135.4	±1.9 %
		Y	71.59	99.7	19.3	·	144.2	
		Z	98.96	91.6	15.1	, ·	148.2	
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	6.44	67.9	19.9	5.67	148.9	±1.4 %
		Y	6.27	67.2	19.6	<u>-</u>	131.4	
	1	. z	6.28	67.3	19.5	*****	137.9	

10103- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	9.52	74.2	25.3	9.29	134.3	±2.5 %
	74	Υ	9.97	75.1	25.7		146.8	
45455		Z	9.47	74.4	25.4	<u> </u>	147.4	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.31	67.5	19.8	5.80	147.4	±1.4 %
···		Ϋ́	6.21	67.1	19.6		131.0	
		Z	6.16	67,0	19.5	<u> </u>	136.4	
10117- CAB	IEEE 8D2.11n (HT Mixed, 18.5 Mbps, BPSK)	Х	10.11	68.9	21.2	8.07	137.9	±2.2 %
		Y	10.26	69.3	21.5		147.7	
10454		Z	9.85	68.3	20.9		126.0	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	8.90	73.2	25.0	9.28	129,8	±3.3 %
		Υ	9.32	74.0	25.2		142.5	""
40454		_ Z	8.86	73.4	25.1		142.1	
10154- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.98	66.9	19.6	5.75	143.7	±1.2 %
		<u>Y</u>	5.91	66.6	19.4		128.0	
10160-	LTE EDD (OD ED)	Z	5.84	66.5	19.3		133.4	
CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.43	67.5	19.8	5.82	148.9	±1.4 %
		Y	6.31	67.0	19.6	:	132.2	
40400		2	6.30	67.1	19.5	<u> </u>	138.0	
10169- CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	ļх	4.93	67.3	20.0	5.73	145.7	±1.2 %
		. Y	4.89	66.9	19.8	Ĺ	131.7	7
10172-	LITE TOP (OA FELLW)	Z	4.82	66.9	19.7		134.9	
CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	7.96	77.5	27.4	9.21	143.6	±2.7 %
		Y.	7.61	75.5	26.3		129.2	
10175-	LTE COD (DO COLO)	Z	7.10	74.5	25.9		129.7	<u> </u>
CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	Х	4.89	67.1	19.9	5.72	138.9	±1.2 %
		Υ	5.02	67.5	20.1		148.1	
10181-	ATE EDD (SO FDM) A DD 45	2	4.77	66.7	19.6	<u></u>	129.3	
CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X		67.3	20,0	5.72	143.8	±1.2 %
		· Y	5.08	67.8	20.3		149.0	
10196-	PETE DAD 44 - AUT NE	Z	4.73	66.5	19.5		129.4	
CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	×	9.73	68.7	21.3	8.10	130.0	±1.9 %
720.	i	Y	9.74	68.6	21 .2		132.7	
10225-	LIMTO FOR ALCONAL	z	9.78	69.0	21.4		138.2	
CAB	UMTS-FDD (HSPA+)	X	6.83	66.9	19.4	5.97	134.3	±1.4 %
		Y	6.98	67.3	19.6		139.3	
10237-	LTE YOU GO EDIM A DO AND	<u>z,</u>	6.92	67.4	19.6	: 	142.7	\ <u>\\\</u>
CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	×	7.94	77.5	27.4	9.21	143.5	±2.7 %
		Υ	7.44	74.8	25.9		125.0	
10252	LIFE TOD (OC COM SON DO 40 - 11	Z	7.14	74.7	26.0		131.4	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB. 10 MHz, QPSK)	X	8.95	74.9	26.1	9.24	140.8	±2.7 % ***
		Y	8,53	72.8	24.7		127.2	
10267-	LITE IDD (CC EDMS 4000) DO 45	<u>Z</u> .	8.14	<u>72.3</u>	24.6		127.1	
CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	9. 6 6	75.7	26.4	9.30	149.7	±3.0 %
	· · · · · · · · · · · · · · · · · · ·	Y	9.20	73.6	25.1		135.1	
		Ζį	8.81	73.3	25.1		134.3	

ES3DV3-SN:3288 September 18, 2015

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Ref8.4)	Х	4.39	67.0	18.8	3.96	138.0	±0.7 %
		ΪΥ	4.51	67.5	19,2	!	141.4	
		Z	4,46	67.3	18.9		146.2	<u> </u>
10291- AAB	CDMA2000, RC3, SO55, Full Rate	X	3.59	67.1	18.7	3.46	128.3	±0.5 %
		Ι. Υ	3.80	68.2	19.5		130.9	! :
		Z	3.74	68.1	19.2		135.6	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	×	3.55	67.3	18.9	3.39	129.6	±0.5 %
		Ϋ́Υ	3.73	68.2	19.4	ļ 	132.7	
		Z	3.63	67.8	19.0		, 137.7	~.
10297- LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	х	6.30	67.4	19.8	5.81	145.6	±1.4 %	
		Y	6.38	67.7	19.9		148.2	 -
		Z	6.12	66.8	i 19.4	ì	129.8	
10311- AAA	LTE-FŐD (SC-FÐMÄ, 100% RB, 15 : MHz, QPSK)	×	6.56	66.9	19.5	6.06	126.9	±1.2 %
		Y	6.71	67.4	19.8	 	129.7	
		Ζ	6.71	67.5	19.8	·	136.5	-~
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	Х	9.96	68.8	21.5	8.37	132.0	±2.2 %
-v		Y	10.06	69.0	21.6		137.4	·
		Ζ ;	10.06	69.3	21.7		140.2	
104 0 3- AAB	CDMA2000 (1xEV-DO, Rev. 0)	Х	4.89	69.6	19.3	3.76	139.4	±0.5 %
	T-1	ļΥ	5.05	70.0	19.6	<u> </u>	143.9	
		Z	4.98	70.0	19.5	""	146.8	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	x	4.81	69.6	19.4	3.77	136.6	±0.7 %
		Y	5.07	70.4	19.9		146.8	
		z "	4,90	70.2	19.6		144.5	
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	×	2.82	69.8	19.4	1.54	136.4	±D.7 %
		Υ	3.19	72.3	20.7	•	145.1	V
*		Z	2.84	69.7	19.1	7.	145.5	-
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	×	9.77	68.6	21.3	8.23	130.4	±2.2 %
		Υ	9.95	69.0	21.5		140.4	•
	<u> </u>	Z	9.88	69.0	21,5		138.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

Numerical linearization parameter: uncertainty not required.

Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^f	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^{'d'} (mm)	Unc (k=2)
750	41.9	0.89	6.69	6.69	6.69	0.80	1.17	± 12.0 %
835	41.5	0.90	6.41	6.41	6.41	0.68	1.22	± 12.0 %
1750	40.1	1.37	5.40	5.40	5,40	0.57	1.39	± 12.0 %
1900	40.0	1.40	5.17	5.17	5.17	0.76	1.14	± 12.0 %
2300	39.5	1.67	4.85	4.85	4.85	0.64	1.32	± 1 2.0 %
2450	39.2	1.80	4.57	4.57	4.57	0.75	1.34	± 12.0 %
2600	39.0	1.96	4.44	4.44	4.44	0.68	1.38	± 12.0 %

Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments \pm t 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (s and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (s and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissu= parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvFY	ConvF Z	Alpha ⁶	Depth ⁶ (mm)	Unç (k=2)
750	55.5	0.96	6.57	6.57	6.57	0.80	1,13	± 12.0 %
835	<u>5</u> 5.2	0.97	6.40	6.40	6.40	0.53	1.45	± 12.0 %
1750	53.4	1.49	4.99	4.99	4.99	0.37	1.82	± 12.0 %
1900	53.3	1.52	4.81	4.81	4.81	0.42	1.72	± 12.0 %
2300	52.9	1.81	4.54	4.54	4 .54	0.80	1.24	± 12.0 %
2450	52.7	1.95	4.37	4.37	4.37	0.80	1.20	± 12.0 %
2600 j	52.5	2.16	4.23	4.23	4.23	0.80	1.18	± 12.0 %


⁶ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.


Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

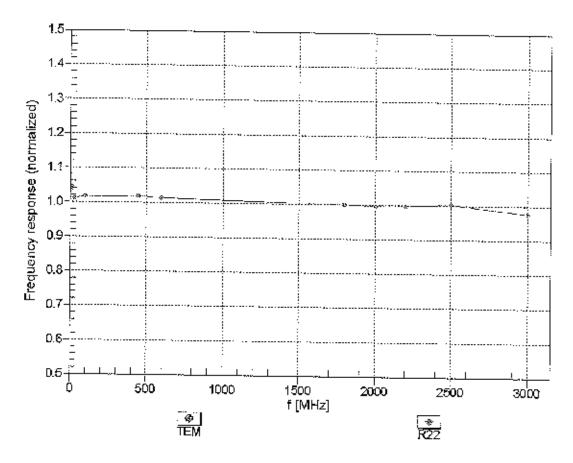

Uncertainty of Frequency Response of E-field: \pm 6.3% (k=2)


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

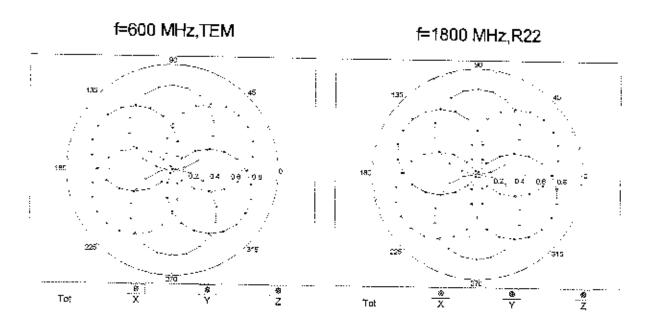


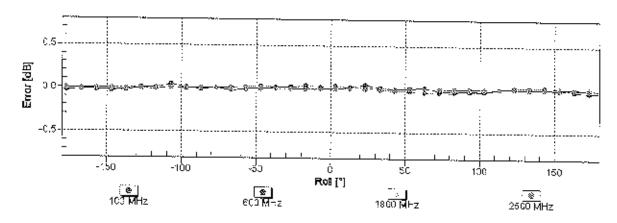

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

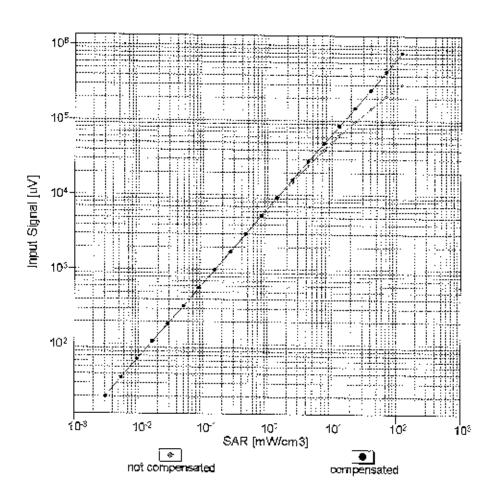

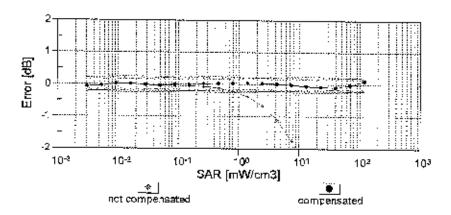


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Conversion Factor Assessment

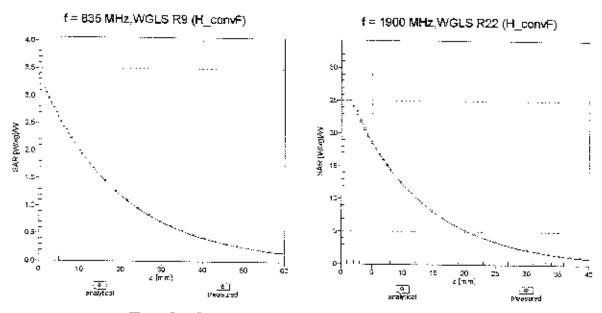

Deviation from Isotropy in Liquid

Error $(\phi, 9)$, f = 900 MHz

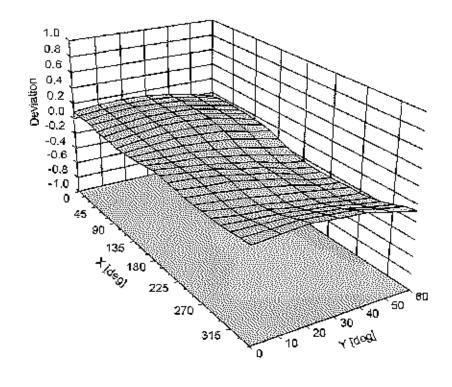



DASY/EASY - Parameters of Probe: ES3DV3 - SN:3288

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	73.1
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kallbrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: ES3-3287_Oct15

CALIBRATION CERTIFICATE

Object | ES3DV3 - SN:3287

Calibration procedure(s) QA CAL-01.v9; QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date: October 29, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility; environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Altenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: 85277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3842U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Issued: October 29, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3287_Oct15

Page 1 of 13

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerlscher Kallbrierdtenst
C Service suisse d'étalonnage
S Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid NORMx,y,z sensitivity in free space

ConvF sensitivity in TSL / NORMx,y,z DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal A, B, C, D modulation dependent linearization parameters

Polarization φ φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center).

i.e., 9 = 0 is normal to probe axis.

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) JEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)". March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 8 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty Inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency not media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip
 (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ES3-3287_Oct15 Page 2 of 13

ES3DV3 - SN:3287

Probe ES3DV3

SN:3287

Manufactured: June 7, 2010

Repaired: October 26, 2015 Calibrated: October 29, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

ES3DV3-- \$N:3287

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) ²) ^A	0.90	1.02	1.03	± 10.1 %
DCP (mV) ⁸	107.9	102.8	106.2	

Modulation Calibration Parameters

uib	Communication System Name		A dB	B , dB√μV	С	D dB	VR mV	Unc [±] (k=2)
0	CW	X	0.0	0.0	1.0	0.00	174.4	±3.3 %
		Υ	0.0	0.0	1.0		182.0	
		Z	0.0	0.0	1.0		190.2	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	Х	0.95	51.7	5.1	10.00	43.9	±2.7 %
		Υ	3.69	64.5	12.4		37.8	
	-	Z	1 .91	60.6	10.6		37.4	
10011- CAB	UMTS-FDD (WCDMA)	Х	3.47	68.1	18.7	2.91	138.9	±0.7 %
		Υ	3.34	66.7	17.8		146.6	
		Z	3.09	66.1	17.9		111.1	
10012- CAB	IEEE 802.11b WiFl 2.4 GHz (DSSS, 1 Mbps)	X '	2.91	68.5	18.3	1,87	14 1 .3	±0.7 %
		Υ	2.89	67.5	17.4		147.4	
	<u> </u>	Z	2.68	67.5	18.0		112.6	
10013- CAB	JEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	X	10.96	70.7	23.2	9.46	134.1	±3.0 %
		Y	11.47	71.3	23.4		146.7	
10001	2011 505 (5011) 011010	Z	10.21	69.0	22.4		101.B	4 - 41
10021- DAB	GSM-FDD (TDMA, GMSK)	Х	7.66	60.9	20.7	9.39	135.4	±1.7 %
		Υ	17.65	94.3	26.1		149.8	
		Z	7.45	82.4	21.8		147.9	/
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	X	6.04	76.8	19.2	9.57	126.0	±1.9 %
		Y	12.07	87.2	23.6		140.2	
1		Z	9.85	87.1	23.5	0.00	141.5	7.00
10024- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	7.78	79.2	17.8	6.56	115.4	±1.7 %
		Y	25.36	94.3	23.2		133.5	
		Z	8.04	80.7	18.5		131.8	-1.4.05
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	Х	63.55	99.9	21.9	4.80	131.7	±1.4 %
	<u></u>	Y	64.01	99.9	22.5		103.3	
	ODDO EDD (TOLL) CHOIC THE A CO	Z	52.80	99.9	22.2		149.1	
10028- DAB	GPRS-FDD (TOMA, GMSK, TN 0-1-2-3)	Х	7.45	76.8	14.5	3.55	141,6	±1.4 %
		Y	52.62	99.8	22.3		109.9	
40020	(CEC DO2 45 4 Divolants (CECV, DU6)	Z	12.72	84.3	17.2	1 16	113.6 115.8	±1.4 %
10032- CAA	1EEE 802.15.1 Bluetooth (GFSK, DH5)	X	94.45	95.7	17.0	1.16		11.4 %
		Y	97.58	91.9	15.8		123.7 131.4	
10100	LTE EDD (00 EDMA 4000/ DD 30	Z	96.27	92.2	15.3	5.67		11 2 97
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.04	66.4	19.0	5.67	105.9	±1.2 %
	1	Y	6.03	65.9	18.6	<u> </u>	112.4	
		Z	6.15	66.9	19.4	1	12 1,2	I

ES3DV3- SN:3287 October 29, 2015

10103- CAB	LTE-TOD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	9.88	74.8	25.6	9.29	132.9	±2.7 %
		Υ	9.08	71.7	23.7		101.1	
		Z	8.43	71.3	24.0		103.5	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	Х	6.48	6 8.D	20.0	5.80	149.4	±1.2 %
		Υ	5.96	65.6	18.5		112.0	
		Z	6.01	66.5	19.3		120.0	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	Х	10.29	69.4	21.5	8.07	138.8	±1.9 %
		Y	9.51	67.1	20.1		100.8	
		Z !	9.72	68.1	20.8		108.8	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	9.12	74.0	25.4	9.28	129.0	±2,5 %
		Υ	10.12	75.5	25.8		146.3	
		Z	9.36	75.5	26.5		146,1	
10154- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	6.14	67.5	19.6	5.75	145.7	±1.2 %
		Υ	5.67	65.1	18.3		110.B	
		Z	5.74	66.2	19.1		117.5	
10160- CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	х	6.02	65.9	18.9	5.82	106.3	±1.2 %
		Υ	6.11	65.7	18.6		1 15.6	
		Z	6.13	66.5	19.2		122.5	
10169- CAB	LTE-FOD (SC-FDMA, 1 RB, 20 MHz, QPSK)	Х	4.92	67.2	19.8	5.73	125.8	±1.2 %
		Υ	4.98	66.5	19.2		135.6	
		Z	4.95	67.5	20,1		142.9	
10172- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	8.18	78.3	27.8	9.21	141.5	±1.9 %
		Υ	7.34	73.2	24.7		111.0	
		Z	6.97	74.4	26.1		113.2	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4,84	66.8	19.6	5.72	124.7	±1.2 %
		Y	4.96	66.5	19.2		133.9	
		Z	4.90	67.3	20.0		141.6	
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	×	4.91	67.1	19.8	5.72	125.6	±1.2 %
	<u> </u>	Y	4.93	66.3	19.0		133.1	
		Z	4.89	67.2	19.9	<u> </u>	141.6	
10196- CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	×	9.85	69.0	21.4	8.10	132.0	±2.2 %
		Y	10.13	69.3	21.4		146.4	
	<u> </u>	Z	9.32	67.8	20.8		103.6	
10225- CAB	UMTS-FDD (HSPA+)	X	6.63	66.2	18.9	5.97	112.6	±1.4 %
		Y	6.86	66.4	18.9		124.6	<u> </u>
		Z	6.77	66.9	19.4		129.8	
10237- CAB	LTE-TOD (SC-FDMA, 1 RB, 10 MHz, QPSK)	х	8.17	78.3	27.8	9.21	141.6	±1.9 %
		Y	7.56	74.1	25.2		114.4	
		Z	7.01	74.5	26.2		114.6	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	8.44	73.0	25.0	9.24	120.9	±2.7 %
		Y	9,42	74.6	25.4		138.7	
		Z	8.64	74.5	26.1		137.8	
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	×	9.13	74.0	25.4	9.30	128.7	±2.7 %
		Υ	10.25	75.8	26.0		148.8	
		Z	9.31	75.3	26.4		145.2	

ES3DV3-SN:3287 October 29, 2015

10275- САВ	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rei8.4)	х	4.56	67.6	19.0	3.96	140.5	±0.7 %
		Υ	4.11	64.9	17.4		107.6	
		Z	4.17	65.9	18.2		114.1	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.71	67.5	18.8	3.46	130.6	±0.7 %
		Υ	3.66	66.4	18.0		138.5	
		ž	3.68	67.6	18.9		147.9	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.68	67.7	18.9	3.39	132.6	±0.7 %
		Υ	3.54	66.0	17.7		142.3	
		Z	3.67	67.9	19. 1		149.2	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	Х	5.99	66.2	19.1	5.81	105.7	±1.2 %
		Υ	6.00	65.7	18.6		113.0	
		Z	6.00	66.4	19.2		120.3	
10311- AAA	LTE-FDD (\$C-FDMA, 100% RB, 15 MHz, QPSK)	Х	6.44	66.4	19.2	6.06	109.3	±1.2 %
		Υ	6.55	66.4	19.0		118.2	
		Z	6.62	67.2	19.7		125.0	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	х	10.23	69.6	21.9	8.37	135.7	±2.5 %
		Υ	10.44	69.6	21.8		149.1	
		Z	9.60	68.1	21.2		104.3	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	4.94	69.5	19.2	3,76	142.7	±0.5 %
		Υ	4.44	66.5	17.5		109.4	
		z	4.57	68.4	18.7		113.6	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	Х	4.97	69.9	19.4	3.77	140.3	±0.5 %
		Y	4.57	67.3	17.9		107.6	
		Z	4.62	69,2	19.2		113.0	
10415- AAA	IEEE 802.11b WiFl 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	Х	3.00	70.3	19.4	1.54	139.9	±0.5 %
		Y	2.56	66.7	17.1		147.2	
		Z	2.91	70.0	19.2		114.2	
10416- AAA	IEEE 802,11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	Х	10.01	69.2	21.6	8.23	134.8	±2.5 %
		Υ	10.23	69.4	21.5		146.8	
		Z	9.44	68.0	21.0		104.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: ES3-3287_Oct15

A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

B Numerical linearization parameter: uncertainty not required.

C Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Depth ^d (mm)	Unc (k=2)
750	41.9	0.89	6.72	6.72	6.72	0.19	2.32	± 12.0 %
835	41.5	0.90	6.57	6.57	6.57	0.15	2.57	± 12.0 %
1750	40.1	1.37	5.30	5.30	5.30	0.31	1.72	± 12,0 %
1900	40.0	1.40	5.08	5.08	5.08	0.50	1.29	± 12.0 %
2300	39.5	1.67	4.69	4.69	4.69	0.37	1.63	± 12,0 %
2450	39.2	1.80	4.38	4.38	4.38	0.65	1.26	± 12,0 %
2600	39.0	1.96	4.25	4.25	4.25	0.44	1.65	± 12.0 %

⁶ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

validity can be extended to \pm 110 MHz.

Fix All frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for Indicated target tissue parameters.

The ConvP uncertainty for Indicated target itssue parameters.

B Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

Calibration Parameter Determined in Body Tissue Simulating Media

			-		•			
f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Dapth ⁹ (mm)	Unc (k=2)
750	55.5	0.96	6.62	6.62	6.62	0.39	1.42	± 12.0 %
835	55.2	0.97	6.34	6.34	6.34	0.20	2.47	± 12.0 %
1750	53.4	1.49	4.96	4.96	4.96	0.35	1.65	± 12.0 %
1900	53.3	1.52	4,72	4.72	4.72	0.31	1.87	± 12.0 %
2300	52.9	1.81	4.38	4.38	4.38	0.49	1.49	± 12.0 %
2450	52.7	1.95	4.20	4.20	4.20	0.75	1.05	± 12.0 %
2600	52.5	2.16	4.00	4.00	4,00	0.68	1.06	± 12.0 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (a and a) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (a and b) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.


Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

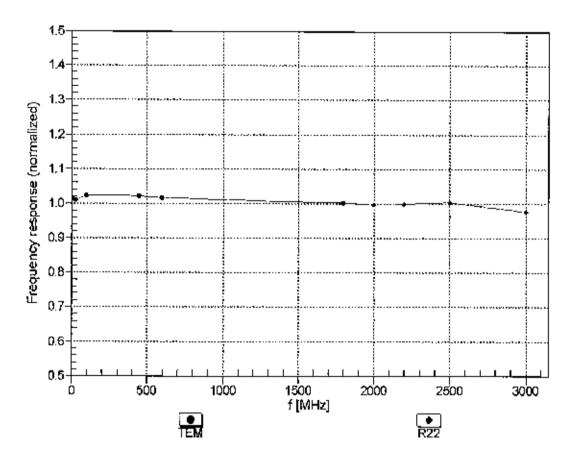

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

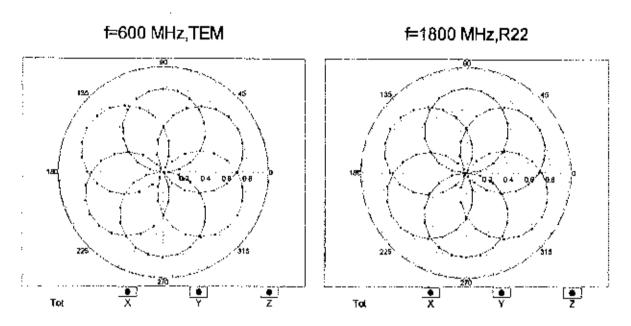


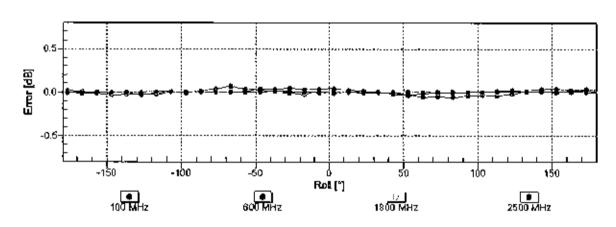

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k≈2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

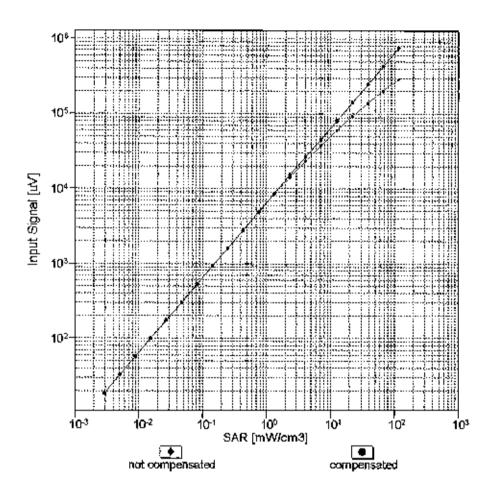

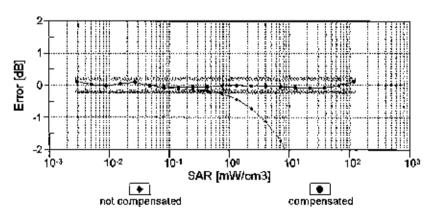


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

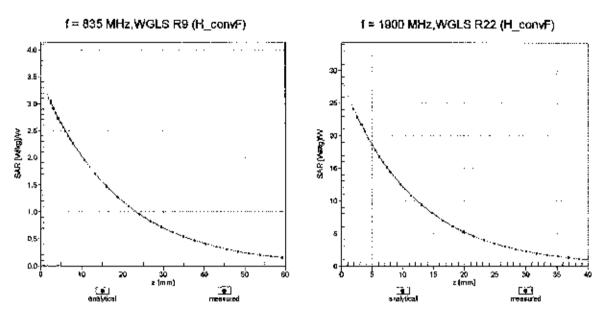

Deviation from Isotropy in Liquid

Error (ϕ , ϑ), f = 900 MHz

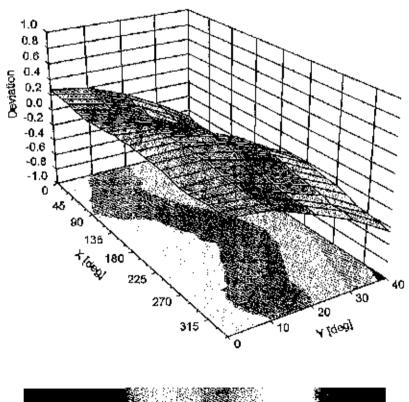

ES3DV3-- \$N:3287

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3287

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	83.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of Schmid & Partner

Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdienst Service suisse d'étalonnage C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS) The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: ES3-3319_Mar15

CALIBRATION CERTIFICATE

Object

ES3DV3 - SN:3319

Calibration procedure(s)

QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes

Calibration date:

March 19, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature $(22 \pm 3)^{\circ}$ C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID.	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN; S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Арг-15
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	, ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Function Name Laboratory Technician Israe Elnaouq Calibrated by: Technical Manager Katja Pokovic Approved by:

Page 1 of 13

Issued: March 19, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of

Certificate No: ES3-3319_Mar15

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z

DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ φ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., $\vartheta = 0$ is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

ES3DV3 - SN:3319 March 19, 2015

Probe ES3DV3

SN:3319

Manufactured: Calibrated:

January 10, 2012 March 19, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

March 19, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	1.12	1.08	1.15	± 10.1 %
DCP (mV) ^B	104.4	106.0	104.4	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	c	D dB	VR mV	Unc ^Ŀ (k=2)
0	CW	Х	0.0	0.0	1.0	0.00	176.1	±3.3 %
		Υ	0.0	0.0	1.0		192.7	
		Z	0.0	0.0	1.0		174.6	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	Х	3.26	64.8	13.4	10.00	41.7	±1.9 %
		Υ	2.66	62.2	11.7		39.5	
		Z	3.51	64.8	13.2		42.1	
10011- CAB	UMTS-FDD (WCDMA)	X	3.47	68.1	19.1	2.91	142.9	±0.5 %
		Υ	3.37	67.9	19.1		133.0	
		Z	3.57	68.7	19.4		138.6	. 0 7 0/
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	3.48	71.8	20.2	1.87	143.9	±0.7 %
		Υ	3.23	70.9	19.9		134.6	
		Z	3.68	72.8	20.6	0.10	140.5	.0.0.0/
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	X	11.18	70.5	23.1	9.46	143.4	±3.3 %
		Υ	10.98	70.5	23.2		129.9	
		Z	11.19	70.6	23.1		138.8	.4 7 0/
10021- DAB	GSM-FDD (TDMA, GMSK)	X	15.55	92.7	26.1	9.39	126.5	±1.7 %
		Υ	21.21	98.0	27.2		142.0	
		Z	19.50	96.1	27.0		125.4	.0.0.04
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	×	23.54	100.0	28.4	9.57	142.6	±2.2 %
		Y	23,24	99.9	28.0		137.4	
		Z	23.57	99.6	28.2	0.50	139.7	10.00
10024- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	×	17.00	90.2	22.7	6.56	128.9	±2.2 %
		Υ	35.20	99.7	24.9		148.2	
		Z	33.12	99.6	25.4		123.8	14.0.0/
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	44.20	99.6	23.6	4.80	146.0	±1.9 %
		Y	49.99	99.9	23.0		136.6	
		Z	41.43	99.6	23.9		141.4	10.000
10028- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	Х	46.56	99.7	22.7	3.55	127.7	±2.2 %
		Y	58.11	99.8	21.9			
		Z	55.65	99.6	22.2	1.40	124.3	14 7 9/
10032- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	34.25	99.4	21.1	1.16	140.3	±1.7 %
		Y	40.72	100.0	20.6		136.4	-
		Z	45.39	100.0	20.8	E 07		±4 / 0/
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	×	6.30	67.1	19.5	5.67	127.4	±1.4 %
		Υ	6.58	68.4	20.3		149.0	
	}	Z	6.55	68.0	19.9		146.3	1

10103-	LTE-TDD (SC-FDMA, 100% RB, 20	Х	10.47	75.6	25.8	9.29	146.6	±3.0 %
CAB	MHz, QPSK)	Υ	10.18	75.8	26.3		136.2	
		z	10.38	75.3	25.6		140.8	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	×	6.18	66.6	19.4	5.80	126.9	±1.4 %
ONO	WITE, GUOTY	Υ	6.40	67.8	20.1		147.0	
		Z	6.44	67.6	19.9		145.7	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	Х	10.24	69.0	21.3	8.07	142.7	±2.5 %
		Υ	10.25	69.2	21.5		136.7	
		Z	10.16	68.8	21.2		136.6	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	×	9.85	74.8	25.6	9.28	140.8	±3.0 %
		Υ	9.49	74.7	25.9		130.5	
		Z	9.90	74.8	25.6		136.8	14 4 0/
10154- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	6.13	67.1	19.7	5.75	146.6	±1.4 %
		Y	6.11	67.4	19.9		142.3	
		Z	6.12	67.1	19.7	5.82	128.9	±1.4 %
10160- CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.33	66.7	19.4	0.02	128.7	±1.4 /0
		Y	6.33	67.1	19.7		147.4	
10169-	LTE-FDD (SC-FDMA, 1 RB, 20 MHz,	Z X	6.57 4.89	67.6 66.4	19.9 19.5	5.73	127.5	±1.2 %
CAB	QPSK)	Y	4.99	67.5	20.2		149.3	
		Z	5.09	67.3	20.0		145.1	
10172- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	7.99	75.8	26.3	9.21	127.6	±2.7 %
		Y	9.29	81.7	29.6		149.8	
		Z	8.04	75.8	26.3		123.6	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	Х	5.08	67.3	20.0	5.72	149.3	±1.4 %
		Y	5.00	67.6	20.3		145.0	
		Z	5.09	67.3	20.0	<u> </u>	145.0	14.4.9/
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	5.08	67.3	20.0	5.72	148.5	±1.4 %
		Y	5.06	67.9	20.4	-	147.1 144.8	
		Z	5.11	67.4	20.0	0.40		+2.2.0/
10196- CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.89	68.7	21.2	8.10	134.6	±2.2 %
		Y	9.84	68.9	21.4		130.4	
10225-	UMTS-FDD (HSPA+)	Z X	9.82 7.02	68.5 67.1	21.1 19.5	5.97	138.0	±1.4 %
CAB		Y	6.88	67.0	19.5		133.2	
		Z	7.01	67.1	19.5		134.6	
10237- CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	8.01	75.9	26.4	9.21	128.0	±2.7 %
U, (D	¬, ¬, ¬	Y	9.39	82.1	29.9		149.7	
		Z	8.34	76.9	26.9		129.1	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	Х	9.05	73.6	25.1	9.24	130.6	±3.0 %
		Y	8.76	73.7	25.5		123.6	1
		Z	9.10	73.6	25.1		127.8	
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	Х	9.81	74.7	25.6	9.30	139.3	±3.0 %
		Υ	9.50	74.8	25.9		130.7	
		Z	9.81	74.6	25.5		135.0	

March 19, 2015 ES3DV3-SN:3319

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	Х	4.49	67.1	18.9	3.96	140.1	±0.7 %
<u> </u>		Υ	4.46	67.2	19.0		137.6	
		Z	4.52	67.1	18.9		137.1	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.68	67.0	18.8	3.46	129.3	±0.7 %
7010		Υ	3.64	67.3	19.0		130.3	
		Z	3.84	67.9	19.2		148.6	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.64	67.2	18.8	3.39	131.8	±0.5 %
7010		Υ	3.60	67.4	19.1		128.2	
		Z	3.71	67.5	19.0		128.0	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	6.43	67.5	19.9	5.81	147.2	±1.7 %
		Υ	6.39	67.7	20.0		145.4	
		Z	6.42	67.5	19.8		143.2	
10311- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	Х	6.73	67.1	19.7	6.06	129.7	±1.4 %
		Υ	6.75	67.5	19.9		130.8	
		Z	6.75	67.3	19.7		126.2	
10400- AAB	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	Х	10.14	68.9	21.5	8.37	136.7	±2.5 %
		Υ	10.23	69.5	22.0		136.5	
		Z	10.13	68.9	21.5		132.8	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	Х	4.97	69.2	19.3	3.76	143.5	±0.5 %
		Υ	4.87	69.3	19.4		141.0	
		Z	5.02	69.2	19.3		139.6	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	Х	4.91	69.3	19.4	3.77	139.8	±0.7 %
		Υ	4.67	68.9	19.1		138.9	
		Z	4.89	69.1	19.3		137.1	
10415- AAA	IEEE 802,11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.93	70.1	19.6	1.54	137.8	±0.7 %
		Y	2.84	69.8	19.6		138.2	
		Z	3.04	70.8	19.9		134.2	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	Х	9.94	68.7	21.3	8.23	134.6	±2.2 %
		Υ	10.00	69.1	21.7		134.1	
		Z	9.89	68.5	21.2		130.1	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

March 19, 2015

Certificate No: ES3-3319_Mar15

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	6.69	6.69	6.69	0.40	1.70	± 12.0 %
835	41.5	0.90	6.41	6.41	6.41	0.43	1.62	± 12.0 %
1750	40.1	1.37	5.29	5.29	5.29	0.80	1.16	± 12.0 %
1900	40.0	1.40	5.10	5.10	5.10	0.80	1.24	± 12.0 %
2300	39.5	1.67	4.77	4.77	4.77	0.64	1.38	± 12.0 %
2450	39.2	1.80	4.55	4.55	4.55	0.80	1.29	± 12.0 %
2600	39.0	1.96	4.39	4.39	4.39	0.80	1.31	± 12.0 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

validity can be extended to \pm 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

March 19, 2015

Certificate No: ES3-3319_Mar15

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	55.5	0.96	6.10	6.10	6.10	0.34	1.80	± 12.0 %
835	55.2	0.97	6.07	6.07	6.07	0.47	1.56	± 12.0 %
1750	53.4	1.49	4.83	4.83	4.83	0.70	1.36	± 12.0 %
1900	53.3	1.52	4.53	4.53	4.53	0.71	1.39	± 12.0 %
2300	52.9	1.81	4.24	4.24	4.24	0.80	1.26	± 12.0 %
2450	52.7	1.95	4.11	4.11	4.11	0.80	1.10	± 12.0 %
2600	52.5	2.16	3.90	3.90	3.90	0.80	1.11	± 12.0 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

validity can be extended to ± 110 MHz.


F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

S Alpha/Depth are determined during colliberation.

⁶ Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Certificate No: ES3-3319_Mar15


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

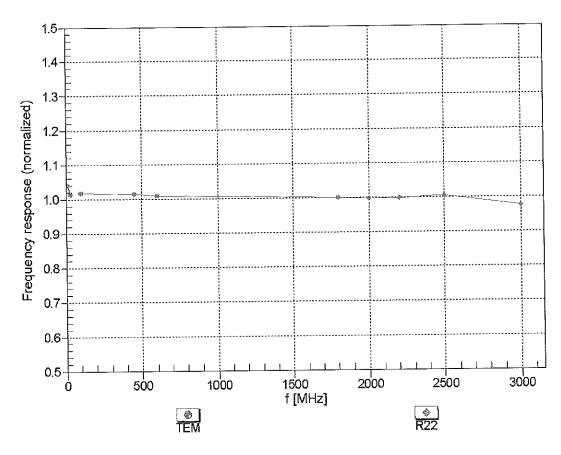


Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Tot

Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$




f=1800 MHz,R22




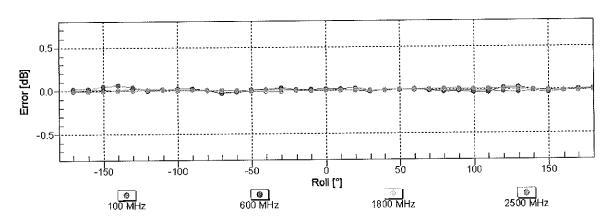

Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

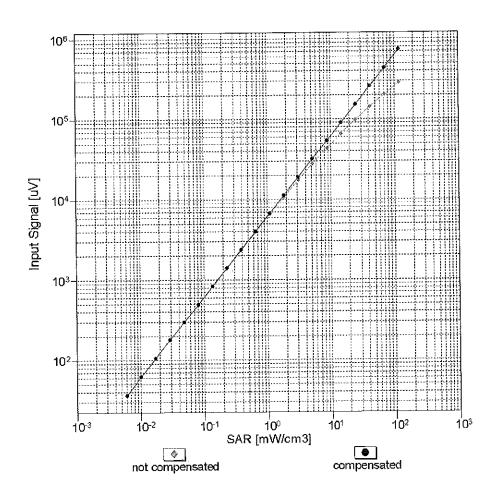


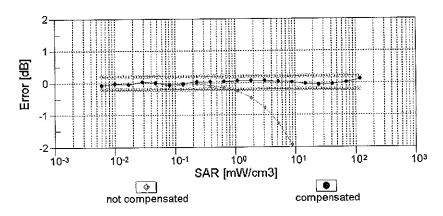


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


ES3DV3-- SN:3319 March 19, 2015

Conversion Factor Assessment

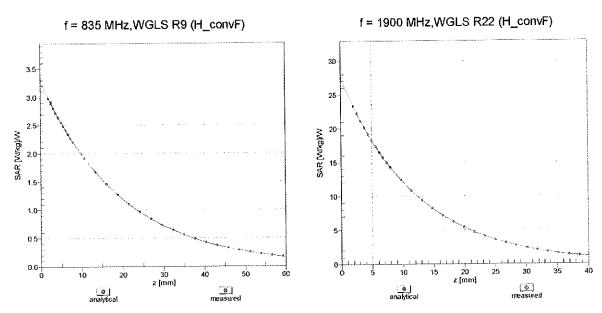

Deviation from Isotropy in Liquid Error (φ, θ), f = 900 MHz

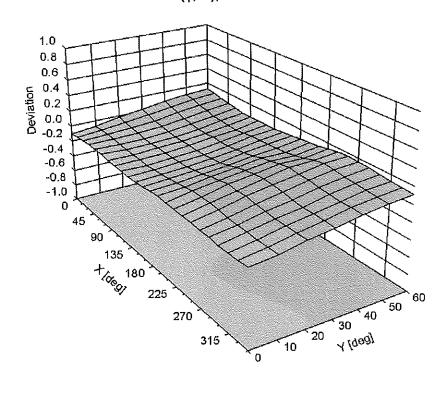



March 19, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3319

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-120.2
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst Service suisse d'étalonnage Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Certificate No: ES3-3263_May15

CALIBRATION CERTIFICATE

Object

ES3DV3 - SN:3263

Calibration procedure(s)

QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes

Calibration date:

May 20, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Name Function Signature

Leif Klysner Laboratory Technician Signature

Approved by: Katja Pokovic Technical Manager

Issued: May 19, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3263_May15

Page 1 of 13

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z

tissue simulating liquid sensitivity in free space

ConvF DCP sensitivity in TSL / NORMx,y,z diode compression point

CF A, B, C, D crest factor (1/duty_cycle) of the RF signal modulation dependent linearization parameters

Polarization ω

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., $\vartheta = 0$ is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- Techniques", June 2013
 b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization θ = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is
 implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included
 in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ES3-3263_May15

ES3DV3 - SN:3263 May 20, 2015

Probe ES3DV3

SN:3263

Manufactured: January 25, 2010 Calibrated: May 20, 2015

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

Certificate No: ES3-3263_May15

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	1.21	1.25	1.13	± 10.1 %
DCP (mV) ^B	106.1	103.6	108.3	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc ^E (k=2)
0	CW	Х	0.0	0.0	1.0	0.00	205.3	±3.3 %
		Y	0.0	0.0	1.0		207.3	
		Z	0.0	0.0	1.0		199.5	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	Х	1.83	58.4	9.4	10.00	41.2	±1.4 %
		Υ	3.88	63.3	12.9		47.5	
		Z	1.42	56.8	8.7		39.5	
10011- CAB	UMTS-FDD (WCDMA)	X	3.27	67.4	18.6	2.91	140.1	±0.7 %
		Y	3.39	67.5	18.7		142.7	
40040	ISSE 000 4	Z	3.32	67.6	18.6		136.9	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	2.85	68.8	18.8	1.87	142.2	±0.7 %
		Y	3.38	70.7	19.5		144.8	
10013-		Z	3.07	70.0	19.1		138.1	
CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	×	10.99	70.8	23.4	9.46	135.9	±2.5 %
		Υ	11.36	70.3	22.8		124.7	
10021-	COM EDD (TDMA, CMC)	Z	10.57	70.0	22.9		129.4	
DAB	GSM-FDD (TDMA, GMSK)	X	9.38	84.7	22.1	9.39	139.8	±1.9 %
		Y	27.79	100.0	28.7		129.4	
10023-	GPRS-FDD (TDMA, GMSK, TN 0)	Z	9.29	86.8	23.8		134.5	
DAB	GPKS-FDD (TDIVIA, GWSK, TN U)	X	9.63	84.9	22.1	9.57	134.1	±2.5 %
		Y	25.29	98.2	28.2		124.0	
10024-	CDDC EDD (TDMA CMOK TN 0.4)	Z	9.65	87.7	24.3		128.2	
DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	16.20	88.9	21.0	6.56	145.2	±1.4 %
		Y	41.82	99.7	25.6		128.5	
10027-	CDDC EDD (TDMA CMOK TNO 4 0)	Z	24.57	96.8	24.1		142.0	
DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	55.77	99.6	22.1	4.80	138.5	±2.2 %
		Y	53.39	99.7	23.9		140.5	
10028-	CDDC CDD (TDMA CMOV TN 0 4 0 0)	Z	40.28	99.6	23.2		134.3	
DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	81.43	99.8	20.7	3.55	148.6	±1.7 %
		Y	60.49	99.7	22.9		146.0	
10032-	JEEE 802 15 1 Physicath (OCO), DUIC	Z	62.69	99.6	21.2		145.0	
CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	96.06	93.7	16.0	1.16	140.3	±1.9 %
		Y	77.08	99.9	20.1		149.0	
10100-	LITE EDD (SC EDMA 4000/ DD 00	Z	99.64	99.9	18.6		138.0	
CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.24	67.2	19.6	5.67	131.7	±1.4 %
		Y	6.39	67.3	19.5		133.8	
	- TOTAL TOTA	Z	6.19	67.2	19.6		126.8	

10103- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	10.13	76.3	26.6	9.29	142.6	±2.7 %
0.15	William Service	Y	12.07	77.9	26.6		138.9	
		Z	9.41	74.3	25.6		134.1	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.13	66.9	19.5	5.80	129.6	±1.4 %
		Υ	6.35	67.1	19.5		133.7	
		Z	6.39	68.0	20.1		150.0	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	Х	10.34	69.6	21.7	8.07	147.0	±1.9 %
		Υ	10.05	68.3	20.9		123.4	
		Z	10.08	69.1	21.3	1000	138.2	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	9.44	75.3	26.3	9.28	137.0	±3.5 %
······································		Y	11.36	76.9	26.3		134.5	
40454	LTE EDD (OO ED) (A TOO)	<u> </u>	8.85	73.5	25.3		130.3	
10154- CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.79	66.2	19.2	5.75	126.9	±1.2 %
		Y	6.05	66.5	19.3		130.9	
10160-	LTE EDD (CO EDMA CON DD 4515)	Z	5.92	66.9	19.5		145.5	
CAB	LTE-FDD (SC-FDMA, 50% RB, 15 MHz, QPSK)	X	6.25	66.9	19.5	5.82	131.8	±1.4 %
		Y	6.47	67.0	19.5		135.4	
10169-	LTE FOR /OO FOMA A DR COMMI	Z	6.09	66.5	19.3		127.5	
CAB	LTE-FDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.78	66.7	19.7	5.73	130.0	±1.2 %
		Y	5.14	66.7	19.5		135.0	
10172-	LTE-TDD (SC-FDMA, 1 RB, 20 MHz,	Z	4.83	67.1	19.9		147.9	
CAB	QPSK)	X	8.63	80.4	29.1	9.21	147.7	±2.7 %
		Υ	9.72	78.5	27.2		123.9	
10175-	LTE-FDD (SC-FDMA, 1 RB, 10 MHz,	Z	7.63	76.7	27.2		142.5	
CAC	QPSK)	X	4.75	66.6	19.6	5.72	128.2	±1.2 %
		Y 7	5.12	66.6	19.5		134.3	
10181-	LTE-FDD (SC-FDMA, 1 RB, 15 MHz,	Z X	4.87	67.1	19.9	F 70	148.0	14.00/
CAB	QPSK)	Y	4.76	66.6	19.6	5.72	127.9	±1.2 %
		Y Z	5.12	66.6	19.5		134.5	
10196-	IEEE 802.11n (HT Mixed, 6.5 Mbps,	X	4.87	67.3	20.0	0.10	147.0	.000
CAB	BPSK)	^ ^	9.87	69.1	21.6	8.10	135.8	±2.2 %
		Z	10.19 9.65	69.1	21.4		145.3	
10225-	UMTS-FDD (HSPA+)	X		68.8	21.3	F 07	130.5	14 7 0/
CAB	Children (1017)	ļ	6.90	67.2	19.5	5.97	139.2	±1.7 %
		Y 7	7.22	67.3	19.6		148.0	
10237-	LTE-TDD (SC-FDMA, 1 RB, 10 MHz,	Z X	6.75	67.0	19.4	0.01	134.1	
CAB	QPSK)		8.68	80.6	29.2	9.21	148.0	±3.0 %
		Y	9.82	78.8	27.3		125.0	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	7.85 8.56	77.6 73.7	27.7 25.6	9.24	143.5 126.6	±3.5 %
		Υ	10.58	76.0	25.9		126.3	
		z	8.84	74.8	26.1		146.7	
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	9.24	74.6	25.9	9.30	133.6	±3.3 %
		Y	11.38	76.9	26.2		134.3	
	No.	Z	8.79	73.2	25.1		128.6	

ES3DV3-SN:3263 May 20, 2015

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	Х	4.39	67.0	18.9	3.96	143.8	±0.9 %
		Y	4.55	67.1	18.8		147.3	
		Z	4.42	67.4	19.0		139.9	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.59	67.2	18.9	3.46	132.2	±0.5 %
		Υ	3.68	66.7	18.5		136.0	<u> </u>
		Z	3.57	67.1	18.6		128.5	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.50	67.0	18.7	3.39	134.0	±0.7 %
		Y	3.62	66.6	18.4		138.6	
		Z	3.50	67.2	18.7		129.8	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	Х	6.11	66.8	19.4	5.81	127.7	±1.4 %
		Υ	6.33	67.0	19.5		132.1	
		Z	6.28	67.6	19.9		146.6	
10311- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	Х	6.71	67.5	19.9	6.06	134.2	±1.7 %
		Y	6.93	67.7	19.9		138.0	
-1/81001		Z	6.57	67.2	19.6	188011	128.0	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	10.17	69.5	21.9	8.37	138.5	±2.5 %
		Υ	10.55	69.5	21.8		148.0	
		Z	9.92	69.0	21.6		132.5	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	X	4.79	69.2	19.1	3.76	144.1	±0.7 %
		Υ	4.71	67.0	18.2		129.2	
····		Z	4.72	69.3	19.2		139.3	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	X	4.69	69.2	19.2	3.77	142.1	±0.7 %
***************************************		Υ	4.71	67.5	18.5		126.7	
		Z	4.51	68.6	18.8		137.3	
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.55	68.0	18.5	1.54	141.7	±0.7 %
		Υ	2.67	68.4	18.6		144.0	
		Z	2.98	70.8	19.5		138.0	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	X	10.01	69.3	21.8	8.23	137.3	±2.5 %
		Υ	10.31	69.3	21.6		146.0	
		Z	9.69	68.8	21.4		129.9	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

B Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	6.27	6.27	6.27	0.29	1.87	± 12.0 %
835	41.5	0.90	6.18	6.18	6.18	0.49	1.42	± 12.0 %
1750	40.1	1.37	5.27	5.27	5.27	0.49	1.46	± 12.0 %
1900	40.0	1.40	4.96	4.96	4.96	0.66	1.28	± 12.0 %
2300	39.5	1.67	4.63	4.63	4.63	0.58	1.41	± 12.0 %
2450	39.2	1.80	4.40	4.40	4.40	0.71	1.34	± 12.0 %
2600	39.0	1.96	4.25	4.25	4.25	0.80	1.25	± 12.0 %

^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	55.5	0.96	6.07	6.07	6.07	0.53	1.42	± 12.0 %
835	55.2	0.97	6.08	6.08	6.08	0.57	1.36	± 12.0 %
1750	53.4	1.49	4.88	4.88	4.88	0.54	1.50	± 12.0 %
1900	53.3	1.52	4.66	4.66	4.66	0.56	1.51	± 12.0 %
2300	52.9	1.81	4.42	4.42	4.42	0.69	1.33	± 12.0 %
2450	52.7	1.95	4.28	4.28	4.28	0.80	1.08	± 12.0 %
2600	52.5	2.16	4.11	4.11	4.11	0.80	1.09	± 12.0 %


^C Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is


always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

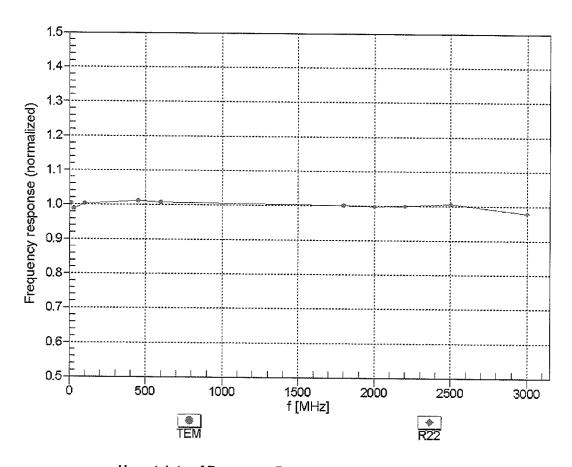

Uncertainty of Frequency Response of E-field: \pm 6.3% (k=2)


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

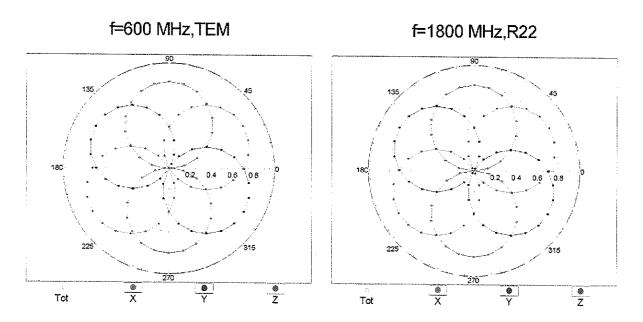


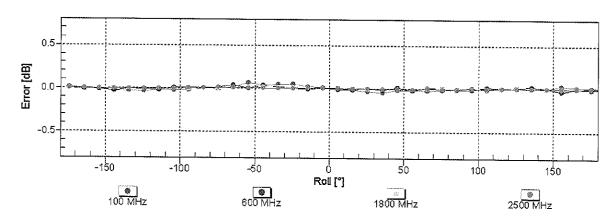

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

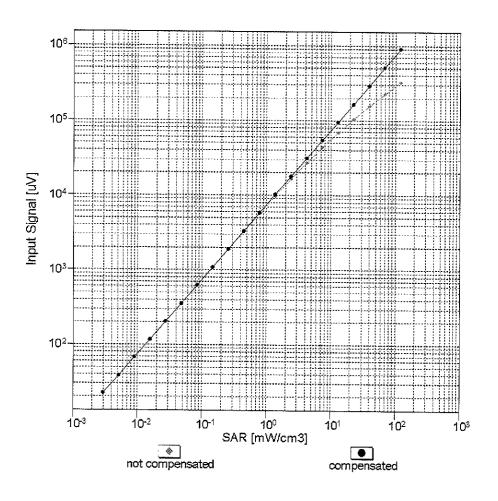

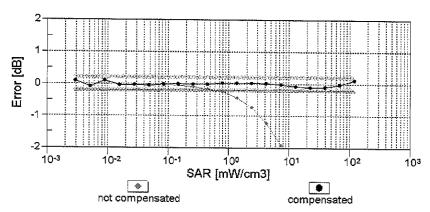


Uncertainty of Linearity Assessment: ± 0.6% (k=2)


Conversion Factor Assessment

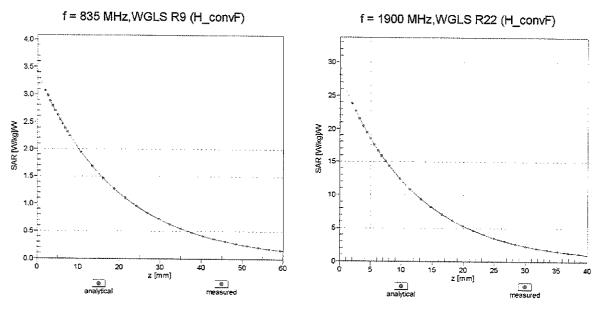

Deviation from Isotropy in Liquid

Error (ϕ, ϑ) , f = 900 MHz

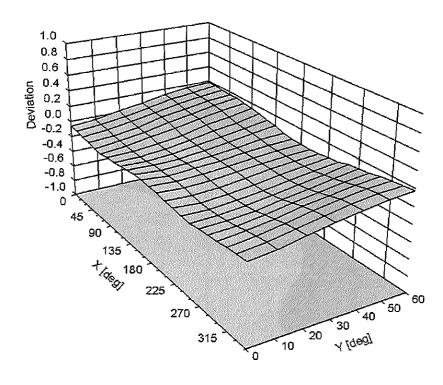



DASY/EASY - Parameters of Probe: ES3DV3 - SN:3263

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	65.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





Schwelzerischer Kalibrierdienst Service sulsse d'étalonnage Servizio svizzero di taretura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multitaleral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

PC Test

Certificate No: ES3-3333_Oct15

~ 4	1001	CI/NRE	CEDT		ATC
IVAL	IBKAI		CERT	ITIQ/	4 I C

Object (ES3DV3 - SN:3333

Calibration procedure(s) QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6

Calibration procedure for dosimetric E-field probes

Calibration date: October 29, 2015

This calibration cartificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 \pm 3)°C and humidity < 70%.

Catibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mer-16
Reference 20 dB Altenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
DAE4	SN: 660	14-Jan-15 (No. DAE4-680_Jan15)	Jan-16
Secondary Standards	1D	Check Dale (in house)	Scheduled Check
RF generator HP 8648C	US3842D01700	4-Aug-99 (In house check Apr-13)	In house check: Apr-16
Natwork Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-15)	In house check: Oct-16

Calibrated by:	Name Lelf Kly sner	Function Laboratory Technicish	Signature Sef They
Approved by:	Katja Pokovic	Technical Manager	R.M.

Issued: October 29, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3333_Oci15 Page 1 of 13

Calibration Laboratory of

Schmid & Partner

Engineering AG

Zeughausstrasse 43, 8004 Zurich, Switzerland





Schweizerischer Kalibrierdtenst S Service suisse d'étalonname C Servizio svizzero di taratura S Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossarv:

tissue simulating liquid T\$L NORMx,y,z sensitivity in free space sensitivity in TSL / NORMx,y,z. ConvF

diode compression point DCP

crest factor (1/duty_cycle) of the RF signal CF modulation dependent linearization parameters A. B. C. D.

φ rotation around probe axis Polarization φ

8 rotation around an axis that is in the plane normal to probe axis (at measurement center), Polarization 9

i.e., $\vartheta = 0$ is normal to probe axis

information used in DASY system to align probe sensor X to the robot coordinate system Connector Angle

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques*, June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- $NORMx_{r}y_{r}z_{r}^{2}$ Assessed for E-field polarization 9 = 0 (f \leq 900 MHz in TEM-cell; f > 1800 MHz; R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E2-field uncertainty inside TSL (see below ConvF).
- $NORM(I)x,y,z = NORMx,y,z * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- $Ax_{x}y_{x}z_{x}^{*}Bx_{x}y_{x}z_{z}^{*}Cx_{x}y_{x}z_{z}^{*}Dx_{x}y_{x}z_{z}^{*}VRx_{x}y_{x}z_{z}^{*}A$, $B_{x}C_{x}D$ are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from \pm 50 MHz to \pm 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset. The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMX (no uncertainty required).

Certificate No: ES3-3333_Oct15 Page 2 of 13 ES3DV3 - SN:3333 October 29, 2015

Probe ES3DV3

SN:3333

Manufactured:

January 24, 2012

Calibrated:

October 29, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3333

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (µV/(V/m)²) ^A	1.07	0.90	0.88	± 10.1 %
DCP (mV) ^B	106.8	108.5	106,8	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc ^E (k=2)
0	cw	×	0.0	0.0	1.0	0.00	201.0	±3.5 %
	<u> </u>	Y	0.D	0.0	1.0		187.1	
		Z	0.0	0.0	1.0	_	184.8	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	х	2.43	60.7	11.4	10.00	41.6	±2.2 %
_		Υ	4.35	67.4	13.2		35.6	
		Z	1.46	57.0	8.7		36.2	
10011- CAB	UMTS-FDD (WCDMA)	х	3.35	67.9	19.1	2.91	138.2	±0.5 %
		Υ	3.48	68.6	19.2		127.5	_
		Z	3.37	67.6	18.6		149.0	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	×	3.60	72.8	20.8	1.87	141.0	±0.7 %
		Y	3.68	73.3	20.8		128.0	
100:0		Z	3.01	69.3	18.8		128.2	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	×	11.52	71.7	23.9	9.46	139.3	±3.0 %
		Y	10.94	70.4	22.9		147.1	
40004		Z	10.95	70.8	23.4		144.5	
10021- DAB	GSM-FDD (TDMA, GMSK)	Х	21.45	95.2	26.5	9.39	139,9	±2.5 %
	<u> </u>	Υ	9.12	82.9	21,9		142.0	
10000		Z	11.47	88.1	23.9		127.6	
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	Х	20.81	95.6	27.0	9.57	135,8	±2.2 %
		Υ	9.78	84.4	22.7		135.3	
40024	CDDQ EDD (TOLU - OLION TV - C)	Z	9.12	83.5	22.1		144.6	
10024- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	39.84	99.6	25.2	6.56	140.9	±1.9 %
		Υ	35.07	100.0	25.0		128.4	
40000		Z	35.20	99.8	24.7		131.9	
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	х	47.16	99.8	23.9	4.80	124.9	±2.5 %
		Υ	49.75	99.6	22.8		145.4	
		Z	45.37	99.9	23.1		148.5	
10028- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	×	56.24	99.6	22.6	3.55	140.4	±2.7 %
	· ·	ĮΥ	56.95	99.7	21.9		129.1	
40000	IEEE 000 45 4 Object of 45500 Exist	Z	48.45	99.6	22.1		133.2	
10032- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	18.03	99.1	22.8	1.16	127.5	±1.9 %
	 	Y	35.17	99.6	20.7		141.1	
40400	LITE FOR (FO FOM) 400% FO 00	Z	21.08	99.9	21.9		127.5	
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.36	67.6	19.8	5.67	137.5	±1.2 %
		Υ	6.29	67.4	19.6		129.9	
	<u> </u>	Z	6.35	67.5	19.7	l	139.5	

10103- CAB	LTE-TOD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	10.85	76.6	26.4	9.29	130.6	±2.7 %
		Υ	9.58	73.7	24.8		143.0	·
		Z	9.94	75.6	26.2	_	149.3	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	Х	6.21	67.0	19.7	5.80	126.9	±1.2 %
	<u> </u>	Υ	6.16	66.9	19.5		129.2	
		Z	6.22	67.2	19.7		138.0	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	Х	10.05	68.7	21.2	8.07	126.1	±2.5 %
	<u> </u>	ΙY	10.13	69.0	21.3		146.1	
40484	LTE TOP (DO EDITA MAN DE CONTRE	Z	9.97	68.7	21,1		126.2	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	10.11	75.5	26.0	9.28	125.8	±3.3 %
		Y	9.08	73.2	24.7	<u> </u>	138.2	
10154-	LTE-FDD (SC-FDMA, 50% RB, 10 MHz,	Z	9.32	74.8	26.0	5.35	143.1	14 O B/
CAC	QPSK)	X	5.97	66.8	19.6	5.75	133.4	±1.2 %
	-	Y	5.92	66.7	19.5	-	127.0	
10160-	LTE-FDD (SC-FDMA, 50% RB, 15 MHz,	Z X	5.91	66.7	19.5	5.82	134.2 137.8	±1.2 %
ÇAB	QPSK)		6.40	67.3	19.9	0.62	137.8	±1.2 %
	 	Y	6.31	67.1	19.6		139.8	
10169-	LTE-FDD (SC-FDMA, 1 RB, 20 MHz,	Z	6.32	67.1	19.6	5 72		14.0.07
CAB	QPSK)	Х.	5.05	67.3	20.1	5.73	136.8 131.1	±1.2 %
	·	Z	4.89 4.93	67.0	19.9		137.4	
10172-	LTE-TOD (\$C-FDMA, 1 RB, 20 MHz,	X	10.74	67.2	20.0	9.21	136.8	±2.7 %
CAB	QPSK)	Y	7.34	83.9 74.3	30,3 25,5	9.21	125.9	12.7 70
		Z	7.74	76.6	27.1		131.2	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.97	66.9	19.9	5.72	130.8	±1.2 %
		Υ	4.66	66.9	19.8		128.5	
		Z	4.97	67.3	20.1		137.0	
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	×	4.99	67.0	19.9	5.72	130.1	±1.2 %
		Υ	4.88	67.0	19.9		127.6	
		Z	4.95	67.2	20.0		136,2	
10196- CAB	JEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	Х	10.00	69.2	21.7	8.10	137.9	±2.2 %
		Υ '	9.75	68.7	21.2		137.5	
		Z	9.94	69.4	21.7		145.3	
10225- CAB	UMTS-FDD (H\$PA+)	х	7.08	67.5	19.8	5.97	147,1	±1.4 %
		Y	7.06	67.7	19.8		142.3	
1000	LEG TOP (OR SOLUTION	Z	7.04	67.7	19.9		148.8	
10237- CAB	LTE-TDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X.	10.66	83.5	30.1	9.21	144.0	±3.0 %
		Y	7.43	74.7	25.7		127.6	
10060	LYE TOO ICC COMA SOU DO AGAIL	Z	7.86	77.1	27.4	0.04	132,3	10.00
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X .	10.81	78.7	27.9	9.24	139.7	±3.0 %
	+	Y	8.48	72.4	24.4		130.1	
10267	LTG TDD (QC-EDMA 4000 DD 40	Z	8.71	74.1	25.8	B 75	135.2	+2.0.04
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	11,73	79,9	28.3	9.30	148.6	±3.3 %
	+	Y	9.11	73.2	24.8		139.0	
		Z	9.38	74.9	26.1		142.7	

ES3DV3-- SN:3333 October 29, 2015

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Ref8.4)	X	4.52	67.6	19.3	3.96	144.5	±0.7 %
		Y	4.67	68.3	19.6		146.0	
		Z	4.41	67.0	18.9		130.0	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.66	67.2	19.0	3.46	134.5	±0.5 %
		Υ	3.91	68.9	19.9		133.2	
		Z	3.86	66.5	19.6		146.9	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.63	67.5	19.1	3.39	134.9	±0.5 %
		Υ	3.93	69.3	20.0		136.0	
		Z	3.81	68.5	19.6		148.6	
10297- AAA	LTE-FDD (SC-FDMA, 50% R8, 20 MHz, QPSK)	Х	6.20	67.1	19.7	5.81	129.0	±1.2 %
		Υ	6.20	67.0	19.6		128.0	
		Z	6.32	67.5	19.9		142.7	
10311- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	Х	6.76	67.6	20.0	6.08	134.7	±1.4 %
		Y	6.75	67.5	19.9		133.5	
		Z	6.90	68.1	20.3		149.2	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	Х	10.30	69.7	22.1	8.37	140.1	±2.5 %
		Υ	10.05	69.0	21.5		141.2	
	<u> </u>	Z	9.94	69.0	2 1.7		126.3	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	Х	4.80	68.5	19.0	3.76	129.3	±0.5 %
		Υ	5.30	71.1	20.2		148,4	
		Z	5,10	70.4	19.9		135.2	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	X :	4.77	68.8	19.2	3.77	127.3	±0.7 %
		Y	5.35	71.7	20.5		145.4	
		Z	5.03	70.6	20.1		133.3	
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	×	2.77	69.7	19.7	1.54	147 .D	±0.7 %
		Υ	3.73	75.4	22.2		143.7	
		Z	3.25	72.2	20.7		133.9	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	X_	10.11	69.4	21.8	8.23	144.7	±2.5 %
		Υ	9.86	8.86	21.4		139.3	
	-	Z	9.72	66.6	21.3		126.0	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of Norm X,Y,Z do not affect the E2-liefd uncertainty inside TSL (see Pages 7 and 8).

Numerical linearization parameter: uncertainty not required.
 Uncertainty is determined using the max, deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3333 October 29, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3333

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Depth ⁶ (mm)	Unc (k=2)
750	41.9	0.89	6.46	6.46	6.46	0.75	1.22	± 12.0 %
835	41.5	0.90	6.16	6.16	6,16	0.36	1.67	± 12.0 %
1750	40.1	1.37	5.21	5.21	5.21	0.80	1.19	± 12.0 <u>%</u>
1900	40.0	1.40	5.03	5.03	5.03_	0.73	1.25	± 12.0 %
2300	39.5	1.67	4.73	4.73	4.73	0.60	1.43	± 12.0 %
2450	39.2	1.80	4.53	4.53	4.53	08.0	1.28	± 12.0 %
2600	39.0	1.96	4.39	4.39	4.39	0.80	1.29	± 12.0 %

⁶ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

Certificate No: ES3-3333_Oct15 Page 7 of 13

validity can be extended to ± 110 MHz.

Fixed At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvE uncertainty for indicated larget tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Apha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- \$N:3333 October 29, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3333

Calibration Parameter Determined in Body Tissue Simulating Media

			-		-			
f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^f	ConvF X	ConvF Y	ConvF Z	Alpha ⁶	Depth ⁶ (mm)	Unc (k=2)
750	65.5	0.96	6,31	6.31	6.31	0.70	1.26	± 12.0 %
835	55.2	0.97	6.25	6.25	6.25	0.47	1.54	±12.0 %
1750	53.4	1,49	4.90	4.90	4.90	0.49	1.63	± 12.0 %
1900	53.3	1.52	4.70	4.70	4.70	0.54	1.49	± 12.0 %
2300	52.9	1.81	4.51	4.51	4.51	08.0	1.15	± 12.0 %
2450	52.7	1.95	4.34	4.34	4.34	0.80	1.15	± 12.0 %
2600	52.5	2.16	4.23	4.23	4.23	0.80	1.03	± 12.0 %

⁶ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is \pm 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to \pm 110 MHz.

Certificate No: ES3-3333_Oct15 Page 8 of 13


validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (s and o) can be released to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (s and o) is restricted to ± 5%. The uncertainty is the RSS of the Copy Exprediciply for indicated terral tissue parameters.

the ConvF uncertainty for indicated larget tissue parameters that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


ES3DV3-SN:3333 October 29, 2015


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

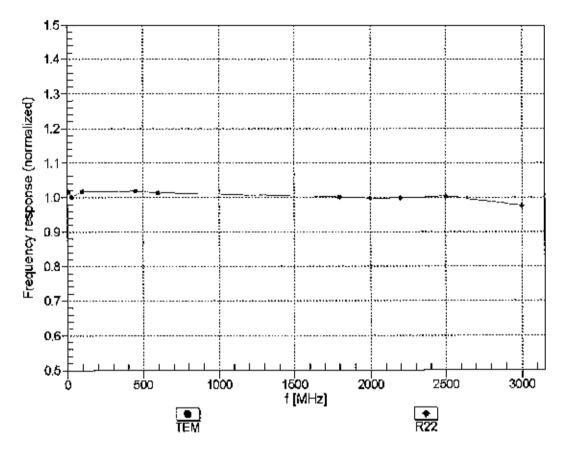

Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

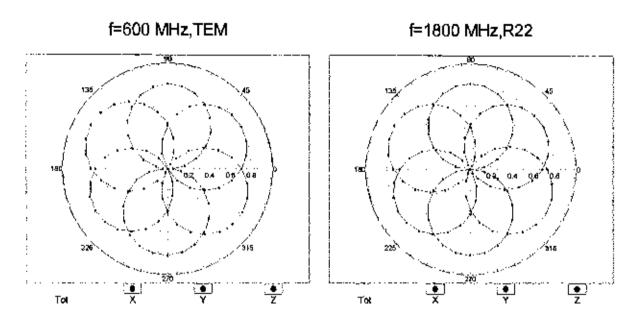


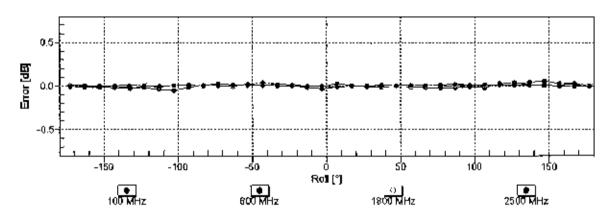

Uncertainty of Axial (sotropy Assessment: ± 0.5% (k=2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

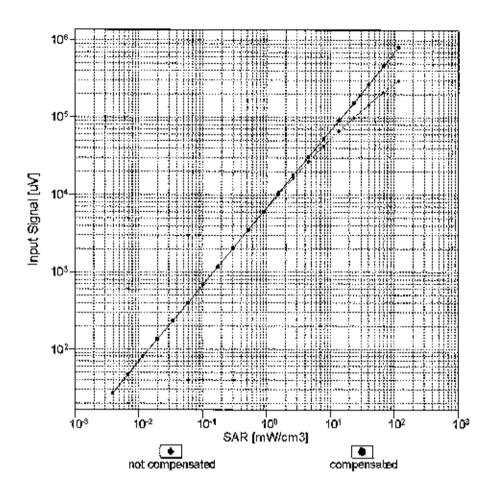

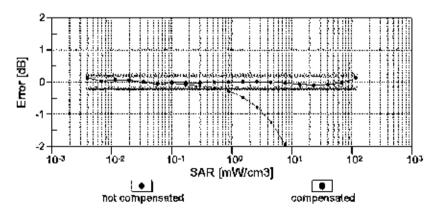


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

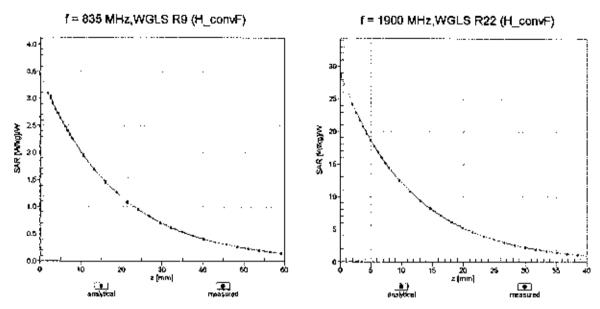

Deviation from Isotropy in Liquid

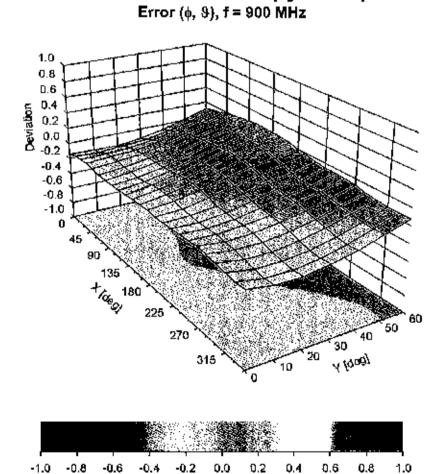

Uncertainty of Spherical Isotropy Assessment: ± 2.6% (k=2)

ES3DV3- SN:3333 October 29, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3333

Other Probe Parameters

Triangular
-32.8
enabled
disabled
337 mm
10 mm
10 mm
4 mm
2 mm
2 mm
2 mm
3 mm

Calibration Laboratory of Schmid & Partner

Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

BN 15/15

Client

PC Test

Certificate No: ES3-3351_Jun15

I	A A L	IDDATI	RTIFICA	TE
ı	LAL	IBRAIII	RIIILA	k I E

Object

ES3DV3 - SN:3351

Calibration procedure(s)

QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6
Calibration procedure for dosimetric E-field probes

Calibration date:

June 22, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Mar-16
Power sensor E4412A	MY41498087	01-Apr-15 (No. 217-02128)	Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02132)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02133)	Mar-16
Reference Probe ES3DV2	SN: 3013	30-Dec-14 (No. ES3-3013_Dec14)	Dec-15 (
DAE4	SN: 660	14-Jan-15 (No. DAE4-660_Jan15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Oct-15

Name Function Signature

Calibrated by: Leif Klysner Laboratory Technician

Approved by: Katja Pokovic Technical Manager

Issued: June 22, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura

Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid
NORMx,y,z sensitivity in free space
ConvF sensitivity in TSL / NORMx,y,z
DCP diode compression point

CF crest factor (1/duty_cycle) of the RF signal modulation dependent linearization parameters

Polarization φ σ rotation around probe axis

Polarization 9 9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., $\vartheta = 0$ is normal to probe axis

Connector Angle information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

 a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORMx,y,z: Assessed for E-field polarization 9 = 0 (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide).
 NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)x,y,z = NORMx,y,z * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Page 2 of 13

June 22, 2015 ES3DV3 - SN:3351

Probe ES3DV3

SN:3351

Manufactured: May 22, 2012

June 22, 2015 Calibrated:

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

E\$3DV3- \$N:3351 June 22, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3351

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm $(\mu V/(V/m)^2)^A$	0.99	1.17	1.19	± 10.1 %
DCP (mV) ^B	113.6	105.2	104.5	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB√μV	С	D dB	VR mV	Unc [±] (k=2)
0	CW	х	0.0	0.0	1.0	0.00	188.8	±3.8 %
		Υ	0.0	0.0	1.0		196.2	
		Z	0.0	0.0	1.0	· · · · · ·	151.3	
10010- CAA	SAR Validation (Square, 100ms, 10ms)	Х	2.73	65.7	12.7	10.00	35.9	±1.2 %
		Υ	1.18	58.1	9.8		37.4	
		Z	2.44	61.9	12.5		42.0	_
10011- CAB	UMTS-FDD (WCDMA)	X	3.43	68.2	18.9	2.91	148.5	±0.5 %
		Υ	3.14	66.5	18.1	<u>_</u>	114.3	
		Z	3.26	66.5	18.1		119.3	
10012- CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	Х	3.13	70.5	19.4	1.87	149.0	±0.5 %
		Υ	2.46	65.9	17.0		115.2	
		Z	3.02	68.7	18.5		120.9	
10013- CAB	IEEE 802.11g WiFi 2.4 GHz (DSSS- OFDM, 6 Mbps)	X	10.59	69.9	22.6	9.46	139.1	±2.5 %
		Υ	10.11	68.9	22.4		103.4	
		Z	10.74	69.4	22.4		114.3	
10021- DAB	GSM-FDD (TDMA, GMSK)	×	4.33	75.1	18.5	9.39	125.5	±1.4 %
		Y	5.13	77.6	20.0	ļ .	144.5	_
10000		Z	17.70	96.1	27.5		123.5	
10023- DAB	GPRS-FDD (TDMA, GMSK, TN 0)	X	4.56	75.8	18.9	9.57	147.7	±2.2 %
		Υ	5.75	78.8	20.2		140.4	
		Z	18.60	97.9	28.5		117.3	
10024- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1)	X	3.42	71.8	15.3	6.56	119.6	±1.4 %
		Y	14.95	90.8	22.0		132.7	
		Z	29.34	98.9	25.6		106.6	
10027- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	X	28.96	99.9	23.5	4.80	135.7	±1.9 %
		Y	55.26	99.9	21.9		107.5	
		Z	35.15	99.9	24.6		120.0	
10028- DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	X	36.32	96.2	20.3	3.55	147.5	±1.9 %
		Y	73.22	99.9	20.7		117.0	
10000		Z	52.78	99.6	22.4		128.3	<u> </u>
10032- CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	×	31.23	99.5	20.1	1.16	122.8	±1.4 %
	<u> </u>	Y	0.74	62.4	7.0	ļ. <u> </u>	135.2	
		Z	56.68	99.6	20.2		141.5	
10100- CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	×	6.01	66.4	18.9	5.67	112.7	±1.2 %
		Y	6.14	66.9	19.3		124.6	
		Z	6.37	67.2	19.4		129.3	

Page 4 of 13

Certificate No: ES3-3351_Jun15

10103-	LTE-TDD (SC-FDMA, 100% RB, 20			-, -	_,			June 22, 20
CAB	MHz, QPSK)	X	8.50	71.4	23.6	9.29	137.9	±2.7 %
	- 	Y	8.12	70.6	23.6		105.2	
10108-	LTE EDD (SC EDMA 4000) ED 40	Z	9.68	73.4	24.7		118.6	
CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	5.88	66.0	18.8	5.80	111.2	±1.2 %
		Y	5.99	66.5	19.2		122.8	
10117-	IEEE 200 41- (UTAE) 40 5 10	Z	6.28	66.9	19.4		128.7	
CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	10.19	69.3	21.2	8.07	149.1	±2.2 %
	· 	Y	9.73	68.2	20.9		111.5	
10151-	LTE-TDD (SC-FDMA, 50% RB, 20 MHz,	Z	9.97	68.3	20.8		117.7	
CAB	QPSK)	X	8.07	71.0	23.5	9.28	132.7	±2.5 %
		Y	8.82	74.2	25.9	<u> </u>	147.0	
10154-	LTE-FDD (SC-FDMA, 50% RB, 10 MHz,	Z	9.11	72.5	24.4	<u> </u>	115.3	
CAC	QPSK)	X	5.55	65.4	18.6	5.75	107.9	±0.9 %
		Y	5.67	66.0	19.0		120.3	
10160-	LTE-FDD (SC-FDMA, 50% RB, 15 MHz,	Z X	5.96	66.3	19.1	 	126.2	
CAB	QPSK)	ļ	5.96	65.9	18.7	5.82	111.9	±1.2 %
		Y	6.12	66.6	19.3	<u> </u>	125.0	
10169-	LTE-FDD (SC-FDMA, 1 RB, 20 MHz,	Z	6.38	66.8	19.3	 	131.2	
CAB	QPSK)	X	4.68	66.6	19.4	5.73	130.7	±0.9 %
		Z	4.81	67.2	20.0	<u> </u>	144.7	
10172- CAB	LTE-TDD (SC-FDMA, 1 RB, 20 MHz, QPSK)	X	4.74 6.59	65.5 73.2	18.9 25.1	9.21	109.9 143.9	±2.5 %
		Ý	6.42	72.7	25.3	 	113.3	
		Z	7.92	75.5	26.2	 	127.2	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	X	4.68	66.5	19.4	5.72	128.6	±0.9 %
		Y	4.80	67.2	20.0		144.2	
10101		Z	4.73	65.5	18.9		109.1	
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	Х	4.71	66.7	19.5	5.72	128.9	±1.2 %
		Υ	4.78	67.1	19.9		143.9	
10196-	IEEE 000 44 / // This	Z	5.12	67.3	19.9		149.9	
CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	X	9.72	68.8	21.1	8.10	138.3	±1.9 %
		Y	9.32	67.9	20.9		105.9	
10225-	UMTS-FDD (HSPA+)	Z	9.58	67.8	20.6		111.2	
CAB	OWIS-FDD (HSPA+)	Х	6.60	66.5	18.9	5.97	117.6	±1.2 %
<u>-</u>	 	Y	6.69	66.9	19.3		132.0	
10237-	LTE-TDD (SC-FDMA, 1 RB, 10 MHz,	_Z	7.08	67.2	19.5		139.9	
CAB	QPSK)	X	6.57	73.1	25.0	9.21	144.5	±2.2 %
	·	Y	6.59	73.6	25.8		114.3	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	Z X	7.44	76.0 70.0	26.4 23.2	9.24	127.7 122.9	±2.5 %
		Ŷ	8.16	73.3			400 0	
		$\frac{1}{z}$	8.43		25.5		138.8	
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	8.01	71.6	24.1	9.30	108.3 130.5	±2.7 %
		Y	8.86	74.4	26.1	 -	146.7	
		Ż	9.12	72.6	24.5		114.0	

June 22, 2015 ES3DV3-SN:3351

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	Х	4.49	67.5	18.8	3.96	146.9	±0.7 %
•		Υ_	4.13	65.9	18.1		117.5	
		Z	4.36	66.2	18.2		121.1	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.66	67.7	18.9	3.46	133.9	±0.5 %
		Υ	3.37	66.1	18.1		109.3	
		Z	3.54	66.0	18.0		112.1	
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.55	67.5	18.7	3.39	136.7	±0.7 %
		Υ	3.35	66.4	18.2		110.1	
		Z	3.44	65.7	17.9		112.9	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	Х	5.86	65.9	18.8	5.81	109.3	±1.2 %
		Υ	6.00	66.5	19.3		122.6	
	-	Z	6.23	66.7	19.3		126.8	
103 1 1- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	Х	6.42	66.5	19.1	6.06	114.1	±1.2 %
		Υ	6.60	67.2	19.7		127.9	
		Z	6.85	67.4	19.7		132.6	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	10.03	69.2	21.5	8.37	141.2	±1.9 %
		Υ	9.51	68.0	21.1		106.9	
		Z	9.90	68.2	21.1		114.0	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	Х	5.00	70.6	19.6	3.76	146.5	±0.5 %
		Y	4.32	67.9	18.3		115.0	
		Z	4.63	67.5	18.3		121.9	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	Х	4.99	71.0	19.8	3.77	143.8	±0.5 %
		Y	4.37	68.5	18.7		113.5	
		Z	4.56	67.5	18.2		120.2	
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	Х	3.07	71.2	19.9	1.54	145.7	±0.5 %
		Y	2.43	66.6	17.4		116.6	
		Z	2.59	67.1	17.8		124.3	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	X	9.84	69.0	21.3	8.23	139.6	±1.9 %
		Υ	9.37	67.9	21.0		106.5	
		Z	9.84	68.4	21.1		117.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of NormX,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

B Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

ES3DV3- SN:3351 June 22, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3351

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	6.43	6.43	6.43	0.31	1.96	± 12.0 %
835	41.5	0.90	6.17	6.17	6.17	0.21	2.59	± 12.0 %
1750	40.1	1.37	5.24	5.24	5.24	0.55	1.35	± 12.0 %
1900	40.0	1.40	5.07	5.07	5.07	0.54_	1.42	± 12.0 %
2300	39.5	1.67	4.74	4.74	4.74	0.69	1.31	± 12.0 %
2450	39.2	1.80	4.46	4.46_	4.46	0.80	1.26	± 12.0 %
2600	39.0	1.96	4.35	4.35	4.35	0.80	1.26	± 12.0 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the CopyE uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

ES3DV3- SN:3351 June 22, 2015

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3351

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	55.5	0.96	6.21	6.21	6.21	0.29_	1.98	± 12.0 %
835	55.2	0.97	6.11	6.11	6.11	0.77	1.20	± 12.0 %
1750	53.4	1.49	4.88	4.88	4.88	0.68	1.30	± 12.0 %
1900	53.3	1.52	4.68	4.68	4.68	0.61_	1.46	± 12.0 %
2300	52.9	1.81	4.47	4.47	4.47	0.80	1.16	± 12.0 %
2450	52.7	1.95	4.30	4.30	4.30 _	0.80	1.16	± 12.0 %
2600	52.5	2.16	4.16	4.16	4.16	0.80	1.20	± 12.0 %


^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.

F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the CopyE uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Galpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

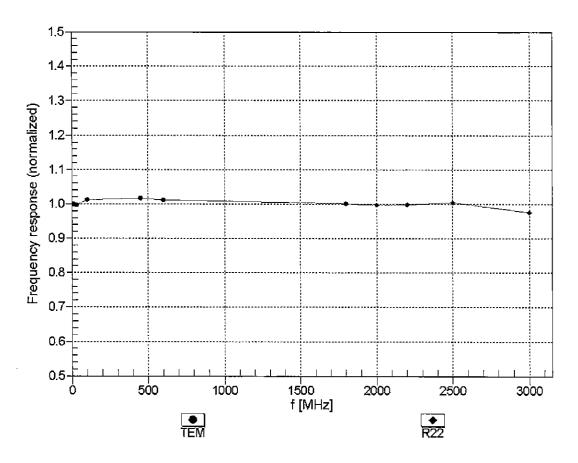



Uncertainty of Frequency Response of E-field: ± 6.3% (k=2)


Receiving Pattern (ϕ), ϑ = 0°

f=600 MHz,TEM

f=1800 MHz,R22

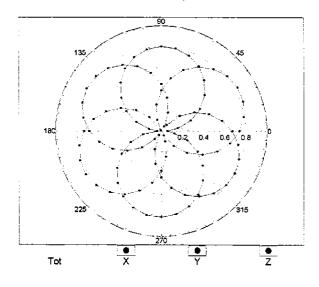





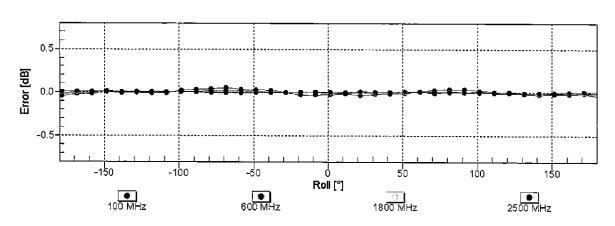

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

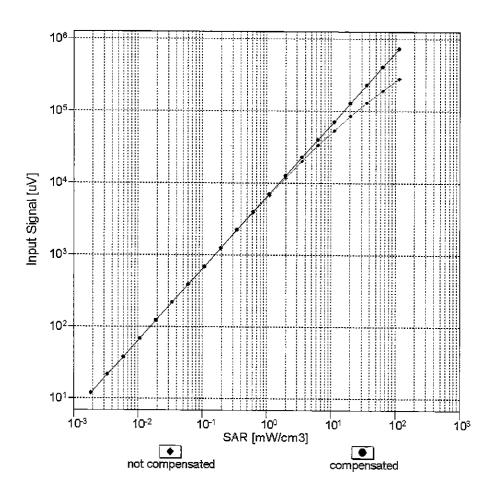

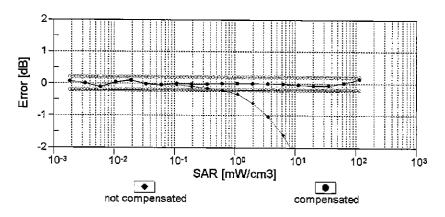


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

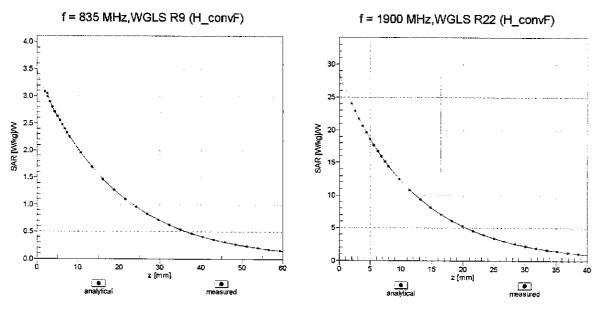

Deviation from Isotropy in Liquid

Error (ϕ , ϑ), f = 900 MHz

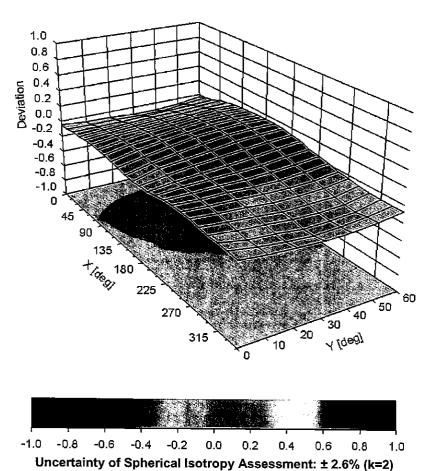

ES3DV3-SN:3351

DASY/EASY - Parameters of Probe: ES3DV3 - SN:3351

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	21.5
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst

C Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA

Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: SCS 0108

Client

PC Test

Certificate No: ES3-3022_Aug15

CALIBRATION CERTIFICATE

Object

ES3DV2 - SN:3022

Calibration procedure(s)

QA CAL-01.v9, QA CAL-23.v5, QA CAL-25.v6 Calibration procedure for dosimetric E-field probes

Calibration date:

August 26, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	C-L-1110
Power meter E4419B	GB41293874	01-Apr-15 (No. 217-02128)	Scheduled Calibration
Power sensor E4412A	MY41498087		Mar-16
Reference 3 dB Attenuator	SN: S5054 (3c)	01-Apr-15 (No. 217-02128)	Mar-16
Reference 20 dB Attenuator	SN: S5277 (20x)	01-Apr-15 (No. 217-02129)	Mar-16
Reference 30 dB Attenuator	SN: S5129 (30b)	01-Apr-15 (No. 217-02132)	Mar-16
Reference Probe ES3DV2	SN: 3013	01-Apr-15 (No. 217-02133)	Mar-16
DAE4		30-Dec-14 (No. ES3-3013_Dec14)	Dec-15
UNET	SN: 660	14-Jan-15 (No. DAE4-660_Jaп15)	Jan-16
Secondary Standards	ID	Check Date (in house)	Cohodulad Ol
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	Scheduled Check
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-14)	In house check: Apr-16

Name Function
Calibrated by: Michael Weber Laboratory T

Laboratory Technician

Signature

Approved by:

Katja Pokovic

Technical Manager

Issued: August 27, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Certificate No: ES3-3022_Aug15

Page 1 of 13

Calibration Laboratory of

Schmid & Partner Engineering AG Zeughausstrasse 43, 8004 Zurich, Switzerland





C

Schweizerischer Kalibrierdienst S

Service suisse d'étalonnage

Servizio svizzero di taratura Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL NORMx,y,z

tissue simulating liquid sensitivity in free space

ConvF DCP

sensitivity in TSL / NORMx, y, z diode compression point

CF A, B, C, D

crest factor (1/duty_cycle) of the RF signal modulation dependent linearization parameters

Polarization or

φ rotation around probe axis

Polarization 9

9 rotation around an axis that is in the plane normal to probe axis (at measurement center),

i.e., $\vartheta = 0$ is normal to probe axis

Connector Angle

information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013

b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

c) IEC 62209-2, "Procedure to determine the Specific Absorption Rate (SAR) for wireless communication devices used in close proximity to the human body (frequency range of 30 MHz to 6 GHz)", March 2010

d) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Methods Applied and Interpretation of Parameters:

- NORMx, y, z: Assessed for E-field polarization $\vartheta = 0$ (f ≤ 900 MHz in TEM-cell; f > 1800 MHz: R22 waveguide). NORMx,y,z are only intermediate values, i.e., the uncertainties of NORMx,y,z does not affect the E²-field uncertainty inside TSL (see below ConvF).
- $NORM(f)x,y,z = NORMx,y,z * frequency_response$ (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCPx,y,z: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- Ax,y,z; Bx,y,z; Cx,y,z; Dx,y,z; VRx,y,z: A, B, C, D are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters: Assessed in flat phantom using E-field (or Temperature Transfer Standard for f ≤ 800 MHz) and inside waveguide using analytical field distributions based on power measurements for f > 800 MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORMx,y,z * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from \pm 50 MHz to \pm 100
- Spherical isotropy (3D deviation from isotropy): in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle: The angle is assessed using the information gained by determining the NORMx (no uncertainty required).

Certificate No: ES3-3022_Aug15 Page 2 of 13

Probe ES3DV2

SN:3022

Manufactured: April 15, 2003 Calibrated:

August 26, 2015

Calibrated for DASY/EASY Systems

(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm (μV/(V/m) ²) ^A	1.00	1.03	0.95	± 10.1 %
DCP (mV) ^B	99.9	99.7	100.9	= 10.1 /8

Modulation Calibration Parameters

UID	Communication System Name		Α	В	С	D	T 1/5	T E
0	CW	<u> </u>	đВ	dB√μV		dB	VR mV	Unc ^E (k=2)
ļ -	CVV	X_	0.0	0.0	1.0	0.00	179.6	±3.3 %
		Y	0.0	0.0	1.0		183.9	*
10010-	SAP Validation (Cause 400	Z	0.0	0.0	1.0		179.0	
CAA	SAR Validation (Square, 100ms, 10ms)	X	3.60	65.9	14.2	10.00	43.5	±2.2 %
		Y	2.84	63.5	13.0		43.3	
10011-	UMTS-FDD (WCDMA)	Z	2.76	63.7	12.7		41.7	
CAB	OWIS-FDD (WCDMA)	X	3.32	67.0	18.7	2.91	144.4	±0.7 %
		<u> </u>	3.24	66.3	18.0		147.3	
10012-	IEEE 902 44b WEE; O 4 OU (DODG)	Z	3.19	66.3	18.0		143.5	
CAB	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps)	X	3.15	69.9	19.5	1.87	146.1	±0.7 %
		Y	2.88	67.7	18.0		147.9	
10013-	IEEE 802.11g WiFi 2.4 GHz (DSSS-	Z	2.78	67.4	17.8		145.6	
CAB	OFDM, 6 Mbps)	X	11.40	71.3	23.8	9.46	144.9	±3.3 %
		Y	11,15	70.5	23.1		146.9	
10021-	GSM-FDD (TDMA, GMSK)	Z	10.95	70.5	23.3		140.3	
DAB	CONFI DD (TDIVIA, GIVISK)	X	20.66	99.8	29.2	9.39	132.6	±2.2 %
		Y	14.36	93.3	26.6		145.3	
10023-	GPRS-FDD (TDMA, GMSK, TN 0)	Z	17.17	97.2	27.8		145.4	
DAB	GING-I DD (I DIVIA, GIVISK, IN U)	X	17.22	96.5	28.2	9.57	125.4	±1.9 %
		Y	11.06	88.6	25.0		136.0	
10024-	GPRS-FDD (TDMA, GMSK, TN 0-1)	Z	8.71	84.6	23.4		130.7	
DAB	G. TO TOD (TOWA, GIVISK, TN 0-1)	X	31.05	99.5	25.9	6.56	135.2	±2.2 %
		Y	25.28	97.4	25.0		132.5	
10027-	GPRS-FDD (TDMA, GMSK, TN 0-1-2)	Z	21.58	95.7	24.5		144.4	
DAB	GING-PDD (TDIVIA, GIVISK, TN 0-1-2)	X	42.88	99.9	24.0	4.80	129.5	±1.9 %
		Y	40.80	99.6	23.7		124.9	***
10028-	GDDS EDD (TDMA CMSK TALO 4 0 0)	Z	38.42	99.7	23.7		137.8	
DAB	GPRS-FDD (TDMA, GMSK, TN 0-1-2-3)	Х	44.48	100.0	23.2	3.55	138.2	±1.9 %
		Y	44.03	99.7	22.8		133.0	
10032-	JEEE 200 45 4 DL (OFO)	Z	41.36	99.8	22.8		147.5	
CAA	IEEE 802.15.1 Bluetooth (GFSK, DH5)	X	16.08	99.5	23.3	1.16	127.5	±1.4 %
		Υ	79.69	99.6	19.3		146.2	· · · · · · · · · · · · · · · · · · ·
10100-	LTE FDD (OC FDMA 4000) DE -	Z	45.81	99.9	20.4		138.2	.,,,,
CAB	LTE-FDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	X	6.43	67.4	19.8	5.67	138.7	±1.4 %
777		Y	6.27	66.8	19.2		134.9	
		Z	6.16	66.6	19.2		127.6	

Certificate No: ES3-3022_Aug15

10103- CAB	LTE-TDD (SC-FDMA, 100% RB, 20 MHz, QPSK)	Х	10.13	75.0	25.9	9.29	129.4	±3.3 %
		Y	9.46	73.0	24.5		121.0	
		Z	9.52	74.0	25.4		131.8 137.0	
10108- CAC	LTE-FDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	6.27	66.9	19.7	5.80	137.0	±1.7 %
***		İΥ	6.24	66.7	19.3		140.0	<u> </u>
		Z	6.06	66.3	19.2		127.1	
10117- CAB	IEEE 802.11n (HT Mixed, 13.5 Mbps, BPSK)	X	10.16	68.7	21.3	8.07	127.7	±2.2 %
		Υ	9.99	68.2	20.9		131.5	
10454	LITE TOP (OCT	Z	10.22	69.1	21.4		141.6	
10151- CAB	LTE-TDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	X	9.34	73.4	25.2	9.28	125.0	±3.3 %
		Y	8.92	72.2	24.3		127.2	
10154-	LITE EDD (CC FDM) FOX FD (CAN)	<u></u>	8.95	73.1	25.1		131.9	*
CAC	LTE-FDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	X	5.95	66.4	19.4	5.75	134.4	±1.4 %
		Y	5.92	66.2	19.1		137.0	
10160-	LTE-FDD (SC-FDMA, 50% RB, 15 MHz,	Z	5.98	66.7	19.5	<u> </u>	146.8	
CAB	QPSK)	X	6.39	66.9	19.6	5.82	139.9	±1.7 %
		Y	6.35	66.7	19.3		141.9	
10169-	LTE-FDD (SC-FDMA, 1 RB, 20 MHz,	Z	6.15	66.2	19.2		128.4	
CAB	QPSK)	X	4.96	66.6	19.8	5.73	137.3	±1.4 %
		Y	4.85	66.1	19.3		139.8	
10172-	LTE-TDD (SC-FDMA, 1 RB, 20 MHz,	Z	4.85	66.6	19.7		146.7	
CAB	QPSK)	X	8.75	78.7	28.3	9.21	138.9	±3.0 %
		Y	7.69	75.1	26.1		140.1	
10175- CAC	LTE-FDD (SC-FDMA, 1 RB, 10 MHz, QPSK)	Z	7.80 4.88	76.6 66.2	27.2 19.6	5.72	144.0 132.0	±1.4 %
		Y	4.77	65.8	19.1		132.6	
		Z	4.83	66.5	19.1		146.0	****
10181- CAB	LTE-FDD (SC-FDMA, 1 RB, 15 MHz, QPSK)	X	4.91	66.3	19.7	5.72	131.7	±1.4 %
		Υ	4.82	66.0	19.2		138.4	
10100		Z	4.86	66.7	19.7		145.7	
10196- CAB	IEEE 802.11n (HT Mixed, 6.5 Mbps, BPSK)	Х	10.04	69.1	21.7	8.10	140.9	±2.2 %
		Υ	9.62	67.9	20.8		125.2	
10225-	LIMTS FDD (HODA)	Z	9.74	68.6	21.3		133.3	
CAB	UMTS-FDD (HSPA+)	Х	7.01	67.1	19.6	5.97	143.7	±1.4 %
		Υ	6.78	66.2	19.0		129.3	
10237-	LTE-TDD (SC-FDMA, 1 RB, 10 MHz,	Z	6.80	66.7	19.3		136.5	
CAB	QPSK)	Х	8.55	78.0	27.9	9.21	134.6	±3.0 %
		_ <u>Y</u>	7.79	75.6	26.3		141.6	
10252- CAB	LTE-TDD (SC-FDMA, 50% RB, 10 MHz, QPSK)	Z X	7.89 9.30	76.9 74.8	27.4 26.1	9.24	145.2 134.8	±3.3 %
		Y	8.65	72.5	24.5		136.4	
**********		z	8.33	72.3	24.5		126.6	
10267- CAB	LTE-TDD (SC-FDMA, 100% RB, 10 MHz, QPSK)	X	10.20	76.2	24.8 26.8	9.30	144.8	±3.3 %
		Y	9.41	73.7	25.1		145.9	
		Z	9.18	73.9	25.6		138.6	

ES3DV2-SN:3022 August 26, 2015

10275- CAB	UMTS-FDD (HSUPA, Subtest 5, 3GPP Rel8.4)	X	4.45	66.7	18.9	3.96	147.0	±0.9 %
		Y	4.21	65.5	17.9		126.5	
40004		Z	4.36	66.5	18.5		148.0	
10291- AAB	CDMA2000, RC3, SO55, Full Rate	Х	3.57	66.3	18.5	3.46	134.3	±0.7 %
		Y	3.48	65.6	17.8	<u> </u>	136.8	
40000		Z	3.51	66.2	18.3		136.4	1
10292- AAB	CDMA2000, RC3, SO32, Full Rate	Х	3.53	66.4	18.6	3.39	135.8	±0.7 %
		Y	3.45	65.8	17.9		140.4	
4000=		Z	3.50	66.5	18.5		137.0	
10297- AAA	LTE-FDD (SC-FDMA, 50% RB, 20 MHz, QPSK)	Х	6.18	66.5	19.5	5.81	129.4	±1.4 %
		Y	6.15	66.3	19.1		133.6	1
40044		Z	6.13	66.5	19.3		131.2	
10311- AAA	LTE-FDD (SC-FDMA, 100% RB, 15 MHz, QPSK)	X	6.77	67.2	19.9	6.06	134.8	±1.7 %
		Y	6.81	67.3	19.7		144.8	
40400		Z	6.68	67.1	19.7	ļ	136.7	
10400- AAC	IEEE 802.11ac WiFi (20MHz, 64-QAM, 99pc duty cycle)	X	10.30	69.4	22.0	8.37	142.0	±2.5 %
		Υ	9.90	68.2	21.1		126.8	
40400		Z	10.15	69.3	21.9		142.6	
10403- AAB	CDMA2000 (1xEV-DO, Rev. 0)	Х	4.72	68.1	18.9	3.76	147.8	±0.7 %
		Υ	4.56	67.5	18.2		133.6	
10101		Z	4.61	68.2	18.7		147.4	
10404- AAB	CDMA2000 (1xEV-DO, Rev. A)	Х	4.57	67.8	18.8	3.77	144.3	±0.7 %
		Υ	4.43	67.3	18.1		131.3	***************************************
40445		Z	4.57	68.3	18.8		145.0	
10415- AAA	IEEE 802.11b WiFi 2.4 GHz (DSSS, 1 Mbps, 99pc duty cycle)	X	2.64	67.9	18.7	1.54	142.1	±0.5 %
		Υ	2.36	65.4	16.8		130.3	·····
40440		Z	2.50	66.7	17.7		145.0	
10416- AAA	IEEE 802.11g WiFi 2.4 GHz (ERP- OFDM, 6 Mbps, 99pc duty cycle)	Х	10.04	69.0	21.7	8.23	138.8	±2.2 %
		Υ	9.71	68.0	20.9		125.6	
		Z	9.94	69.0	21.6		140.4	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

A The uncertainties of Norm X,Y,Z do not affect the E²-field uncertainty inside TSL (see Pages 7 and 8).

B Numerical linearization parameter: uncertainty not required.

E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G	Unc
		3,,,,,,	OUIIVI X	CONVE	CONVP Z	Alpha	(mm)	(k=2)
750	41.9	0.89	6.33	6.33	6.33	0.46	1.43	± 12.0 %
835	41.5	0.90	6.11	6.11	6.11	0.24	2.08	± 12.0 %
1750	40.1	1.37	5.08	5.08	5.08	0.45	1.47	± 12.0 %
1900	40.0	1.40	4.93	4.93	4.93	0.59	1.25	± 12.0 %
2300	39.5	1.67	4.63	4.63	4.63	0.55	1.39	± 12.0 %
2450	39.2	1.80	4.30	4.30	4.30	0.51	1,47	± 12.0 %
2600	39.0	1.96	4.12	4.12	4.12	0.57	1.46	± 12.0 %

 $^{^{\}rm C}$ Frequency validity above 300 MHz of \pm 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to \pm 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity validity can be extended to \pm 110 MHz.

validity can be extended to ± 110 MHz.

At frequencies below 3 GHz, the validity of tissue parameters (ε and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ε and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Calibration Parameter Determined in Body Tissue Simulating Media

f (MHz) ^c	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unc (k≃2)
750	55.5	0.96	6.16	6.16	6.16	0.50	1.34	± 12.0 %
835	55.2	0.97	6.13	6.13	6.13	0.25	2.16	± 12.0 %
1750	53.4	1.49	4.79	4.79	4.79	0.61	1.33	± 12.0 %
1900	53.3	1.52	4.56	4.56	4.56	0.31	2.02	± 12.0 %
2300	52.9	1.81	4.32	4.32	4.32	0.79	1.19	± 12.0 %
2450	52.7	1.95	4.08	4.08	4.08	0.80	1.12	± 12.0 %
2600	52.5	2.16	3.96	3.96	3.96	0.80	1.10	± 12.0 %

^c Frequency validity above 300 MHz of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band. Frequency validity below 300 MHz is ± 10, 25, 40, 50 and 70 MHz for ConvF assessments at 30, 64, 128, 150 and 220 MHz respectively. Above 5 GHz frequency validity can be extended to ± 110 MHz.


At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to \pm 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to \pm 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is

always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Frequency Response of E-Field


(TEM-Cell:ifi110 EXX, Waveguide: R22)

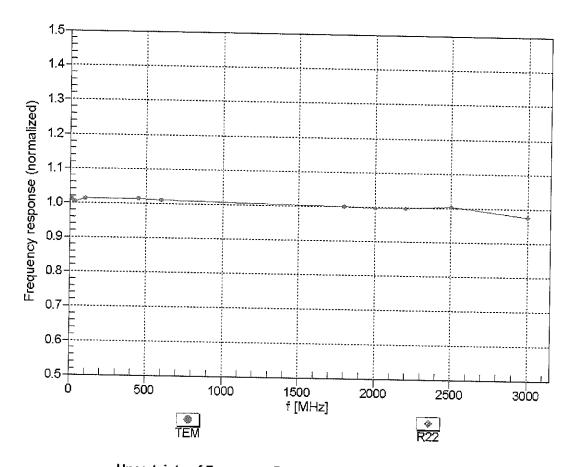

Uncertainty of Frequency Response of E-field: \pm 6.3% (k=2)


Receiving Pattern (ϕ), $\vartheta = 0^{\circ}$

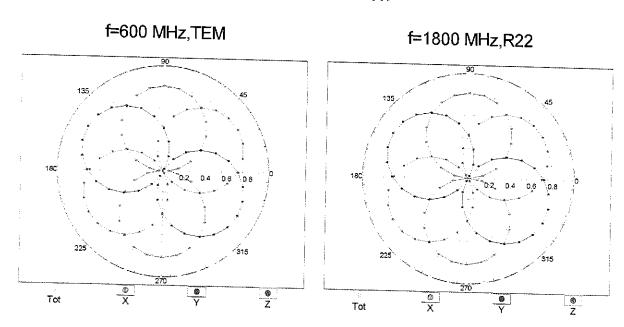


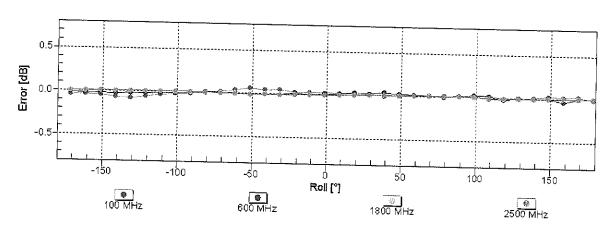

Uncertainty of Axial Isotropy Assessment: ± 0.5% (k=2)


Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

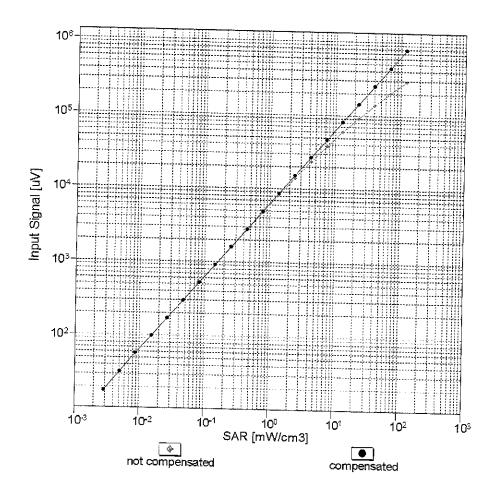

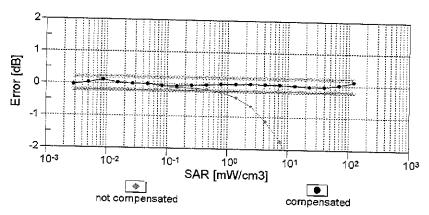



Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

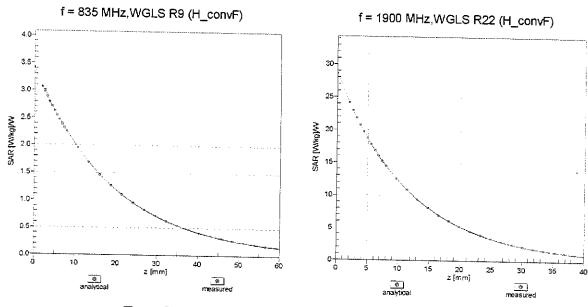

Deviation from Isotropy in Liquid Error (\$\phi\$, \$\text{9}\$), f = 900 MHz

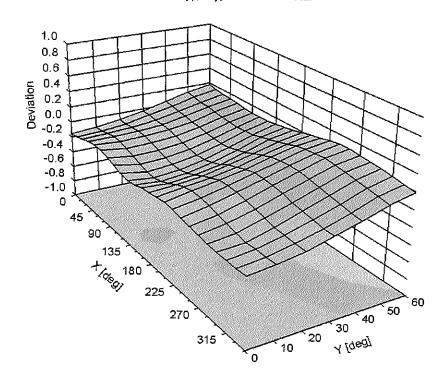



DASY/EASY - Parameters of Probe: ES3DV2 - SN:3022

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	98.5
Mechanical Surface Detection Mode	
Optical Surface Detection Mode	enabled
Probe Overall Length	disabled
Probe Body Diameter	337 mm
Tip Length	10 mm
	10 mm
Tip Diameter	4 mm
Probe Tip to Sensor X Calibration Point	2 mm
Probe Tip to Sensor Y Calibration Point	2 mm
Probe Tip to Sensor Z Calibration Point	2 mm
Recommended Measurement Distance from Surface	3 mm

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Client

PC Test

Accreditation No.: SCS 0108

Certificate No: D1900V2-5d141_Apr15

Object D1900V2 - SN:5d141

Calibration procedure(s)

QA CAL-05.v9

Calibration procedure for dipole validation kits above 700 MHz

4/29/15

Calibration date:

April 14, 2015

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI). The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID#	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	US37292783	07-Oct-14 (No. 217-02020)	Oct-15
Power sensor HP 8481A	MY41092317	07-Oct-14 (No. 217-02021)	Oct-15
Reference 20 dB Attenuator	SN: 5058 (20k)	01-Apr-15 (No. 217-02131)	Mar-16
Type-N mismatch combination	SN: 5047.2 / 06327	01-Apr-15 (No. 217-02134)	Mar-16
Reference Probe ES3DV3	SN: 3205	30-Dec-14 (No. ES3-3205_Dec14)	Dec-15
DAE4	SN: 601	18-Aug-14 (No. DAE4-601_Aug14)	Aug-15
Secondary Standards	ID#	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-14)	In house check: Oct-15
	Name	Function	Signature 3
Calibrated by:	Claudio Leubler	Laboratory Technician	(X)

Issued: April 14, 2015

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.

Katja Pokovic

Approved by:

Calibration Laboratory of

Schmid & Partner
Engineering AG
Zeughausstrasse 43, 8004 Zurich, Switzerland





S Schweizerischer Kalibrierdienst
C Service suisse d'étalonnage
Servizio svizzero di taratura
Swiss Calibration Service

Accreditation No.: SCS 0108

Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the sign:

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL tissue simulating liquid

ConvF sensitivity in TSL / NORM x,y,z N/A not applicable or not measured

Calibration is Performed According to the Following Standards:

- a) IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- b) IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- c) KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

d) DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions: Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL: The dipole is mounted with the spacer to position its feed
 point exactly below the center marking of the flat phantom section, with the arms oriented
 parallel to the body axis.
- Feed Point Impedance and Return Loss: These parameters are measured with the dipole
 positioned under the liquid filled phantom. The impedance stated is transformed from the
 measurement at the SMA connector to the feed point. The Return Loss ensures low
 reflected power. No uncertainty required.
- Electrical Delay: One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured: SAR measured at the stated antenna input power.
- SAR normalized: SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters: The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor k=2, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Certificate No: D1900V2-5d141_Apr15 Page 2 of 8

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy , $dz = 5 mm$	
Frequency	1900 MHz ± 1 MHz	,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,,

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity 1.40 mho/m	
Nominal Head TSL parameters	22.0 °C	40.0		
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.6 ± 6 %	1.37 mho/m ± 6 %	
Head TSL temperature change during test	< 0.5 °C	a u 12.20		

SAR result with Head TSL

SAR averaged over 1 cm ³ (1 g) of Head TSL	Condition			
SAR measured	250 mW input power	9.93 W/kg		
SAR for nominal Head TSL parameters	normalized to 1W	39.9 W/kg ± 17.0 % (k=2)		

SAR averaged over 10 cm ³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.20 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	20.9 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity	
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m	
Measured Body TSL parameters	(22.0 ± 0.2) °C	52.8 ± 6 %	1.50 mho/m ± 6 %	
Body TSL temperature change during test	< 0.5 °C			

SAR result with Body TSL

SAR averaged over 1 cm ³ (1 g) of Body TSL	Condition			
SAR measured	250 mW input power	9.94 W/kg		
SAR for nominal Body TSL parameters	normalized to 1W	40.0 W/kg ± 17.0 % (k=2)		

SAR averaged over 10 cm ³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.29 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	21.2 W/kg ± 16.5 % (k=2)

Certificate No: D1900V2-5d141_Apr15

Appendix (Additional assessments outside the scope of SCS 0108)

Antenna Parameters with Head TSL

Impedance, transformed to feed point	53.0 Ω + 4.6 jΩ
Return Loss	- 25.5 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.2 Ω + 5.6 jΩ
Return Loss	- 24.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.198 ns
	1.130115

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	March 11, 2011

Certificate No: D1900V2-5d141_Apr15

DASY5 Validation Report for Head TSL

Date: 14.04.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d141

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.37$ S/m; $\epsilon_r = 38.6$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(5, 5, 5); Calibrated: 30.12.2014;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001

• DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 98.18 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 18.2 W/kg


SAR(1 g) = 9.93 W/kg; SAR(10 g) = 5.2 W/kg

Maximum value of SAR (measured) = 12.5 W/kg

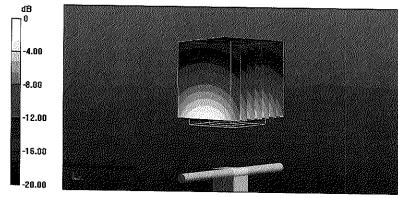

0 dB = 12.5 W/kg = 10.97 dBW/kg

Impedance Measurement Plot for Head TSL

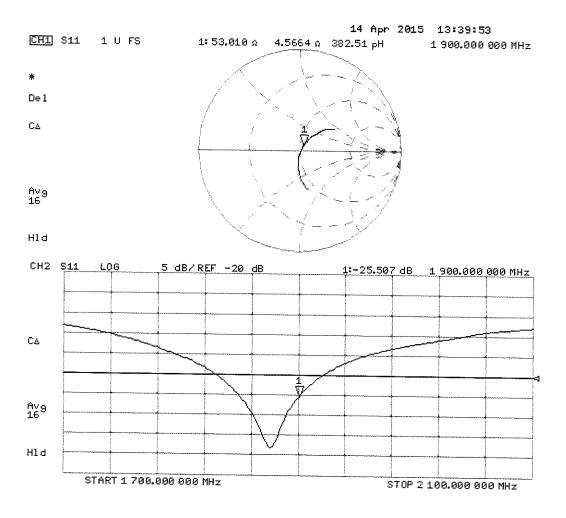

DASY5 Validation Report for Body TSL

Date: 14.04.2015

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN:5d141

Communication System: UID 0 - CW; Frequency: 1900 MHz

Medium parameters used: f = 1900 MHz; $\sigma = 1.5$ S/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

Probe: ES3DV3 - SN3205; ConvF(4.65, 4.65, 4.65); Calibrated: 30.12.2014;

• Sensor-Surface: 3mm (Mechanical Surface Detection)

• Electronics: DAE4 Sn601; Calibrated: 18.08.2014

Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002

DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 95.73 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 16.9 W/kg


SAR(1 g) = 9.94 W/kg; SAR(10 g) = 5.29 W/kg

Maximum value of SAR (measured) = 12.5 W/kg

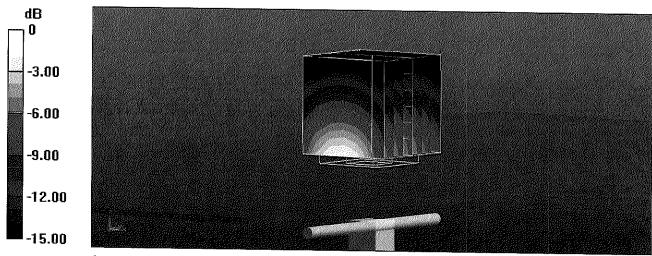

0 dB = 12.5 W/kg = 10.97 dBW/kg

Impedance Measurement Plot for Body TSL

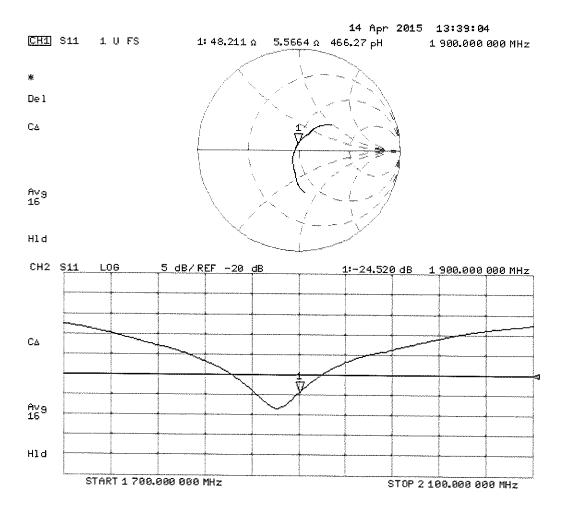

APPENDIX D: SAR TISSUE SPECIFICATIONS

Measurement Procedure for Tissue verification:

- 1) The network analyzer and probe system was configured and calibrated.
- 2) The probe was immersed in the tissue. The tissue was placed in a nonmetallic container. Trapped air bubbles beneath the flange were minimized by placing the probe at a slight angle.
- 3) The complex admittance with respect to the probe aperture was measured
- 4) The complex relative permittivity ε can be calculated from the below equation (Pournaropoulos and Misra):

$$Y = \frac{j2\omega\varepsilon_{r}\varepsilon_{0}}{\left[\ln(b/a)\right]^{2}} \int_{a}^{b} \int_{a}^{b} \int_{0}^{\pi} \cos\phi' \frac{\exp\left[-j\omega r(\mu_{0}\varepsilon_{r}\varepsilon_{0})^{1/2}\right]}{r} d\phi' d\rho' d\rho$$

where Y is the admittance of the probe in contact with the sample, the primed and unprimed coordinates refer to source and observation points, respectively, $r^2 = \rho^2 + \rho'^2 - 2\rho\rho'\cos\phi'$, ω is the angular frequency, and $j = \sqrt{-1}$.

Table D-I Composition of the Tissue Equivalent Matter

Frequency (MHz)	835	835	1900	1900	2450	2450
Tissue	Head	Body	Head	Body	Head	Body
Ingredients (% by weight)						
Bactericide	0.1	0.1				
DGBE			44.92	29.44	See page 2	26.7
HEC	1	1				
NaCl	1.45	0.94	0.18	0.39		0.1
Sucrose	57	44.9				
Water	40.45	53.06	54.9	70.17		73.2

FCC ID: ZNFL17AG	CAPCTEST* SA	AR EVALUATION REPORT	(LG	Reviewed by: Quality Manager
Test Dates:	DUT Type:			APPENDIX D:
11/09/15 - 11/18/15	Portable Handset			Page 1 of 2

2 Composition / Information on ingredients

The Item is composed of the following ingredients:

H2O Water, 52 – 75%

C8H18O3 Diethylene glycol monobutyl ether (DGBE), 25 – 48%

(CAS-No. 112-34-5, EC-No. 203-961-6, EC-index-No. 603-096-00-8)

Relevant for safety; Refer to the respective Safety Data Sheet*.

NaCl Sodium Chloride, <1.0%

Figure D-1

Composition of 2.4 GHz Head Tissue Equivalent Matter

Note: 2.4 GHz head liquid recipes are proprietary SPEAG. Since the composition is approximate to the actual liquids utilized, the manufacturer tissue-equivalent liquid data sheets are provided below.

Measurement Certificate / Material Test Head Tissue Simulating Liquid (HSL2450V2) Product No. SL AAH 245 BA (Charge: 150206-3) Manufacturer SPEAG surement Method TSL dielectric parameters measured using calibrated OCP probe. Validation results were within $\pm 2.5\%$ towards the target values of Methanol. Target Parameters Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards. **Test Condition** Ambient TSL Temperature Environment temperatur (22 ± 3)°C and humidity < 70%. 11-Feb-15 Test Date Operator IEN Additional Information TSL Density 0.988 a/cm TSL Heat-capacity 3,680 kJ/(kg*K) Target Diff.to Target [%] f [MHz] HP-e' HP-e" sigma eps sigma Δ-eps Δ-sigma 7.5 5.0 11.89 1.26 -10.2 1925 40.3 11.98 1.28 40.0 -8.3 2.5 40.2 1950 12.07 1.31 40.0 1.40 0.4 -6.4 1975 40.1 12.15 1.34 40.0 0.2 -4.6 -2.5 2000 40.0 12.23 1.36 40.0 1.40 -0.1 -2.8 Dev. -5.0 39.9 2025 12.32 1.39 40.0 1.42 -0.2 -2.4 2050 39.8 1.42 39.9 -0.3 -2.0 1900 2000 2100 2200 2300 2400 2500 2600 2700 2075 39.7 12.50 1.44 39.9 1.47 -0.4 -1.6 39.6 Frequency MHz 2100 12.59 1.47 39.8 1.49 -0.5 -1.2 2125 39.5 12.66 1.50 39.8 1.51 -0.7 -0.9 2150 39.4 39.3 12.73 1.52 39.7 1.53 -0.8 2175 12.83 10.0 1.55 39.7 1.56 -0.9 -0.2 7.5 5.0 2200 39.2 12.92 1.58 39.6 1.58 Conductivity % -1.1 0.2 2225 39.1 13.00 1.61 39.6 1.60 0.6 2.5 2250 39.0 13.08 1.64 39.6 1.62 -1.3 0.9 0.0 2275 38.9 1.67 39.5 -1.5 1.4 -2.5 2300 38.8 13.26 1.70 39.5 1.67 1.8 38.7 13.34 1.73 39.4 1.69 2.2 38.6 13.42 1.75 39.4 1.71 -2.0 2.5 2375 38.5 13.50 1.78 39.3 1.73 1900 2000 2100 2200 2300 2400 2500 2600 2700 2.9 2400 38.4 13.58 1.81 39.3 1.76 -2.3 3.3 Frequency MHz 38.3 13.65 1.84 1.78 39.2 2450 38.2 13.73 1.87 1.80 -2.6 2475 38.1 13.80 1.90 39.2 1.83 4.0 38.0 13.87 1.93 39.1 1.85 -3.0 4.0 2525 37.9 13.90 1.95 39.1 1.88 -3.1 3.8 2550 37.8 13.93 1.98 39.1 1.91 -3.2 3.5 2.01 2575 37.7 14.05 39.0 2600 37.6 14.17 2.05 39.0 1.96 37.4 14.23 2.08 39.0 4.4 4.4 37.3 14.29 2.11 38.9 2.02 2675 37.2 14.37 2.14 38.9 2.05 37.1 14.45

Figure D-2
2.4 GHz Head Tissue Equivalent Matter

FCC ID: ZNFL17AG	PCTEST	SAR EVALUATION REPORT		Reviewed by: Quality Manager
Test Dates:	DUT Type:			APPENDIX D:
11/09/15 - 11/18/15	Portable Handset			Page 2 of 2

APPENDIX E: SAR SYSTEM VALIDATION

Per FCC KDB 865664 D02v01, SAR system validation status should be documented to confirm measurement accuracy. The SAR systems (including SAR probes, system components and software versions) used for this device were validated against its performance specifications prior to the SAR measurements. Reference dipoles were used with the required tissue- equivalent media for system validation, according to the procedures outlined in FCC KDB 865664 D01v01r04 and IEEE 1528-2013. Since SAR probe calibrations are frequency dependent, each probe calibration point was validated at a frequency within the valid frequency range of the probe calibration point, using the system that normally operates with the probe for routine SAR measurements and according to the required tissue-equivalent media.

A tabulated summary of the system validation status including the validation date(s), measurement frequencies, SAR probes and tissue dielectric parameters has been included.

Table E-I SAR System Validation Summary

SAR FREQ.		DDODE	DDODE			COND.	PERM.	CW VALIDATION			MOD. VALIDATION			
SYSTEM #	[MHz]	DATE	PROBE SN	PROBE TYPE	PROBE CAL. POINT	AL. POINT	(σ)	(Er)	SENSITIVITY	PROBE LINEARITY	PROBE ISOTROPY	MOD. TYPE	DUTY FACTOR	PAR
С	835	10/9/2015	3288	ES3DV3	835	Head	0.895	40.311	PASS	PASS	PASS	GMSK	PASS	N/A
В	1900	11/5/2015	3287	ES3DV3	1900	Head	1.412	38.093	PASS	PASS	PASS	GMSK	PASS	N/A
J	1900	5/25/2015	3319	ES3DV3	1900	Head	1.447	39.423	PASS	PASS	PASS	GMSK	PASS	N/A
I	2450	11/16/2015	3333	ES3DV3	2450	Head	1.862	39.522	PASS	PASS	PASS	OFDM	N/A	PASS
Н	835	7/22/2015	3263	ES3DV3	835	Body	0.992	53.114	PASS	PASS	PASS	GMSK	PASS	N/A
K	835	9/8/2015	3022	ES3DV2	835	Body	1.005	53.292	PASS	PASS	PASS	GMSK	PASS	N/A
1	1900	11/4/2015	3333	ES3DV3	1900	Body	1.579	51.524	PASS	PASS	PASS	GMSK	PASS	N/A
E	2450	9/15/2015	3351	ES3DV3	2450	Body	2.005	50.900	PASS	PASS	PASS	OFDM	N/A	PASS

NOTE: While the probes have been calibrated for both CW and modulated signals, all measurements were performed using communication systems calibrated for CW signals only. Modulations in the table above represent test configurations for which the measurement system has been validated per FCC KDB Publication 865664 D01v01r04 for scenarios when CW probe calibrations are used with other signal types. SAR systems were validated for modulated signals with a periodic duty cycle, such as GMSK, or with a high peak to average ratio (>5 dB), such as OFDM according to FCC KDB Publication 865664 D01v01r04.

FCC ID: ZNFL17AG	PCTEST*	SAR EVALUATION REPORT	(LG	Reviewed by: Quality Manager
Test Dates:	DUT Type:			APPENDIX E:
11/09/15 - 11/18/15	Portable Handset			Page 1 of 1