




Appendix D




Photographs

1. SAR measurement System
2. Photographs of Tissue Simulate Liquid
3. Photographs of EUT test position
4. EUT Constructional Details

1. SAR measurement System

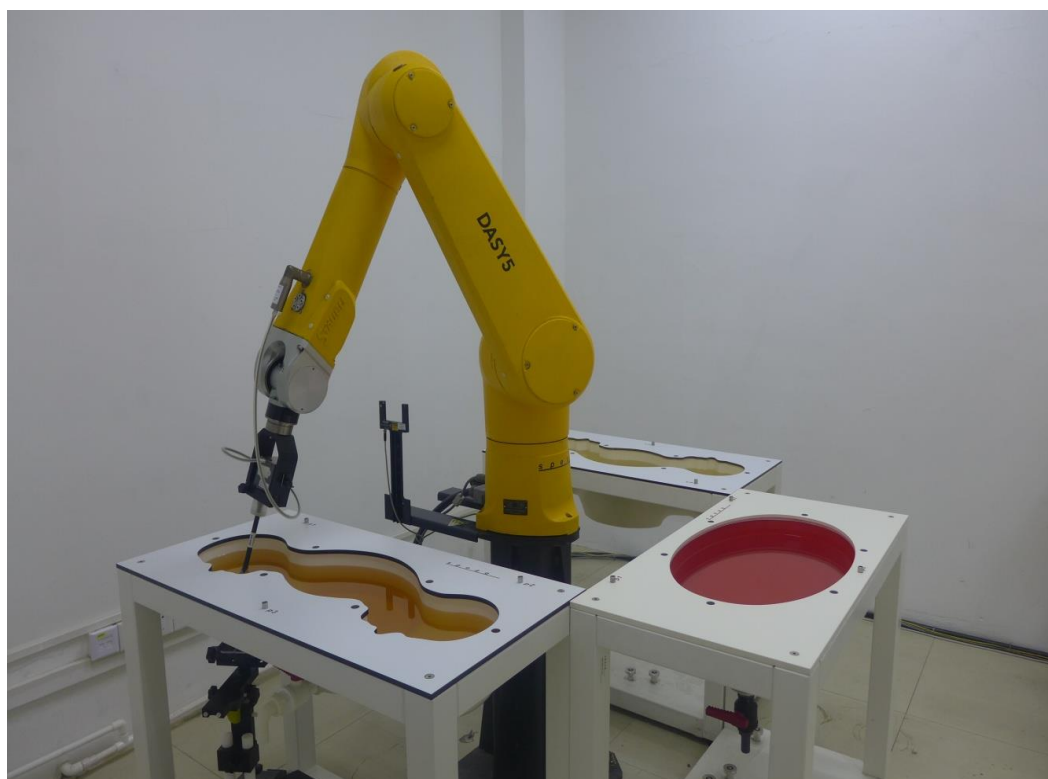

2. Photographs of Tissue Simulate Liquid

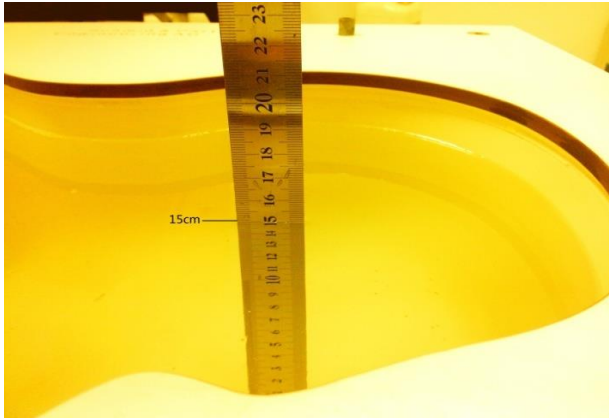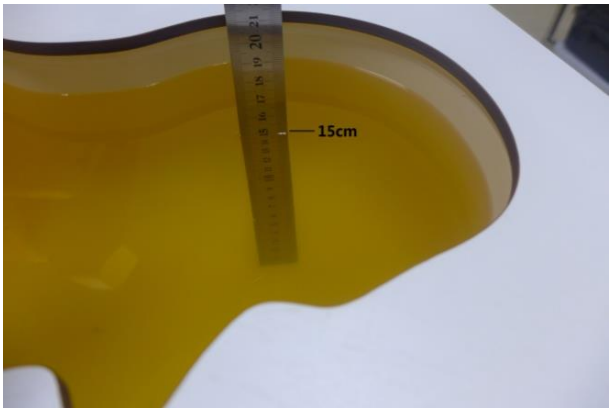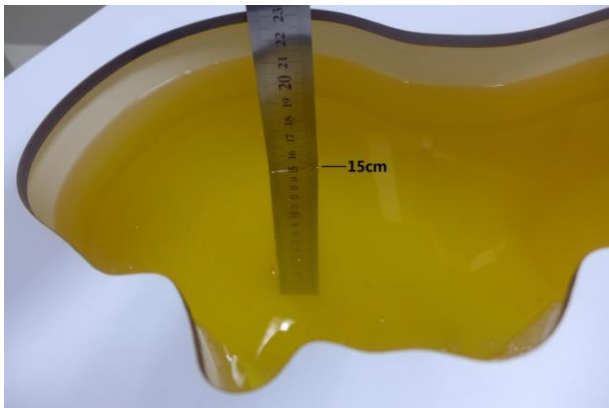Photo 1: Tissue Simulant Liquid for Head 835	Photo 2: Tissue Simulant Liquid for Head 1900
	
Photo 3: Tissue Simulant Liquid for Head 2450	NA
	NA

3. Photographs of EUT test position

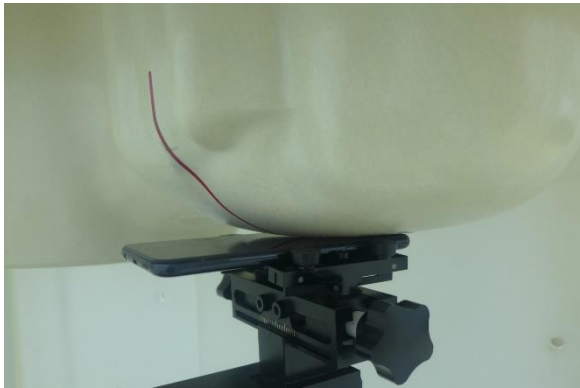
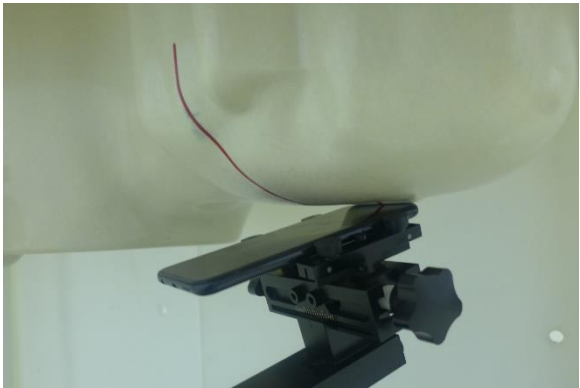
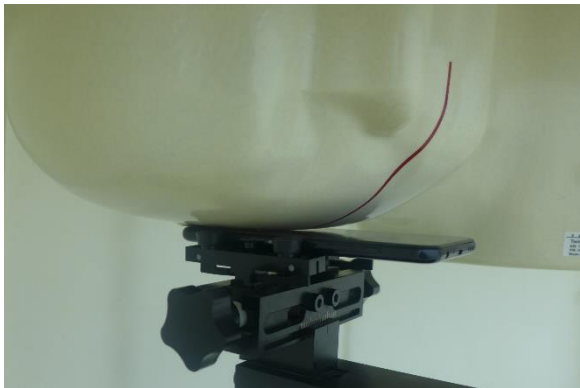
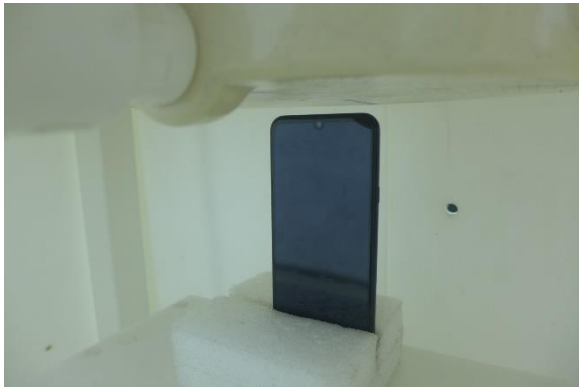
Photo 4: Left touch cheek	Photo 5: Left tilted 15 degree
	
Photo 6: Right touch cheek	Photo 7: Right tilted 15 degree
	
Photo 8: Front side 10mm	Photo 9: Back side 10mm
	

Photo 10: Left side 10mm	Photo 11: Right side 10mm
	
Photo 12: Top side 10mm	Photo 13: Bottom side 10mm
	

4. EUT Constructional Details

Photo 14: Front View	Photo 15: Back View
	
Photo 16: Accessory	NA
	NA