


## Dipole 900MHz (D900V2) Annual Check



Head 900

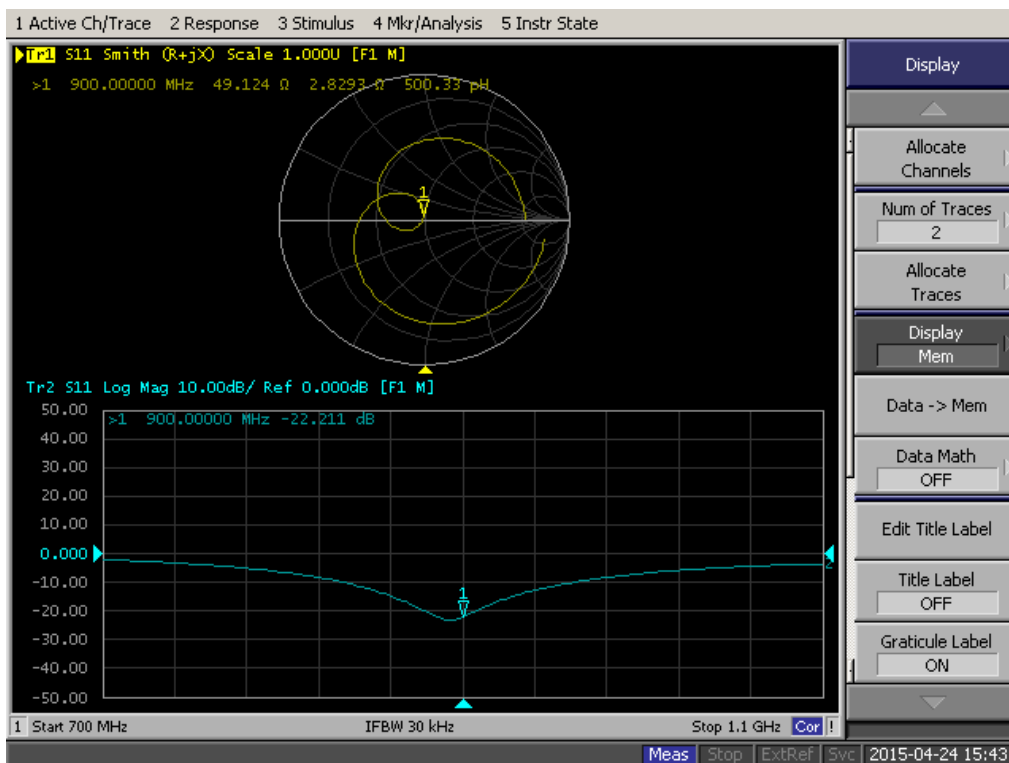


Head 900

Calibration results: Return Loss:-22.3 dB Impedance: 49.2 ohm

Annual check results: Return Loss:-22.2 dB Impedance: 49.1 ohm



Body 900

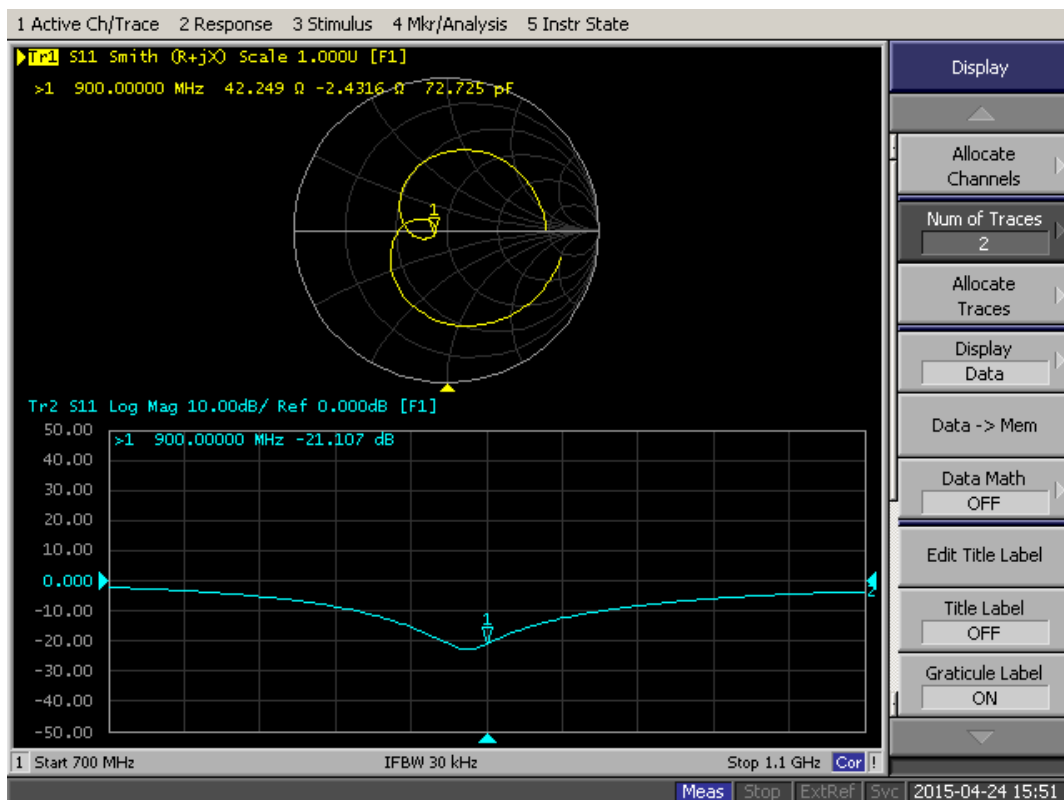

Body 900

Calibration results: Return Loss:-21.3 dB Impedance: 42.1 ohm

Annual check results: Return Loss:-21.1dB Impedance: 42.2 ohm