


20141006_SystemPerformanceCheck-D2450V2 SN 706

Frequency: 2450 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used: $f = 2450 \text{ MHz}$; $\sigma = 2.013 \text{ S/m}$; $\epsilon_r = 50.42$; $\rho = 1000 \text{ kg/m}^3$
 DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE3 Sn427; Calibrated: 1/21/2014
- Probe: EX3DV4 - SN3902; ConvF(7.35, 7.35, 7.35); Calibrated: 5/19/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI-B v5.0; Type: QDOVA002AA; Serial: TP:1195

Body/Pin=100 mW/Area Scan (8x8x1): Measurement grid: dx=12mm, dy=12mm
 Maximum value of SAR (measured) = 6.52 W/kg

Body/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 56.136 V/m; Power Drift = 0.00 dB
 Peak SAR (extrapolated) = 11.1 W/kg
SAR(1 g) = 5.37 W/kg; SAR(10 g) = 2.49 W/kg
 Maximum value of SAR (measured) = 7.68 W/kg

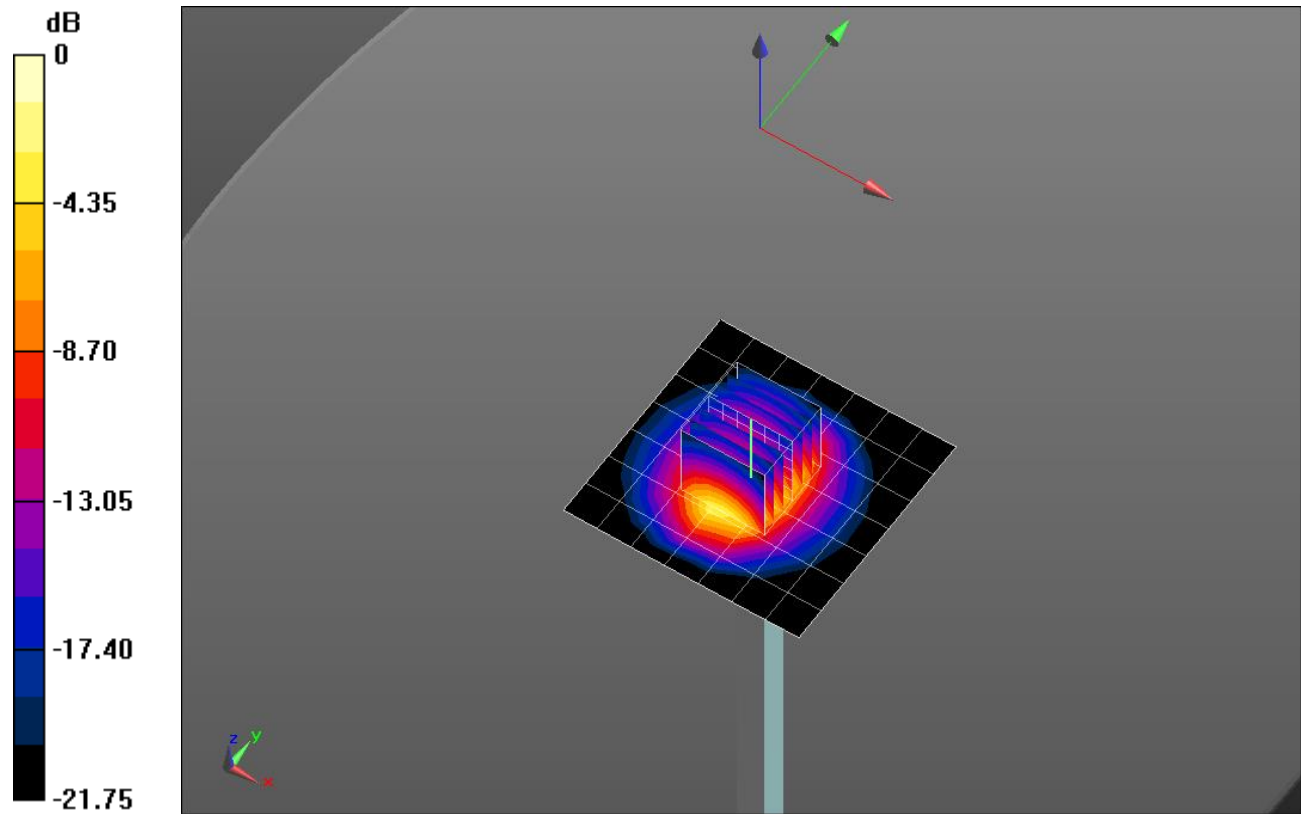


0 dB = 7.68 W/kg = 8.85 dBW/kg

20141006_SystemPerformanceCheck-D2450V2 SN 706

Frequency: 2450 MHz; Duty Cycle: 1:1

Body/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm

Maximum value of SAR (measured) = 7.11 W/kg

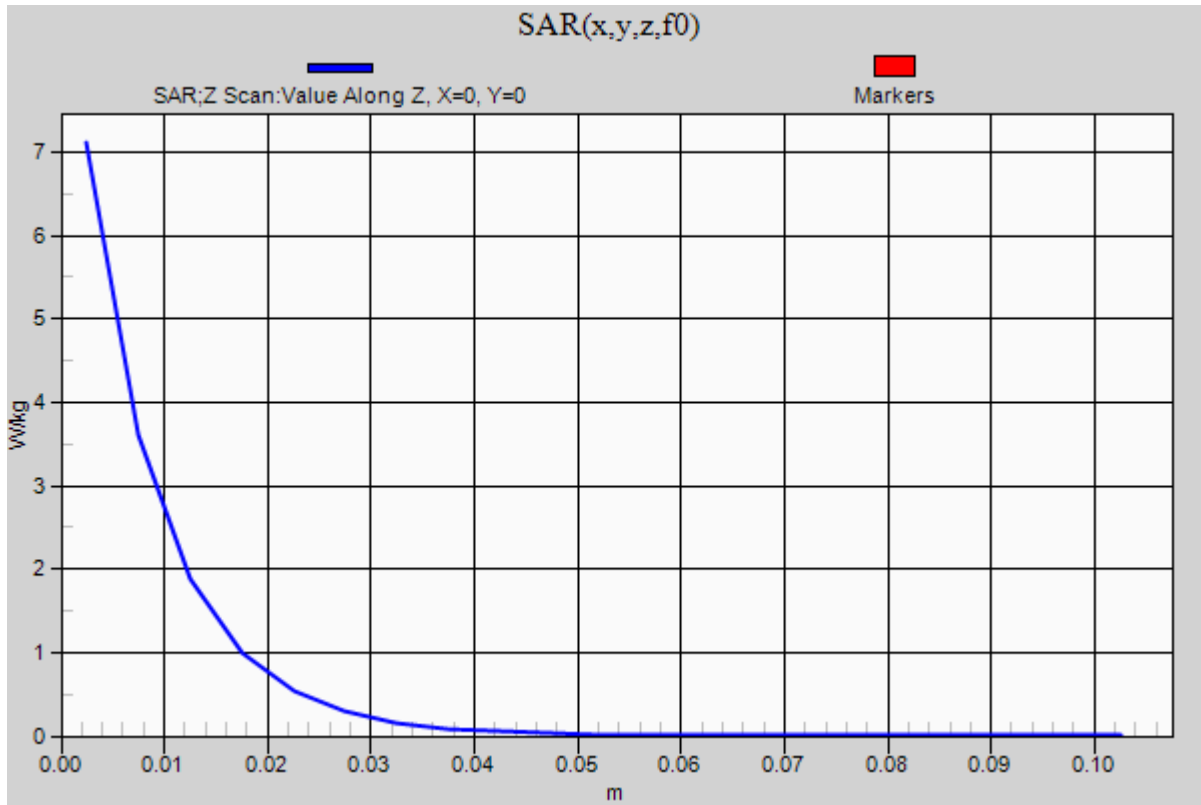

20141006_SystemPerformanceCheck-D835V2 SN 4d117

Frequency: 835 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 1.015 \text{ S/m}$; $\epsilon_r = 52.829$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(8.77, 8.77, 8.77); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Body/Pin=100 mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 1.25 W/kg


Body/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 35.69 V/m; Power Drift = -0.01 dB

Peak SAR (extrapolated) = 1.54 W/kg

SAR(1 g) = 1.03 W/kg; SAR(10 g) = 0.681 W/kg

Maximum value of SAR (measured) = 1.26 W/kg

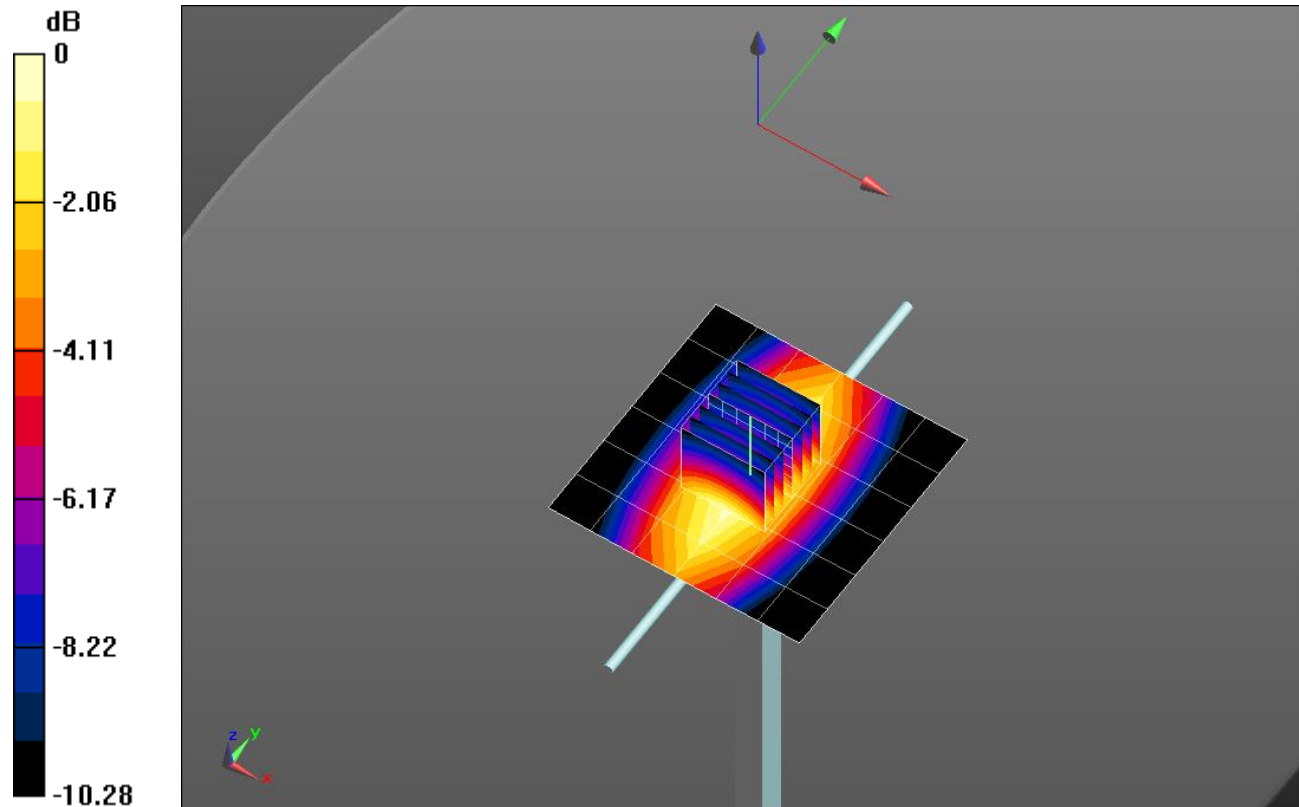


0 dB = 1.26 W/kg = 1.00 dBW/kg

20141006_SystemPerformanceCheck-D835V2 SN 4d117

Frequency: 835 MHz; Duty Cycle: 1:1

Body/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 1.26 W/kg

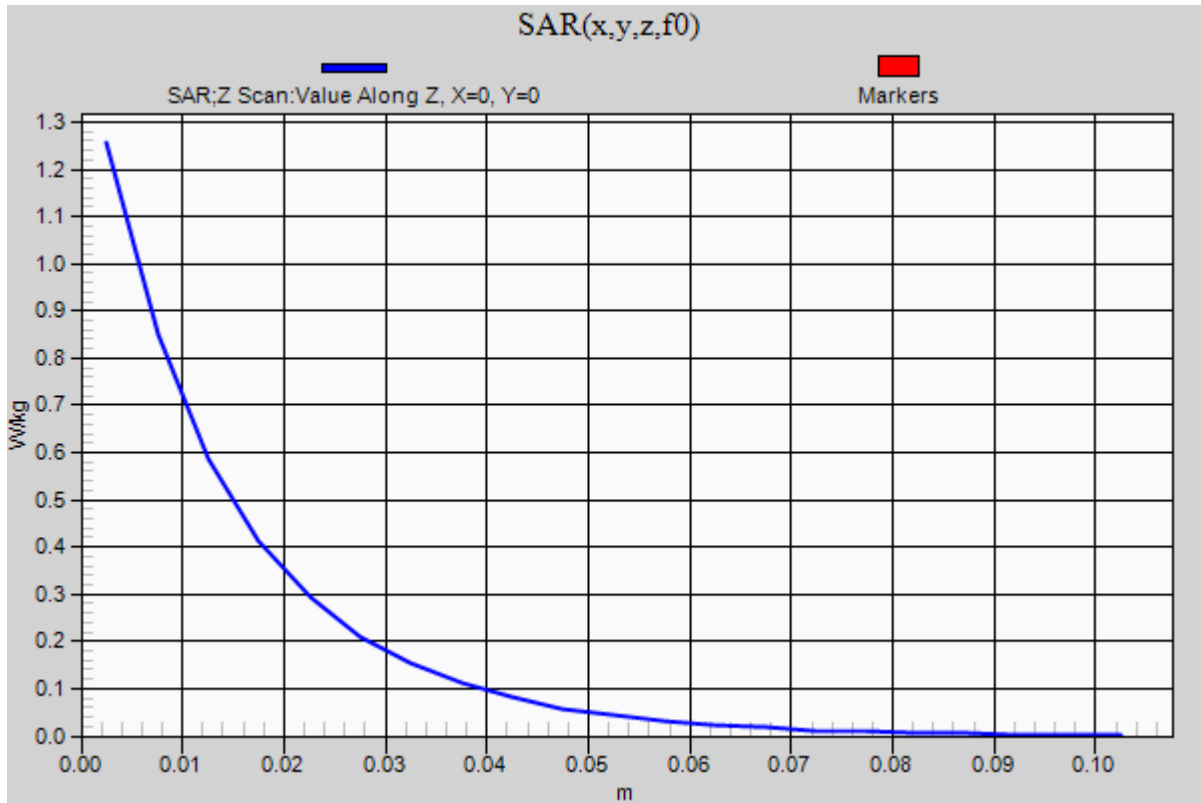


20141003_SystemPerformanceCheck-D1900V2 SN 5d043

Frequency: 1900 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used: $f = 1900 \text{ MHz}$; $\sigma = 1.57 \text{ S/m}$; $\epsilon_r = 51.05$; $\rho = 1000 \text{ kg/m}^3$
 DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(6.9, 6.9, 6.9); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Body/Pin=100 mW/Area Scan (7x7x1): Measurement grid: dx=15mm, dy=15mm
 Maximum value of SAR (measured) = 5.38 W/kg

Body/Pin=100 mW/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm
 Reference Value = 59.63 V/m; Power Drift = -0.03 dB
 Peak SAR (extrapolated) = 7.27 W/kg
SAR(1 g) = 4.01 W/kg; SAR(10 g) = 2.08 W/kg
 Maximum value of SAR (measured) = 5.43 W/kg

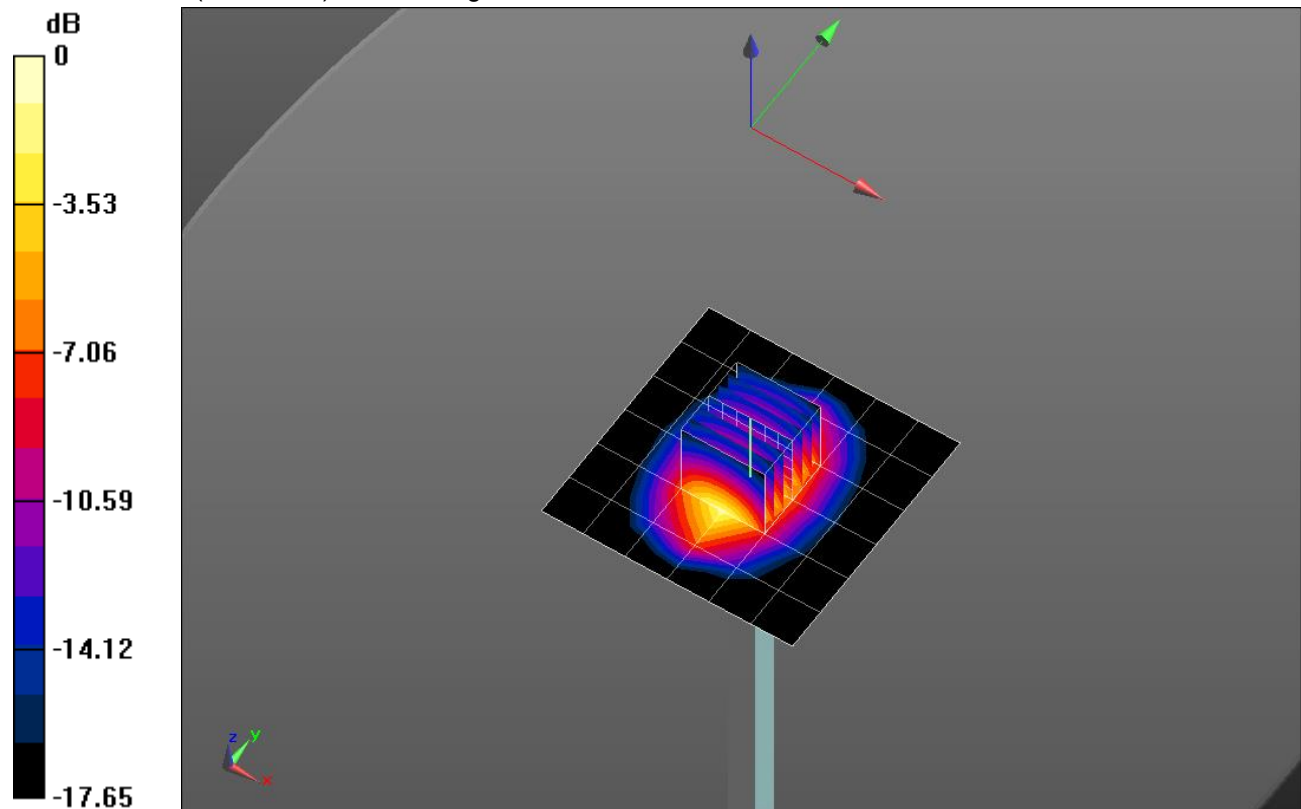


0 dB = 5.43 W/kg = 7.35 dBW/kg

20141003_SystemPerformanceCheck-D1900V2 SN 5d043

Frequency: 1900 MHz; Duty Cycle: 1:1

Body/Pin=100 mW/Z Scan (1x1x21): Measurement grid: dx=20mm, dy=20mm, dz=5mm
Maximum value of SAR (measured) = 5.46 W/kg

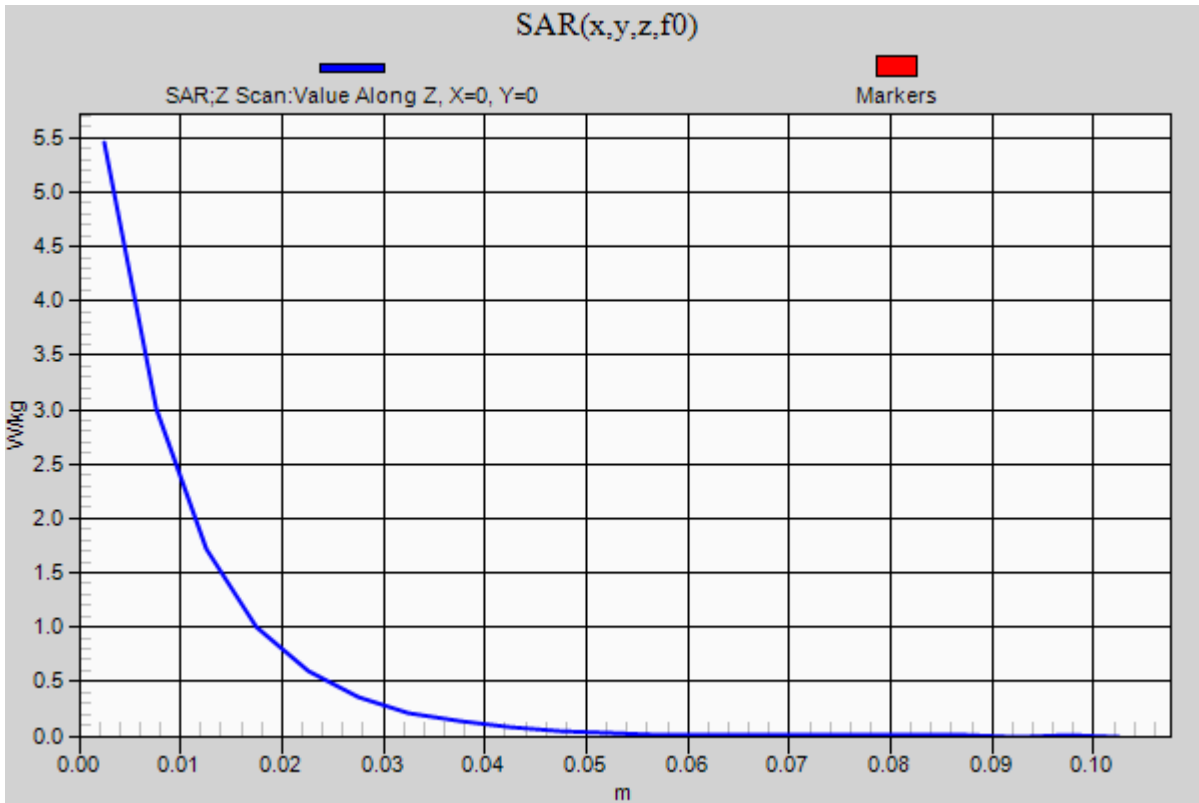

GSM 850

Frequency: 836.6 MHz; Duty Cycle: 1:8.00018; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 836.6$ MHz; $\sigma = 0.915$ S/m; $\epsilon_r = 41.699$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(8.91, 8.91, 8.91); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: SAM with CRP; Type: SAM;

RHS/Touch_GSM Voice_ch 190/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.329 W/kg

RHS/Touch_GSM Voice_ch 190/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 19.05 V/m; Power Drift = 0.05 dB

Peak SAR (extrapolated) = 0.388 W/kg

SAR(1 g) = 0.292 W/kg; SAR(10 g) = 0.215 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.332 W/kg

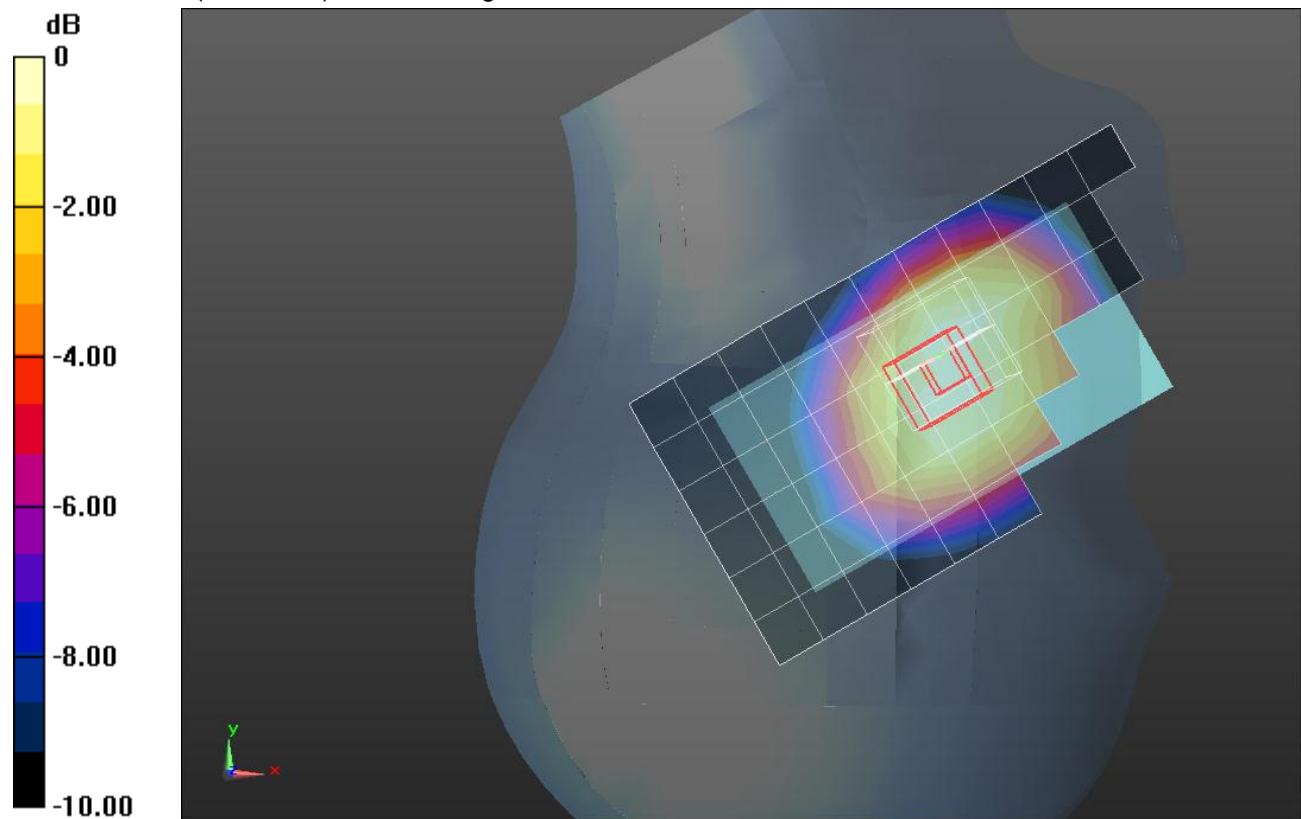

0 dB = 0.332 W/kg = -4.79 dBW/kg

GSM 850

Frequency: 836.6 MHz; Duty Cycle: 1:2.60016; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 836.6$ MHz; $\sigma = 0.915$ S/m; $\epsilon_r = 41.699$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(8.91, 8.91, 8.91); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: SAM with CRP; Type: SAM;

RHS/Touch_GPRS_3 Slot ch 190/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.356 W/kg

RHS/Touch_GPRS_3 Slot ch 190/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 19.73 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 0.409 W/kg

SAR(1 g) = 0.316 W/kg; SAR(10 g) = 0.235 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.358 W/kg

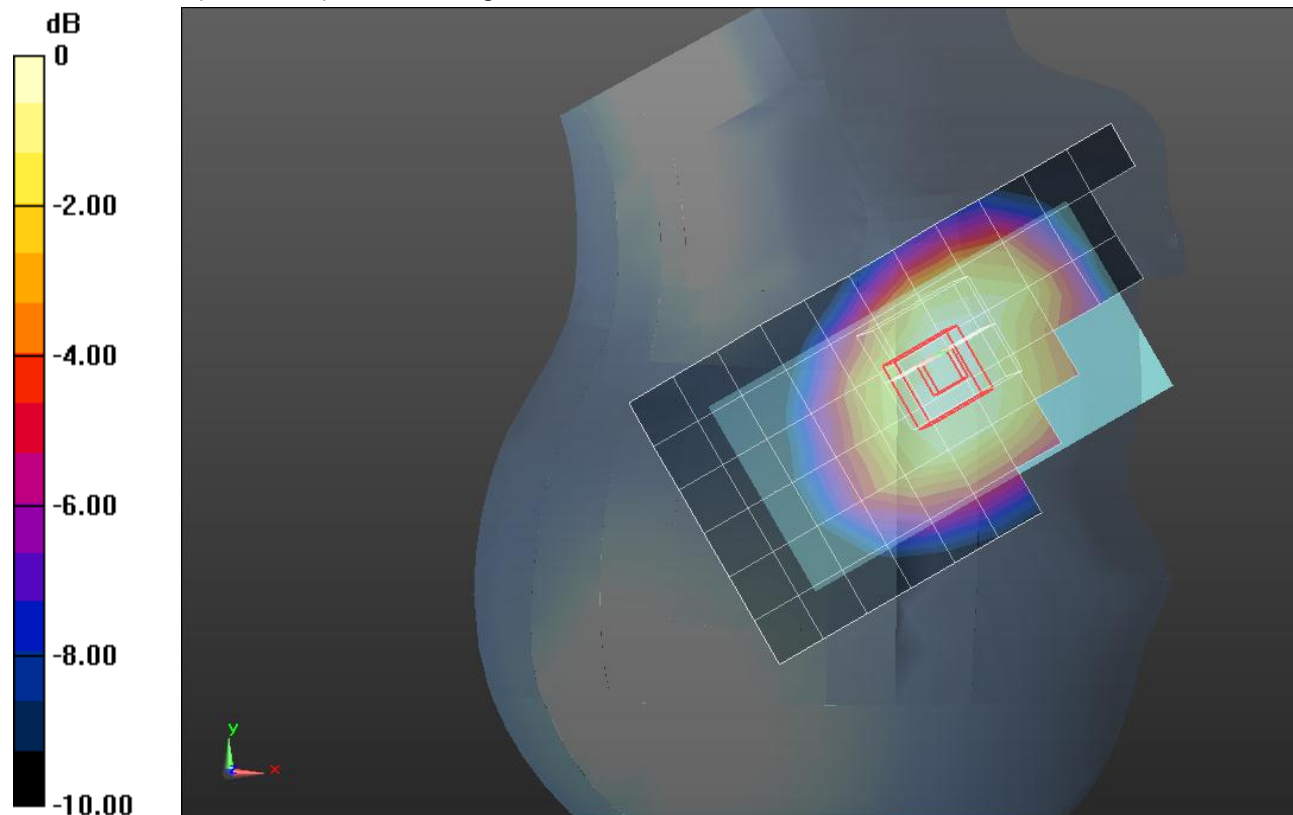

0 dB = 0.358 W/kg = -4.46 dBW/kg

GSM 850

Frequency: 836.6 MHz; Duty Cycle: 1:8.00018; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 836.6$ MHz; $\sigma = 1.018$ S/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(8.77, 8.77, 8.77); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection (Locations From Previous Scan Used)), Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Rear/GSM_Voice ch 190/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.537 W/kg

Rear/GSM_Voice ch 190/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 23.15 V/m; Power Drift = -0.02 dB

Peak SAR (extrapolated) = 0.634 W/kg

SAR(1 g) = 0.482 W/kg; SAR(10 g) = 0.355 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.548 W/kg

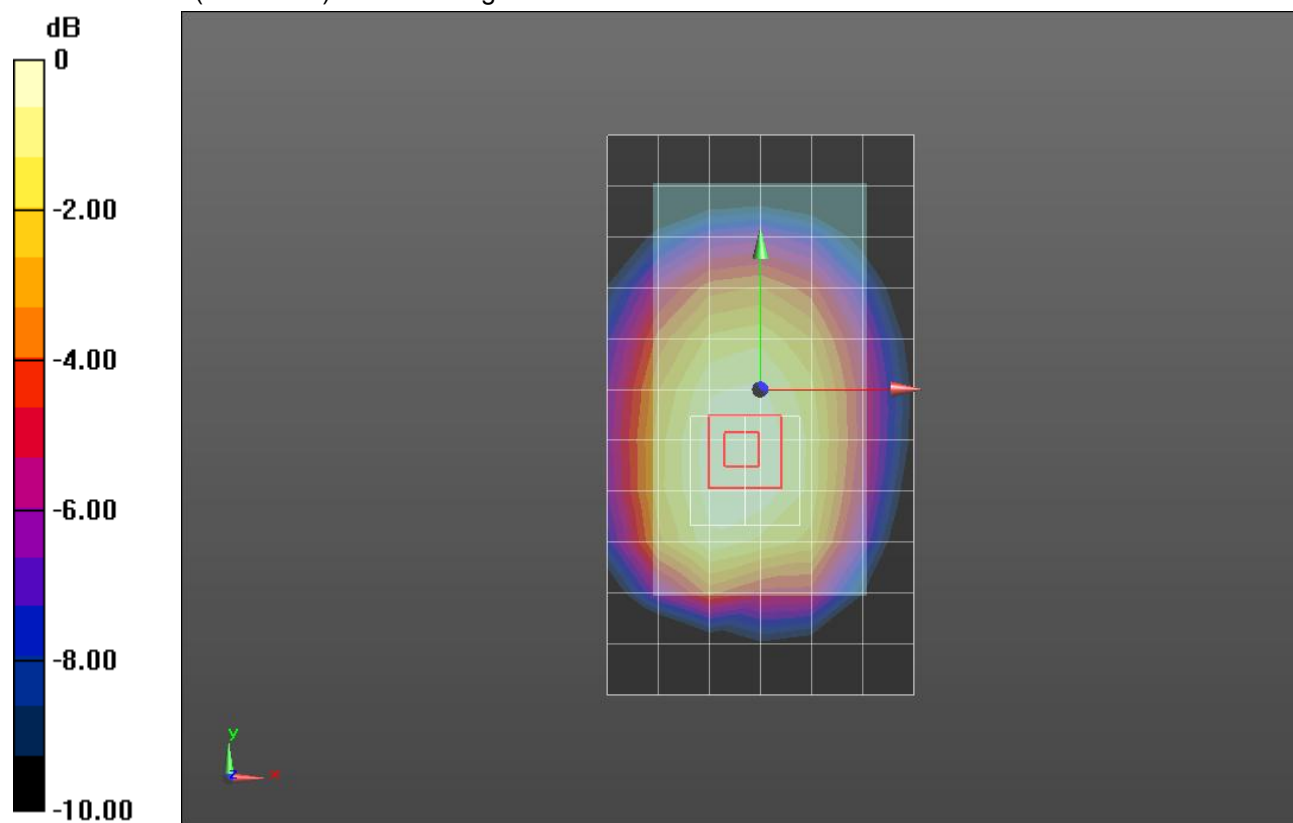

0 dB = 0.548 W/kg = -2.61 dBW/kg

GSM 850

Frequency: 836.6 MHz; Duty Cycle: 1:2.60016; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 836.6$ MHz; $\sigma = 1.018$ S/m; $\epsilon_r = 52.8$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(8.77, 8.77, 8.77); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Rear/GPRS_3 Slot ch 190/Area Scan (7x12x1):

Measurement grid: dx=15mm, dy=15mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.574 W/kg

Rear/GPRS_3 Slot ch 190/Zoom Scan (5x5x7)/Cube 0:

Measurement grid: dx=8mm, dy=8mm, dz=5mm


Reference Value = 24.16 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 0.693 W/kg

SAR(1 g) = 0.525 W/kg; SAR(10 g) = 0.385 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.595 W/kg

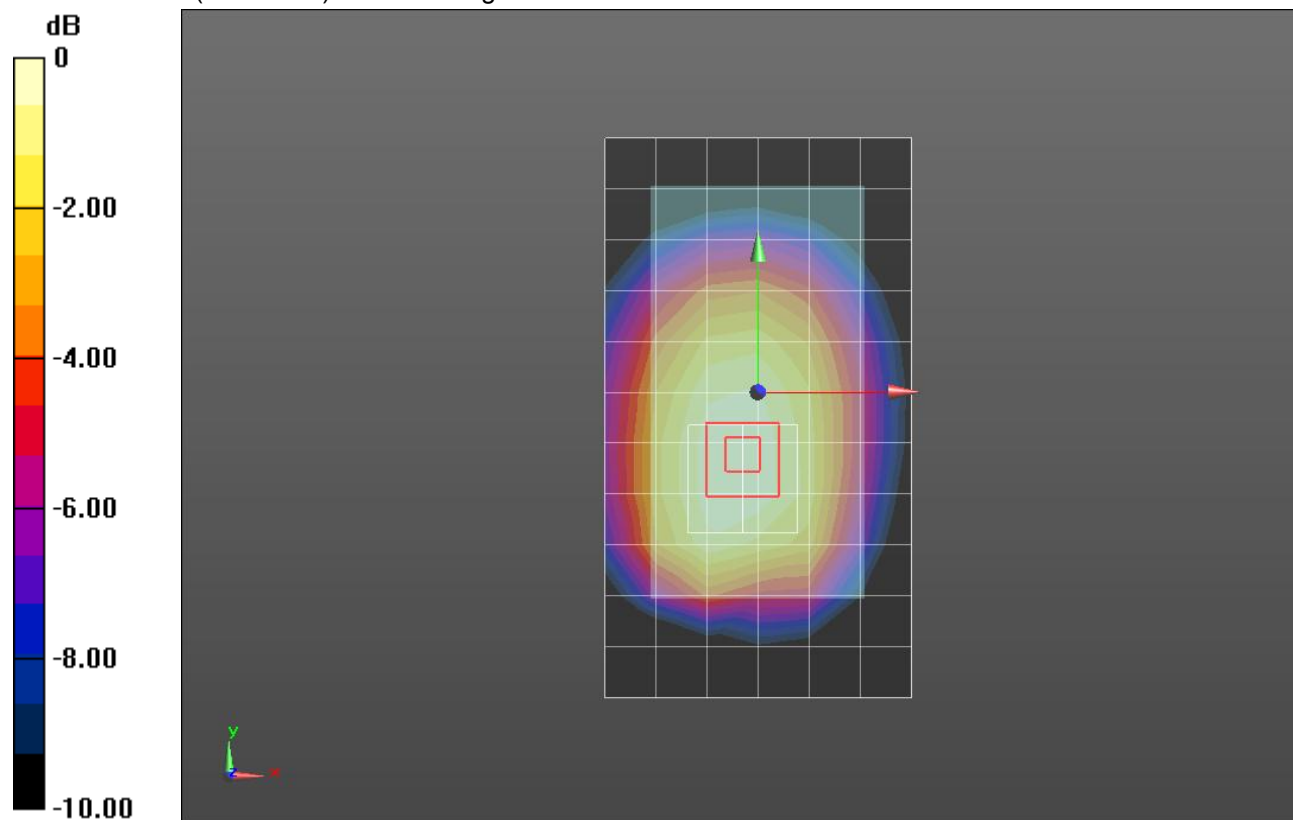

0 dB = 0.595 W/kg = -2.25 dBW/kg

GSM 1900

Frequency: 1880 MHz; Duty Cycle: 1:8.00018; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.402 \text{ S/m}$; $\epsilon_r = 40.216$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(7.26, 7.26, 7.26); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: SAM with CRP; Type: SAM;

RHS/Touch_GSM Voice_ch 661/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.408 W/kg

RHS/Touch_GSM Voice_ch 661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm,


dz=5mm

Reference Value = 17.34 V/m; Power Drift = 0.12 dB

Peak SAR (extrapolated) = 0.509 W/kg

SAR(1 g) = 0.337 W/kg; SAR(10 g) = 0.205 W/kg

Maximum value of SAR (measured) = 0.410 W/kg

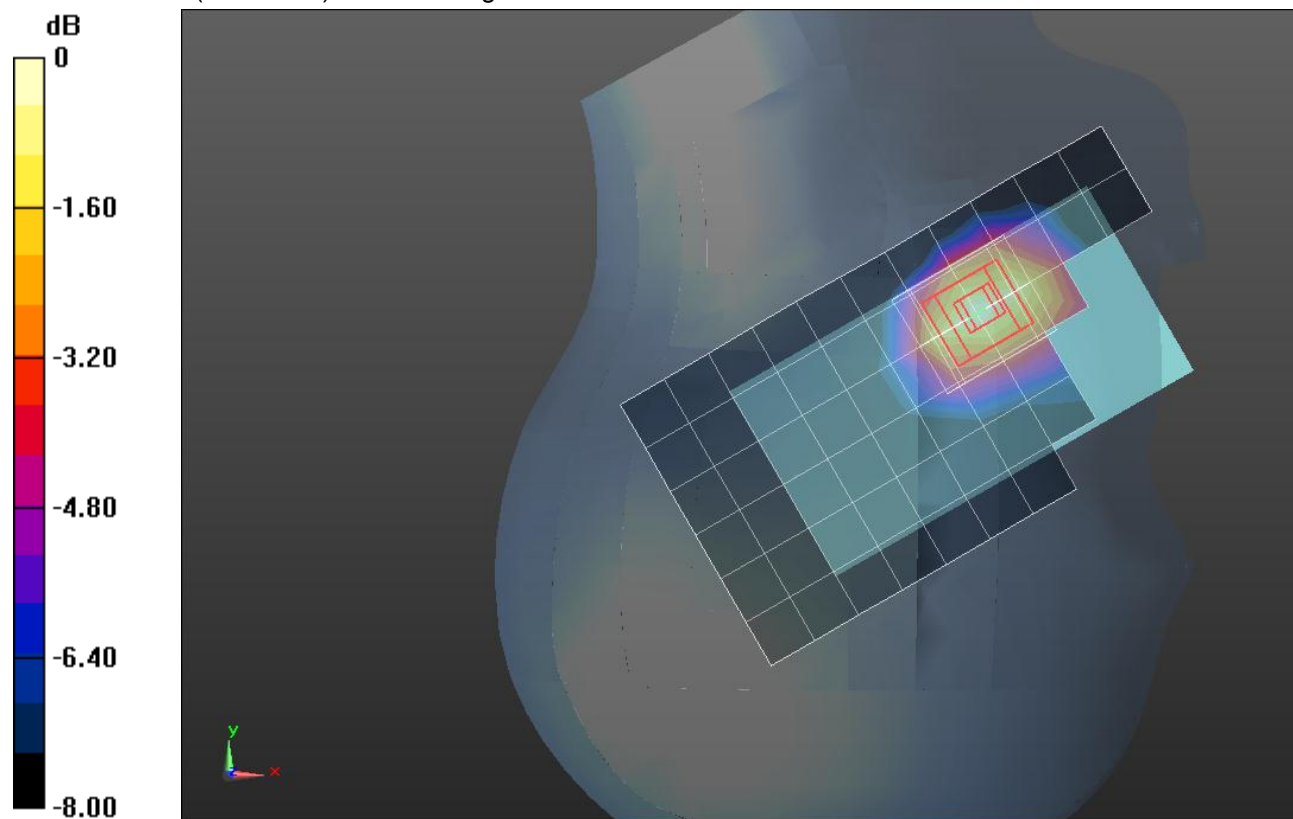

0 dB = 0.410 W/kg = -3.87 dBW/kg

GSM 1900

Frequency: 1880 MHz; Duty Cycle: 1:4.00037; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.402 \text{ S/m}$; $\epsilon_r = 40.216$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(7.26, 7.26, 7.26); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: SAM with CRP; Type: SAM;

RHS/Touch_GPRS_2 Slot ch 661/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.481 W/kg

RHS/Touch_GPRS_2 Slot ch 661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm,


dz=5mm

Reference Value = 19.21 V/m; Power Drift = -0.09 dB

Peak SAR (extrapolated) = 0.604 W/kg

SAR(1 g) = 0.402 W/kg; SAR(10 g) = 0.244 W/kg

Maximum value of SAR (measured) = 0.485 W/kg

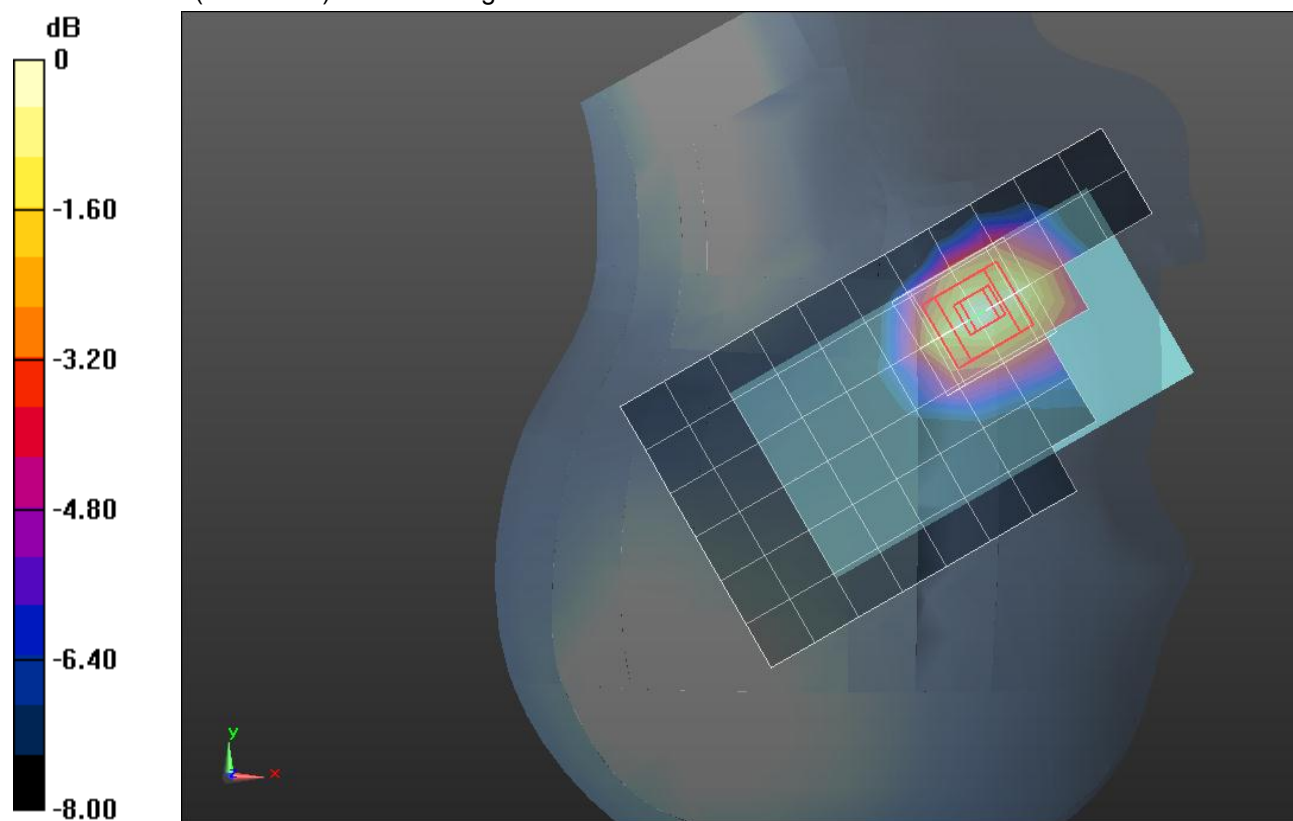

0 dB = 0.485 W/kg = -3.14 dBW/kg

GSM 1900

Frequency: 1880 MHz; Duty Cycle: 1:8.00018; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.48 \text{ S/m}$; $\epsilon_r = 53.231$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(6.9, 6.9, 6.9); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Rear/GSM_Voice ch 661/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.792 W/kg


Rear/GSM_Voice ch 661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 23.57 V/m; Power Drift = -0.06 dB

Peak SAR (extrapolated) = 1.00 W/kg

SAR(1 g) = 0.651 W/kg; SAR(10 g) = 0.396 W/kg

Maximum value of SAR (measured) = 0.796 W/kg

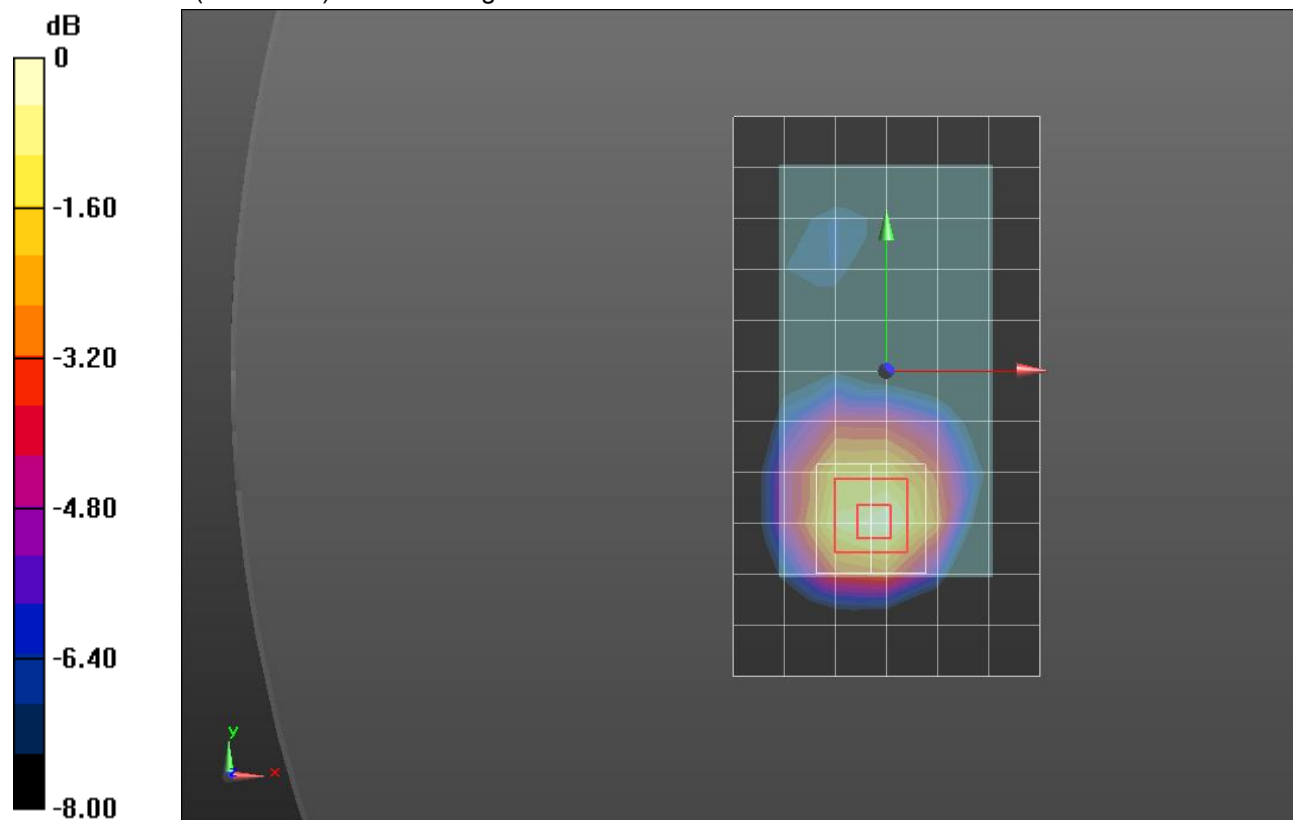

0 dB = 0.796 W/kg = -0.99 dBW/kg

GSM 1900

Frequency: 1880 MHz; Duty Cycle: 1:4.00037; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used: $f = 1880 \text{ MHz}$; $\sigma = 1.48 \text{ S/m}$; $\epsilon_r = 53.231$; $\rho = 1000 \text{ kg/m}^3$

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE4 Sn1380; Calibrated: 7/23/2014
- Probe: EX3DV4 - SN3773; ConvF(6.9, 6.9, 6.9); Calibrated: 4/22/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI v5.0 (A); Type: QDOVA001BB; Serial: 1213

Rear/GPRS_2 Slot ch 661/Area Scan (7x12x1): Measurement grid: dx=15mm, dy=15mm

Maximum value of SAR (measured) = 0.995 W/kg


Rear/GPRS_2 Slot ch 661/Zoom Scan (5x5x7)/Cube 0: Measurement grid: dx=8mm, dy=8mm, dz=5mm

Reference Value = 26.40 V/m; Power Drift = -0.04 dB

Peak SAR (extrapolated) = 1.29 W/kg

SAR(1 g) = 0.817 W/kg; SAR(10 g) = 0.492 W/kg

Maximum value of SAR (measured) = 1.02 W/kg

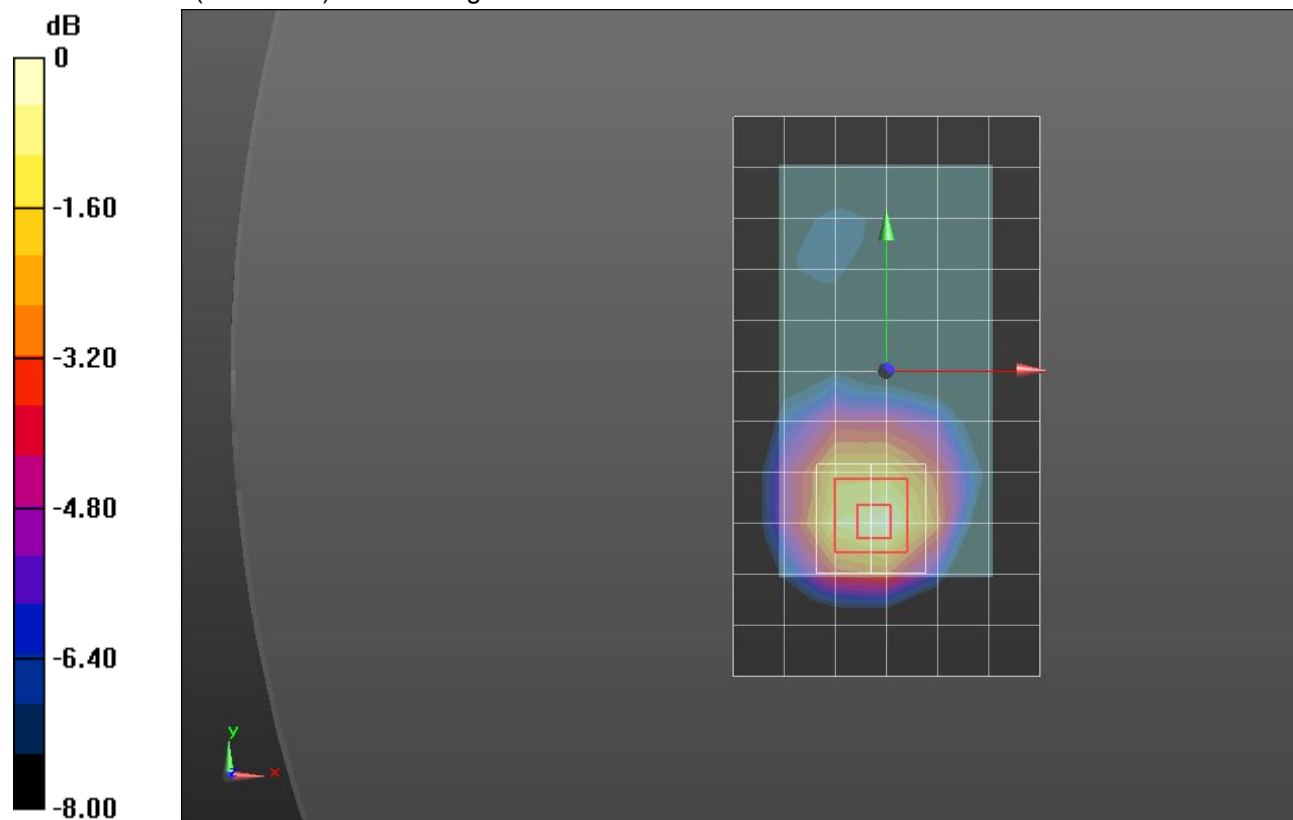

0 dB = 1.02 W/kg = 0.09 dBW/kg

Wi-Fi 2.4GHz

Frequency: 2437 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 1.723$ S/m; $\epsilon_r = 37.387$; $\rho = 1000$ kg/m³

DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE3 Sn427; Calibrated: 1/21/2014
- Probe: EX3DV4 - SN3902; ConvF(7.29, 7.29, 7.29); Calibrated: 5/19/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: SAM; Type: QD000P40CD; Serial: TP 1751

RHS/Touch_802.11b_ch 6/Area Scan (9x14x1): Measurement grid: dx=12mm, dy=12mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.536 W/kg

RHS/Touch_802.11b_ch 6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 17.330 V/m; Power Drift = 0.09 dB

Peak SAR (extrapolated) = 0.879 W/kg

SAR(1 g) = 0.424 W/kg; SAR(10 g) = 0.209 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.584 W/kg

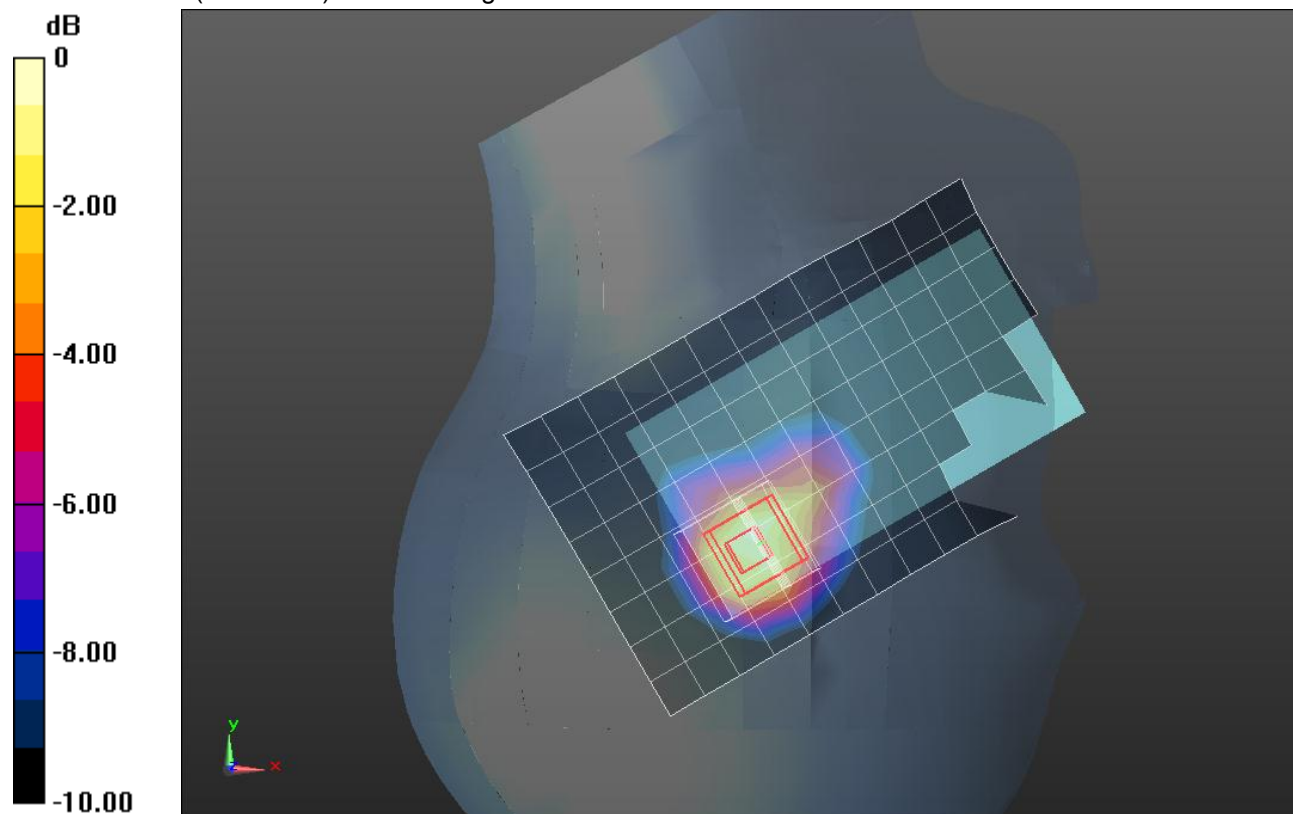

0 dB = 0.584 W/kg = -2.34 dBW/kg

Wi-Fi 2.4GHz

Frequency: 2437 MHz; Duty Cycle: 1:1; Room Ambient Temperature: 24.0°C; Liquid Temperature: 23.0°C
 Medium parameters used (interpolated): $f = 2437$ MHz; $\sigma = 2.001$ S/m; $\epsilon_r = 50.467$; $\rho = 1000$ kg/m³
 DASY5 Configuration:

- Area Scan Setting: Find Secondary Maximum Within: 2.0 dB and with a peak SAR value greater than 0.0012W/kg
- Electronics: DAE3 Sn427; Calibrated: 1/21/2014
- Probe: EX3DV4 - SN3902; ConvF(7.35, 7.35, 7.35); Calibrated: 5/19/2014;
- Sensor-Surface: 2.5mm (Mechanical Surface Detection)
- Phantom: ELI-B v5.0; Type: QDOVA002AA; Serial: TP:1195

Rear/802.11b_ch 6/Area Scan (10x15x1): Measurement grid: dx=12mm, dy=12mm

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.168 W/kg

Rear/802.11b_ch 6/Zoom Scan (7x7x7)/Cube 0: Measurement grid: dx=5mm, dy=5mm, dz=5mm


Reference Value = 9.160 V/m; Power Drift = 0.13 dB

Peak SAR (extrapolated) = 0.238 W/kg

SAR(1 g) = 0.134 W/kg; SAR(10 g) = 0.081 W/kg

[Info: Interpolated medium parameters used for SAR evaluation.](#)

Maximum value of SAR (measured) = 0.172 W/kg

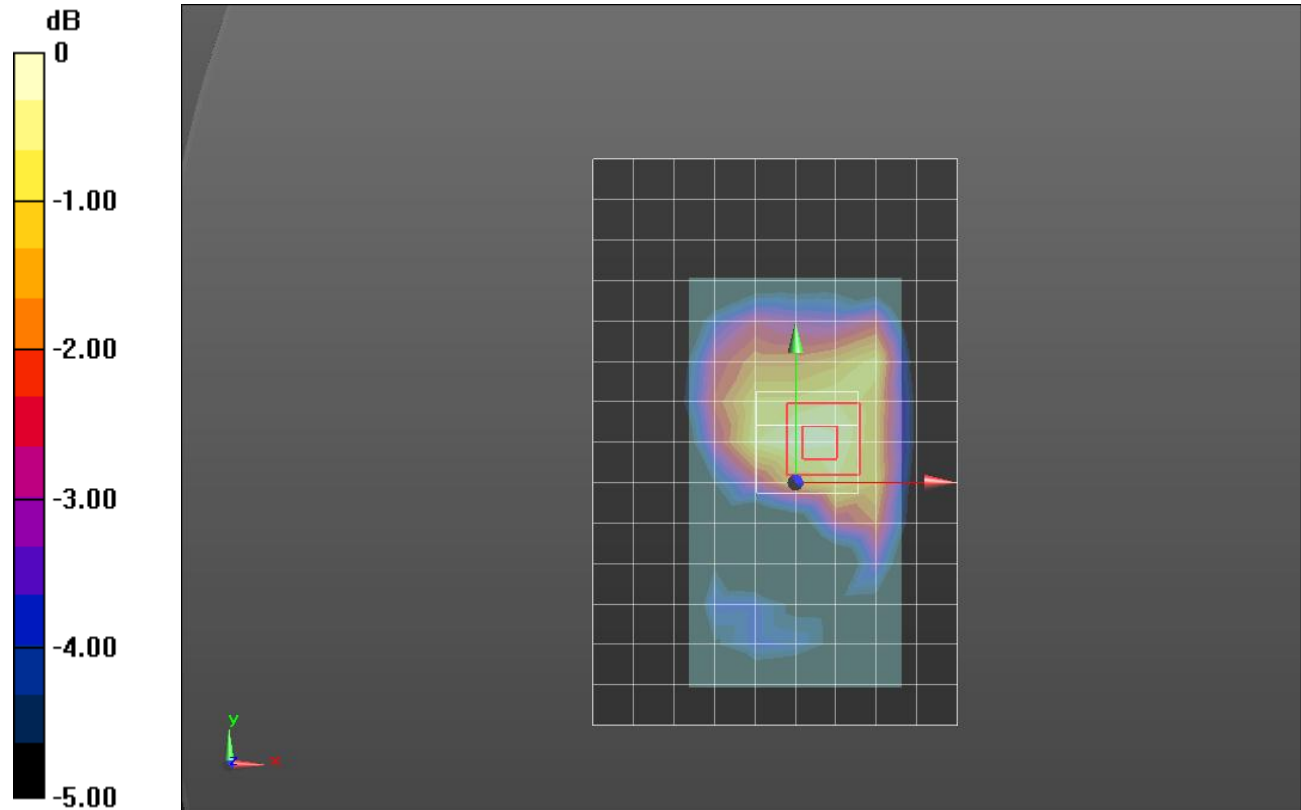

0 dB = 0.172 W/kg = -7.64 dBW/kg

Head Tissue Simulating Liquids

Head Tissue	Parameters according to IEEE Std 1528-2013 / IEC 62209 / FCC KDB 865664 D01		
Narrow-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	HSL300V2	300	Water, Sugar
	HSL450V2	450	Water, Sugar
	HSL750V2	750	Water, Sugar
	HSL900V2	835, 900	Water, Sugar
	HSL1450V2	1450, 1500, 1640	Water, DGBE
	HSL1750V2	1750	Water, DGBE
	HSL1800V2	1800, 1900	Water, DGBE
	HSL1900V2	1900	Water, DGBE
	HSL1950V2	1950, 2000	Water, DGBE
HSL2450V2	2450, 2600	Water, DGBE	
Broad-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	HBBL30-250V3	30-250	Water, Tween
	HBBL1350-1850V3	1400-1800	Water, Tween
	HBBL1550-1950V3	1750-1900	Water, Tween
	HBBL1900-3800V3	1950-3000	Water, Tween
HBBL3500-5800V5	3500-5800	Water, Oil	

Body Tissue Simulating Liquids

Body Tissue (Muscle)	Parameters according to FCC KDB 865664 D01		
Narrow-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	MSL300V2	300	Water, Sugar
	MSL450V2	400, 450	Water, Sugar
	MSL750V2	750	Water, Sugar
	MSL900V2	835, 900	Water, Sugar
	MSL1450V2	1450, 1500, 1640	Water, DGBE
	MSL1750V2	1750	Water, DGBE
	MSL1800V2	1800, 1900	Water, DGBE
	MSL1900V2	1900	Water, DGBE
	MSL1950V2	1950, 2100	Water, DGBE
MSL2450V2	2450, 2600	Water, DGBE	
Broad-Band Solutions (±5% tolerance)	Product	Test Frequency (MHz)	Main Ingredients
	MBBL130-250V3	130-250	Water, Tween
	MBBL1350-1850V3	1350-1800	Water, Tween
	MBBL1550-1950V3	1550-1850	Water, Tween
	MBBL1900-3800V3	1950-3800	Water, Tween
MBBL3500-5800V5	3500-5800	Water, Oil	

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL750V2)
Product No.	SL AAH 075 AA (Charge: 140210-5)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

Additional Information

TSL Density	1.284 g/cm ³
TSL Heat-capacity	2.701 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
600	44.4	23.49	0.78	42.7	0.88	3.9	-11.1
625	44.1	23.23	0.81	42.6	0.88	3.5	-8.6
650	43.7	22.96	0.83	42.5	0.89	3.0	-6.2
675	43.3	22.68	0.85	42.3	0.89	2.4	-4.1
700	42.9	22.40	0.87	42.2	0.89	1.7	-1.9
725	42.6	22.25	0.90	42.1	0.89	1.3	0.7
750	42.3	22.10	0.92	41.9	0.89	0.9	3.2
775	42.0	21.89	0.94	41.8	0.90	0.4	5.4
800	41.6	21.67	0.96	41.7	0.90	-0.1	7.5
825	41.3	21.55	0.99	41.6	0.91	-0.6	9.0
838	41.2	21.49	1.00	41.5	0.91	-0.8	9.8
850	41.1	21.42	1.01	41.5	0.92	-1.1	10.6
875	40.8	21.29	1.04	41.5	0.94	-1.8	9.9
900	40.5	21.15	1.06	41.5	0.97	-2.5	9.2
925	40.2	21.01	1.08	41.5	0.98	-3.1	10.0
950	39.9	20.87	1.10	41.4	0.99	-3.7	10.9
975	39.6	20.79	1.13	41.4	1.00	-4.3	12.2
1000	39.4	20.71	1.15	41.3	1.01	-4.8	13.5

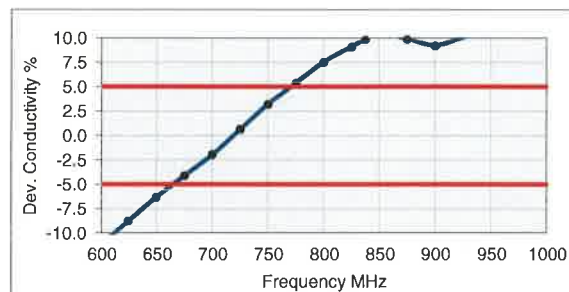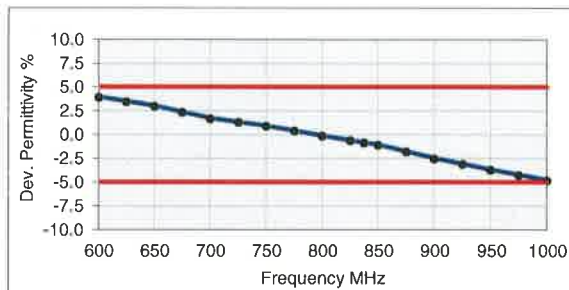

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL900V2)
Product No.	SL AAH 090 BB (Charge: 140205-4)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	12-Feb-14
Operator	IEN

Additional Information

TSL Density	1.280 g/cm ³
TSL Heat-capacity	2.942 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
700	42.9	19.58	0.76	42.2	0.89	1.6	-14.3
725	42.6	19.52	0.79	42.1	0.89	1.2	-11.7
750	42.3	19.47	0.81	41.9	0.89	0.8	-9.1
775	41.9	19.35	0.83	41.8	0.90	0.3	-6.8
800	41.6	19.23	0.86	41.7	0.90	-0.3	-4.6
825	41.3	19.18	0.88	41.6	0.91	-0.7	-2.9
838	41.1	19.16	0.89	41.5	0.91	-1.0	-2.1
850	41.0	19.13	0.90	41.5	0.92	-1.2	-1.2
875	40.7	19.07	0.93	41.5	0.94	-1.9	-1.6
900	40.4	19.00	0.95	41.5	0.97	-2.7	-1.9
925	40.1	18.92	0.97	41.5	0.98	-3.3	-0.9
950	39.8	18.85	1.00	41.4	0.99	-3.9	0.2
975	39.6	18.82	1.02	41.4	1.00	-4.4	1.6
1000	39.3	18.80	1.05	41.3	1.01	-5.0	3.0
1025	39.0	18.71	1.07	41.3	1.03	-5.5	4.0
1050	38.8	18.62	1.09	41.2	1.04	-6.0	5.0
1075	38.5	18.59	1.11	41.2	1.05	-6.5	6.3
1100	38.3	18.55	1.14	41.2	1.06	-7.0	7.5
1125	38.0	18.50	1.16	41.1	1.07	-7.5	8.5
1150	37.8	18.44	1.18	41.1	1.08	-8.0	9.6
1175	37.5	18.39	1.20	41.0	1.09	-8.4	10.6
1200	37.3	18.35	1.22	41.0	1.10	-8.9	11.6

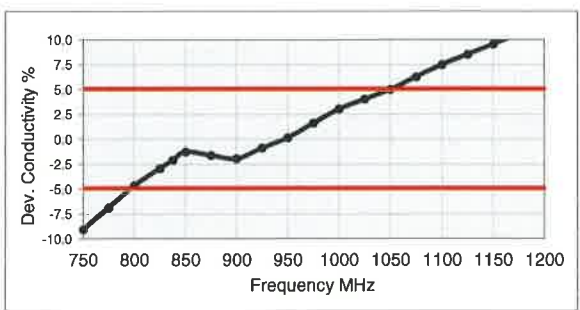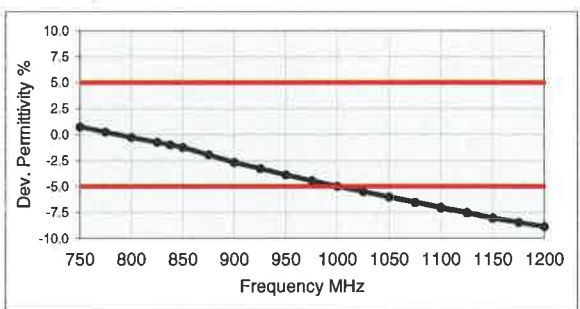

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HSL1750V2)**
 Product No. SL AAH 175 (Charge: 120907-2)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 13-Sep-12
 Operator CL

Additional Information

TSL Density 0.998 g/cm³
 TSL Heat-capacity 3.572 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1400	41.2	13.09	1.02	40.6	1.18	1.4	-13.6
1425	41.0	13.14	1.04	40.5	1.19	1.2	-12.4
1450	40.9	13.19	1.06	40.5	1.20	1.1	-11.3
1475	40.8	13.26	1.09	40.5	1.21	0.8	-10.3
1500	40.7	13.34	1.11	40.4	1.23	0.6	-9.4
1525	40.6	13.39	1.14	40.4	1.24	0.4	-8.6
1550	40.5	13.44	1.16	40.4	1.26	0.3	-7.8
1575	40.3	13.49	1.18	40.3	1.27	0.0	-6.9
1600	40.2	13.55	1.21	40.3	1.28	-0.2	-6.1
1613	40.2	13.58	1.22	40.3	1.29	-0.3	-5.7
1625	40.1	13.62	1.23	40.3	1.30	-0.4	-5.2
1638	40.1	13.65	1.24	40.3	1.31	-0.5	-4.8
1650	40.0	13.68	1.26	40.2	1.31	-0.5	-4.3
1663	40.0	13.70	1.27	40.2	1.32	-0.6	-4.1
1675	39.9	13.71	1.28	40.2	1.33	-0.7	-3.8
1688	39.8	13.72	1.29	40.2	1.33	-0.8	-3.5
1700	39.8	13.73	1.30	40.2	1.34	-0.9	-3.2
1713	39.7	13.77	1.31	40.1	1.35	-1.0	-2.7
1725	39.7	13.81	1.33	40.1	1.36	-1.1	-2.3
1738	39.6	13.85	1.34	40.1	1.36	-1.2	-1.8
1750	39.6	13.89	1.35	40.1	1.37	-1.3	-1.4
1763	39.5	13.91	1.36	40.1	1.38	-1.3	-1.0
1775	39.5	13.93	1.38	40.0	1.39	-1.4	-0.7
1788	39.4	13.95	1.39	40.0	1.39	-1.4	-0.4
1800	39.4	13.97	1.40	40.0	1.40	-1.5	-0.1
1813	39.3	14.01	1.41	40.0	1.40	-1.7	0.9
1825	39.3	14.04	1.43	40.0	1.40	-1.8	1.8
1838	39.2	14.08	1.44	40.0	1.40	-2.0	2.8
1850	39.2	14.11	1.45	40.0	1.40	-2.1	3.8
1863	39.1	14.14	1.47	40.0	1.40	-2.2	4.7
1875	39.1	14.17	1.48	40.0	1.40	-2.3	5.6
1888	39.0	14.19	1.49	40.0	1.40	-2.5	6.5
1900	39.0	14.22	1.50	40.0	1.40	-2.6	7.4

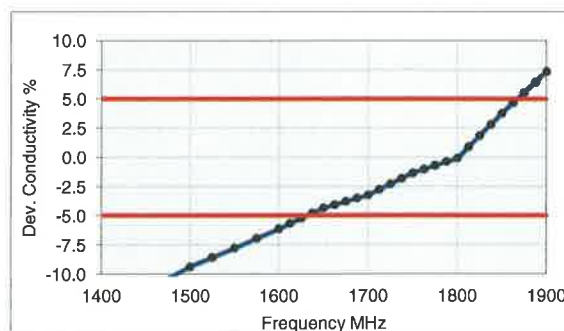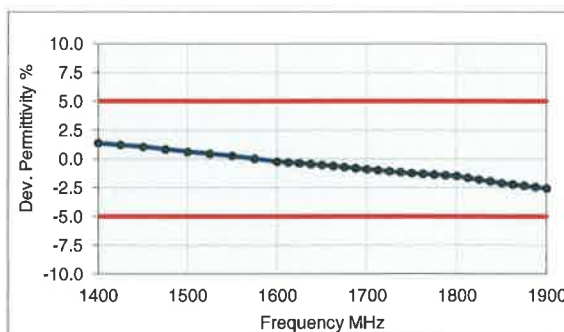

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL 1900)
Product No.	SL AAH 190 AA (Charge: 120112-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe (type DAK).

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition



Ambient Condition 22°C ; 30% humidity
 TSL Temperature 22°C
 Test Date 18-Jan-12

Additional Information

TSL Density 0.985 g/cm³
 TSL Heat-capacity 3.710 kJ/(kg*K)

Results

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-ε'	HP-ε''	sigma	eps	sigma	Δ-eps	Δ-sigma
1600	41.2	12.84	1.14	40.3	1.28	2.1	-11.0
1613	41.1	12.88	1.16	40.3	1.29	2.0	-10.5
1625	41.1	12.93	1.17	40.3	1.30	1.9	-10.0
1638	41.0	12.97	1.18	40.3	1.31	1.8	-9.5
1650	40.9	13.01	1.19	40.2	1.31	1.8	-9.1
1663	40.9	13.05	1.21	40.2	1.32	1.7	-8.6
1675	40.8	13.10	1.22	40.2	1.33	1.6	-8.1
1688	40.8	13.14	1.23	40.2	1.33	1.4	-7.6
1700	40.7	13.18	1.25	40.2	1.34	1.3	-7.1
1713	40.6	13.22	1.26	40.1	1.35	1.2	-6.7
1725	40.6	13.25	1.27	40.1	1.36	1.1	-6.3
1738	40.5	13.28	1.28	40.1	1.36	1.0	-5.9
1750	40.5	13.31	1.30	40.1	1.37	0.9	-5.5
1763	40.4	13.35	1.31	40.1	1.38	0.9	-5.1
1775	40.4	13.38	1.32	40.0	1.39	0.8	-4.7
1788	40.3	13.41	1.33	40.0	1.39	0.7	-4.3
1800	40.3	13.44	1.35	40.0	1.40	0.6	-3.9
1813	40.2	13.48	1.36	40.0	1.40	0.5	-2.9
1825	40.2	13.52	1.37	40.0	1.40	0.4	-2.0
1838	40.1	13.55	1.39	40.0	1.40	0.3	-1.0
1850	40.1	13.59	1.40	40.0	1.40	0.1	-0.1
1863	40.0	13.63	1.41	40.0	1.40	0.0	0.9
1875	39.9	13.67	1.43	40.0	1.40	-0.1	1.9
1888	39.9	13.71	1.44	40.0	1.40	-0.3	2.9
1900	39.8	13.75	1.45	40.0	1.40	-0.4	3.8
1913	39.8	13.79	1.47	40.0	1.40	-0.5	4.8
1925	39.7	13.83	1.48	40.0	1.40	-0.7	5.8
1938	39.7	13.86	1.49	40.0	1.40	-0.8	6.7
1950	39.6	13.90	1.51	40.0	1.40	-0.9	7.7
1975	39.5	13.97	1.53	40.0	1.40	-1.2	9.6
2000	39.4	14.04	1.56	40.0	1.40	-1.5	11.6

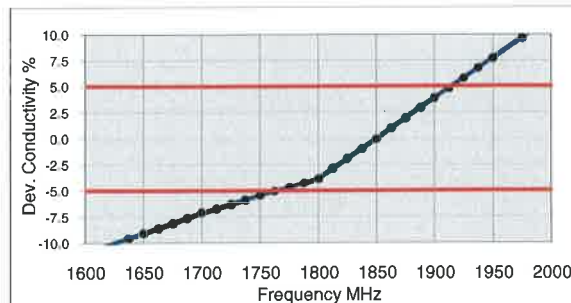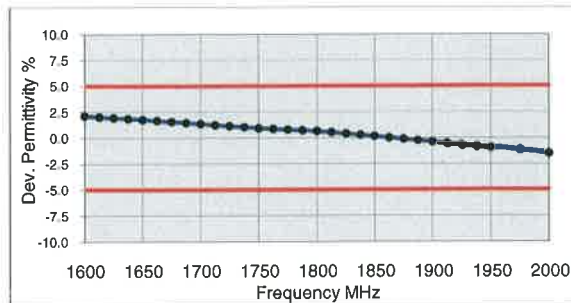

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HSL1950V2)**
 Product No. SL AAH 195 CA (Charge: 120717-3)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters



Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 18-Jul-12
 Operator DI

TSL Density 0.995 g/cm³
 TSL Heat-capacity 3.720 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
1850	40.6	12.43	1.28	40.0	1.40	1.5	-8.6
1875	40.5	12.53	1.31	40.0	1.40	1.2	-6.7
1900	40.3	12.62	1.33	40.0	1.40	0.9	-4.7
1925	40.2	12.71	1.36	40.0	1.40	0.6	-2.8
1950	40.1	12.80	1.39	40.0	1.40	0.3	-0.8
1975	40.0	12.89	1.42	40.0	1.40	0.0	1.1
2000	39.9	12.98	1.44	40.0	1.40	-0.3	3.1
2025	39.8	13.07	1.47	40.0	1.42	-0.4	3.5
2050	39.7	13.16	1.50	39.9	1.44	-0.6	3.9
2075	39.6	13.23	1.53	39.9	1.47	-0.8	4.2
2100	39.5	13.30	1.55	39.8	1.49	-0.9	4.4
2125	39.3	13.37	1.58	39.8	1.51	-1.1	4.6
2150	39.2	13.44	1.61	39.7	1.53	-1.2	4.9
2175	39.1	13.52	1.64	39.7	1.56	-1.4	5.2
2200	39.1	13.61	1.67	39.6	1.58	-1.5	5.5
2225	38.9	13.68	1.69	39.6	1.60	-1.7	5.9
2250	38.8	13.76	1.72	39.6	1.62	-1.9	6.2
2275	38.7	13.83	1.75	39.5	1.64	-2.0	6.5
2300	38.6	13.91	1.78	39.5	1.67	-2.2	6.8
2325	38.5	13.98	1.81	39.4	1.69	-2.3	7.1
2350	38.4	14.06	1.84	39.4	1.71	-2.5	7.4
2375	38.3	14.13	1.87	39.3	1.73	-2.7	7.7
2400	38.2	14.21	1.90	39.3	1.76	-2.8	8.0
2425	38.1	14.28	1.93	39.2	1.78	-3.0	8.4
2450	38.0	14.36	1.96	39.2	1.80	-3.1	8.7
2475	37.9	14.42	1.99	39.2	1.83	-3.3	8.7
2500	37.8	14.49	2.02	39.1	1.85	-3.5	8.7
2525	37.6	14.56	2.04	39.1	1.88	-3.7	8.7
2550	37.5	14.62	2.07	39.1	1.91	-3.9	8.7
2575	37.4	14.69	2.10	39.0	1.94	-4.1	8.7
2600	37.3	14.76	2.13	39.0	1.96	-4.3	8.7

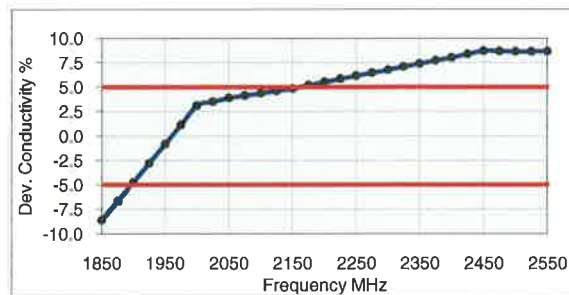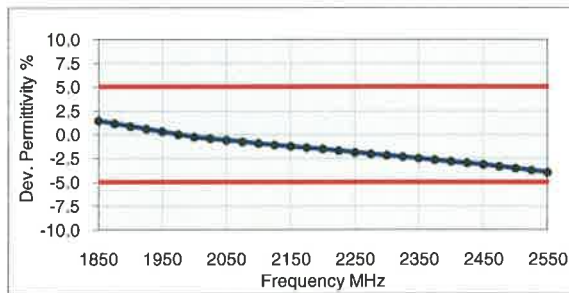

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HSL2450V2)
Product No.	SL AAH 245 BA (Charge: 130430-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	23°C
Test Date	2-May-13
Operator	CL

Additional Information

TSL Density	0.988 g/cm ³
TSL Heat-capacity	3.680 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1900	41.6	11.98	1.27	40.0	1.40	4.0	-9.6
1925	41.5	12.06	1.29	40.0	1.40	3.8	-7.7
1950	41.4	12.15	1.32	40.0	1.40	3.5	-5.9
1975	41.3	12.24	1.35	40.0	1.40	3.3	-3.9
2000	41.2	12.34	1.37	40.0	1.40	3.0	-1.9
2025	41.1	12.44	1.40	40.0	1.42	2.9	-1.5
2050	41.0	12.54	1.43	39.9	1.44	2.8	-1.0
2075	40.9	12.62	1.46	39.9	1.47	2.6	-0.6
2100	40.8	12.71	1.48	39.8	1.49	2.5	-0.3
2125	40.7	12.80	1.51	39.8	1.51	2.3	0.1
2150	40.6	12.88	1.54	39.7	1.53	2.2	0.5
2175	40.5	12.97	1.57	39.7	1.56	2.0	0.9
2200	40.4	13.05	1.60	39.6	1.58	1.9	1.3
2225	40.3	13.13	1.63	39.6	1.60	1.7	1.6
2250	40.2	13.21	1.65	39.6	1.62	1.6	1.9
2275	40.1	13.30	1.68	39.5	1.64	1.5	2.4
2300	40.0	13.39	1.71	39.5	1.67	1.3	2.8
2325	39.9	13.48	1.74	39.4	1.69	1.2	3.2
2350	39.8	13.56	1.77	39.4	1.71	1.0	3.6
2375	39.7	13.64	1.80	39.3	1.73	0.9	4.0
2400	39.6	13.72	1.83	39.3	1.76	0.8	4.3
2425	39.5	13.80	1.86	39.2	1.78	0.6	4.8
2450	39.4	13.89	1.89	39.2	1.80	0.5	5.2
2475	39.3	13.96	1.92	39.2	1.83	0.3	5.2
2500	39.2	14.03	1.95	39.1	1.85	0.1	5.2
2525	39.1	14.12	1.98	39.1	1.88	-0.1	5.4
2550	39.0	14.22	2.02	39.1	1.91	-0.3	5.6
2575	38.9	14.28	2.05	39.0	1.94	-0.5	5.6
2600	38.7	14.34	2.07	39.0	1.96	-0.7	5.6
2625	38.6	14.41	2.10	39.0	1.99	-0.9	5.7
2650	38.5	14.48	2.13	38.9	2.02	-1.1	5.8
2675	38.4	14.55	2.17	38.9	2.05	-1.3	5.9
2700	38.3	14.62	2.20	38.9	2.07	-1.4	6.0

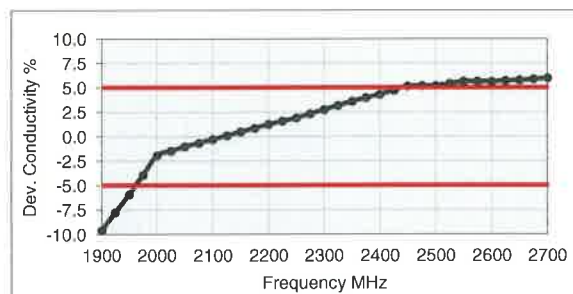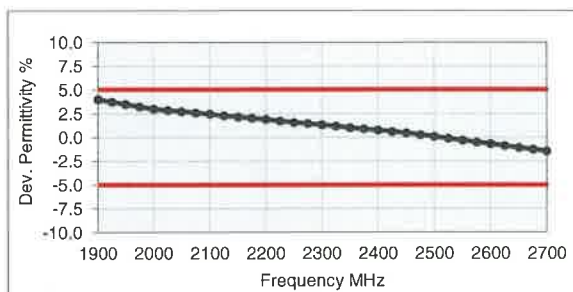

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speg.com, http://www.speg.com

Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HBBL1550-1950V3)**
 Product No. SL AAH 181 AA (Charge: 140206-3)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 12-Feb-14
 Operator IEN

Additional Information

TSL Density 1.052 g/cm³
 TSL Heat-capacity 3.322 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1500	40.8	13.29	1.11	40.4	1.23	0.9	-9.7
1525	40.7	13.34	1.13	40.4	1.24	0.7	-8.9
1550	40.6	13.38	1.15	40.4	1.26	0.6	-8.2
1575	40.5	13.41	1.17	40.3	1.27	0.4	-7.5
1600	40.4	13.44	1.20	40.3	1.28	0.2	-6.9
1625	40.3	13.48	1.22	40.3	1.30	0.1	-6.2
1650	40.2	13.53	1.24	40.2	1.31	-0.1	-5.4
1675	40.1	13.54	1.26	40.2	1.33	-0.3	-5.0
1700	40.0	13.55	1.28	40.2	1.34	-0.4	-4.5
1725	39.9	13.60	1.30	40.1	1.36	-0.6	-3.8
1750	39.8	13.64	1.33	40.1	1.37	-0.7	-3.1
1775	39.7	13.67	1.35	40.0	1.39	-0.9	-2.6
1800	39.6	13.70	1.37	40.0	1.40	-1.0	-2.0
1825	39.5	13.75	1.40	40.0	1.40	-1.2	-0.3
1850	39.4	13.81	1.42	40.0	1.40	-1.5	1.5
1875	39.3	13.84	1.44	40.0	1.40	-1.7	3.1
1900	39.2	13.88	1.47	40.0	1.40	-2.0	4.8
1925	39.1	13.92	1.49	40.0	1.40	-2.2	6.5
1950	39.0	13.97	1.52	40.0	1.40	-2.4	8.3
1975	38.9	14.01	1.54	40.0	1.40	-2.6	10.0
2000	38.8	14.05	1.56	40.0	1.40	-2.9	11.6

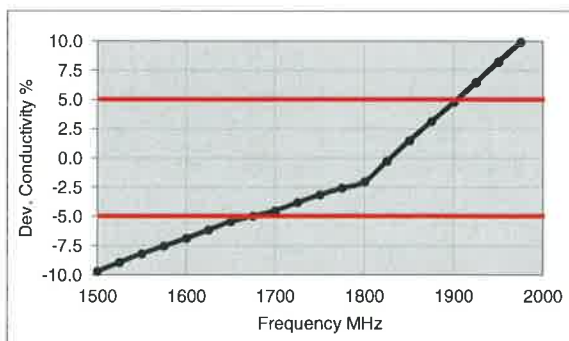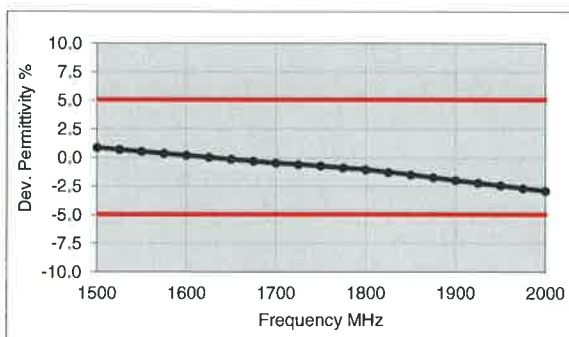

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Head Tissue Simulating Liquid (HBBL1900-3800V3)**
 Product No. SL AAH 196 AB (Charge: 131212-1)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 18-Dec-13
 Operator IEN

Additional Information

TSL Density 1.054 g/cm³
 TSL Heat-capacity 3.389 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1900	41.0	12.2	1.3	40.0	1.4	2.5	-7.9
1950	40.8	12.3	1.3	40.0	1.4	2.1	-4.7
2000	40.7	12.4	1.4	40.0	1.4	1.7	-1.3
2050	40.5	12.6	1.4	39.9	1.4	1.6	-0.6
2100	40.4	12.7	1.5	39.8	1.5	1.4	-0.6
2150	40.2	12.8	1.5	39.7	1.5	1.2	-0.4
2200	40.0	12.9	1.6	39.6	1.6	1.0	0.1
2250	39.9	13.0	1.6	39.6	1.6	0.8	0.4
2300	39.7	13.2	1.7	39.5	1.7	0.5	1.3
2350	39.5	13.3	1.7	39.4	1.7	0.3	1.8
2400	39.3	13.5	1.8	39.3	1.8	0.1	2.4
2450	39.1	13.6	1.9	39.2	1.8	-0.1	2.8
2500	39.0	13.7	1.9	39.1	1.9	-0.4	2.6
2550	38.8	13.8	2.0	39.1	1.9	-0.6	2.7
2600	38.6	14.0	2.0	39.0	2.0	-1.0	2.8
2650	38.4	14.0	2.1	38.9	2.0	-1.4	2.5
2700	38.2	14.2	2.1	38.9	2.1	-1.7	2.7
2750	38.0	14.3	2.2	38.8	2.1	-2.1	2.5
2800	37.8	14.4	2.2	38.8	2.2	-2.4	2.6
2850	37.6	14.5	2.3	38.7	2.2	-2.7	2.6
2900	37.5	14.6	2.4	38.6	2.3	-2.9	2.6
2950	37.3	14.6	2.4	38.6	2.3	-3.3	2.5
3000	37.1	14.7	2.5	38.5	2.4	-3.6	2.3
3050	36.9	14.8	2.5	38.4	2.5	-3.9	2.6
3100	36.7	14.9	2.6	38.4	2.5	-4.3	2.6
3150	36.6	15.0	2.6	38.3	2.6	-4.6	2.8
3200	36.4	15.0	2.7	38.3	2.6	-4.9	2.8
3250	36.2	15.1	2.7	38.2	2.7	-5.2	3.0
3300	36.1	15.2	2.8	38.2	2.7	-5.5	3.0
3350	35.9	15.2	2.8	38.1	2.8	-5.8	2.9
3400	35.7	15.3	2.9	38.0	2.8	-6.0	2.8
3450	35.6	15.3	2.9	38.0	2.9	-6.3	2.8
3500	35.4	15.4	3.0	37.9	2.9	-6.6	2.8
3550	35.3	15.4	3.0	37.9	3.0	-6.9	2.9
3600	35.1	15.5	3.1	37.8	3.0	-7.2	2.9
3650	34.9	15.5	3.2	37.8	3.1	-7.5	2.9
3700	34.7	15.6	3.2	37.7	3.1	-7.8	3.2
3750	34.6	15.7	3.3	37.6	3.2	-8.1	3.2
3800	34.5	15.7	3.3	37.6	3.2	-8.3	3.4
3850	34.3	15.8	3.4	37.5	3.3	-8.5	3.2

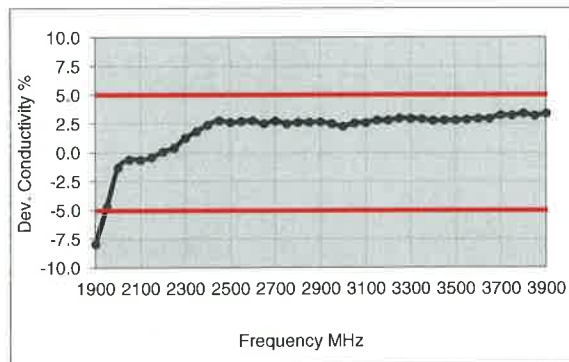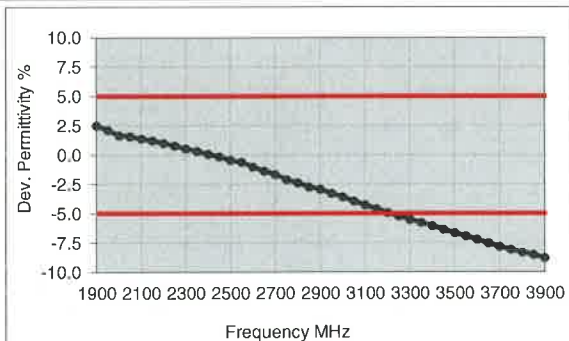

Measurement Certificate / Material Test

Item Name	Head Tissue Simulating Liquid (HBBL3500-5800V5)
Product No.	SL AAH 502 AB (Charge: 130123-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 23-Jan-13
 Operator DI

Additional Information

TSL Density 0.985 g/cm³
 TSL Heat-capacity 3.383 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
3400	38.8	15.03	2.84	38.0	2.81	1.9	1.2
3500	38.6	15.00	2.92	37.9	2.91	1.8	0.3
3600	38.5	14.98	3.00	37.8	3.02	1.7	-0.5
3700	38.4	14.97	3.08	37.7	3.12	1.7	-1.2
3800	38.2	14.95	3.16	37.6	3.22	1.7	-1.8
3900	38.1	14.96	3.25	37.5	3.32	1.7	-2.3
4000	38.0	14.99	3.34	37.4	3.43	1.8	-2.6
4100	37.9	15.03	3.43	37.2	3.53	1.8	-2.8
4200	37.8	15.06	3.52	37.1	3.63	1.8	-3.0
4300	37.7	15.13	3.62	37.0	3.73	1.8	-3.1
4400	37.6	15.20	3.72	36.9	3.84	1.8	-3.0
4500	37.4	15.23	3.81	36.8	3.94	1.7	-3.2
4600	37.3	15.30	3.92	36.7	4.04	1.6	-3.1
4700	37.1	15.35	4.01	36.6	4.14	1.5	-3.1
4800	37.0	15.41	4.11	36.4	4.25	1.5	-3.1
4850	36.9	15.45	4.17	36.4	4.30	1.5	-3.0
4900	36.8	15.49	4.22	36.3	4.35	1.4	-2.9
4950	36.8	15.51	4.27	36.3	4.40	1.4	-2.9
5000	36.7	15.54	4.32	36.2	4.45	1.4	-2.9
5050	36.6	15.57	4.37	36.2	4.50	1.3	-2.8
5100	36.6	15.60	4.42	36.1	4.55	1.3	-2.8
5150	36.5	15.63	4.48	36.0	4.60	1.2	-2.7
5200	36.4	15.67	4.53	36.0	4.66	1.2	-2.6
5250	36.3	15.68	4.58	35.9	4.71	1.1	-2.7
5300	36.2	15.71	4.63	35.9	4.76	1.0	-2.6
5350	36.2	15.74	4.68	35.8	4.81	1.0	-2.6
5400	36.1	15.78	4.74	35.8	4.86	0.9	-2.5
5450	36.0	15.78	4.78	35.7	4.91	0.9	-2.6
5500	36.0	15.79	4.83	35.6	4.96	0.9	-2.6
5550	35.9	15.84	4.89	35.6	5.01	0.9	-2.5
5600	35.8	15.86	4.94	35.5	5.07	0.8	-2.5
5650	35.8	15.91	5.00	35.5	5.12	0.8	-2.2
5700	35.7	15.91	5.05	35.4	5.17	0.8	-2.4
5750	35.6	15.97	5.11	35.4	5.22	0.7	-2.1
5800	35.5	15.98	5.16	35.3	5.27	0.7	-2.1
5850	35.5	16.01	5.21	35.3	5.34	0.5	-2.4
5900	35.4	16.05	5.27	35.3	5.40	0.3	-2.4

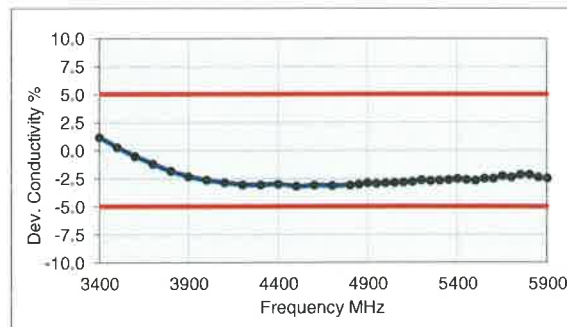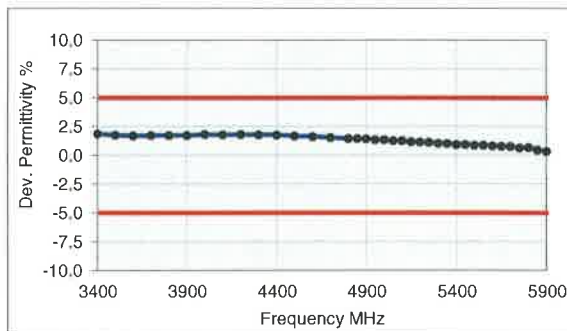

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL750V2)**
 Product No. SL AAM 075 (Charge: 120831-2)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 5-Sep-12
 Operator CL

Additional Information

TSL Density 1.212 g/cm³
 TSL Heat-capacity 3.006 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
600	57.4	24.67	0.82	56.1	0.95	2.2	-13.5
625	57.1	24.34	0.85	56.0	0.95	1.9	-11.3
650	56.8	24.01	0.87	55.9	0.96	1.6	-9.1
675	56.6	23.71	0.89	55.8	0.96	1.3	-7.1
700	56.3	23.41	0.91	55.7	0.96	1.0	-5.0
725	56.0	23.20	0.94	55.6	0.96	0.7	-2.7
750	55.8	22.99	0.96	55.5	0.96	0.5	-0.4
775	55.5	22.81	0.98	55.4	0.97	0.2	1.9
800	55.3	22.64	1.01	55.3	0.97	-0.1	4.2
825	55.1	22.47	1.03	55.2	0.98	-0.3	5.5
838	54.9	22.39	1.04	55.2	0.98	-0.5	6.1
850	54.8	22.31	1.05	55.2	0.99	-0.6	6.7
875	54.6	22.19	1.08	55.1	1.02	-0.9	6.0
900	54.4	22.07	1.10	55.0	1.05	-1.1	5.2
925	54.1	21.96	1.13	55.0	1.06	-1.5	6.3
950	53.9	21.85	1.15	54.9	1.08	-1.9	7.4
975	53.7	21.75	1.18	54.9	1.09	-2.2	8.5
1000	53.5	21.64	1.20	54.8	1.10	-2.5	9.6

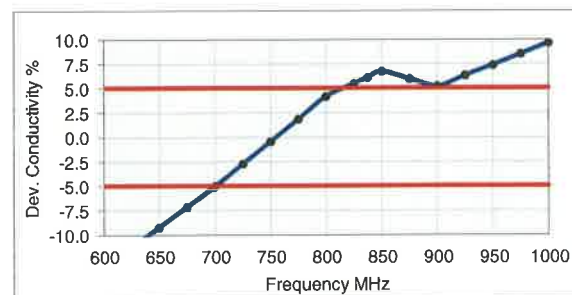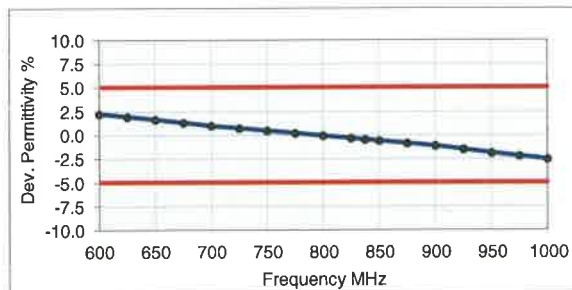

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL900V2)**
 Product No. SL AAM 090 CA (Charge: 140124-1)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 29-Jan-14
 Operator IEN

Additional Information

TSL Density 1.208 g/cm³
 TSL Heat-capacity 3.113 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
700	56.5	22.21	0.86	55.7	0.96	1.4	-9.9
725	56.3	22.03	0.89	55.6	0.96	1.1	-7.6
750	56.0	21.85	0.91	55.5	0.96	0.9	-5.4
775	55.8	21.71	0.94	55.4	0.97	0.6	-3.1
800	55.5	21.57	0.96	55.3	0.97	0.3	-0.8
825	55.3	21.47	0.99	55.2	0.98	0.1	0.8
838	55.2	21.42	1.00	55.2	0.98	-0.1	1.5
850	55.1	21.37	1.01	55.2	0.99	-0.2	2.2
875	54.8	21.28	1.04	55.1	1.02	-0.5	1.6
900	54.6	21.19	1.06	55.0	1.05	-0.8	1.0
925	54.3	21.10	1.09	55.0	1.06	-1.1	2.1
950	54.1	21.01	1.11	54.9	1.08	-1.5	3.2
975	53.9	20.96	1.14	54.9	1.09	-1.8	4.6
1000	53.7	20.90	1.16	54.8	1.10	-2.1	5.9
1025	53.5	20.82	1.19	54.8	1.11	-2.4	7.0
1050	53.3	20.75	1.21	54.7	1.12	-2.7	8.1
1075	53.0	20.70	1.24	54.7	1.13	-3.0	9.4
1100	52.8	20.66	1.26	54.7	1.14	-3.4	10.6
1125	52.6	20.57	1.29	54.6	1.15	-3.7	11.5
1150	52.4	20.48	1.31	54.6	1.17	-3.9	12.4
1175	52.2	20.47	1.34	54.5	1.18	-4.2	13.7
1200	52.0	20.46	1.37	54.5	1.19	-4.5	15.0

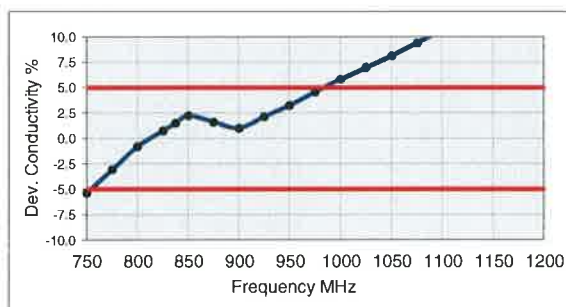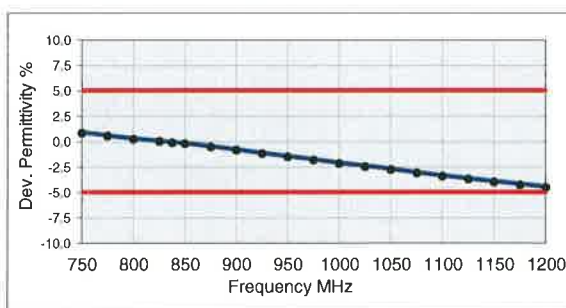

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL1750V2)
Product No.	SL AAM 175 (Charge: 120919-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	20-Sep-12
Operator	CL

Additional Information

TSL Density	0.998 g/cm ³
TSL Heat-capacity	3.893 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1400	54.2	14.23	1.11	54.1	1.28	0.2	-13.2
1425	54.1	14.30	1.13	54.0	1.29	0.1	-12.1
1450	54.0	14.36	1.16	54.0	1.30	0.0	-10.9
1475	53.9	14.42	1.18	54.0	1.32	-0.1	-10.0
1500	53.8	14.49	1.21	53.9	1.33	-0.2	-9.2
1525	53.7	14.54	1.23	53.9	1.35	-0.3	-8.4
1550	53.7	14.59	1.26	53.9	1.36	-0.4	-7.7
1575	53.6	14.67	1.29	53.8	1.38	-0.5	-6.8
1600	53.5	14.74	1.31	53.8	1.39	-0.6	-5.9
1613	53.4	14.77	1.32	53.8	1.40	-0.7	-5.5
1625	53.4	14.79	1.34	53.8	1.41	-0.7	-5.1
1638	53.3	14.82	1.35	53.7	1.42	-0.7	-4.7
1650	53.3	14.85	1.36	53.7	1.43	-0.8	-4.4
1663	53.2	14.88	1.38	53.7	1.43	-0.8	-4.0
1675	53.2	14.91	1.39	53.6	1.44	-0.8	-3.6
1688	53.1	14.94	1.40	53.6	1.45	-0.8	-3.2
1700	53.1	14.97	1.42	53.6	1.46	-0.9	-2.8
1713	53.1	15.01	1.43	53.5	1.46	-0.9	-2.4
1725	53.0	15.04	1.44	53.5	1.47	-0.9	-2.0
1738	53.0	15.07	1.46	53.5	1.48	-1.0	-1.6
1750	52.9	15.10	1.47	53.4	1.49	-1.0	-1.2
1763	52.9	15.14	1.48	53.4	1.50	-1.0	-0.8
1775	52.8	15.17	1.50	53.4	1.50	-1.0	-0.4
1788	52.8	15.21	1.51	53.3	1.51	-1.0	0.0
1800	52.7	15.24	1.53	53.3	1.52	-1.1	0.4
1813	52.7	15.27	1.54	53.3	1.52	-1.1	1.3
1825	52.7	15.30	1.55	53.3	1.52	-1.2	2.2
1838	52.6	15.33	1.57	53.3	1.52	-1.3	3.1
1850	52.6	15.37	1.58	53.3	1.52	-1.4	4.0
1863	52.5	15.40	1.60	53.3	1.52	-1.5	5.0
1875	52.5	15.44	1.61	53.3	1.52	-1.5	6.0
1888	52.4	15.48	1.63	53.3	1.52	-1.6	6.9
1900	52.4	15.51	1.64	53.3	1.52	-1.7	7.9

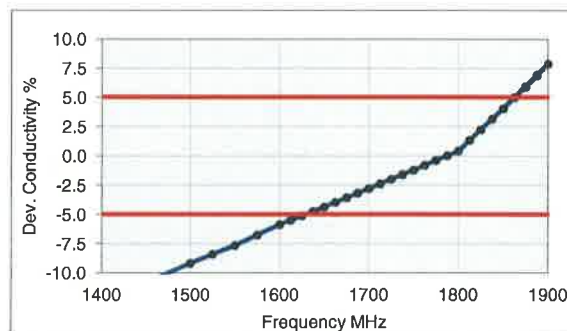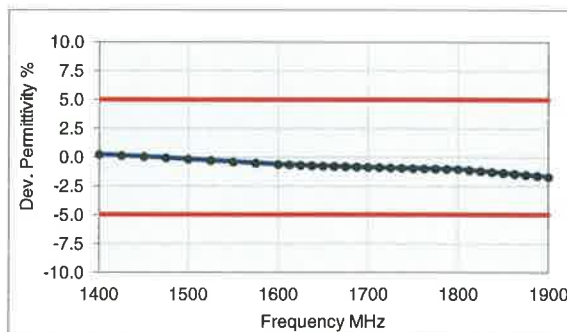

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL1900V2)
Product No.	SL AAM 190 (Charge: 120913-1)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	20-Sep-12
Operator	CL

Additional Information

TSL Density	0.996 g/cm ³
TSL Heat-capacity	3.947 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1600	54.1	13.80	1.23	53.8	1.39	0.5	-11.8
1613	54.1	13.84	1.24	53.8	1.40	0.5	-11.4
1625	54.0	13.87	1.25	53.8	1.41	0.5	-11.0
1638	54.0	13.91	1.27	53.7	1.42	0.5	-10.6
1650	53.9	13.95	1.28	53.7	1.43	0.4	-10.2
1663	53.9	13.99	1.29	53.7	1.43	0.4	-9.7
1675	53.8	14.02	1.31	53.6	1.44	0.4	-9.3
1688	53.8	14.06	1.32	53.6	1.45	0.4	-8.9
1700	53.8	14.10	1.33	53.6	1.46	0.4	-8.4
1713	53.7	14.14	1.35	53.5	1.46	0.3	-8.0
1725	53.7	14.19	1.36	53.5	1.47	0.3	-7.6
1738	53.6	14.23	1.38	53.5	1.48	0.3	-7.1
1750	53.6	14.27	1.39	53.4	1.49	0.3	-6.7
1763	53.5	14.31	1.40	53.4	1.50	0.3	-6.2
1775	53.5	14.35	1.42	53.4	1.50	0.3	-5.8
1788	53.5	14.40	1.43	53.3	1.51	0.2	-5.3
1800	53.4	14.44	1.45	53.3	1.52	0.2	-4.9
1813	53.4	14.48	1.46	53.3	1.52	0.2	-3.9
1825	53.3	14.52	1.47	53.3	1.52	0.1	-3.0
1838	53.3	14.56	1.49	53.3	1.52	0.0	-2.0
1850	53.3	14.61	1.50	53.3	1.52	-0.1	-1.1
1863	53.2	14.65	1.52	53.3	1.52	-0.1	-0.1
1875	53.2	14.69	1.53	53.3	1.52	-0.2	0.8
1888	53.1	14.74	1.55	53.3	1.52	-0.3	1.8
1900	53.1	14.78	1.56	53.3	1.52	-0.4	2.8
1913	53.0	14.83	1.58	53.3	1.52	-0.5	3.8
1925	53.0	14.87	1.59	53.3	1.52	-0.5	4.8
1938	53.0	14.91	1.61	53.3	1.52	-0.6	5.7
1950	52.9	14.95	1.62	53.3	1.52	-0.7	6.7
1975	52.8	15.03	1.65	53.3	1.52	-0.9	8.7
2000	52.7	15.11	1.68	53.3	1.52	-1.0	10.6

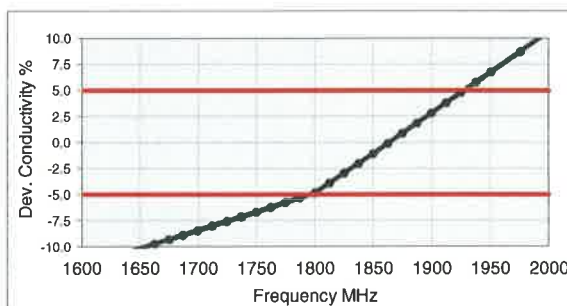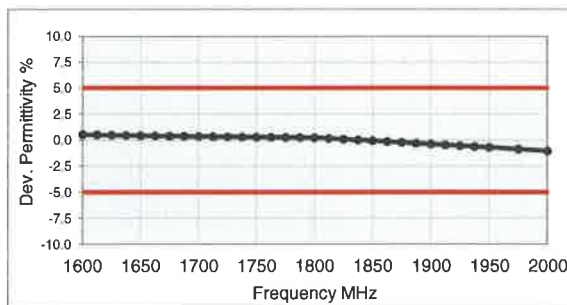

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MSL1950V2)**
 Product No. SL AAM 195 (Charge: 120919-2)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 20-Sep-12
 Operator CL

Additional Information

TSL Density 0.997 g/cm³
 TSL Heat-capacity 3.970 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1850	53.3	13.47	1.39	53.3	1.52	-0.1	-8.8
1875	53.2	13.58	1.42	53.3	1.52	-0.2	-6.8
1900	53.1	13.68	1.45	53.3	1.52	-0.4	-4.9
1925	53.0	13.77	1.47	53.3	1.52	-0.6	-3.0
1950	52.9	13.86	1.50	53.3	1.52	-0.7	-1.1
1975	52.8	13.94	1.53	53.3	1.52	-0.9	0.8
2000	52.7	14.03	1.56	53.3	1.52	-1.1	2.7
2025	52.6	14.13	1.59	53.3	1.54	-1.2	3.1
2050	52.6	14.23	1.62	53.2	1.57	-1.3	3.5
2075	52.5	14.32	1.65	53.2	1.59	-1.4	3.9
2100	52.4	14.41	1.68	53.2	1.62	-1.5	4.2
2125	52.3	14.51	1.72	53.1	1.64	-1.6	4.7
2150	52.2	14.61	1.75	53.1	1.66	-1.7	5.1
2175	52.1	14.70	1.78	53.1	1.69	-1.8	5.5
2200	52.0	14.79	1.81	53.0	1.71	-1.9	5.8
2225	51.9	14.88	1.84	53.0	1.74	-2.0	6.1
2250	51.8	14.96	1.87	53.0	1.76	-2.2	6.5
2275	51.7	15.05	1.91	52.9	1.78	-2.3	6.9
2300	51.6	15.14	1.94	52.9	1.81	-2.4	7.2
2325	51.5	15.24	1.97	52.9	1.83	-2.5	7.7
2350	51.4	15.33	2.00	52.8	1.85	-2.6	8.1
2375	51.4	15.42	2.04	52.8	1.88	-2.7	8.5
2400	51.3	15.50	2.07	52.8	1.90	-2.8	8.8
2425	51.2	15.60	2.10	52.7	1.93	-2.9	9.2
2450	51.1	15.69	2.14	52.7	1.95	-3.1	9.7
2475	51.0	15.78	2.17	52.7	1.99	-3.2	9.4
2500	50.9	15.87	2.21	52.6	2.02	-3.3	9.2
2525	50.8	15.96	2.24	52.6	2.06	-3.4	9.1
2550	50.7	16.06	2.28	52.6	2.09	-3.5	8.9
2575	50.6	16.14	2.31	52.5	2.13	-3.7	8.7
2600	50.5	16.23	2.35	52.5	2.16	-3.9	8.6

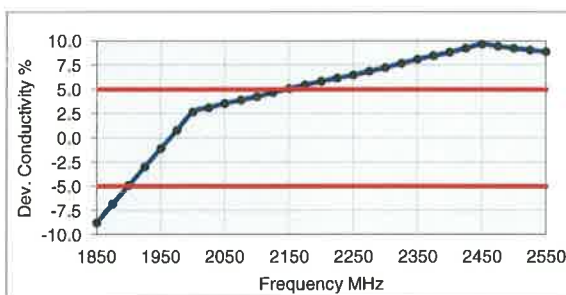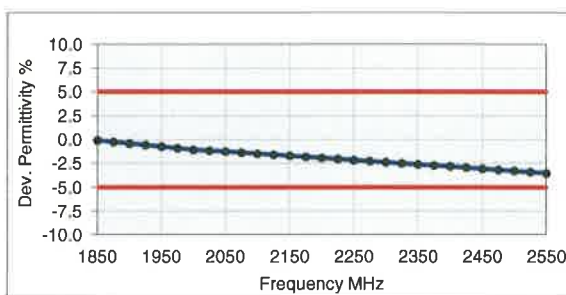

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MSL2450V2)
Product No.	SL AAM 245 BA (Charge: 130510-2)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 15-May-13
 Operator IEN

Additional Information

TSL Density 0.996 g/cm³
 TSL Heat-capacity 3.987 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
1900	52.4	12.21	1.29	53.3	1.52	-1.7	-15.1
1925	52.3	12.32	1.32	53.3	1.52	-1.9	-13.2
1950	52.2	12.43	1.35	53.3	1.52	-2.1	-11.3
1975	52.1	12.55	1.38	53.3	1.52	-2.2	-9.3
2000	52.0	12.67	1.41	53.3	1.52	-2.4	-7.3
2025	51.9	12.75	1.44	53.3	1.54	-2.5	-6.9
2050	51.8	12.84	1.46	53.2	1.57	-2.6	-6.6
2075	51.7	12.96	1.50	53.2	1.59	-2.7	-6.0
2100	51.7	13.09	1.53	53.2	1.62	-2.8	-5.4
2125	51.6	13.17	1.56	53.1	1.64	-2.9	-5.0
2150	51.5	13.25	1.58	53.1	1.66	-3.0	-4.7
2175	51.4	13.37	1.62	53.1	1.69	-3.1	-4.1
2200	51.3	13.50	1.65	53.0	1.71	-3.3	-3.5
2225	51.2	13.58	1.68	53.0	1.74	-3.3	-3.1
2250	51.2	13.65	1.71	53.0	1.76	-3.3	-2.8
2275	51.1	13.78	1.74	52.9	1.78	-3.5	-2.2
2300	51.0	13.90	1.78	52.9	1.81	-3.6	-1.5
2325	50.9	14.01	1.81	52.9	1.83	-3.7	-1.0
2350	50.9	14.12	1.85	52.8	1.85	-3.8	-0.5
2375	50.7	14.21	1.88	52.8	1.88	-3.9	0.0
2400	50.6	14.31	1.91	52.8	1.90	-4.1	0.5
2425	50.5	14.44	1.95	52.7	1.93	-4.2	1.1
2450	50.5	14.56	1.99	52.7	1.95	-4.3	1.9
2475	50.4	14.64	2.02	52.7	1.99	-4.4	1.6
2500	50.3	14.72	2.05	52.6	2.02	-4.5	1.3
2525	50.2	14.79	2.08	52.6	2.06	-4.6	1.0
2550	50.1	14.86	2.11	52.6	2.09	-4.7	0.7
2575	50.0	15.00	2.15	52.5	2.13	-4.8	1.0
2600	49.9	15.14	2.19	52.5	2.16	-4.9	1.2
2625	49.8	15.23	2.22	52.5	2.20	-5.1	1.2
2650	49.6	15.33	2.26	52.4	2.23	-5.3	1.2
2675	49.6	15.45	2.30	52.4	2.27	-5.4	1.3
2700	49.5	15.56	2.34	52.4	2.30	-5.5	1.4

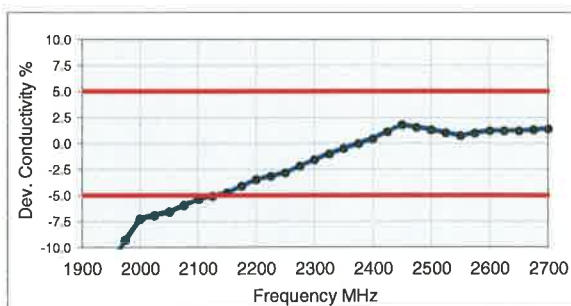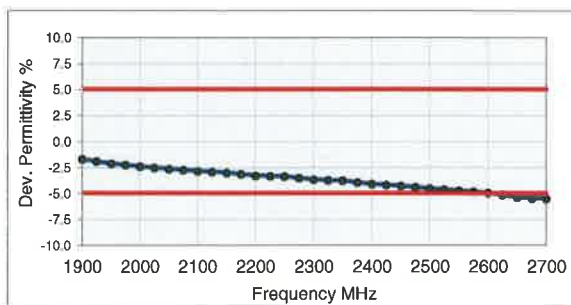

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MBBL1550-1950V3)**
 Product No. SL AAM 181 AA (Charge: 140218-3)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 19-Feb-14
 Operator IEN

Additional Information

TSL Density 1.042 g/cm³
 TSL Heat-capacity 3.475 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-ε'	HP-ε''	sigma	eps	sigma	Δ-eps	Δ-sigma
1500	53.5	14.88	1.24	53.9	1.33	-0.9	-6.7
1525	53.4	14.88	1.26	53.9	1.35	-0.9	-6.2
1550	53.4	14.89	1.28	53.9	1.36	-1.0	-5.8
1575	53.2	14.89	1.30	53.8	1.38	-1.1	-5.3
1600	53.1	14.90	1.33	53.8	1.39	-1.2	-4.8
1625	53.1	14.89	1.35	53.8	1.41	-1.2	-4.5
1650	53.0	14.88	1.37	53.7	1.43	-1.3	-4.2
1675	52.9	14.86	1.38	53.6	1.44	-1.3	-3.9
1700	52.9	14.84	1.40	53.6	1.46	-1.3	-3.7
1725	52.8	14.87	1.43	53.5	1.47	-1.3	-3.1
1750	52.7	14.90	1.45	53.4	1.49	-1.4	-2.6
1775	52.6	14.90	1.47	53.4	1.50	-1.4	-2.2
1800	52.8	14.91	1.49	53.3	1.52	-1.4	-1.8
1825	52.5	14.99	1.52	53.3	1.52	-1.5	0.1
1850	52.4	15.07	1.55	53.3	1.52	-1.7	2.0
1875	52.3	15.06	1.57	53.3	1.52	-1.8	3.3
1900	52.3	15.05	1.59	53.3	1.52	-1.9	4.6
1925	52.2	15.09	1.62	53.3	1.52	-2.1	6.3
1950	52.1	15.13	1.64	53.3	1.52	-2.2	8.0
1975	52.1	15.17	1.67	53.3	1.52	-2.3	9.7
2000	52.0	15.21	1.69	53.3	1.52	-2.4	11.3

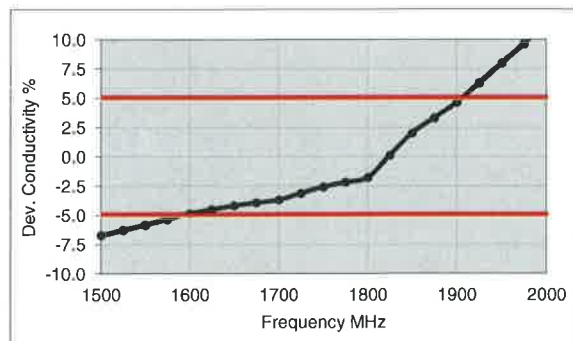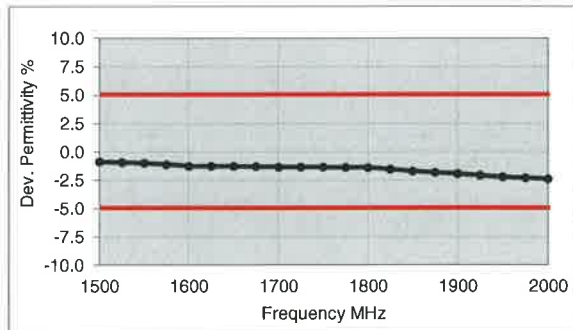

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name	Body Tissue Simulating Liquid (MBBL1900-3800V3)
Product No.	SL AAM 196 AB (Charge: 140219-3)
Manufacturer	SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.

Test Condition



Ambient	Environment temperatur (22 ± 3)°C and humidity < 70%.
TSL Temperature	22°C
Test Date	19-Feb-14
Operator	IEN

Additional Information

TSL Density 1.036 g/cm³

TSL Heat-capacity 3.508 kJ/(kg*K)

f [MHz]	Measured			Target		Diff. to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ -eps	Δ -sigma
1900	53.5	13.3	1.41	53.3	1.52	0.5	-7.3
1950	53.4	13.4	1.46	53.3	1.52	0.2	-4.1
2000	53.3	13.5	1.51	53.3	1.52	0.0	-0.8
2050	53.2	13.6	1.55	53.2	1.57	0.0	-1.1
2100	53.1	13.7	1.60	53.2	1.62	-0.1	-0.7
2150	53.0	13.8	1.65	53.1	1.66	-0.2	-0.9
2200	52.8	13.9	1.70	53.0	1.71	-0.4	-0.5
2250	52.7	14.0	1.76	53.0	1.76	-0.4	0.0
2300	52.6	14.2	1.82	52.9	1.81	-0.6	0.7
2350	52.4	14.4	1.88	52.8	1.85	-0.7	1.3
2400	52.3	14.5	1.94	52.8	1.90	-0.9	2.0
2450	52.2	14.7	2.00	52.7	1.95	-1.0	2.4
2500	52.0	14.8	2.05	52.6	2.02	-1.1	1.6
2550	52.0	14.8	2.10	52.6	2.09	-1.1	0.3
2600	51.8	15.0	2.17	52.5	2.16	-1.4	0.1
2650	51.6	15.1	2.23	52.4	2.23	-1.6	-0.3
2700	51.5	15.2	2.29	52.4	2.30	-1.8	-0.8
2750	51.2	15.3	2.34	52.3	2.38	-2.1	-1.5
2800	51.1	15.4	2.40	52.3	2.45	-2.2	-1.7
2850	50.9	15.6	2.47	52.2	2.52	-2.4	-2.0
2900	50.8	15.7	2.53	52.1	2.59	-2.5	-2.2
2950	50.7	15.8	2.59	52.1	2.66	-2.7	-2.8
3000	50.5	15.9	2.65	52.0	2.73	-2.8	-3.0
3050	50.4	16.0	2.71	51.9	2.79	-3.0	-2.9
3100	50.2	16.1	2.78	51.9	2.85	-3.2	-2.4
3150	50.1	16.2	2.85	51.8	2.91	-3.3	-2.0
3200	49.9	16.3	2.90	51.7	2.96	-3.6	-2.1
3250	49.8	16.5	2.98	51.7	3.02	-3.6	-1.5
3300	49.6	16.5	3.02	51.6	3.08	-3.8	-1.8
3350	49.5	16.6	3.09	51.5	3.14	-3.9	-1.5
3400	49.4	16.6	3.15	51.5	3.20	-4.0	-1.5
3450	49.2	16.7	3.21	51.4	3.26	-4.2	-1.4
3500	49.1	16.8	3.28	51.3	3.31	-4.3	-1.0
3550	48.9	16.9	3.34	51.3	3.37	-4.5	-0.9
3600	48.8	17.1	3.42	51.2	3.43	-4.6	-0.4
3650	48.7	17.1	3.47	51.1	3.49	-4.8	-0.5
3700	48.5	17.2	3.55	51.1	3.55	-4.9	0.0
3750	48.4	17.3	3.61	51.0	3.61	-5.0	0.0
3800	48.3	17.4	3.67	50.9	3.66	-5.1	0.1
3850	48.2	17.5	3.74	50.8	3.72	-5.2	0.5

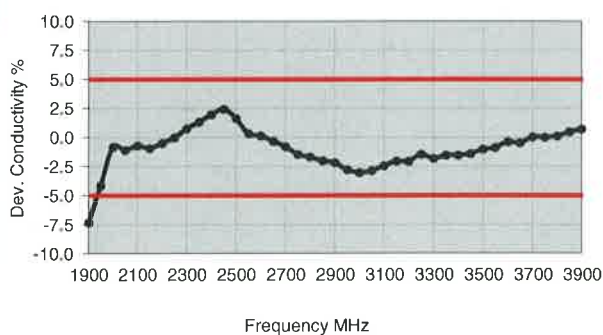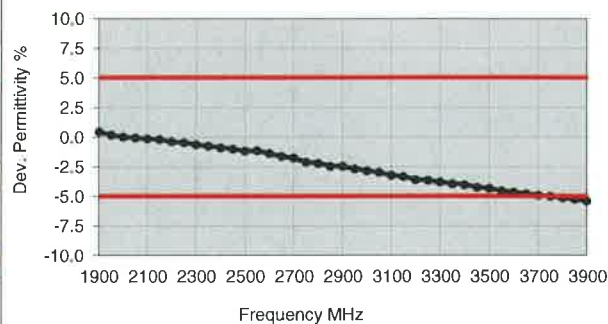

Zeughausstrasse 43, 8004 Zurich, Switzerland
 Phone +41 44 245 9700, Fax +41 44 245 9779
 info@speag.com, http://www.speag.com

Measurement Certificate / Material Test

Item Name **Body Tissue Simulating Liquid (MBBL3500-5800V5)**
 Product No. SL AAM 501 EA (Charge: 140114-1)
 Manufacturer SPEAG

Measurement Method

TSL dielectric parameters measured using calibrated OCP probe.

Setup Validation

Validation results were within $\pm 2.5\%$ towards the target values of Methanol.

Target Parameters

Target parameters as defined in the IEEE 1528 and IEC 62209 compliance standards.



Test Condition

Ambient Environment temperatur (22 ± 3)°C and humidity < 70%.
 TSL Temperature 22°C
 Test Date 15-Jan-14
 Operator IEN

Additional Information

TSL Density 0.996 g/cm³
 TSL Heat-capacity 3.765 kJ/(kg*K)

f [MHz]	Measured			Target		Diff.to Target [%]	
	HP-e'	HP-e''	sigma	eps	sigma	Δ-eps	Δ-sigma
3400	52.2	16.63	3.14	51.5	3.20	1.4	-1.8
3500	52.0	16.67	3.25	51.3	3.31	1.3	-1.9
3600	51.9	16.74	3.35	51.2	3.43	1.4	-2.4
3700	51.7	16.81	3.46	51.1	3.55	1.3	-2.5
3800	51.6	16.90	3.57	50.9	3.66	1.3	-2.6
3900	51.5	16.99	3.69	50.8	3.78	1.4	-2.4
4000	51.3	17.08	3.80	50.6	3.90	1.3	-2.5
4100	51.2	17.18	3.92	50.5	4.01	1.4	-2.4
4200	51.1	17.32	4.05	50.4	4.13	1.4	-2.0
4300	50.9	17.47	4.18	50.2	4.25	1.3	-1.6
4400	50.8	17.61	4.31	50.1	4.37	1.4	-1.3
4500	50.6	17.73	4.44	50.0	4.48	1.3	-0.9
4600	50.4	17.86	4.57	49.8	4.60	1.1	-0.6
4700	50.3	18.00	4.71	49.7	4.72	1.2	-0.1
4800	50.1	18.14	4.84	49.6	4.83	1.1	0.2
4850	50.0	18.20	4.91	49.5	4.89	1.0	0.4
4900	49.9	18.28	4.98	49.4	4.95	1.0	0.6
4950	49.8	18.31	5.04	49.4	5.01	0.9	0.7
5000	49.7	18.38	5.11	49.3	5.07	0.8	0.9
5050	49.6	18.44	5.18	49.2	5.12	0.8	1.1
5100	49.5	18.50	5.25	49.2	5.18	0.7	1.3
5150	49.4	18.57	5.32	49.1	5.24	0.6	1.5
5200	49.4	18.63	5.39	49.0	5.30	0.8	1.7
5250	49.3	18.68	5.46	48.9	5.36	0.7	1.9
5300	49.2	18.75	5.53	48.9	5.42	0.7	2.1
5350	49.1	18.79	5.59	48.8	5.47	0.6	2.1
5400	49.0	18.86	5.66	48.7	5.53	0.5	2.3
5450	48.9	18.90	5.73	48.7	5.59	0.5	2.5
5500	48.8	18.94	5.80	48.6	5.65	0.4	2.7
5550	48.7	19.01	5.87	48.5	5.71	0.3	2.8
5600	48.7	19.06	5.94	48.5	5.77	0.5	3.0
5650	48.6	19.13	6.01	48.4	5.82	0.4	3.2
5700	48.5	19.18	6.08	48.3	5.88	0.3	3.3
5750	48.4	19.26	6.16	48.3	5.94	0.3	3.7
5800	48.3	19.30	6.23	48.2	6.00	0.2	3.8
5850	48.2	19.37	6.30	48.1	6.06	0.1	4.0
5900	48.1	19.43	6.38	48.1	6.12	0.1	4.3

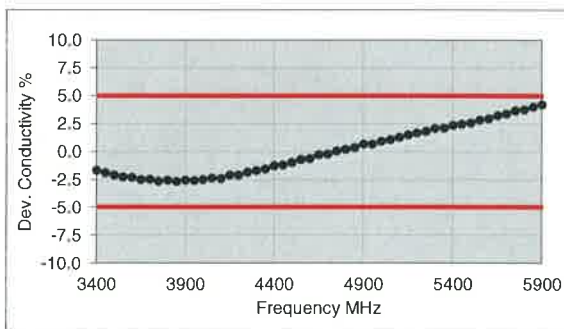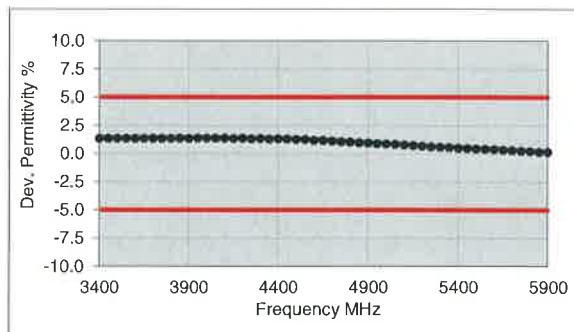



Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: SCS 108

Client **UL CCS USA**

Certificate No: **EX3-3773_Apr14**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3773**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-12.v9, QA CAL-14.v4, QA CAL-23.v5,
QA CAL-25.v6
Calibration procedure for dosimetric E-field probes**

Calibration date: **April 22, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

	Name	Function	Signature
Calibrated by:	Jeton Kastrati	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	
			Issued: April 23, 2014
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization φ	φ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

Probe EX3DV4

SN:3773

Manufactured: January 10, 2011
Calibrated: April 22, 2014

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3773

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.57	0.56	0.52	$\pm 10.1 \%$
DCP (mV) ^B	98.9	98.0	100.8	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	149.1	$\pm 3.5 \%$
		Y	0.0	0.0	1.0		145.4	
		Z	0.0	0.0	1.0		147.5	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3773

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
450	43.5	0.87	10.03	10.03	10.03	0.18	1.20	± 13.3 %
750	41.9	0.89	9.34	9.34	9.34	0.23	1.26	± 12.0 %
835	41.5	0.90	8.91	8.91	8.91	0.34	0.92	± 12.0 %
900	41.5	0.97	8.75	8.75	8.75	0.22	1.23	± 12.0 %
1450	40.5	1.20	7.76	7.76	7.76	0.80	0.61	± 12.0 %
1640	40.3	1.29	7.52	7.52	7.52	0.76	0.61	± 12.0 %
1750	40.1	1.37	7.44	7.44	7.44	0.68	0.70	± 12.0 %
1900	40.0	1.40	7.26	7.26	7.26	0.47	0.82	± 12.0 %
1950	40.0	1.40	7.01	7.01	7.01	0.72	0.66	± 12.0 %
2000	40.0	1.40	7.21	7.21	7.21	0.44	0.86	± 12.0 %
2300	39.5	1.67	6.90	6.90	6.90	0.34	1.02	± 12.0 %
2450	39.2	1.80	6.52	6.52	6.52	0.35	1.08	± 12.0 %
2600	39.0	1.96	6.37	6.37	6.37	0.29	1.36	± 12.0 %
3500	37.9	2.91	6.55	6.55	6.55	0.46	0.89	± 13.1 %
3700	37.7	3.12	6.20	6.20	6.20	0.44	0.93	± 13.1 %
4950	36.3	4.40	4.99	4.99	4.99	0.25	1.80	± 13.1 %
5200	36.0	4.66	4.88	4.88	4.88	0.30	1.80	± 13.1 %
5300	35.9	4.76	4.69	4.69	4.69	0.30	1.80	± 13.1 %
5500	35.6	4.96	4.60	4.60	4.60	0.30	1.80	± 13.1 %
5600	35.5	5.07	4.33	4.33	4.33	0.35	1.80	± 13.1 %
5800	35.3	5.27	4.36	4.36	4.36	0.35	1.80	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3773

Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
450	56.7	0.94	10.02	10.02	10.02	0.10	1.20	± 13.3 %
750	55.5	0.96	8.79	8.79	8.79	0.30	1.07	± 12.0 %
835	55.2	0.97	8.77	8.77	8.77	0.52	0.80	± 12.0 %
900	55.0	1.05	8.58	8.58	8.58	0.40	0.86	± 12.0 %
1450	54.0	1.30	7.38	7.38	7.38	0.23	1.20	± 12.0 %
1640	53.8	1.40	7.59	7.59	7.59	0.63	0.66	± 12.0 %
1750	53.4	1.49	7.13	7.13	7.13	0.34	0.96	± 12.0 %
1900	53.3	1.52	6.90	6.90	6.90	0.39	0.89	± 12.0 %
1950	53.3	1.52	7.18	7.18	7.18	0.44	0.81	± 12.0 %
2000	53.3	1.52	7.03	7.03	7.03	0.39	0.87	± 12.0 %
2300	52.9	1.81	6.78	6.78	6.78	0.63	0.66	± 12.0 %
2450	52.7	1.95	6.67	6.67	6.67	0.78	0.61	± 12.0 %
2600	52.5	2.16	6.44	6.44	6.44	0.80	0.50	± 12.0 %
3500	51.3	3.31	5.95	5.95	5.95	0.44	1.06	± 13.1 %
3700	51.0	3.55	5.97	5.97	5.97	0.41	1.09	± 13.1 %
4950	49.4	5.01	4.40	4.40	4.40	0.30	1.90	± 13.1 %
5200	49.0	5.30	4.39	4.39	4.39	0.35	1.90	± 13.1 %
5300	48.9	5.42	4.19	4.19	4.19	0.35	1.90	± 13.1 %
5500	48.6	5.65	3.92	3.92	3.92	0.40	1.90	± 13.1 %
5600	48.5	5.77	3.75	3.75	3.75	0.40	1.90	± 13.1 %
5800	48.2	6.00	4.12	4.12	4.12	0.40	1.90	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe diameter from the boundary.


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

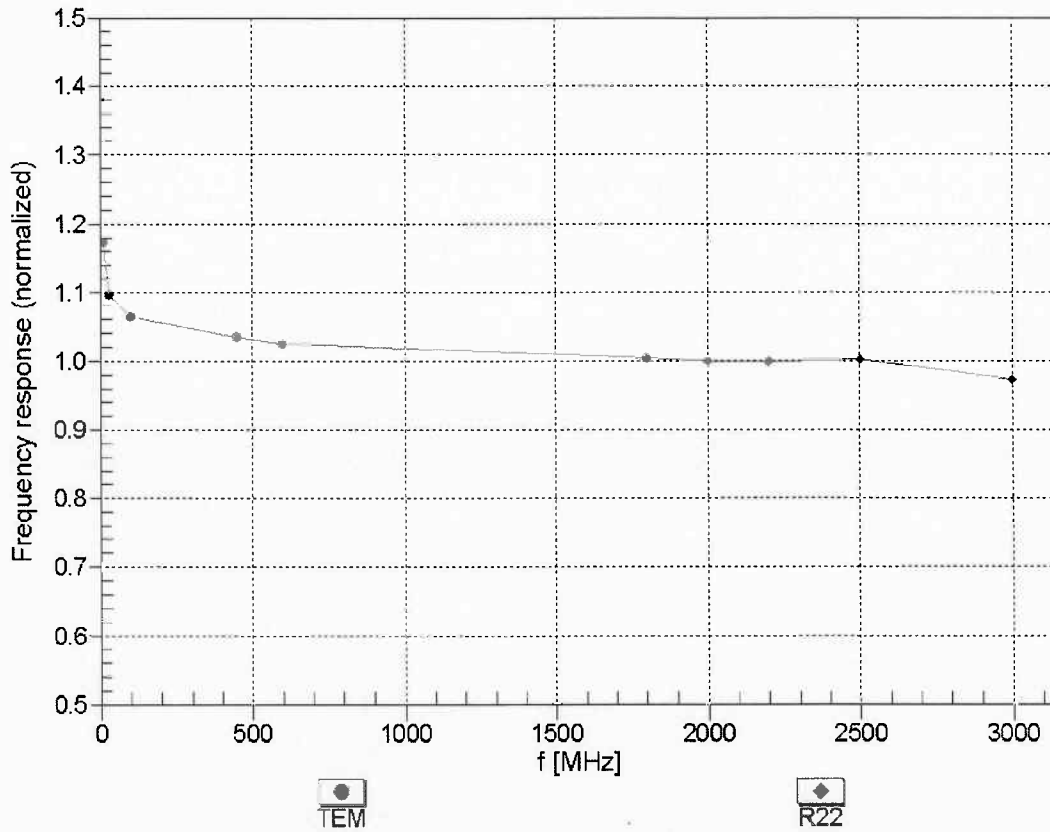



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ ($k=2$)

Receiving Pattern (ϕ), $\theta = 0^\circ$

f=600 MHz,TEM


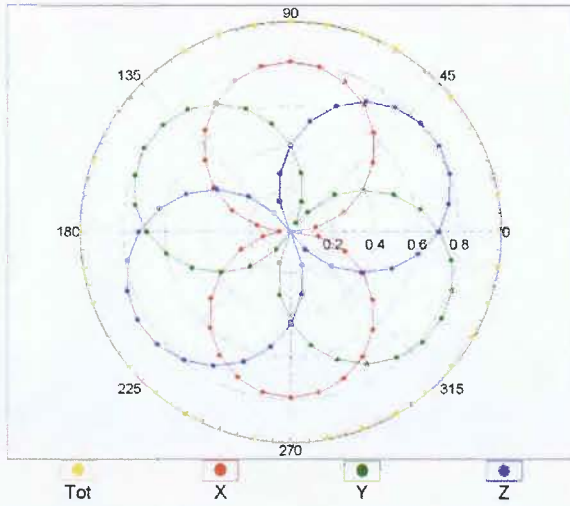


f=1800 MHz,R22

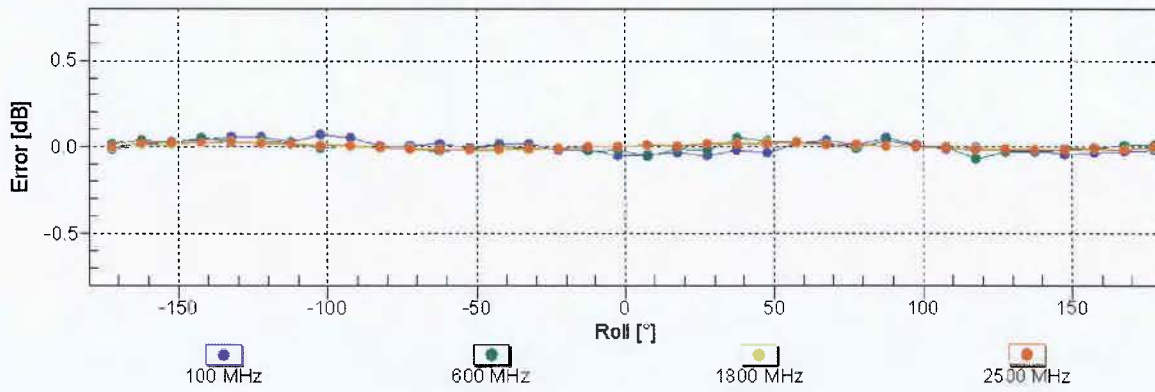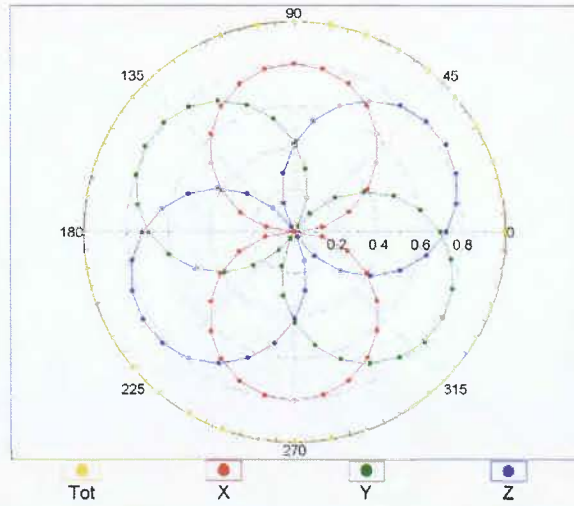



Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range f(SAR_{head}) (TEM cell , f_{eval}= 1900 MHz)

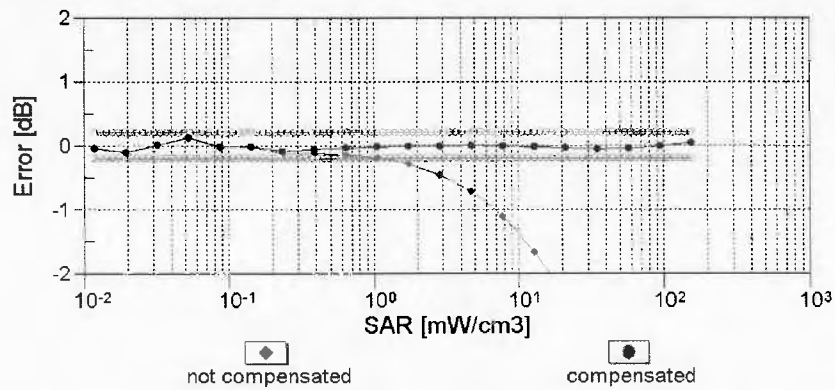
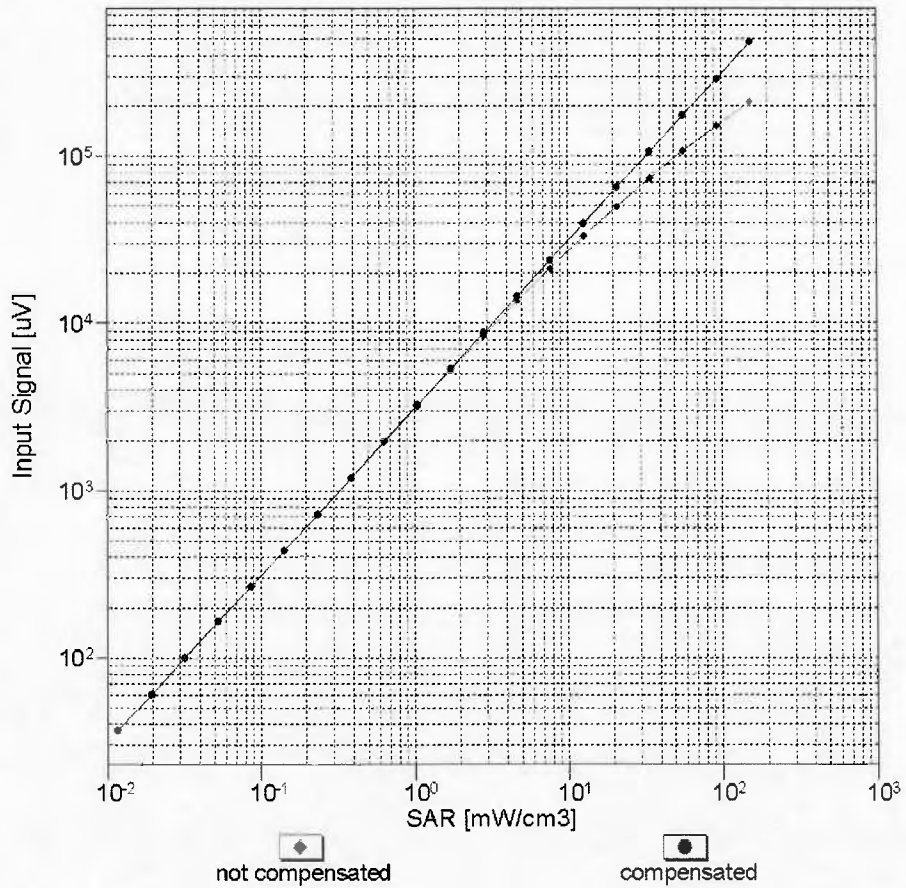


Uncertainty of Linearity Assessment: ± 0.6% (k=2)

Conversion Factor Assessment

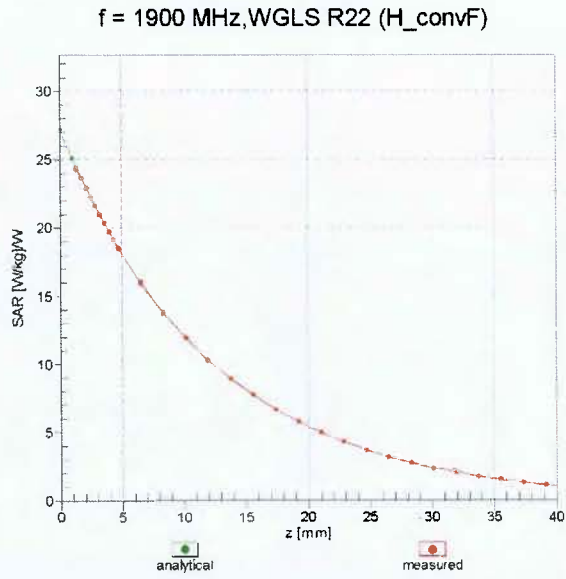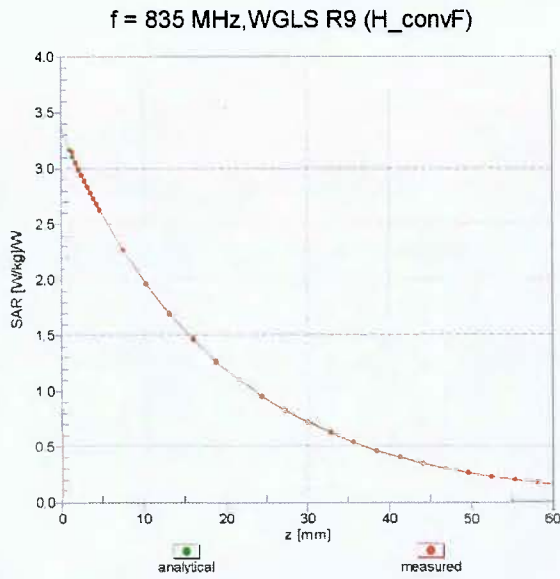

Deviation from Isotropy in Liquid Error (ϕ, θ), f = 900 MHz

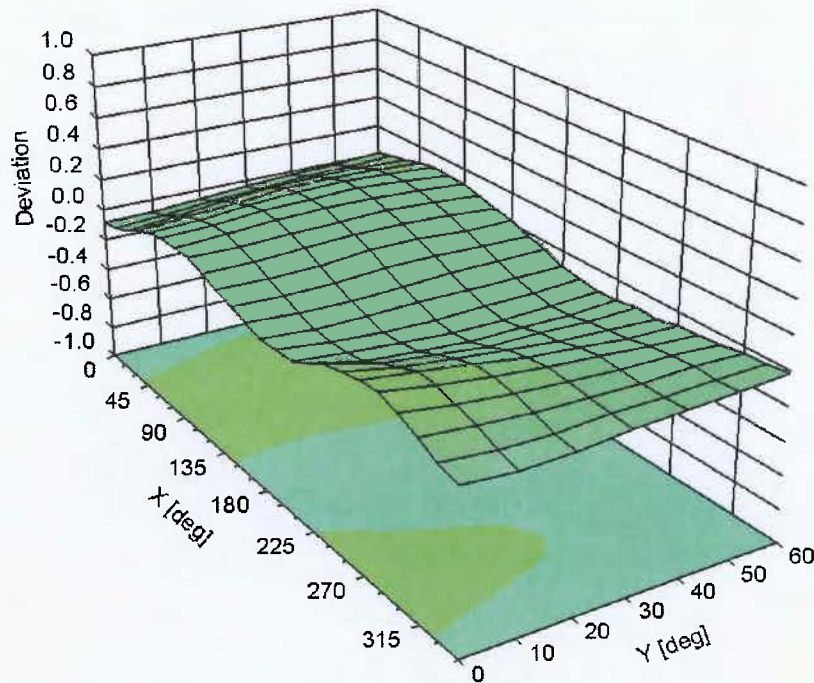

Uncertainty of Spherical Isotropy Assessment: $\pm 2.6\%$ (k=2)

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3773

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	-22.3
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **UL CCS USA**

Certificate No: **EX3-3902_May14**

CALIBRATION CERTIFICATE

Object **EX3DV4 - SN:3902**

Calibration procedure(s) **QA CAL-01.v9, QA CAL-14.v4, QA CAL-23.v5, QA CAL-25.v6**
Calibration procedure for dosimetric E-field probes

Calibration date: **May 19, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID	Cal Date (Certificate No.)	Scheduled Calibration
Power meter E4419B	GB41293874	03-Apr-14 (No. 217-01911)	Apr-15
Power sensor E4412A	MY41498087	03-Apr-14 (No. 217-01911)	Apr-15
Reference 3 dB Attenuator	SN: S5054 (3c)	03-Apr-14 (No. 217-01915)	Apr-15
Reference 20 dB Attenuator	SN: S5277 (20x)	03-Apr-14 (No. 217-01919)	Apr-15
Reference 30 dB Attenuator	SN: S5129 (30b)	03-Apr-14 (No. 217-01920)	Apr-15
Reference Probe ES3DV2	SN: 3013	30-Dec-13 (No. ES3-3013_Dec13)	Dec-14
DAE4	SN: 660	13-Dec-13 (No. DAE4-660_Dec13)	Dec-14
Secondary Standards	ID	Check Date (in house)	Scheduled Check
RF generator HP 8648C	US3642U01700	4-Aug-99 (in house check Apr-13)	In house check: Apr-16
Network Analyzer HP 8753E	US37390585	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Calibrated by:	Name Claudio Leubler	Function Laboratory Technician	Signature
Approved by:	Katja Pokovic	Technical Manager	
			Issued: May 20, 2014
This calibration certificate shall not be reproduced except in full without written approval of the laboratory.			



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
NORM _{x,y,z}	sensitivity in free space
ConvF	sensitivity in TSL / NORM _{x,y,z}
DCP	diode compression point
CF	crest factor (1/duty_cycle) of the RF signal
A, B, C, D	modulation dependent linearization parameters
Polarization ϕ	ϕ rotation around probe axis
Polarization ϑ	ϑ rotation around an axis that is in the plane normal to probe axis (at measurement center), i.e., $\vartheta = 0$ is normal to probe axis
Connector Angle	information used in DASY system to align probe sensor X to the robot coordinate system

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005

Methods Applied and Interpretation of Parameters:

- NORM_{x,y,z}**: Assessed for E-field polarization $\vartheta = 0$ ($f \leq 900$ MHz in TEM-cell; $f > 1800$ MHz: R22 waveguide). NORM_{x,y,z} are only intermediate values, i.e., the uncertainties of NORM_{x,y,z} does not affect the E²-field uncertainty inside TSL (see below ConvF).
- NORM(f)_{x,y,z}** = NORM_{x,y,z} * frequency_response (see Frequency Response Chart). This linearization is implemented in DASY4 software versions later than 4.2. The uncertainty of the frequency response is included in the stated uncertainty of ConvF.
- DCP_{x,y,z}**: DCP are numerical linearization parameters assessed based on the data of power sweep with CW signal (no uncertainty required). DCP does not depend on frequency nor media.
- PAR**: PAR is the Peak to Average Ratio that is not calibrated but determined based on the signal characteristics
- A_{x,y,z}; B_{x,y,z}; C_{x,y,z}; D_{x,y,z}; VR_{x,y,z}; A, B, C, D** are numerical linearization parameters assessed based on the data of power sweep for specific modulation signal. The parameters do not depend on frequency nor media. VR is the maximum calibration range expressed in RMS voltage across the diode.
- ConvF and Boundary Effect Parameters**: Assessed in flat phantom using E-field (or Temperature Transfer Standard for $f \leq 800$ MHz) and inside waveguide using analytical field distributions based on power measurements for $f > 800$ MHz. The same setups are used for assessment of the parameters applied for boundary compensation (alpha, depth) of which typical uncertainty values are given. These parameters are used in DASY4 software to improve probe accuracy close to the boundary. The sensitivity in TSL corresponds to NORM_{x,y,z} * ConvF whereby the uncertainty corresponds to that given for ConvF. A frequency dependent ConvF is used in DASY version 4.4 and higher which allows extending the validity from ± 50 MHz to ± 100 MHz.
- Spherical isotropy (3D deviation from isotropy)**: in a field of low gradients realized using a flat phantom exposed by a patch antenna.
- Sensor Offset**: The sensor offset corresponds to the offset of virtual measurement center from the probe tip (on probe axis). No tolerance required.
- Connector Angle**: The angle is assessed using the information gained by determining the NORM_x (no uncertainty required).

Probe EX3DV4

SN:3902

Manufactured: September 4, 2012
Calibrated: May 19, 2014

Calibrated for DASY/EASY Systems
(Note: non-compatible with DASY2 system!)

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3902

Basic Calibration Parameters

	Sensor X	Sensor Y	Sensor Z	Unc (k=2)
Norm ($\mu\text{V}/(\text{V}/\text{m})^2$) ^A	0.45	0.46	0.46	$\pm 10.1 \%$
DCP (mV) ^B	101.3	100.1	97.9	

Modulation Calibration Parameters

UID	Communication System Name		A dB	B dB $\sqrt{\mu\text{V}}$	C	D dB	VR mV	Unc ^E (k=2)
0	CW	X	0.0	0.0	1.0	0.00	132.5	$\pm 2.5 \%$
		Y	0.0	0.0	1.0		142.7	
		Z	0.0	0.0	1.0		139.7	

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

^A The uncertainties of NormX,Y,Z do not affect the E^2 -field uncertainty inside TSL (see Pages 5 and 6).

^B Numerical linearization parameter: uncertainty not required.

^E Uncertainty is determined using the max. deviation from linear response applying rectangular distribution and is expressed for the square of the field value.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3902

Calibration Parameter Determined in Head Tissue Simulating Media

f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	41.9	0.89	10.36	10.36	10.36	0.47	0.76	± 12.0 %
835	41.5	0.90	10.04	10.04	10.04	0.18	1.45	± 12.0 %
900	41.5	0.97	9.91	9.91	9.91	0.40	0.84	± 12.0 %
1640	40.3	1.29	8.59	8.59	8.59	0.44	0.84	± 12.0 %
1750	40.1	1.37	8.46	8.46	8.46	0.48	0.78	± 12.0 %
1900	40.0	1.40	8.19	8.19	8.19	0.45	0.77	± 12.0 %
1950	40.0	1.40	7.91	7.91	7.91	0.49	0.75	± 12.0 %
2000	40.0	1.40	8.16	8.16	8.16	0.36	0.90	± 12.0 %
2300	39.5	1.67	7.75	7.75	7.75	0.39	0.75	± 12.0 %
2450	39.2	1.80	7.29	7.29	7.29	0.34	0.90	± 12.0 %
2600	39.0	1.96	7.06	7.06	7.06	0.36	0.89	± 12.0 %
5200	36.0	4.66	5.30	5.30	5.30	0.35	1.80	± 13.1 %
5300	35.9	4.76	5.12	5.12	5.12	0.35	1.80	± 13.1 %
5500	35.6	4.96	5.00	5.00	5.00	0.40	1.80	± 13.1 %
5600	35.5	5.07	4.78	4.78	4.78	0.40	1.80	± 13.1 %
5800	35.3	5.27	4.75	4.75	4.75	0.40	1.80	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3902

Calibration Parameter Determined in Body Tissue Simulating Media


f (MHz) ^C	Relative Permittivity ^F	Conductivity (S/m) ^F	ConvF X	ConvF Y	ConvF Z	Alpha ^G	Depth ^G (mm)	Unct. (k=2)
750	55.5	0.96	9.90	9.90	9.90	0.46	0.79	± 12.0 %
835	55.2	0.97	9.86	9.86	9.86	0.39	0.86	± 12.0 %
900	55.0	1.05	9.65	9.65	9.65	0.40	0.86	± 12.0 %
1640	53.8	1.40	8.67	8.67	8.67	0.59	0.69	± 12.0 %
1750	53.4	1.49	8.06	8.06	8.06	0.73	0.62	± 12.0 %
1900	53.3	1.52	7.80	7.80	7.80	0.33	0.93	± 12.0 %
1950	53.3	1.52	8.05	8.05	8.05	0.27	1.05	± 12.0 %
2000	53.3	1.52	7.94	7.94	7.94	0.38	0.87	± 12.0 %
2300	52.9	1.81	7.55	7.55	7.55	0.72	0.59	± 12.0 %
2450	52.7	1.95	7.35	7.35	7.35	0.80	0.58	± 12.0 %
2600	52.5	2.16	7.18	7.18	7.18	0.80	0.50	± 12.0 %
5200	49.0	5.30	4.49	4.49	4.49	0.45	1.90	± 13.1 %
5300	48.9	5.42	4.33	4.33	4.33	0.45	1.90	± 13.1 %
5500	48.6	5.65	3.93	3.93	3.93	0.50	1.90	± 13.1 %
5600	48.5	5.77	3.73	3.73	3.73	0.50	1.90	± 13.1 %
5800	48.2	6.00	4.11	4.11	4.11	0.50	1.90	± 13.1 %

^C Frequency validity of ± 100 MHz only applies for DASY v4.4 and higher (see Page 2), else it is restricted to ± 50 MHz. Above 5 GHz frequency validity can be extended to ± 110 MHz. The uncertainty is the RSS of the ConvF uncertainty at calibration frequency and the uncertainty for the indicated frequency band.

^F At frequencies below 3 GHz, the validity of tissue parameters (ϵ and σ) can be relaxed to ± 10% if liquid compensation formula is applied to measured SAR values. At frequencies above 3 GHz, the validity of tissue parameters (ϵ and σ) is restricted to ± 5%. The uncertainty is the RSS of the ConvF uncertainty for indicated target tissue parameters.

^G Alpha/Depth are determined during calibration. SPEAG warrants that the remaining deviation due to the boundary effect after compensation is always less than ± 1% for frequencies below 3 GHz and below ± 2% for frequencies between 3-6 GHz at any distance larger than half the probe tip diameter from the boundary.


Frequency Response of E-Field (TEM-Cell:ifi110 EXX, Waveguide: R22)

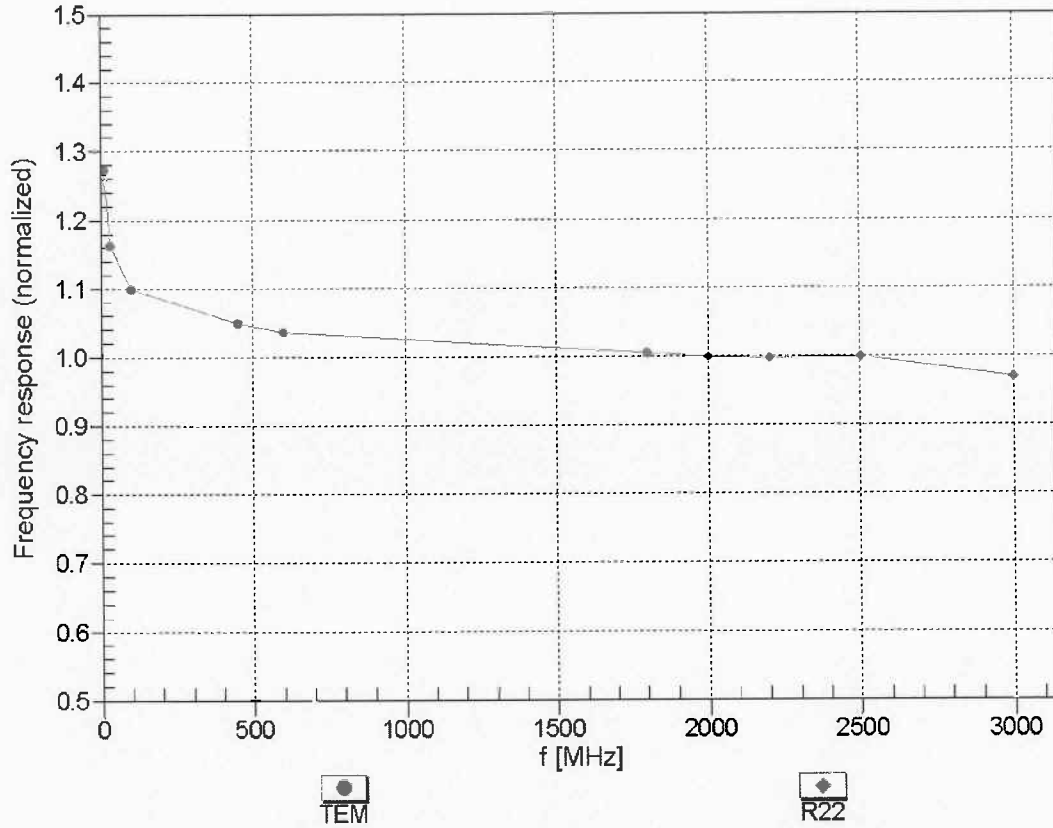



Uncertainty of Frequency Response of E-field: $\pm 6.3\%$ (k=2)

Receiving Pattern (ϕ), $\vartheta = 0^\circ$

f=600 MHz,TEM


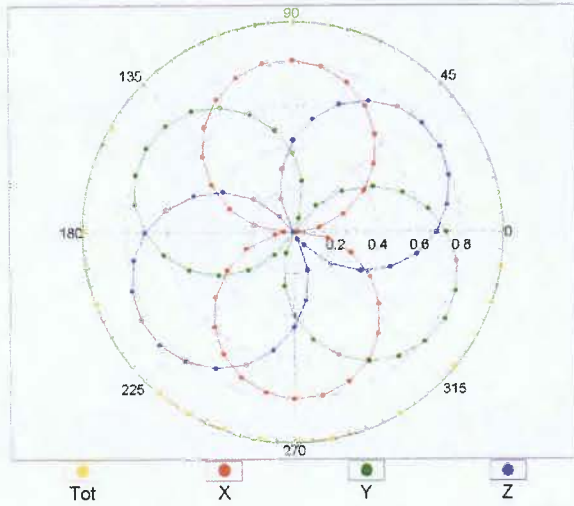


f=1800 MHz,R22

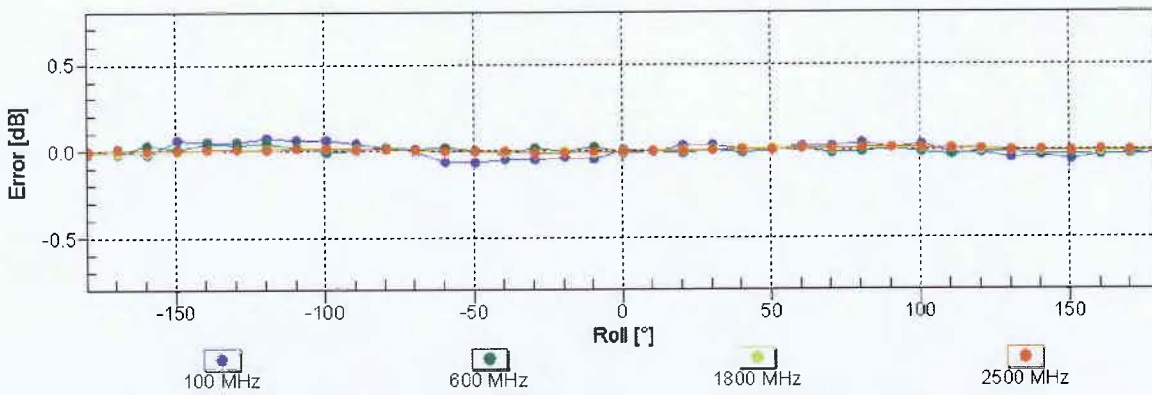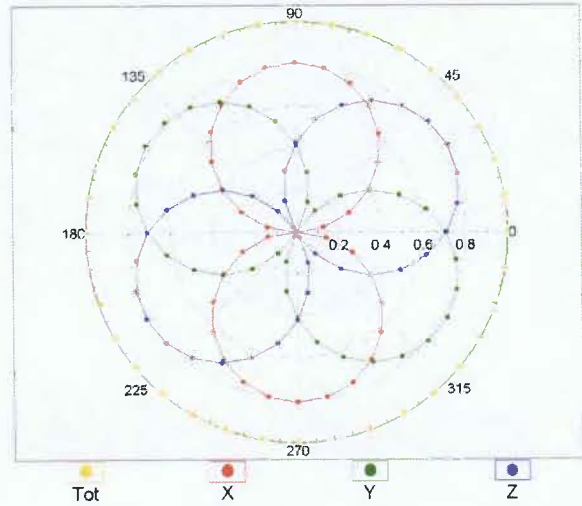


Uncertainty of Axial Isotropy Assessment: $\pm 0.5\%$ (k=2)

Dynamic Range $f(\text{SAR}_{\text{head}})$ (TEM cell , $f_{\text{eval}} = 1900 \text{ MHz}$)

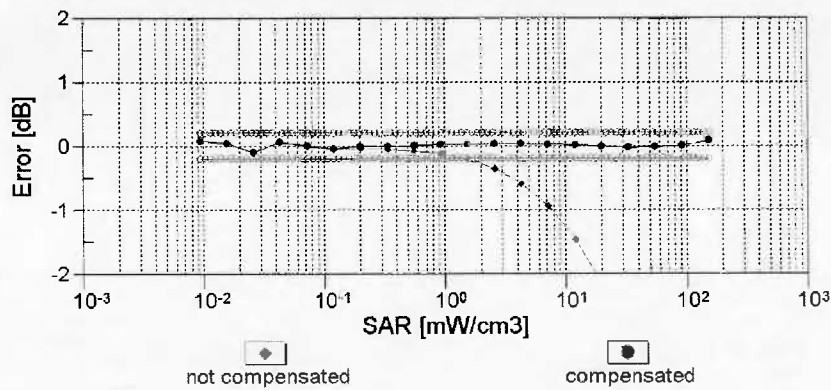
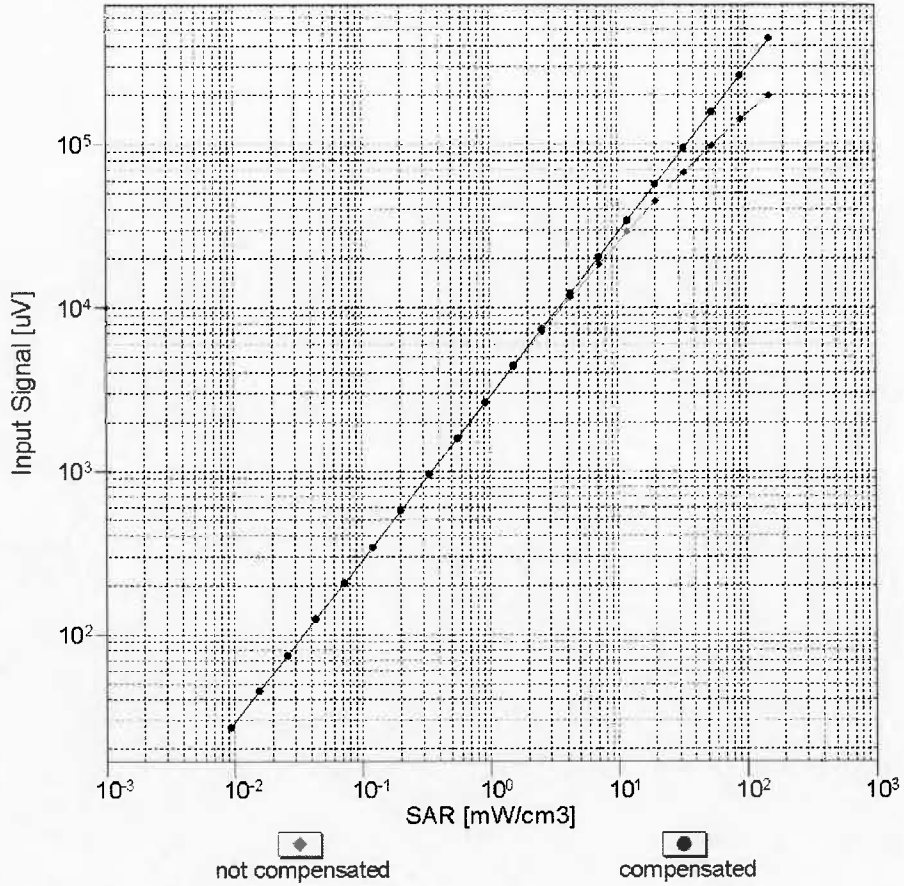


Uncertainty of Linearity Assessment: $\pm 0.6\%$ ($k=2$)

Conversion Factor Assessment

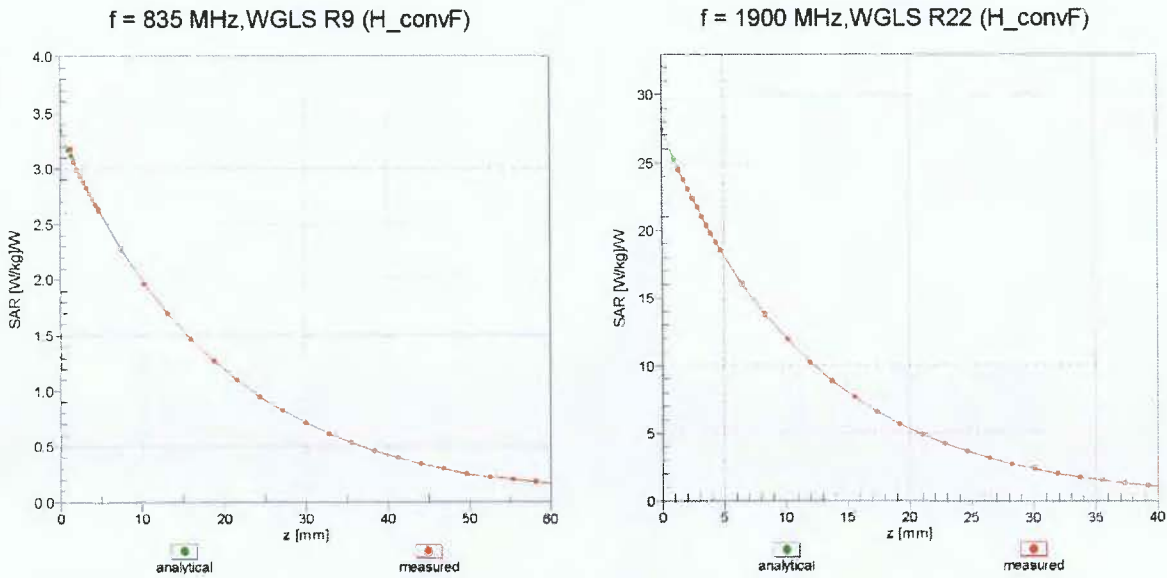

Deviation from Isotropy in Liquid Error (ϕ, ϑ), f = 900 MHz

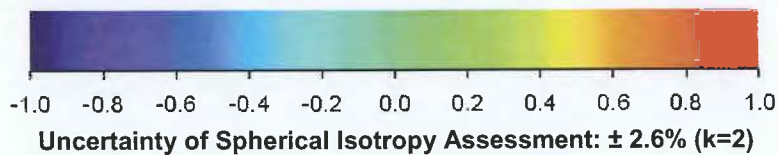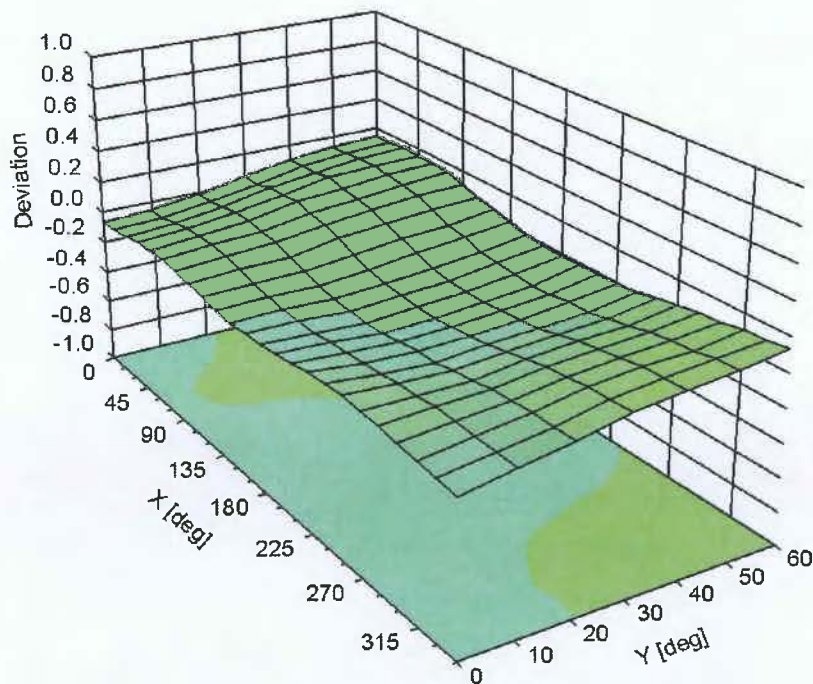

DASY/EASY - Parameters of Probe: EX3DV4 - SN:3902

Other Probe Parameters

Sensor Arrangement	Triangular
Connector Angle (°)	0.6
Mechanical Surface Detection Mode	enabled
Optical Surface Detection Mode	disabled
Probe Overall Length	337 mm
Probe Body Diameter	10 mm
Tip Length	9 mm
Tip Diameter	2.5 mm
Probe Tip to Sensor X Calibration Point	1 mm
Probe Tip to Sensor Y Calibration Point	1 mm
Probe Tip to Sensor Z Calibration Point	1 mm
Recommended Measurement Distance from Surface	2 mm



Accredited by the Swiss Accreditation Service (SAS)
**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Accreditation No.: **SCS 108**

Client **UL CCS USA**

Certificate No: **D835V2-4d117_May14**

CALIBRATION CERTIFICATE

Object **D835V2 - SN: 4d117**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 16, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Calibrated by: **Name** Claudio Leubler **Function** Laboratory Technician

Approved by: **Name** Katja Pokovic **Function** Technical Manager

Signature

Issued: May 20, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	15 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	835 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	41.5	0.90 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	40.2 ± 6 %	0.94 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	2.40 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	9.23 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	1.54 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	5.98 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	55.2	0.97 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	56.6 ± 6 %	1.02 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	2.48 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	9.61 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	1.62 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	6.31 W/kg ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.5 Ω - 2.5 $j\Omega$
Return Loss	- 29.2 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.1 Ω - 5.1 $j\Omega$
Return Loss	- 24.4 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.390 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	June 29, 2010

DASY5 Validation Report for Head TSL

Date: 16.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d117

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 0.94 \text{ S/m}$; $\epsilon_r = 40.2$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.22, 6.22, 6.22); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 56.42 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.63 W/kg

SAR(1 g) = 2.4 W/kg; SAR(10 g) = 1.54 W/kg

Maximum value of SAR (measured) = 2.82 W/kg

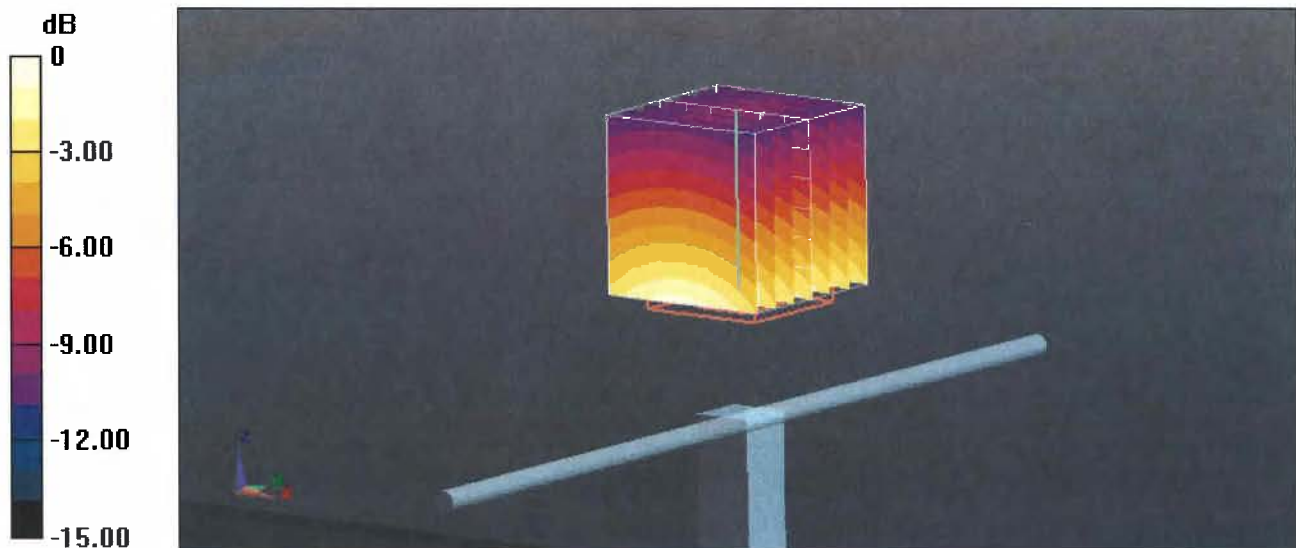


0 dB = 2.82 W/kg = 4.50 dBW/kg

Impedance Measurement Plot for Head TSL

16 May 2014 12:59:07
[CH1] S11 1 U FS 1: 52.523 Ω -2.5176 Ω 75.710 pF 835.000 000 MHz

*
De1
Ca

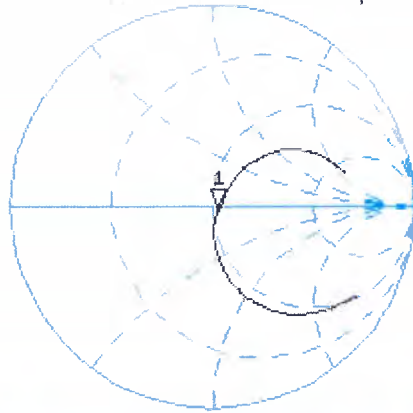

Avg
16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1:-29.168 dB 835.000 000 MHz

Ca

Avg
16

H1d

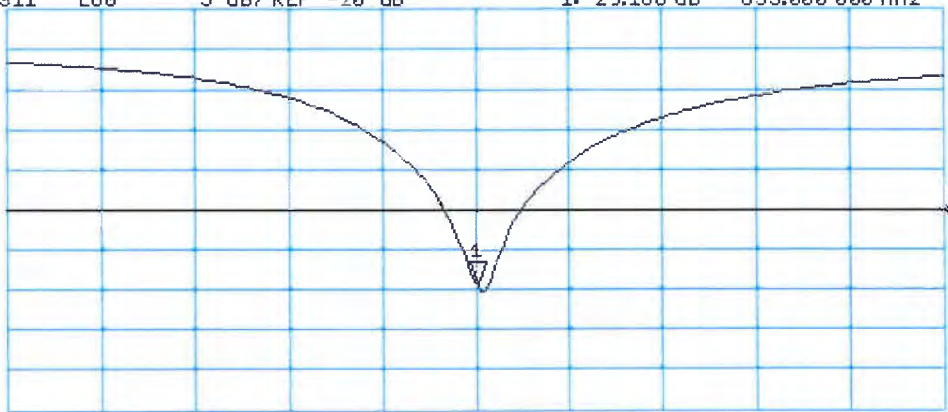

START 635.000 000 MHz

STOP 1 035.000 000 MHz

DASY5 Validation Report for Body TSL

Date: 15.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 835 MHz; Type: D835V2; Serial: D835V2 - SN: 4d117

Communication System: UID 0 - CW; Frequency: 835 MHz

Medium parameters used: $f = 835 \text{ MHz}$; $\sigma = 1.02 \text{ S/m}$; $\epsilon_r = 56.6$; $\rho = 1000 \text{ kg/m}^3$

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(6.09, 6.09, 6.09); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 4.9L; Type: QD000P49AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=15mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: $dx=5\text{mm}$, $dy=5\text{mm}$, $dz=5\text{mm}$

Reference Value = 55.09 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 3.71 W/kg

SAR(1 g) = 2.48 W/kg; SAR(10 g) = 1.62 W/kg

Maximum value of SAR (measured) = 2.90 W/kg

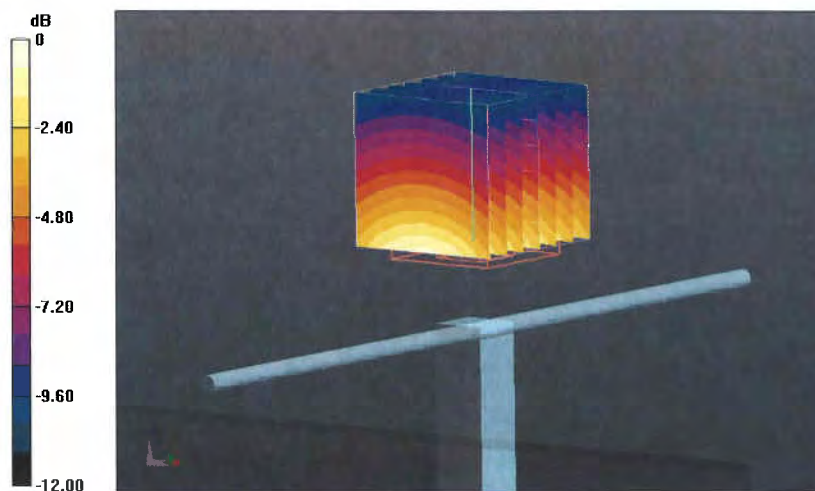


0 dB = 2.90 W/kg = 4.62 dBW/kg

Impedance Measurement Plot for Body TSL

15 May 2014 12:19:23
CH1 S11 1 U FS 2: 47.127 Ω -5.0820 Ω 37.506 pF 835.000 000 MHz

*
De1
CA

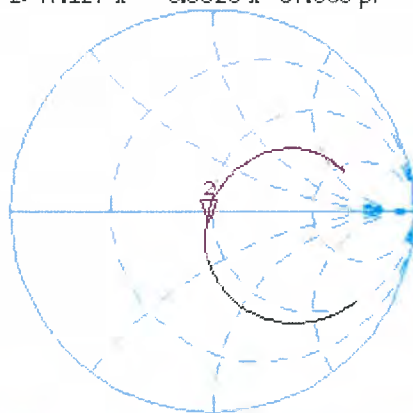

Av9
16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 2:-24.430 dB 835.000 000 MHz

CA

Av9
16

H1d

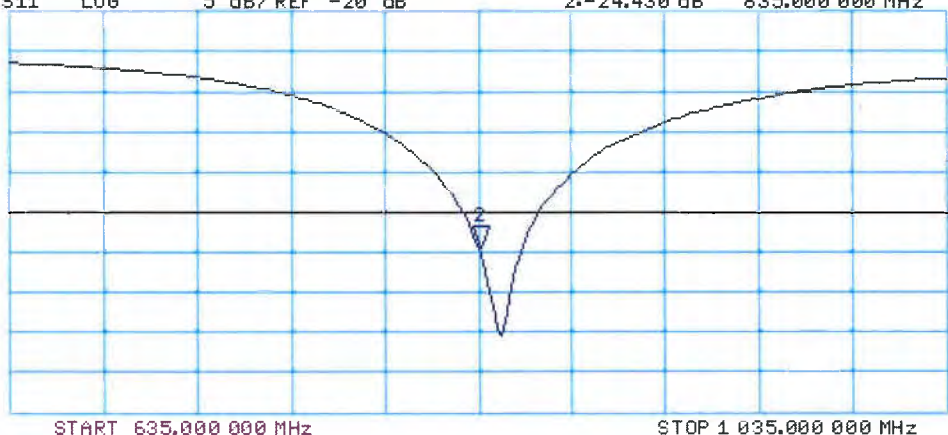



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

**The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates**

Client **UL CCS USA**

Certificate No: **D1900V2-5d043_Nov13**

CALIBRATION CERTIFICATE

Object **D1900V2 - SN: 5d043**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **November 12, 2013**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	04-Apr-13 (No. 217-01736)	Apr-14
Type-N mismatch combination	SN: 5047.3 / 06327	04-Apr-13 (No. 217-01739)	Apr-14
Reference Probe ES3DV3	SN: 3205	28-Dec-12 (No. ES3-3205_Dec12)	Dec-13
DAE4	SN: 601	25-Apr-13 (No. DAE4-601_Apr13)	Apr-14
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-15
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

	Name	Function	Signature
Calibrated by:	Leif Klysner	Laboratory Technician	
Approved by:	Katja Pokovic	Technical Manager	

Issued: November 12, 2013

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

Accreditation No.: **SCS 108**

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:* Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:* The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:* These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:* One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:* SAR measured at the stated antenna input power.
- SAR normalized:* SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:* The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.7
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	1900 MHz \pm 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	40.0	1.40 mho/m
Measured Head TSL parameters	(22.0 \pm 0.2) °C	39.8 \pm 6 %	1.39 mho/m \pm 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	10.0 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	40.1 W/kg \pm 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	5.26 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	21.1 W/kg \pm 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	53.3	1.52 mho/m
Measured Body TSL parameters	(22.0 \pm 0.2) °C	53.4 \pm 6 %	1.51 mho/m \pm 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	9.70 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	39.0 W/kg \pm 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.18 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	20.8 W/kg \pm 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	51.9 Ω + 4.7 j Ω
Return Loss	- 26.1 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	47.7 Ω + 5.6 j Ω
Return Loss	- 24.2 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.194 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	December 16, 2003

DASY5 Validation Report for Head TSL

Date: 12.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d043

Communication System: UID 0 - CW ; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.39$ S/m; $\epsilon_r = 39.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.98, 4.98, 4.98); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 93.658 V/m; Power Drift = 0.06 dB

Peak SAR (extrapolated) = 18.3 W/kg

SAR(1 g) = 10 W/kg; SAR(10 g) = 5.26 W/kg

Maximum value of SAR (measured) = 12.4 W/kg

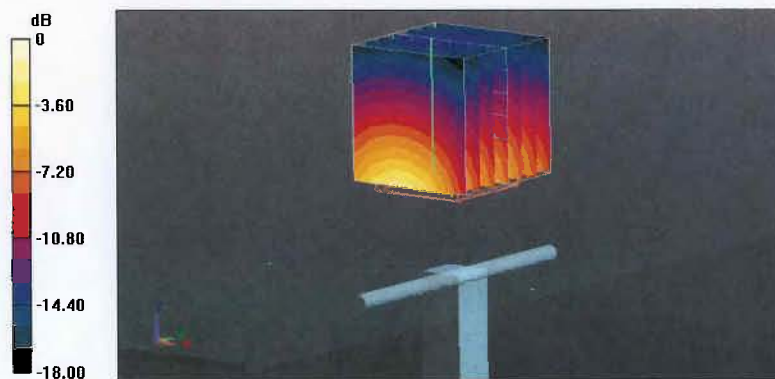


0 dB = 12.4 W/kg = 10.93 dBW/kg

Impedance Measurement Plot for Head TSL

12 Nov 2013 09:06:04

CH1 S11 1 U FS 1: 51.922 Δ 4.6875 Δ 392.65 pH 1 900.000 000 MHz

*
Del
CA

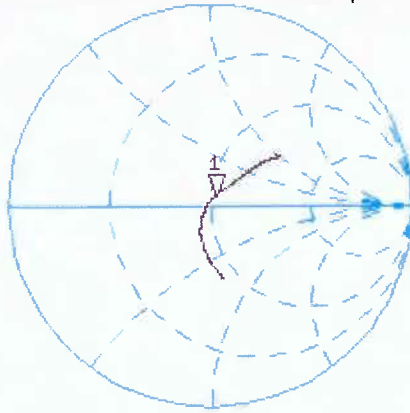

Avg
16


H1 d

CH2 S11 LOG 5 dB/REF -20 dB 1: -26.067 dB 1 900.000 000 MHz

CA

Avg
16

H1 d

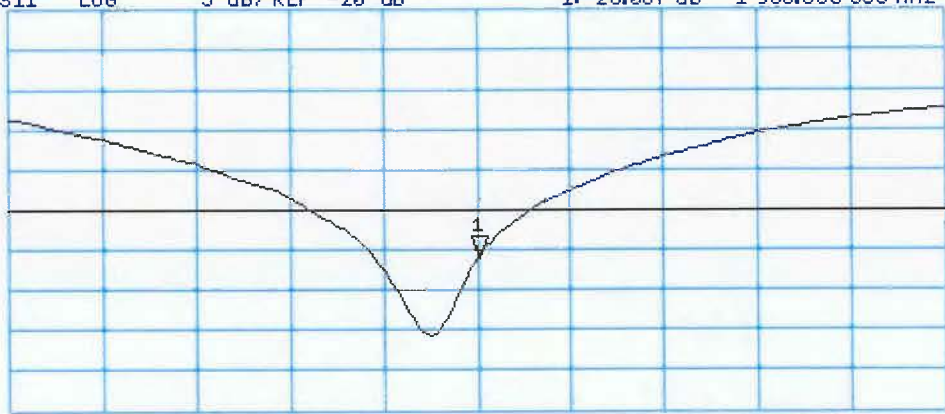

START 1 700.000 000 MHz

STOP 2 100.000 000 MHz

DASY5 Validation Report for Body TSL

Date: 12.11.2013

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 1900 MHz; Type: D1900V2; Serial: D1900V2 - SN: 5d043

Communication System: UID 0 - CW ; Frequency: 1900 MHz

Medium parameters used: $f = 1900$ MHz; $\sigma = 1.51$ S/m; $\epsilon_r = 53.4$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2007)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.6, 4.6, 4.6); Calibrated: 28.12.2012;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 25.04.2013
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.7(1137); SEMCAD X 14.6.10(7164)

Dipole Calibration for Body Tissue/ $P_{in}=250$ mW, $d=10$ mm/Zoom Scan (7x7x7)/Cube 0:

Measurement grid: $dx=5$ mm, $dy=5$ mm, $dz=5$ mm

Reference Value = 93.658 V/m; Power Drift = 0.03 dB

Peak SAR (extrapolated) = 16.6 W/kg

SAR(1 g) = 9.7 W/kg; SAR(10 g) = 5.18 W/kg

Maximum value of SAR (measured) = 12.1 W/kg




0 dB = 12.1 W/kg = 10.83 dBW/kg

Impedance Measurement Plot for Body TSL

12 Nov 2013 09:05:31

CH1 S11 1 U FS 1: 47.674 Ω 5.5703 Ω 466.60 pF 1 900.000 000 MHz

*
Del
CA

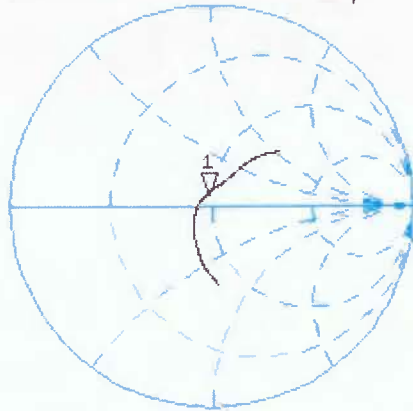

Avg
16


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -24.198 dB 1 900.000 000 MHz

CA

Avg
16

H1d

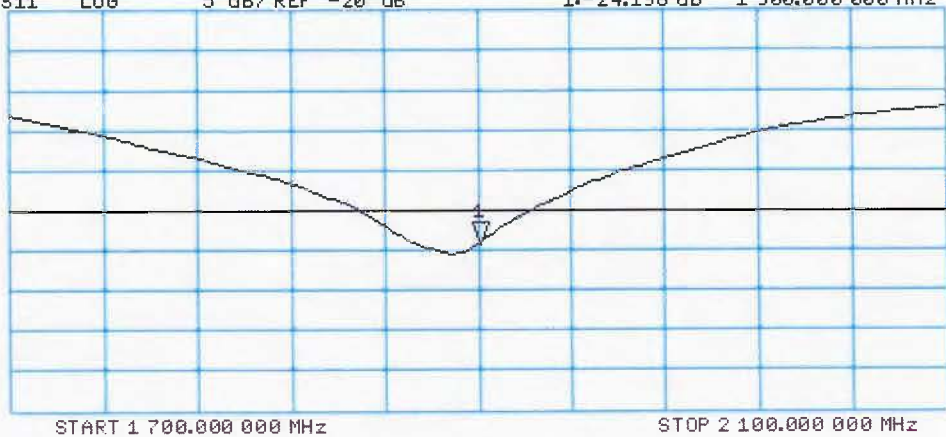



Accredited by the Swiss Accreditation Service (SAS)
The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Client **UL CCS USA**

Certificate No: **D2450V2-706_May14**

CALIBRATION CERTIFICATE

Object **D2450V2 - SN: 706**

Calibration procedure(s) **QA CAL-05.v9
Calibration procedure for dipole validation kits above 700 MHz**

Calibration date: **May 20, 2014**

This calibration certificate documents the traceability to national standards, which realize the physical units of measurements (SI).
The measurements and the uncertainties with confidence probability are given on the following pages and are part of the certificate.

All calibrations have been conducted in the closed laboratory facility: environment temperature (22 ± 3)°C and humidity < 70%.

Calibration Equipment used (M&TE critical for calibration)

Primary Standards	ID #	Cal Date (Certificate No.)	Scheduled Calibration
Power meter EPM-442A	GB37480704	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	US37292783	09-Oct-13 (No. 217-01827)	Oct-14
Power sensor HP 8481A	MY41092317	09-Oct-13 (No. 217-01828)	Oct-14
Reference 20 dB Attenuator	SN: 5058 (20k)	03-Apr-14 (No. 217-01918)	Apr-15
Type-N mismatch combination	SN: 5047.2 / 06327	03-Apr-14 (No. 217-01921)	Apr-15
Reference Probe ES3DV3	SN: 3205	30-Dec-13 (No. ES3-3205_Dec13)	Dec-14
DAE4	SN: 601	30-Apr-14 (No. DAE4-601_Apr14)	Apr-15
Secondary Standards	ID #	Check Date (in house)	Scheduled Check
RF generator R&S SMT-06	100005	04-Aug-99 (in house check Oct-13)	In house check: Oct-16
Network Analyzer HP 8753E	US37390585 S4206	18-Oct-01 (in house check Oct-13)	In house check: Oct-14

Calibrated by: **Name** Claudio Leubler **Function** Laboratory Technician

Signature

Approved by: **Name** Katja Pokovic **Function** Technical Manager

Issued: May 21, 2014

This calibration certificate shall not be reproduced except in full without written approval of the laboratory.



Accredited by the Swiss Accreditation Service (SAS)

The Swiss Accreditation Service is one of the signatories to the EA
Multilateral Agreement for the recognition of calibration certificates

Accreditation No.: **SCS 108**

Glossary:

TSL	tissue simulating liquid
ConvF	sensitivity in TSL / NORM x,y,z
N/A	not applicable or not measured

Calibration is Performed According to the Following Standards:

- IEEE Std 1528-2013, "IEEE Recommended Practice for Determining the Peak Spatial-Averaged Specific Absorption Rate (SAR) in the Human Head from Wireless Communications Devices: Measurement Techniques", June 2013
- IEC 62209-1, "Procedure to measure the Specific Absorption Rate (SAR) for hand-held devices used in close proximity to the ear (frequency range of 300 MHz to 3 GHz)", February 2005
- KDB 865664, "SAR Measurement Requirements for 100 MHz to 6 GHz"

Additional Documentation:

- DASY4/5 System Handbook

Methods Applied and Interpretation of Parameters:

- Measurement Conditions:** Further details are available from the Validation Report at the end of the certificate. All figures stated in the certificate are valid at the frequency indicated.
- Antenna Parameters with TSL:** The dipole is mounted with the spacer to position its feed point exactly below the center marking of the flat phantom section, with the arms oriented parallel to the body axis.
- Feed Point Impedance and Return Loss:** These parameters are measured with the dipole positioned under the liquid filled phantom. The impedance stated is transformed from the measurement at the SMA connector to the feed point. The Return Loss ensures low reflected power. No uncertainty required.
- Electrical Delay:** One-way delay between the SMA connector and the antenna feed point. No uncertainty required.
- SAR measured:** SAR measured at the stated antenna input power.
- SAR normalized:** SAR as measured, normalized to an input power of 1 W at the antenna connector.
- SAR for nominal TSL parameters:** The measured TSL parameters are used to calculate the nominal SAR result.

The reported uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor $k=2$, which for a normal distribution corresponds to a coverage probability of approximately 95%.

Measurement Conditions

DASY system configuration, as far as not given on page 1.

DASY Version	DASY5	V52.8.8
Extrapolation	Advanced Extrapolation	
Phantom	Modular Flat Phantom	
Distance Dipole Center - TSL	10 mm	with Spacer
Zoom Scan Resolution	dx, dy, dz = 5 mm	
Frequency	2450 MHz ± 1 MHz	

Head TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Head TSL parameters	22.0 °C	39.2	1.80 mho/m
Measured Head TSL parameters	(22.0 ± 0.2) °C	38.5 ± 6 %	1.83 mho/m ± 6 %
Head TSL temperature change during test	< 0.5 °C	----	----

SAR result with Head TSL

SAR averaged over 1 cm³ (1 g) of Head TSL	Condition	
SAR measured	250 mW input power	13.4 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	53.0 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Head TSL	condition	
SAR measured	250 mW input power	6.17 W/kg
SAR for nominal Head TSL parameters	normalized to 1W	24.5 W/kg ± 16.5 % (k=2)

Body TSL parameters

The following parameters and calculations were applied.

	Temperature	Permittivity	Conductivity
Nominal Body TSL parameters	22.0 °C	52.7	1.95 mho/m
Measured Body TSL parameters	(22.0 ± 0.2) °C	50.8 ± 6 %	2.03 mho/m ± 6 %
Body TSL temperature change during test	< 0.5 °C	----	----

SAR result with Body TSL

SAR averaged over 1 cm³ (1 g) of Body TSL	Condition	
SAR measured	250 mW input power	12.9 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	50.2 W/kg ± 17.0 % (k=2)

SAR averaged over 10 cm³ (10 g) of Body TSL	condition	
SAR measured	250 mW input power	5.94 W/kg
SAR for nominal Body TSL parameters	normalized to 1W	23.4 W/kg ± 16.5 % (k=2)

Appendix

Antenna Parameters with Head TSL

Impedance, transformed to feed point	52.5 Ω + 4.8 j Ω
Return Loss	- 25.6 dB

Antenna Parameters with Body TSL

Impedance, transformed to feed point	48.4 Ω + 5.6 j Ω
Return Loss	- 24.5 dB

General Antenna Parameters and Design

Electrical Delay (one direction)	1.143 ns
----------------------------------	----------

After long term use with 100W radiated power, only a slight warming of the dipole near the feedpoint can be measured.

The dipole is made of standard semirigid coaxial cable. The center conductor of the feeding line is directly connected to the second arm of the dipole. The antenna is therefore short-circuited for DC-signals. On some of the dipoles, small end caps are added to the dipole arms in order to improve matching when loaded according to the position as explained in the "Measurement Conditions" paragraph. The SAR data are not affected by this change. The overall dipole length is still according to the Standard.

No excessive force must be applied to the dipole arms, because they might bend or the soldered connections near the feedpoint may be damaged.

Additional EUT Data

Manufactured by	SPEAG
Manufactured on	May 28, 2002

DASY5 Validation Report for Head TSL

Date: 20.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 706

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 1.83$ S/m; $\epsilon_r = 38.5$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.53, 4.53, 4.53); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (front); Type: QD000P50AA; Serial: 1001
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Head Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:



Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 101.6 V/m; Power Drift = 0.04 dB

Peak SAR (extrapolated) = 27.8 W/kg

SAR(1 g) = 13.4 W/kg; SAR(10 g) = 6.17 W/kg

Maximum value of SAR (measured) = 17.6 W/kg

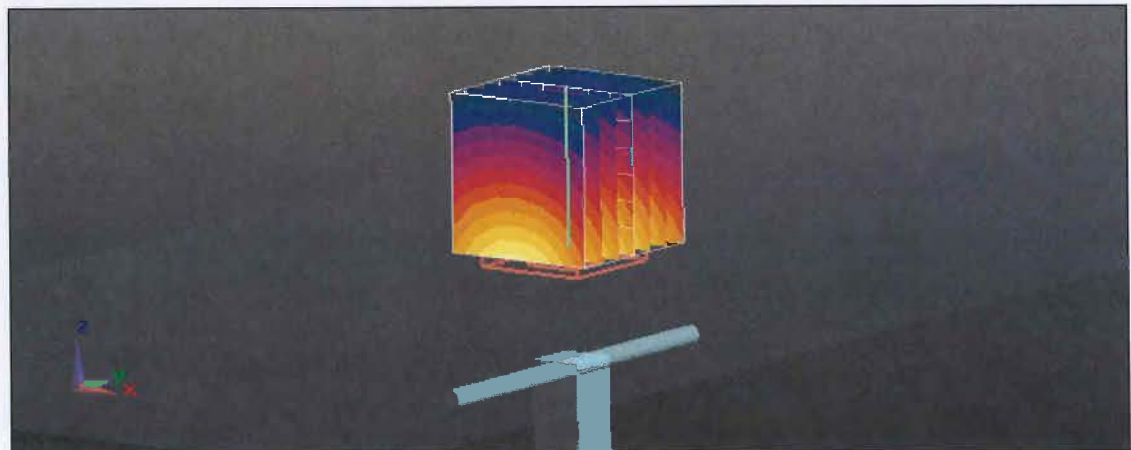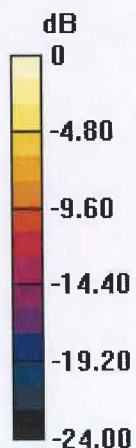

0 dB = 17.6 W/kg = 12.46 dBW/kg


Impedance Measurement Plot for Head TSL

12 May 2014 15:41:29

CH1 S11 1 U FS

1: 52.533 Ω 4.7617 Δ 303.33 pF 2 450.000 000 MHz

*
De1
Cor

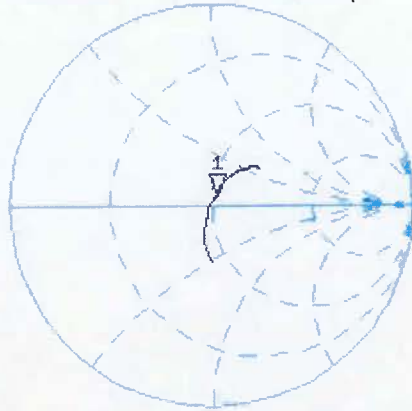

Avg
16

H1d


CH2 S11 LOG 5 dB/REF -20 dB 1:-25.587 dB 2 450.000 000 MHz

De1

Cor

Avg
16

H1d

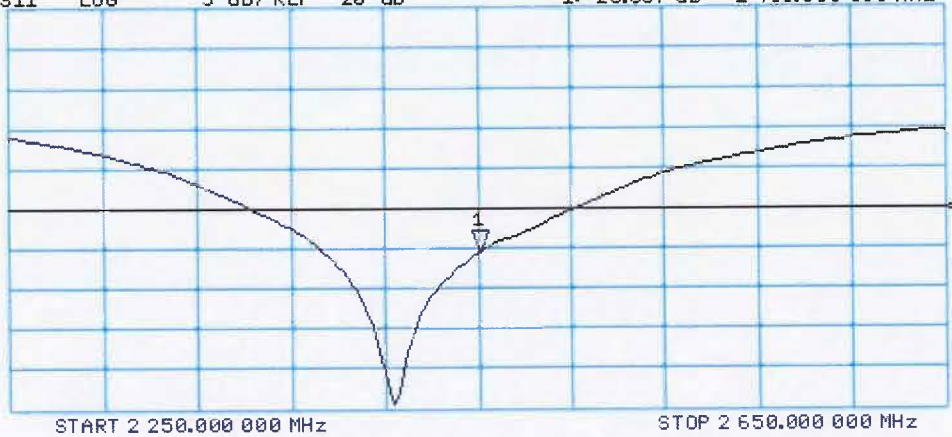

DASY5 Validation Report for Body TSL

Date: 20.05.2014

Test Laboratory: SPEAG, Zurich, Switzerland

DUT: Dipole 2450 MHz; Type: D2450V2; Serial: D2450V2 - SN: 706

Communication System: UID 0 - CW; Frequency: 2450 MHz

Medium parameters used: $f = 2450$ MHz; $\sigma = 2.03$ S/m; $\epsilon_r = 50.8$; $\rho = 1000$ kg/m³

Phantom section: Flat Section

Measurement Standard: DASY5 (IEEE/IEC/ANSI C63.19-2011)

DASY52 Configuration:

- Probe: ES3DV3 - SN3205; ConvF(4.35, 4.35, 4.35); Calibrated: 30.12.2013;
- Sensor-Surface: 3mm (Mechanical Surface Detection)
- Electronics: DAE4 Sn601; Calibrated: 30.04.2014
- Phantom: Flat Phantom 5.0 (back); Type: QD000P50AA; Serial: 1002
- DASY52 52.8.8(1222); SEMCAD X 14.6.10(7331)

Dipole Calibration for Body Tissue/Pin=250 mW, d=10mm/Zoom Scan (7x7x7)/Cube 0:


Measurement grid: dx=5mm, dy=5mm, dz=5mm

Reference Value = 94.57 V/m; Power Drift = 0.01 dB

Peak SAR (extrapolated) = 27.0 W/kg

SAR(1 g) = 12.9 W/kg; SAR(10 g) = 5.94 W/kg

Maximum value of SAR (measured) = 17.0 W/kg

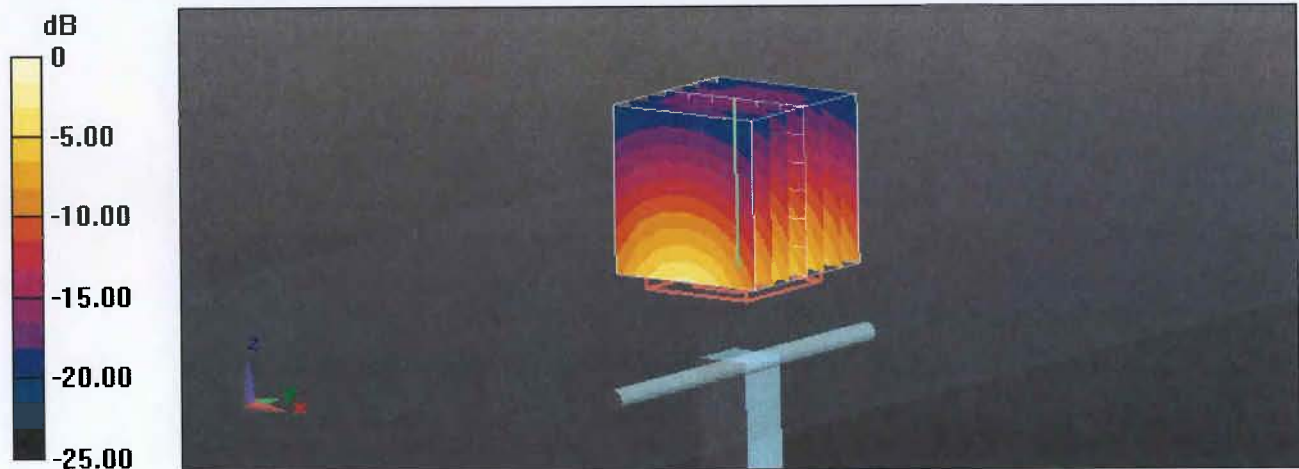

Impedance Measurement Plot for Body TSL


12 May 2014 15:40:14

CH1 S11 1 U FS

1: 48.400 Δ 5.6211 Δ 365.15 pF

2 450.000 000 MHz

*
De1
Cor

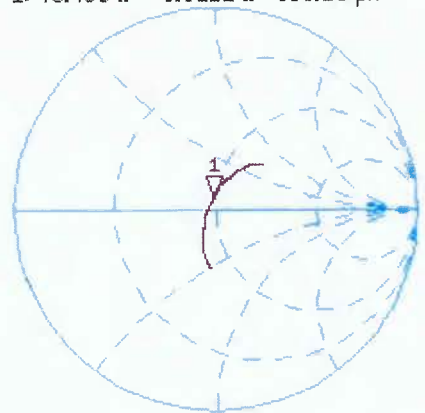

Avg
15


H1d

CH2 S11 LOG 5 dB/REF -20 dB 1: -24.535 dB 2 450.000 000 MHz

De1
Cor

Avg
15

H1d

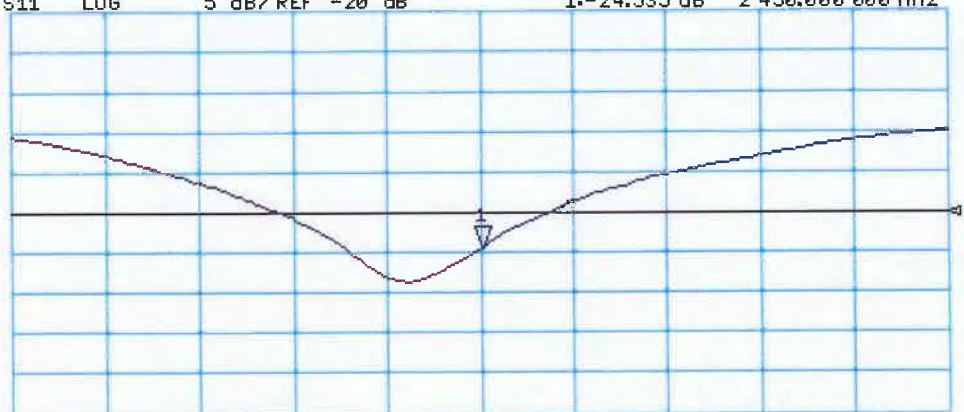

START 2 250.000 000 MHz

STOP 2 650.000 000 MHz